


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:56:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

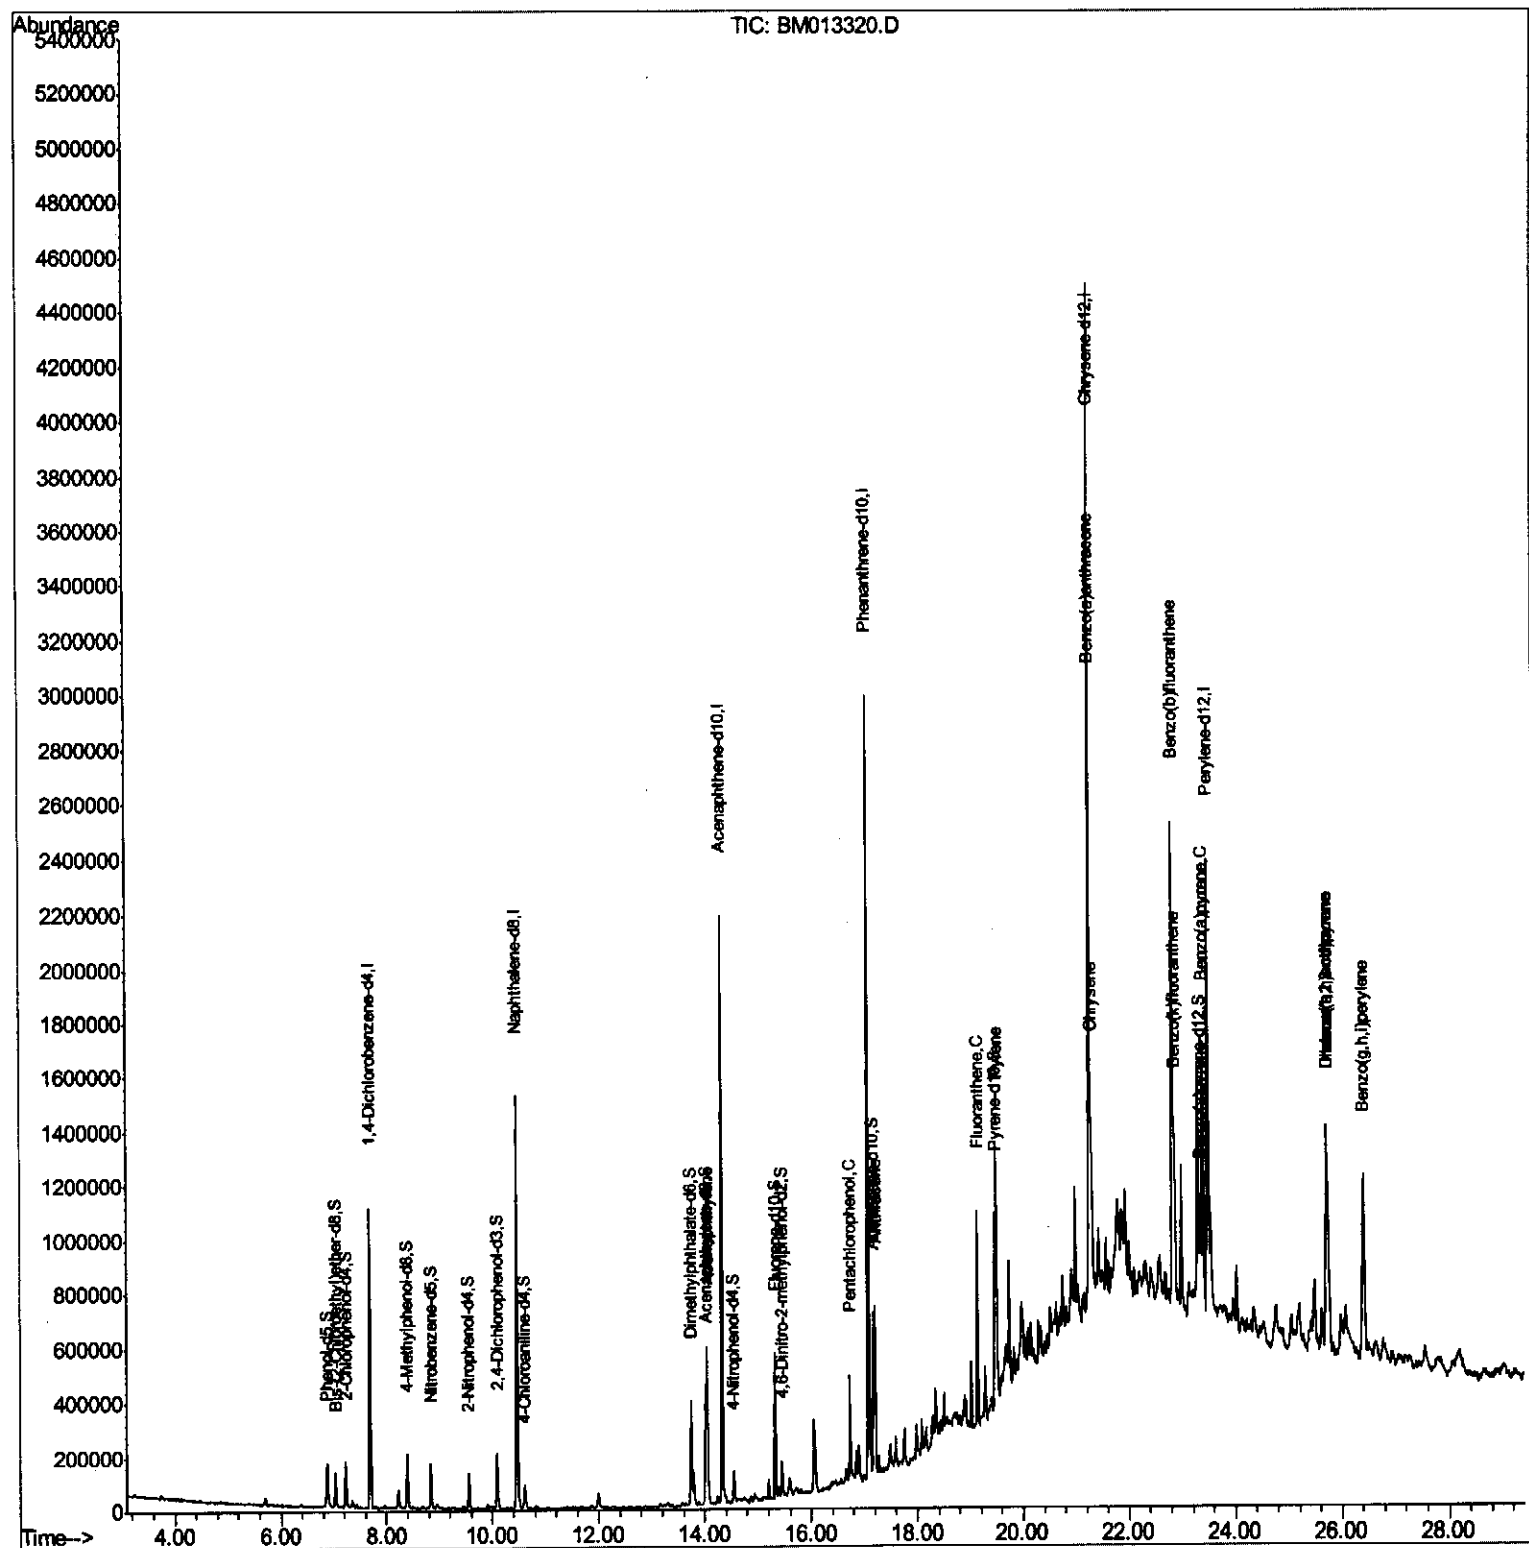




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 02:15:03 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

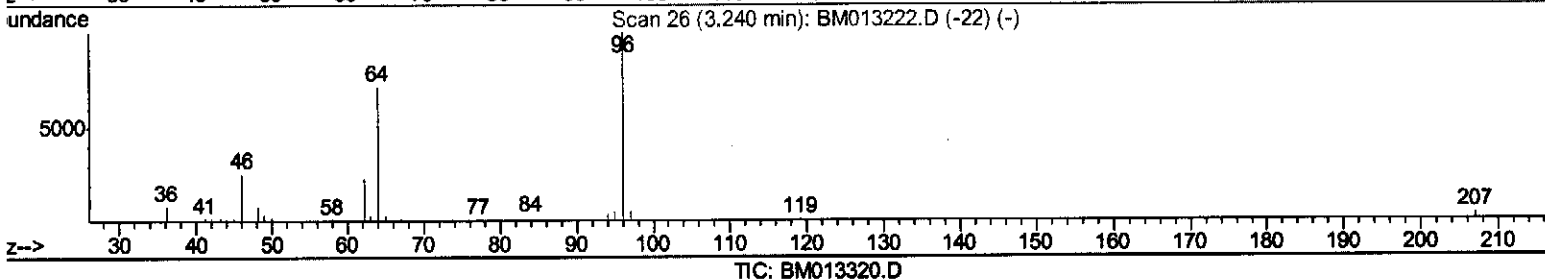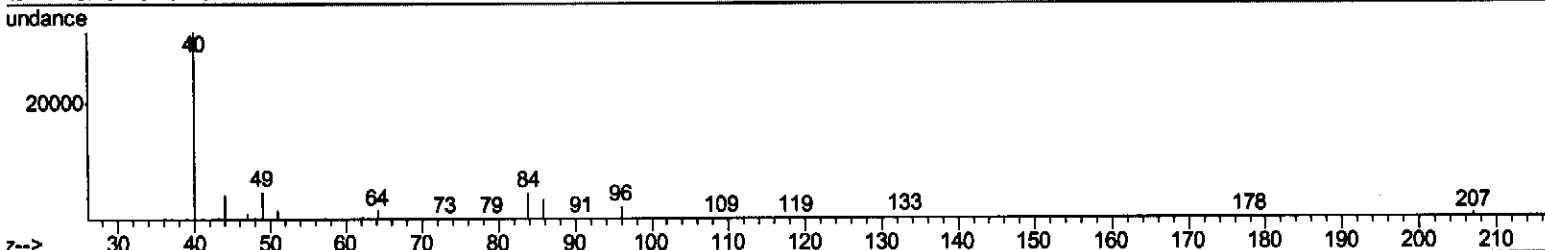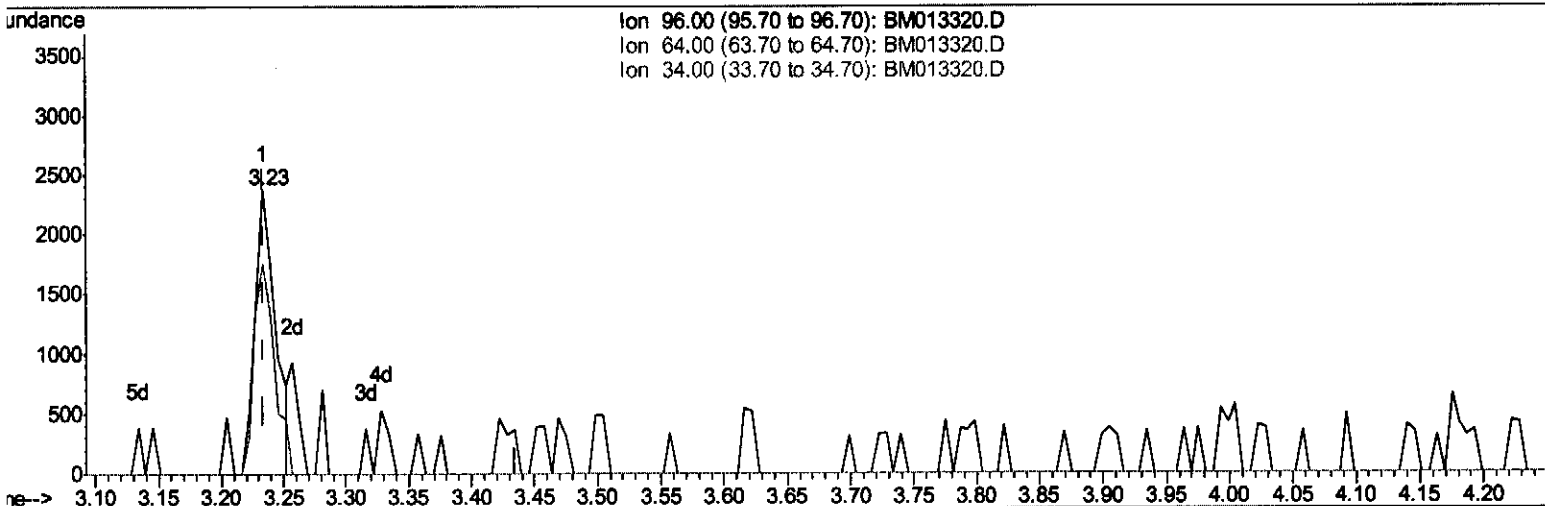

(3) 1,4-Dioxane-d8 (S)

3.234min (-0.001) 0.48ng/uL

response 2717

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	73.57
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 02:15:03 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

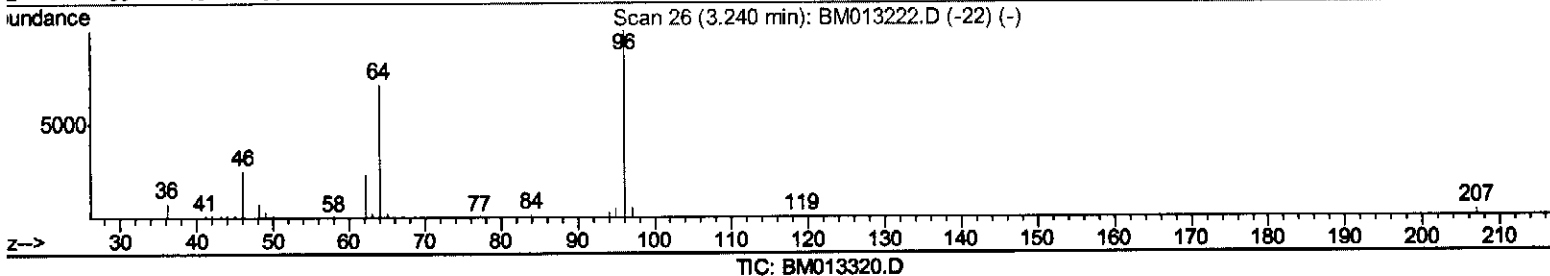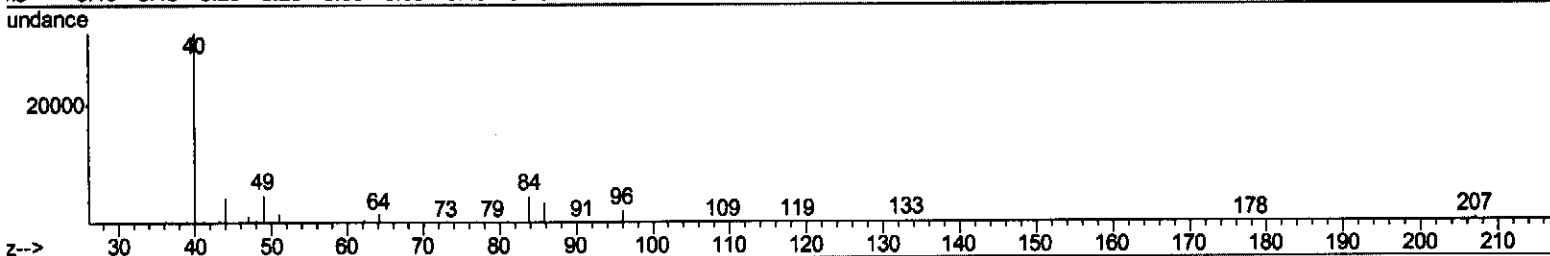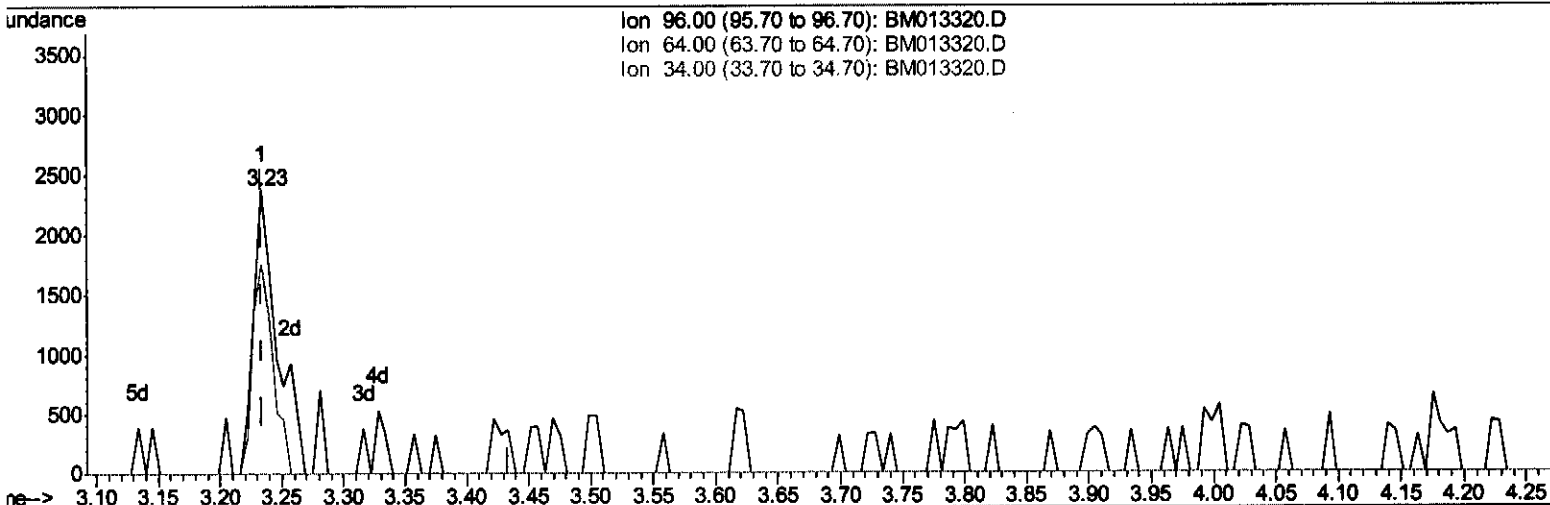

(3) 1,4-Dioxane-d8 (S)

3.234min (-0.001) 0.56ng/uL m

response 3198

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	62.51
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:52:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

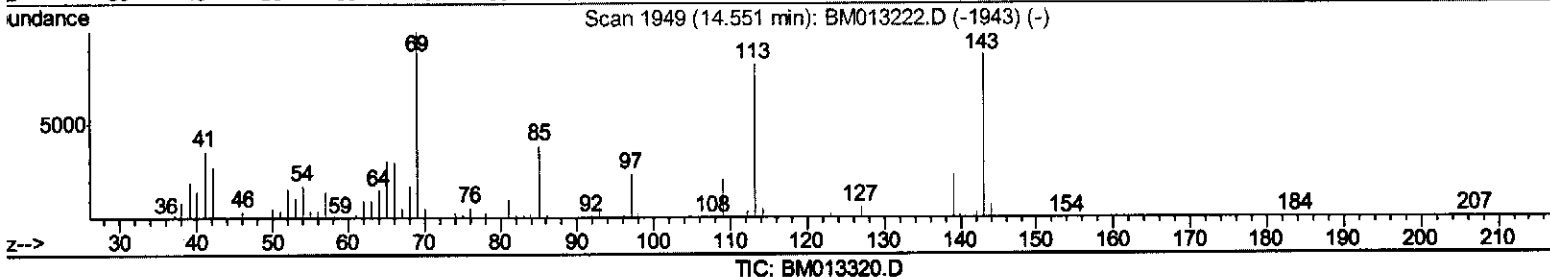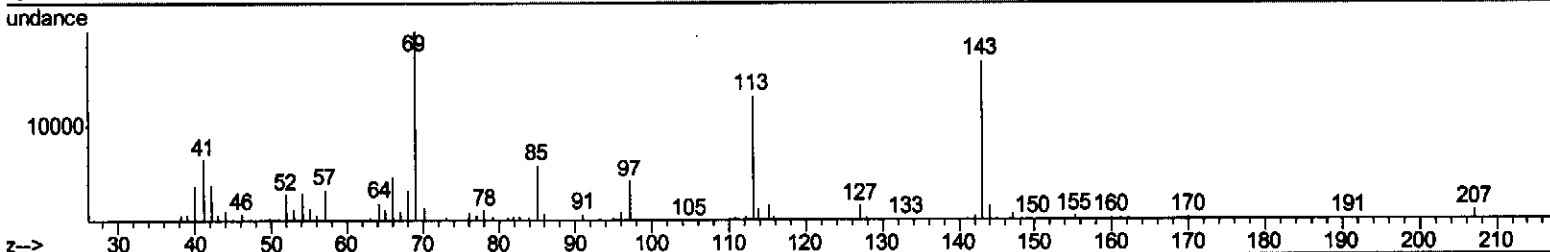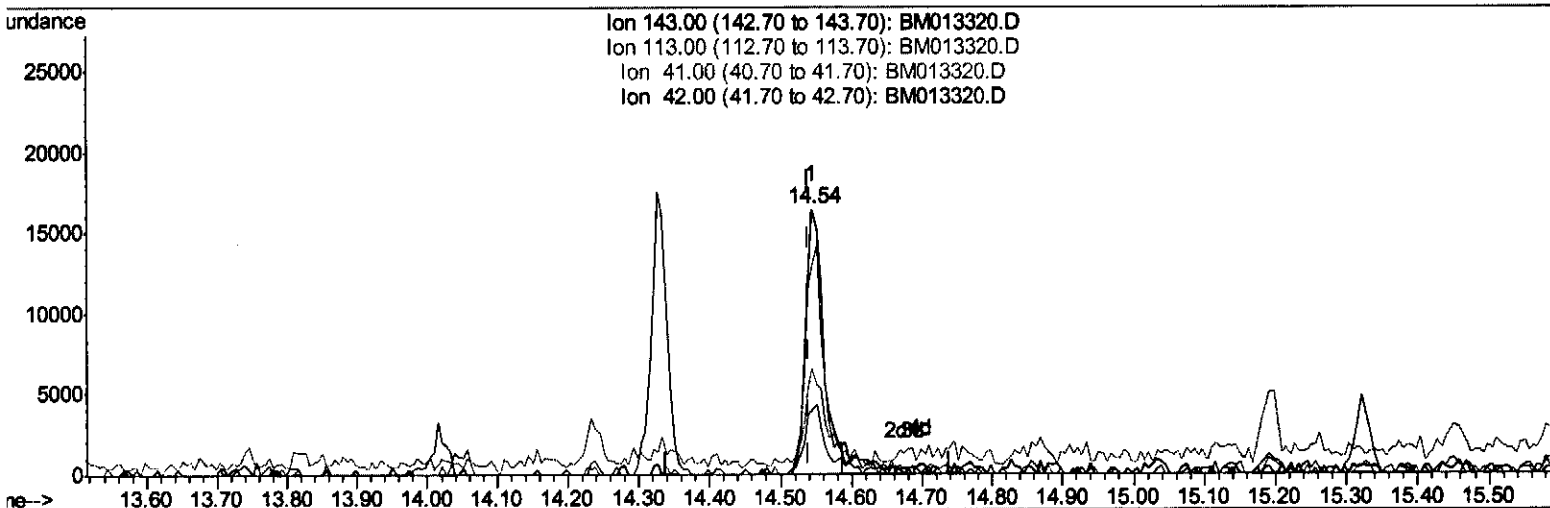

(51) 4-Nitrophenol-d4 (S)

14.545min (+0.005) 2.57ng/ul

response 28830

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	78.45#
41.00	34.80	39.63
42.00	20.50	23.83




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:52:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

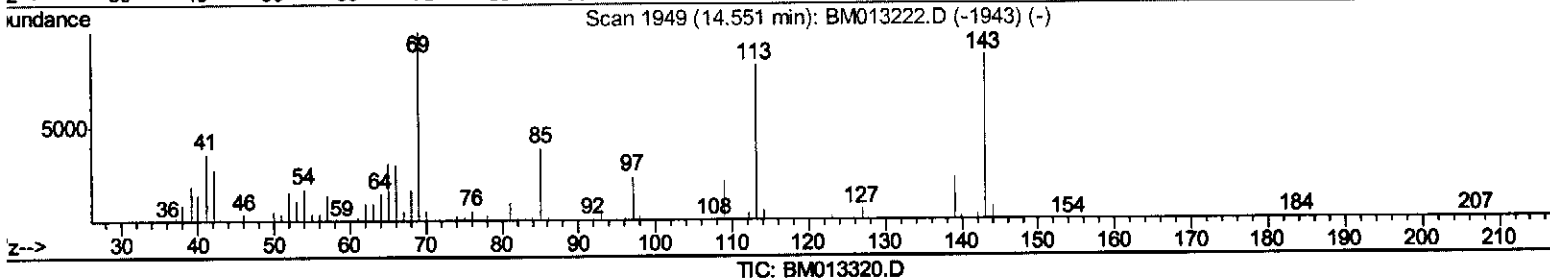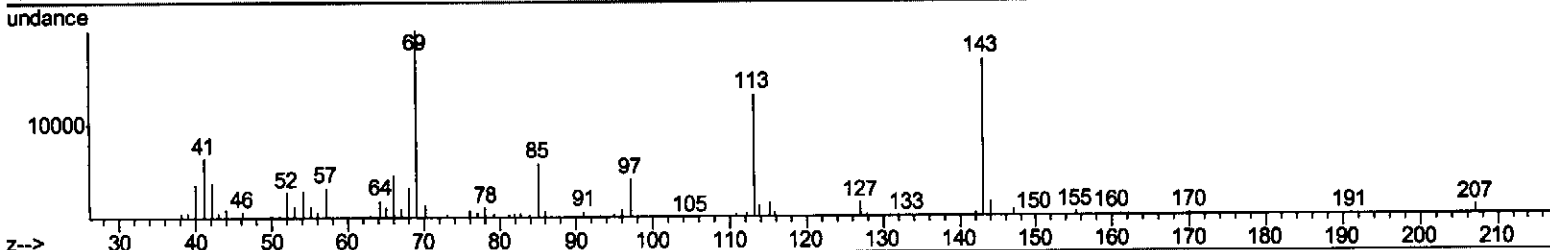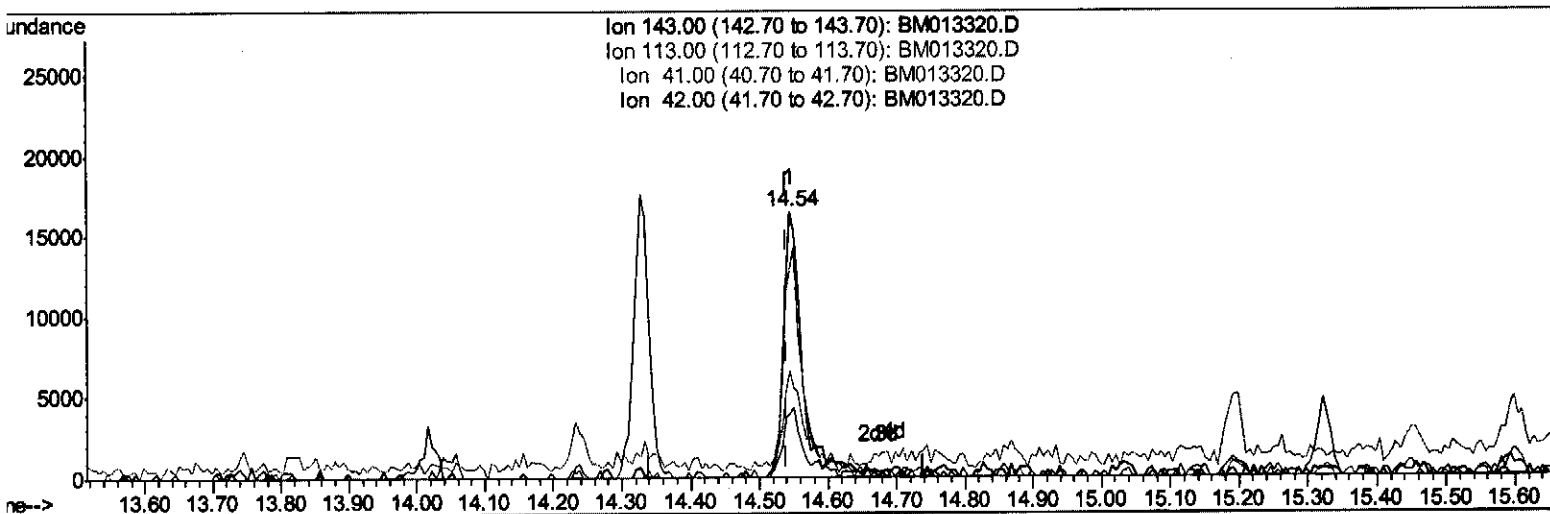

(51) 4-Nitrophenol-d4 (S)

14.545min (+0.005) 2.85ng/ul m

response 32022

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	78.45#
41.00	34.80	39.63
42.00	20.50	23.83




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

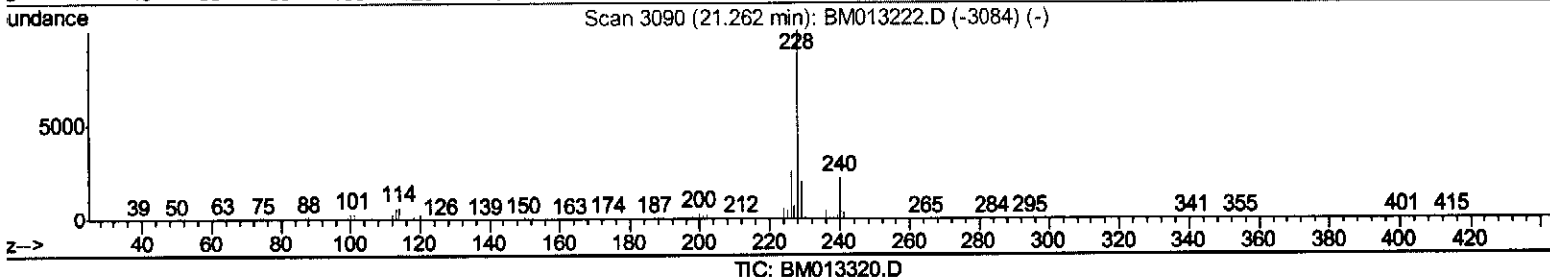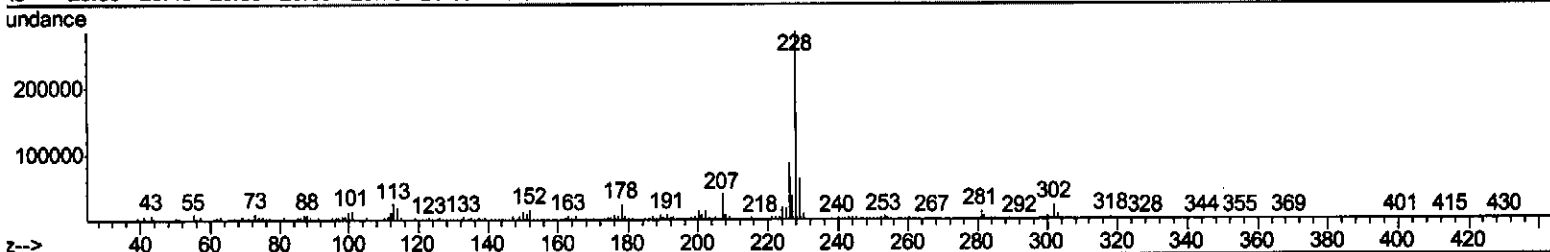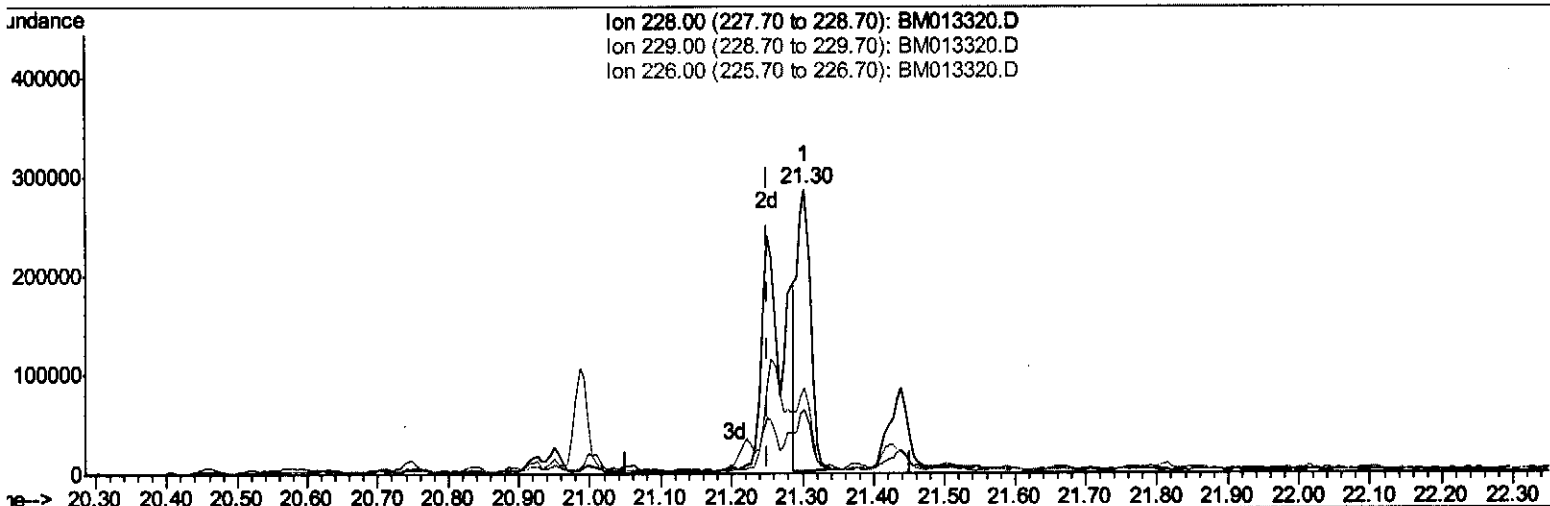

(80) Benzo(a)anthracene

21.303min (+0.052) 3.83ng/ul

response 379531

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	22.31
226.00	26.70	29.91
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

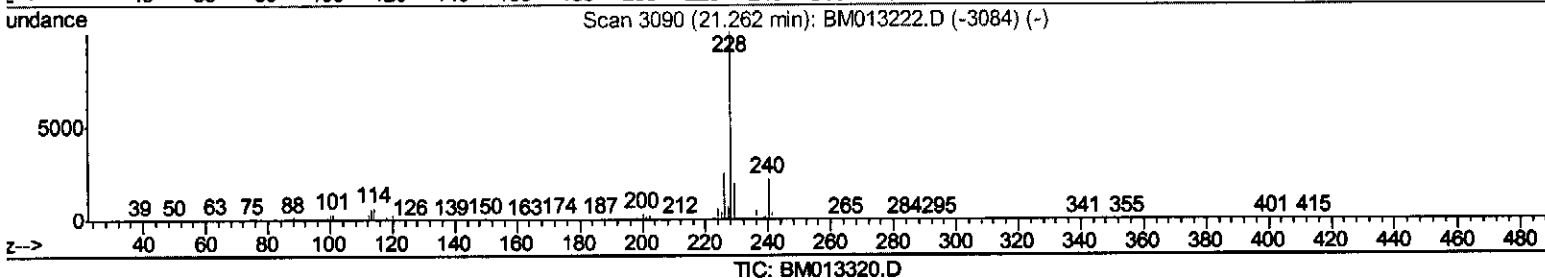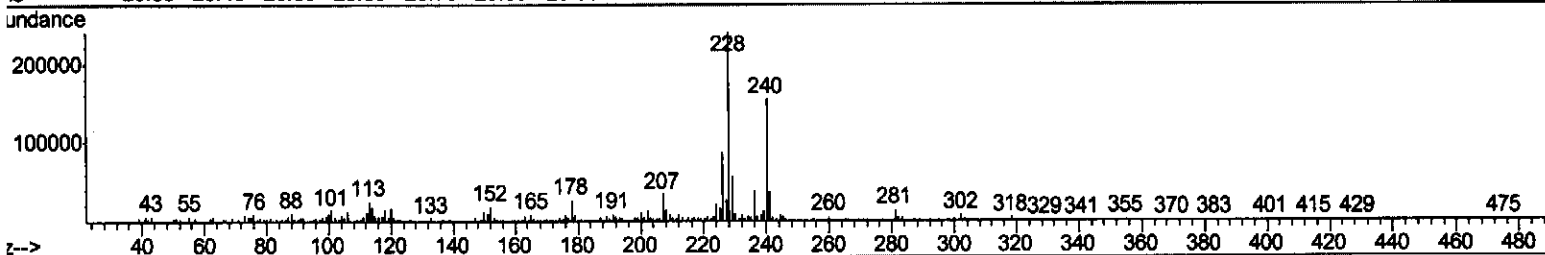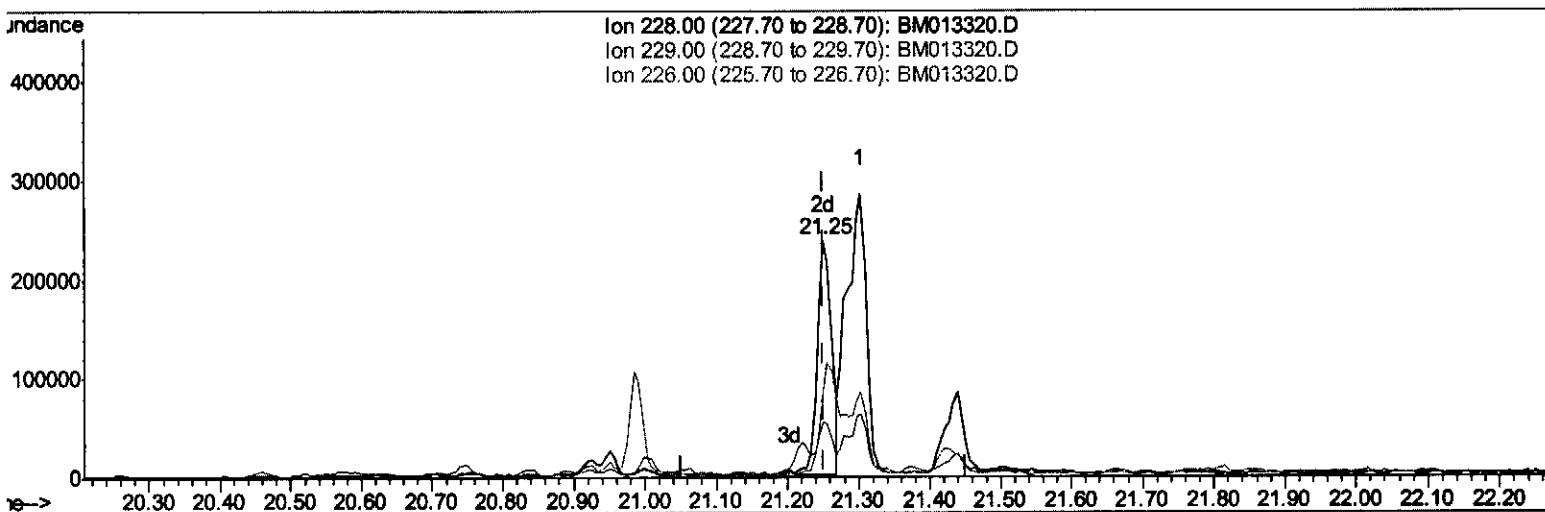

(80) Benzo(a)anthracene

21.250min (-0.001) 3.37ng/ul *5412/15/12*

response 334196

Ion	Exp%	Act%
228.00	100	100
229.00	19.20	23.36#
226.00	26.70	36.17#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

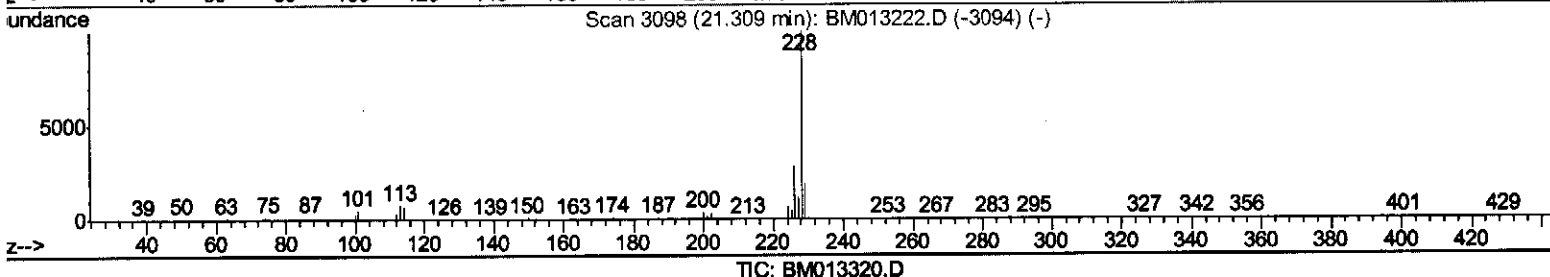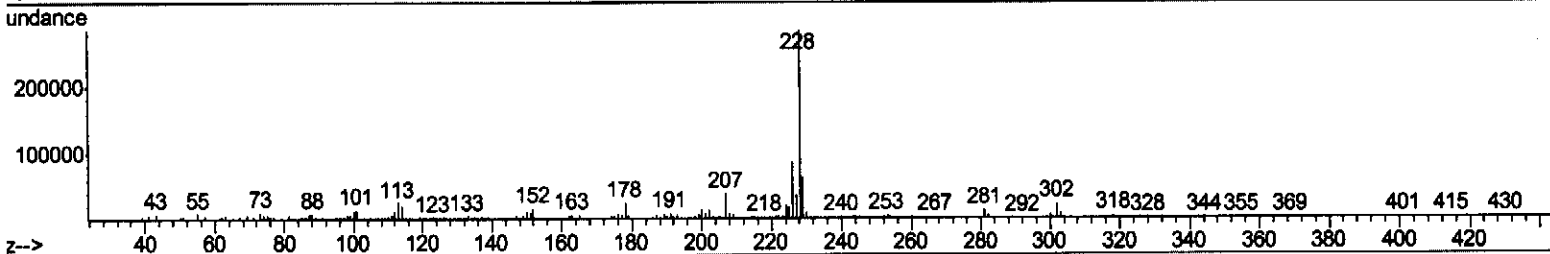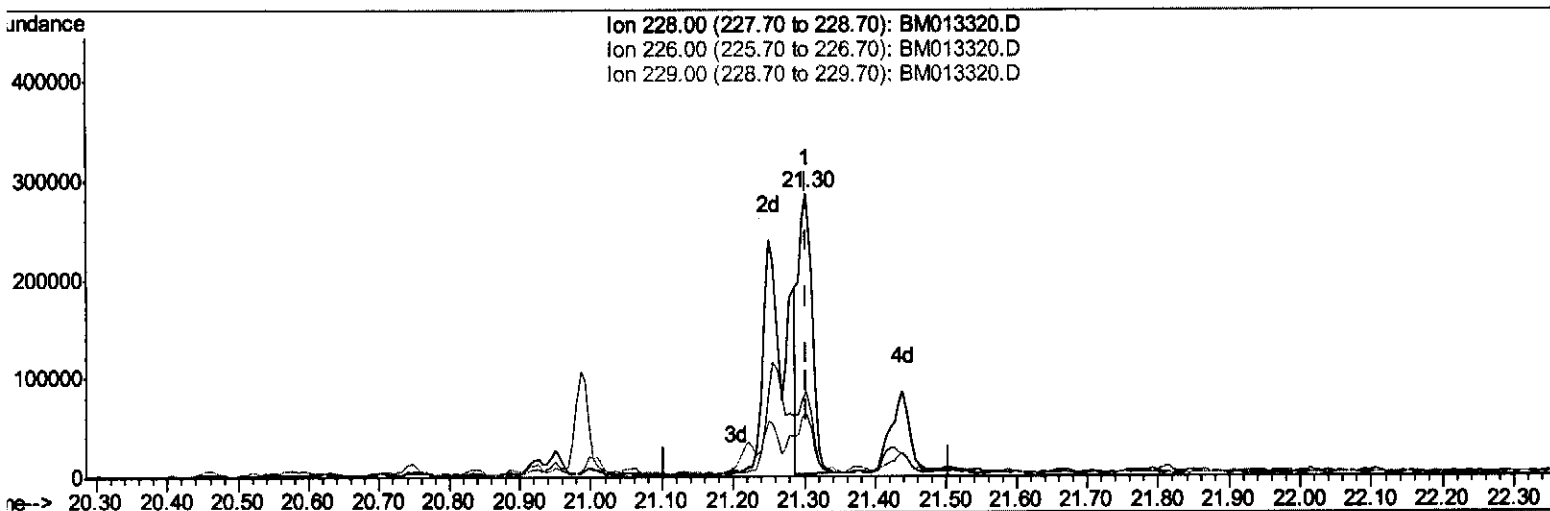

(82) Chrysene

21.303min (-0.001) 4.12ng/ul

response 379531

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	29.91
229.00	19.40	22.31
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration :

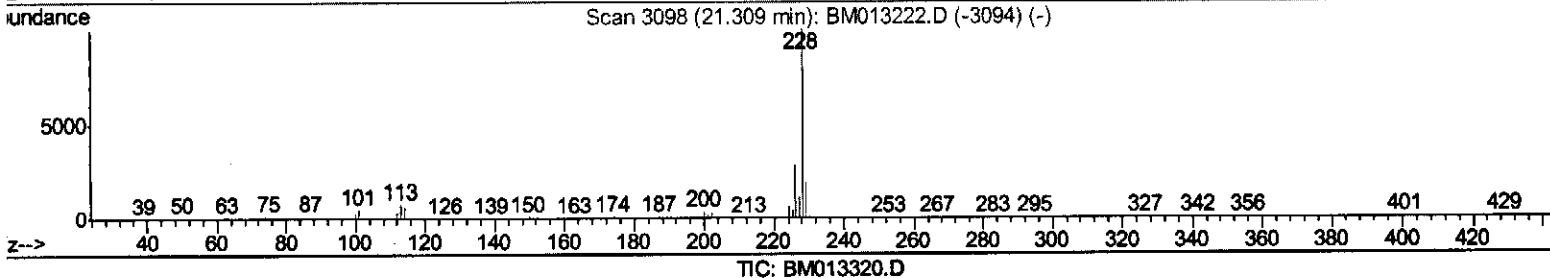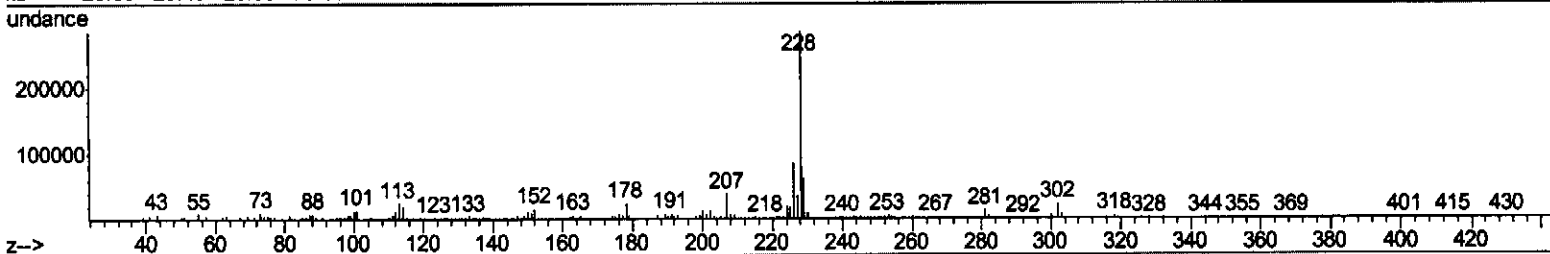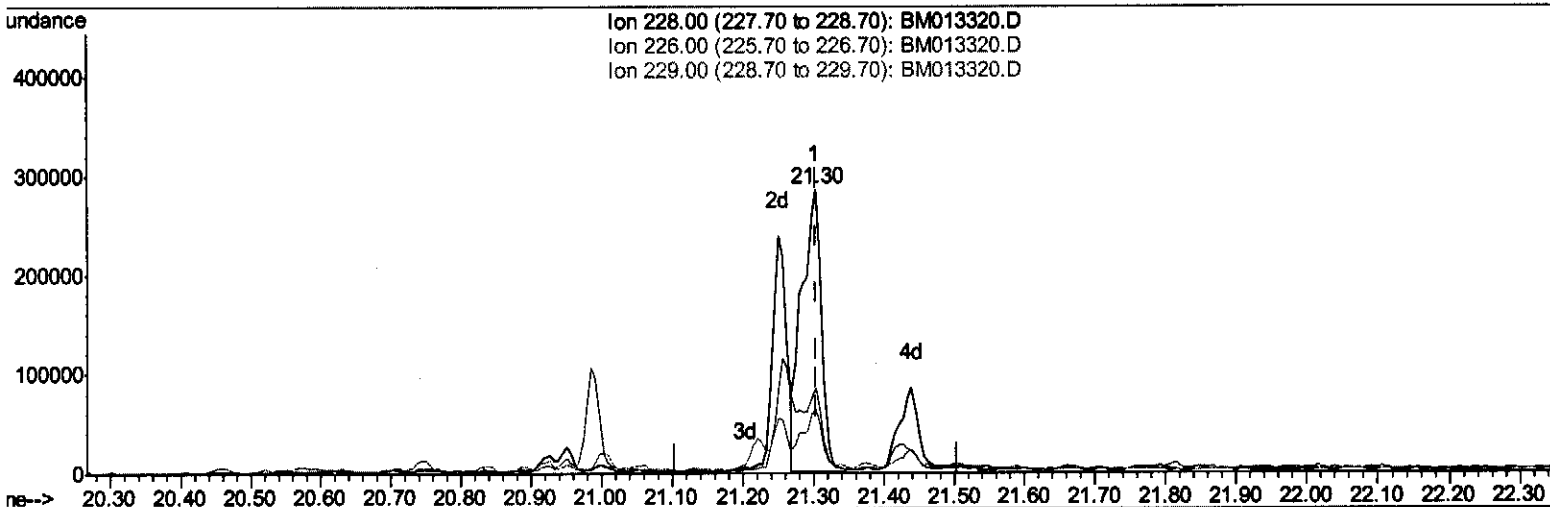

(82) Chrysene

21.303min (-0.001) 6.01ng/ul m

response 552556

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	29.91
229.00	19.40	22.31
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

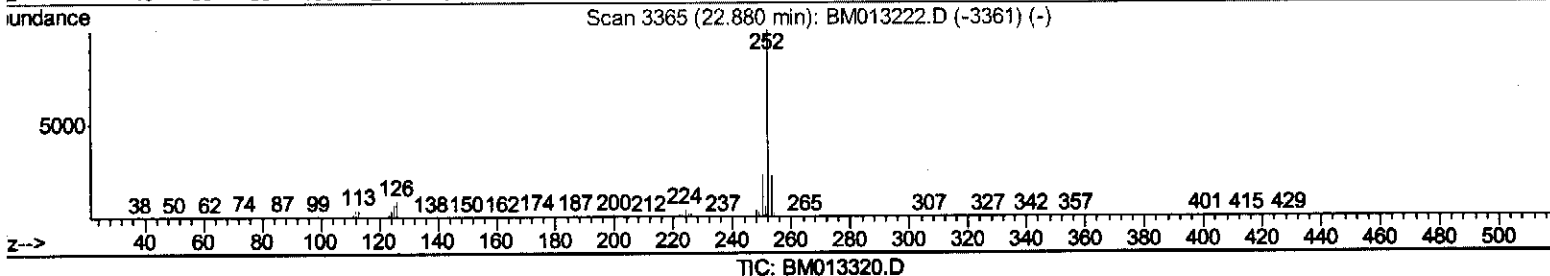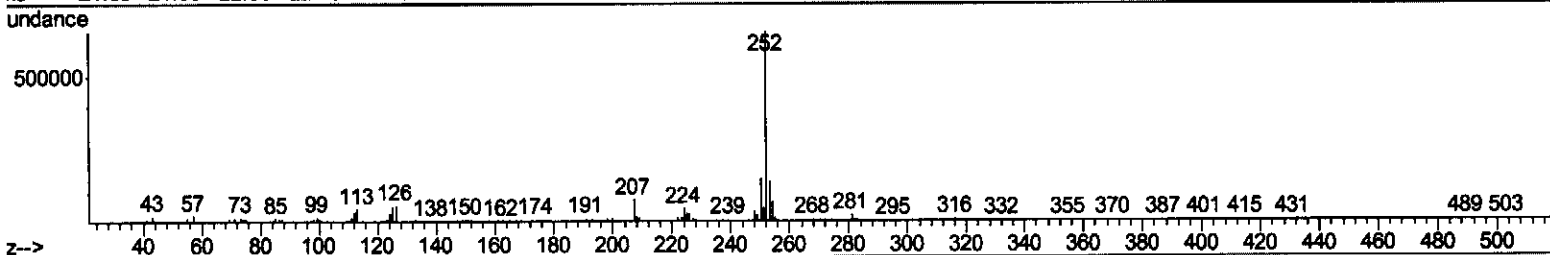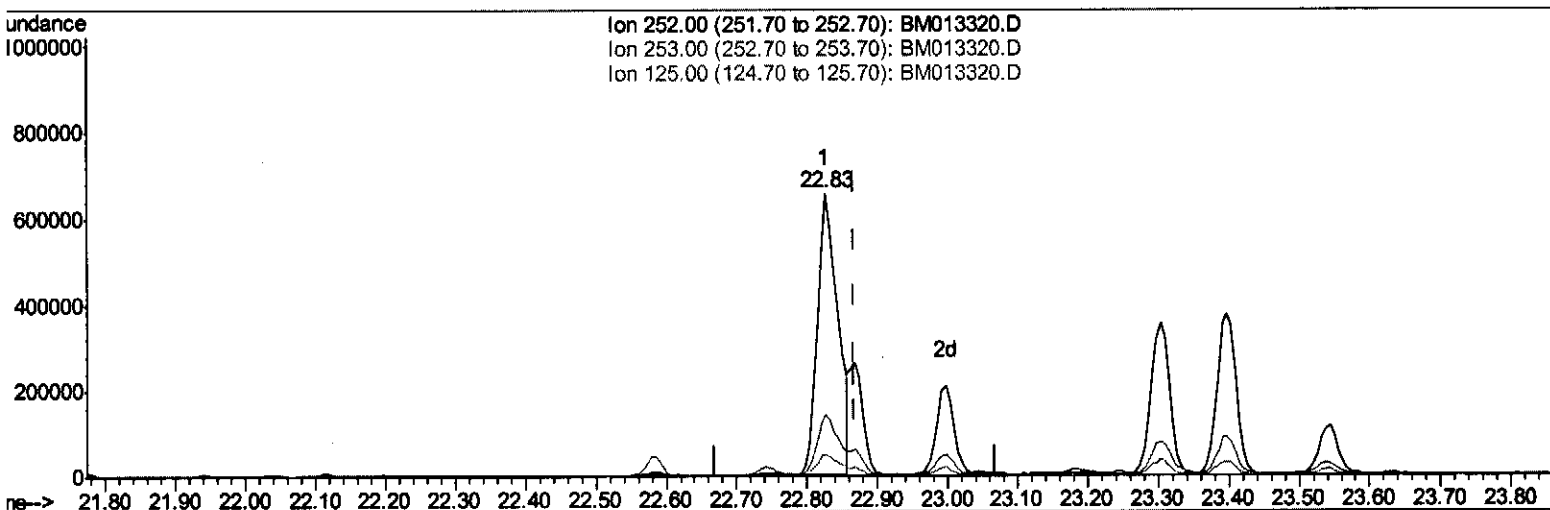

(86) Benzo(k)fluoranthene

22.827min (-0.042) 16.86ng/ul

response 1327936

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.63
125.00	4.30	7.63#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

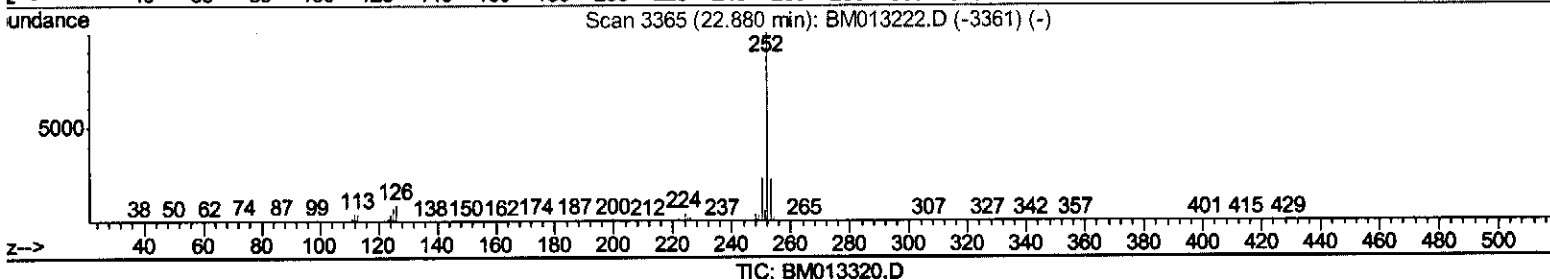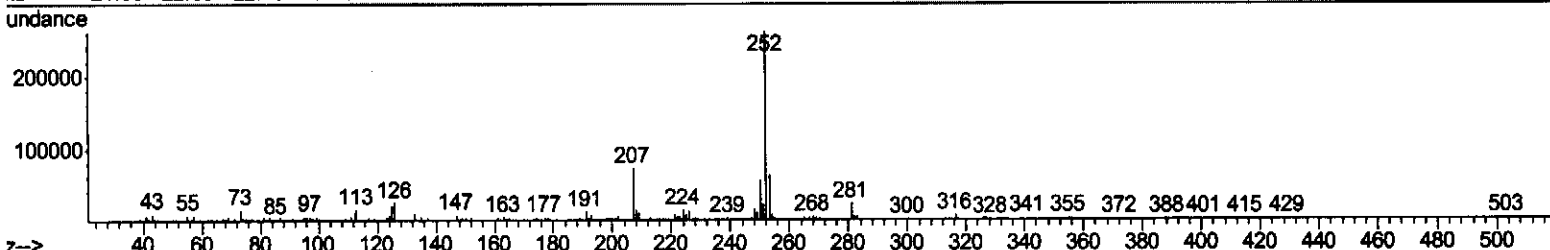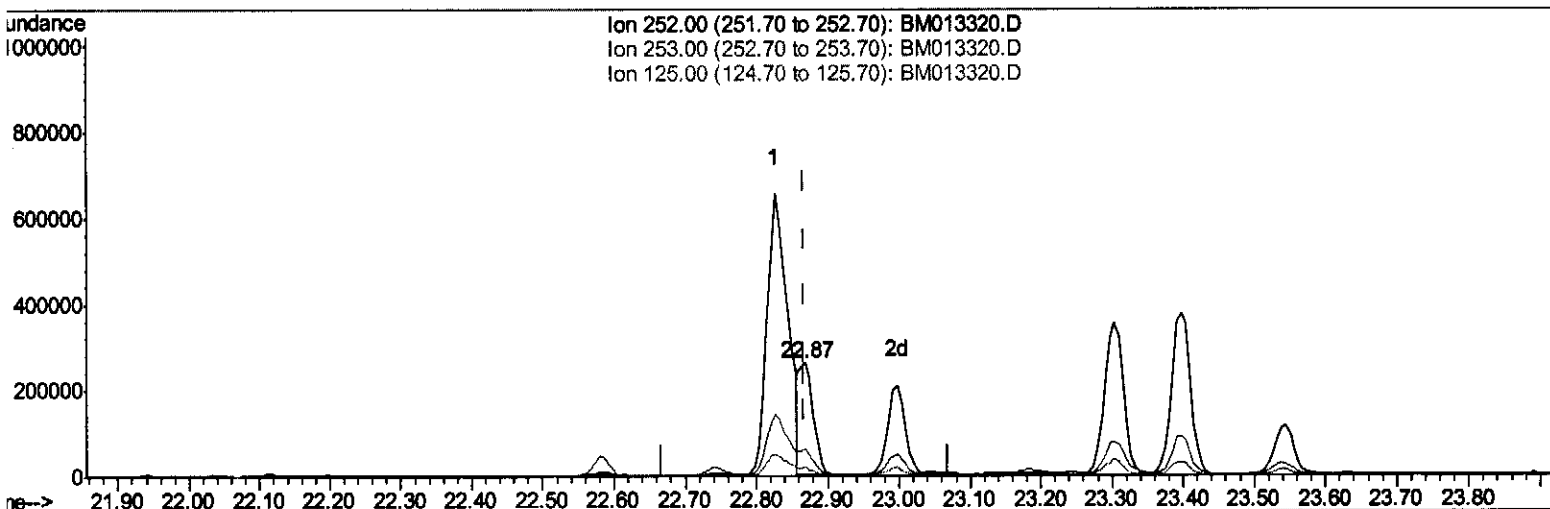

(86) Benzo(k)fluoranthene

22.868min (-0.001) 4.40ng/ul m

response 346373

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.19
125.00	4.30	7.79#
0.00	0.00	0.00

Handwritten signature: Jy 12/15/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

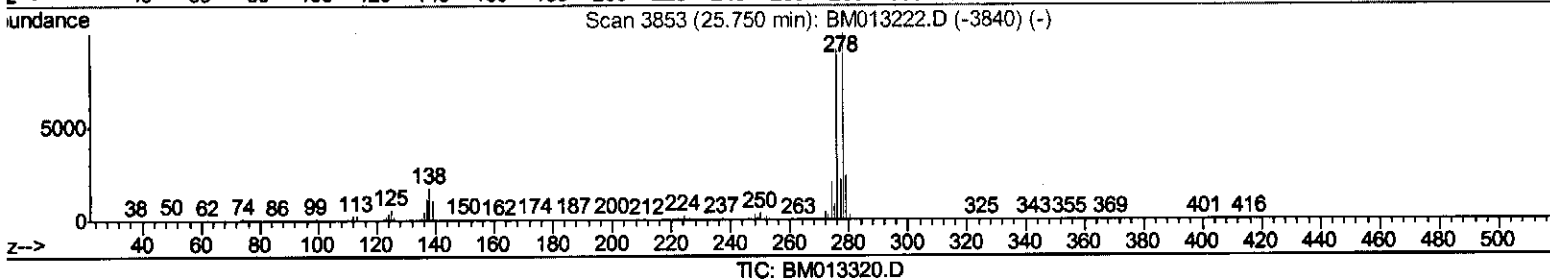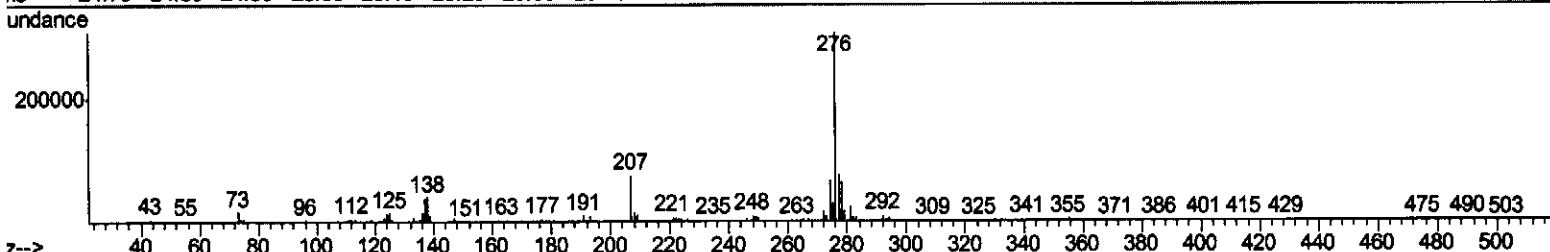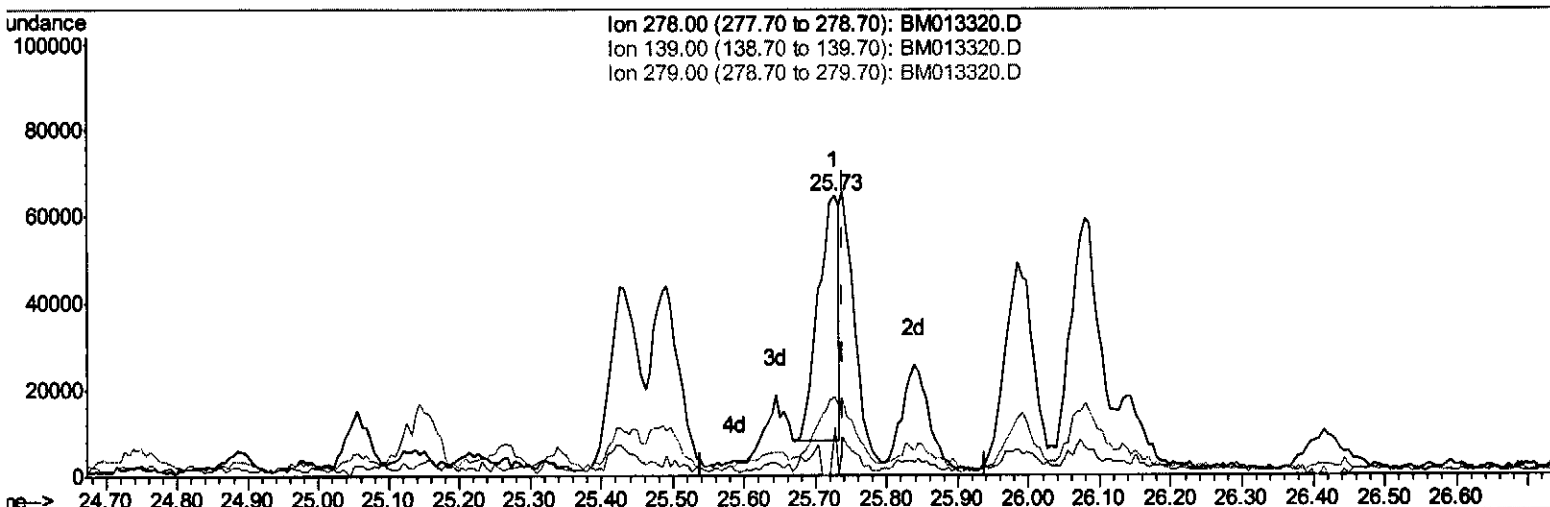

(90) Dibenzo(a,h)anthracene

25.727min (-0.012) 1.81ng/ul

response 115039

Ion	Exp%	Act%
278.00	100	100
139.00	7.30	17.69#
279.00	23.20	27.98#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
 Data File : BM013320.D
 Acq On : 12 Dec 2017 00:45
 Operator : SJ/JU
 Sample : I6758-11 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9B12

Manual Integrations
 APPROVED

Sohil
 12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:53:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 12 02:07:09 2017
 Response via : Initial Calibration

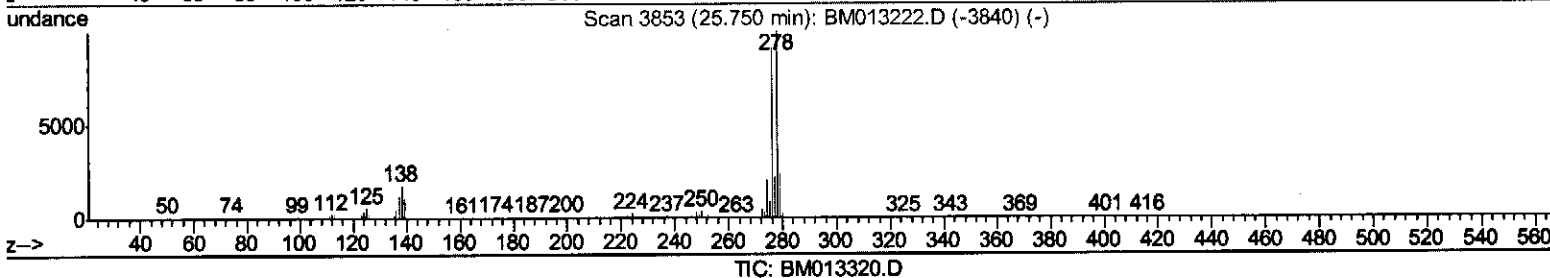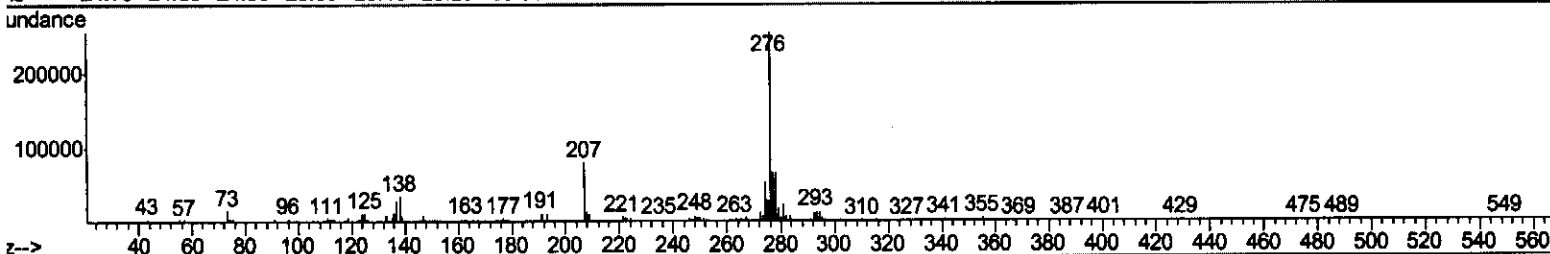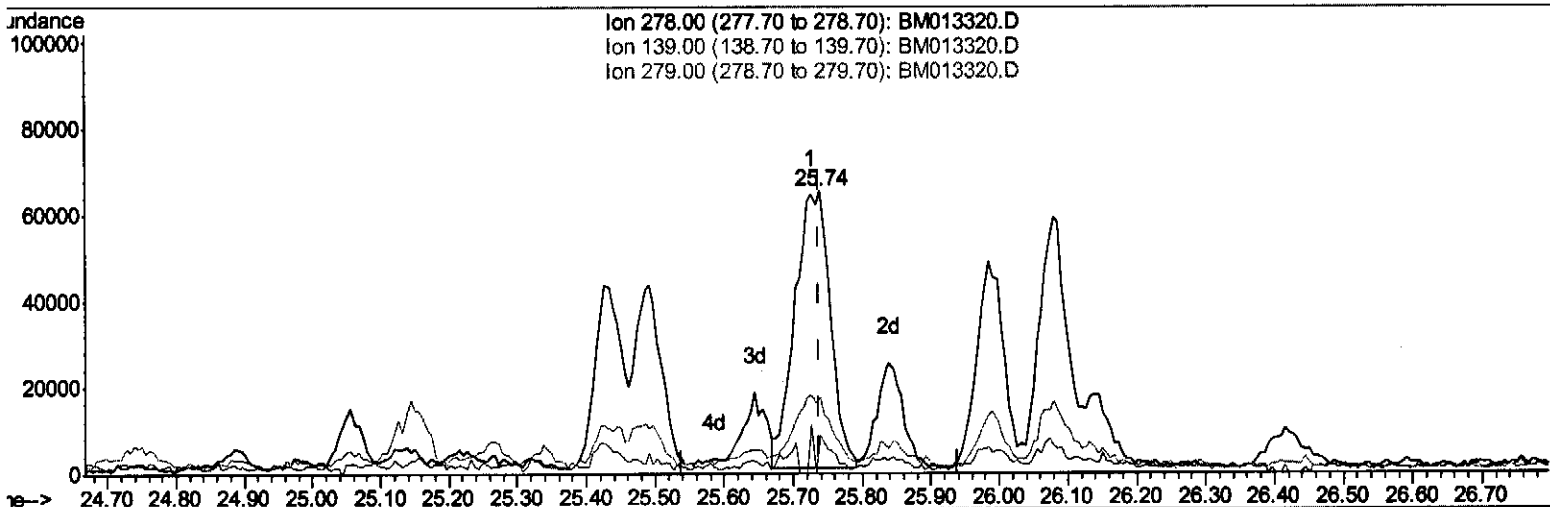

(90) Dibenzo(a,h)anthracene

25.738min (-0.001) 3.62ng/ul m

response 229640

Ion	Exp%	Act%
278.00	100	100
139.00	7.30	13.86#
279.00	23.20	26.93
0.00	0.00	0.00

data Path : Z:\HPCHEM1\BNA M\DATA\BM121117\
data File : BM013320.D
Acq On : 12 Dec 2017 00:45
Operator : SJ/JU
Sample : I6758-11 5X
Disc :
LS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9B12

Manual Integrations
APPROVED

Sohil
12/12/2017 3:57:10 PM

Quant Time: Dec 12 03:56:05 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
Last Update : Tue Dec 12 02:07:09 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	280478	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	1225054	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	725545	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1604394	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1563128	20.00	ng/ul	0.00
83) Perylene-d12	23.50	264	1241298	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	3198m	0.56	ng/ul	0.00
5) Phenol-d5	6.87	99	87972	3.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	51587	3.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	69637	3.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	73333	3.54	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	37401	3.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	39654	3.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	73358	3.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	50483	2.56	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	244866	3.79	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	298452	3.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	32022m	2.85	ng/ul	0.00
57) Fluorene-d10	15.32	176	209758	3.78	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	27043	2.68	ng/ul	0.00
70) Anthracene-d10	17.17	188	319763	3.98	ng/ul	0.00
76) Pyrene-d10	19.47	212	317537	4.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	227302	3.59	ng/ul	0.00

Target Compounds

					Ovalue
47) Acenaphthylene	14.05	152	418794	5.680	ng/ul 97
68) Pentachlorophenol	16.73	266	59183	4.920	ng/ul 95
71) Anthracene	17.21	178	378542	4.063	ng/ul 98
74) Fluoranthene	19.14	202	470923	4.216	ng/ul# 92
77) Pyrene	19.50	202	586573	6.177	ng/ul# 94
80) Benzo(a)anthracene	21.25	228	334196m	3.370	ng/ul } 97
82) Chrysene	21.30	228	552556m	6.005	ng/ul } 92
85) Benzo(b)fluoranthene	22.83	252	1327936	15.870	ng/ul# 97
86) Benzo(k)fluoranthene	22.87	252	346373m	4.399	ng/ul } 92
88) Benzo(a)pyrene	23.40	252	698115	9.287	ng/ul# 96
89) Indeno(1,2,3-cd)pyrene	25.73	276	864757	11.595	ng/ul 98
90) Dibenzo(a,h)anthracene	25.74	278	229640m	3.616	ng/ul } 92
91) Benzo(g,h,i)perylene	26.41	276	866385	14.727	ng/ul# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed