
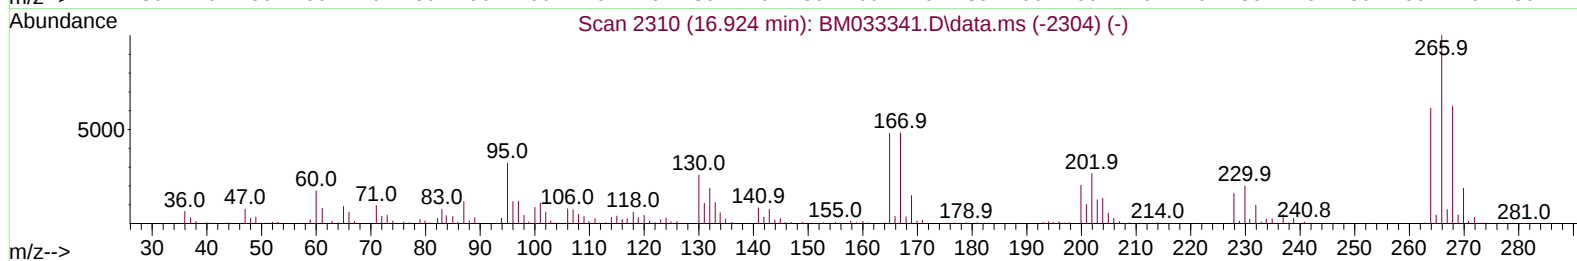
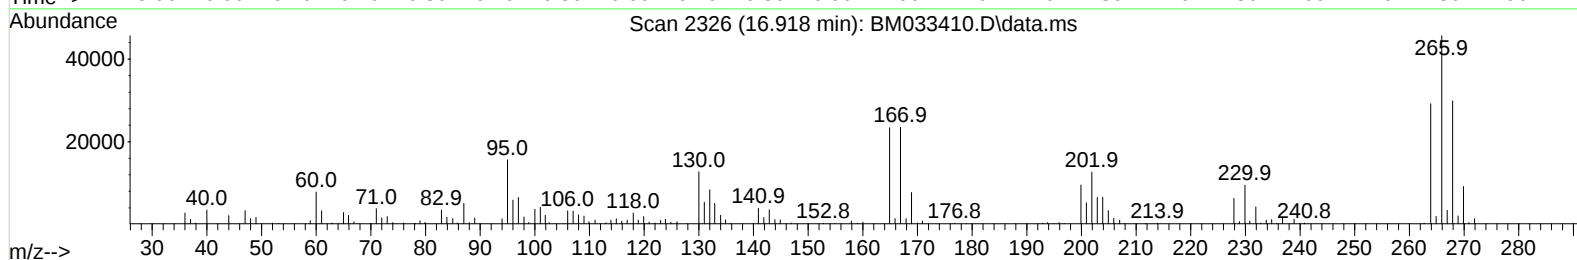


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121121\
 Data File : BM033410.D
 Acq On : 11 Dec 2021 13:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 01:20:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 12 00:15:00 2021
 Response via : Initial Calibration

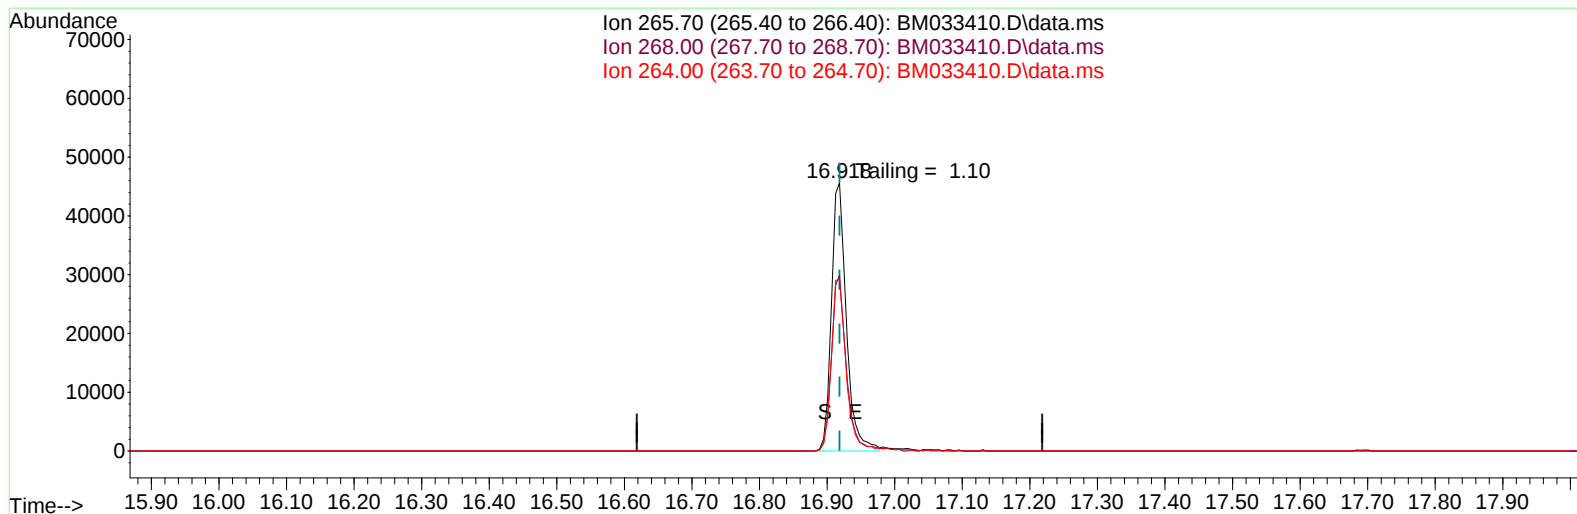

TIC: BM033410.D\data.ms

(70) Pentachlorophenol (C)

16.918min (+ 0.000) 0.00 ng

response 71231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.46
264.00	61.40	63.94
0.00	0.00	0.00