


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121121\
 Data File : BM033410.D
 Acq On : 11 Dec 2021 13:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Dec 12 00:15:00 2021

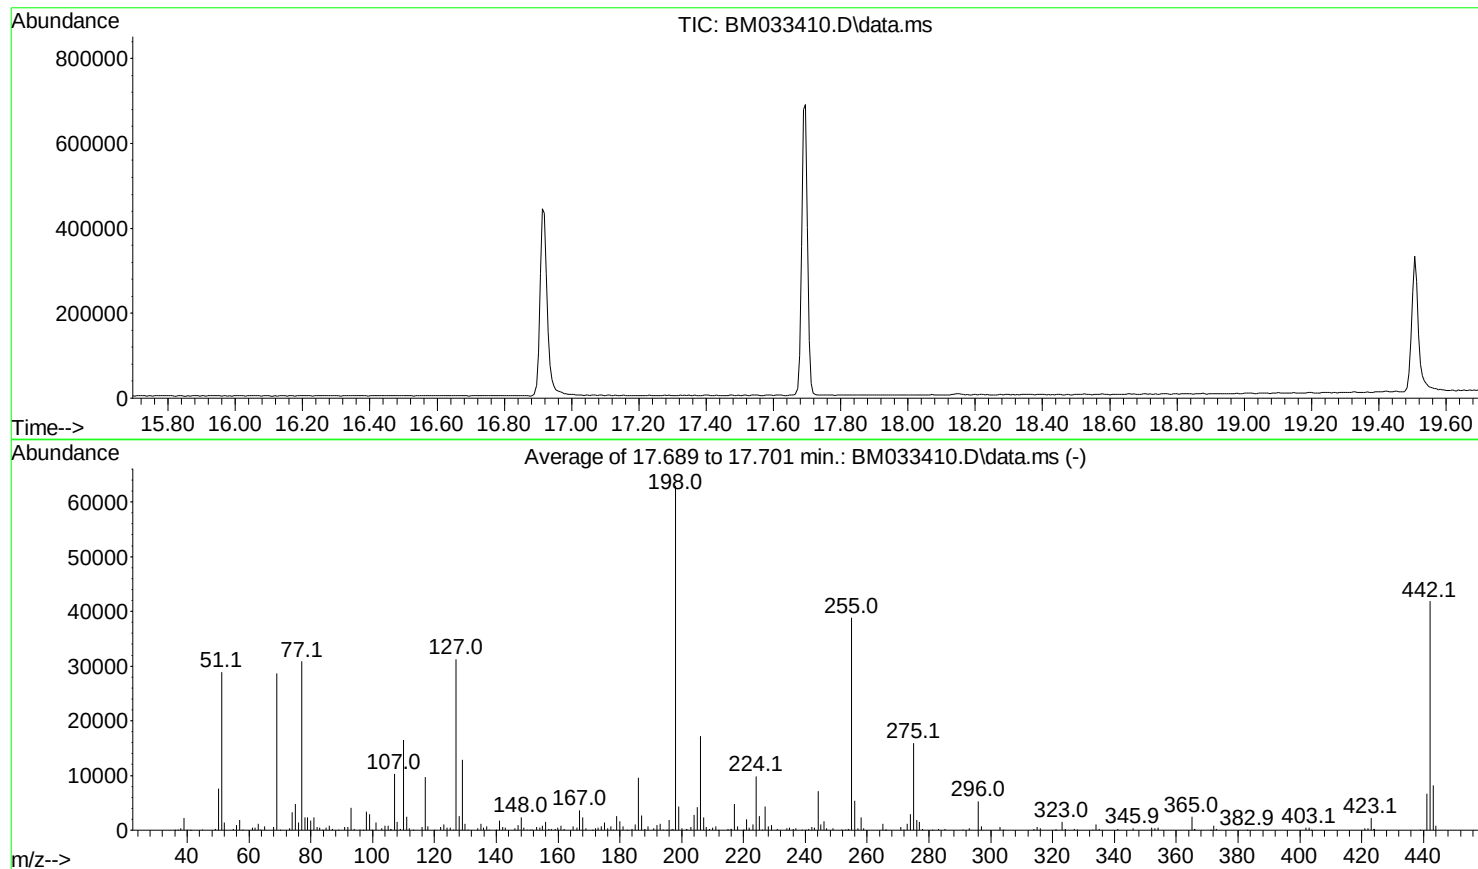




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.9	28914	PASS
68	69	0.00	2	1.9	553	PASS
69	198	0.00	100	45.5	28667	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	49.7	31259	PASS
197	198	0.00	2	0.4	256	PASS
198	198	100	100	100.0	62955	PASS
199	198	5	9	7.0	4378	PASS
275	198	10	60	25.3	15947	PASS
365	198	1	100	3.9	2436	PASS
441	198	0.01	100	10.6	6662	PASS
442	442	50	100	100.0	41864	PASS
443	442	15	24	19.6	8210	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121121\  
Data File : BM033410.D  
Acq On    : 11 Dec 2021  13:45  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 12 01:20:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 12 00:15:00 2021
Response via : Initial Calibration

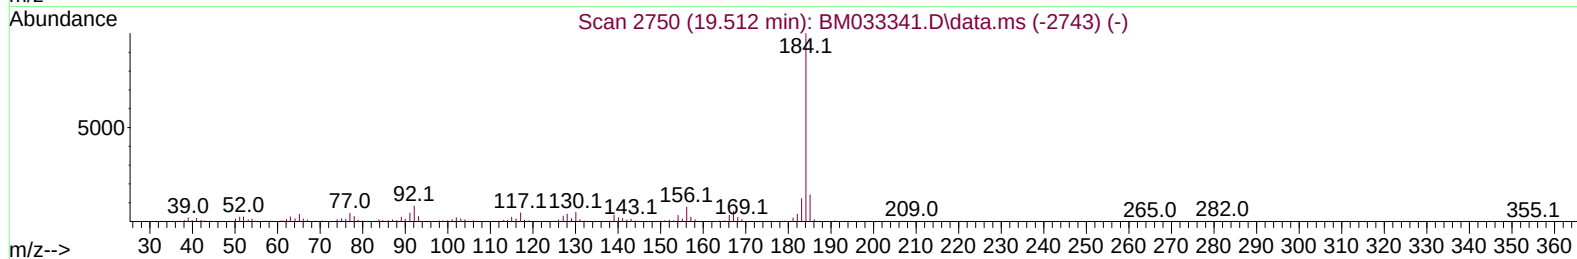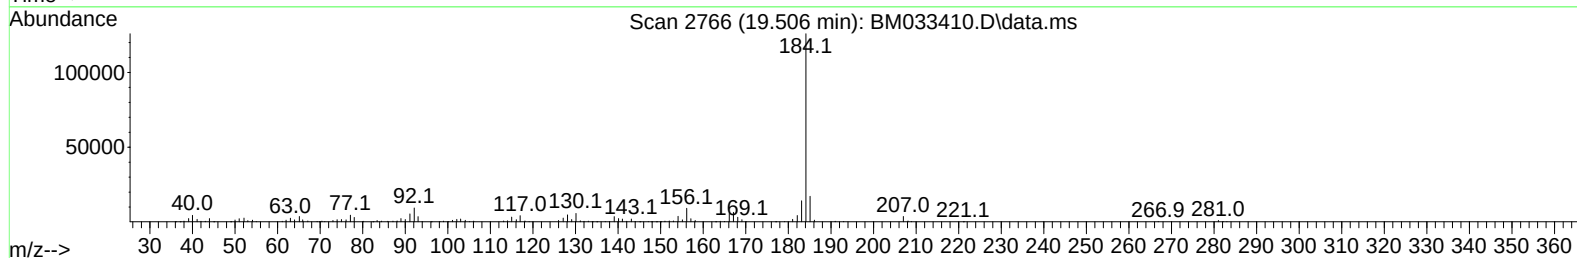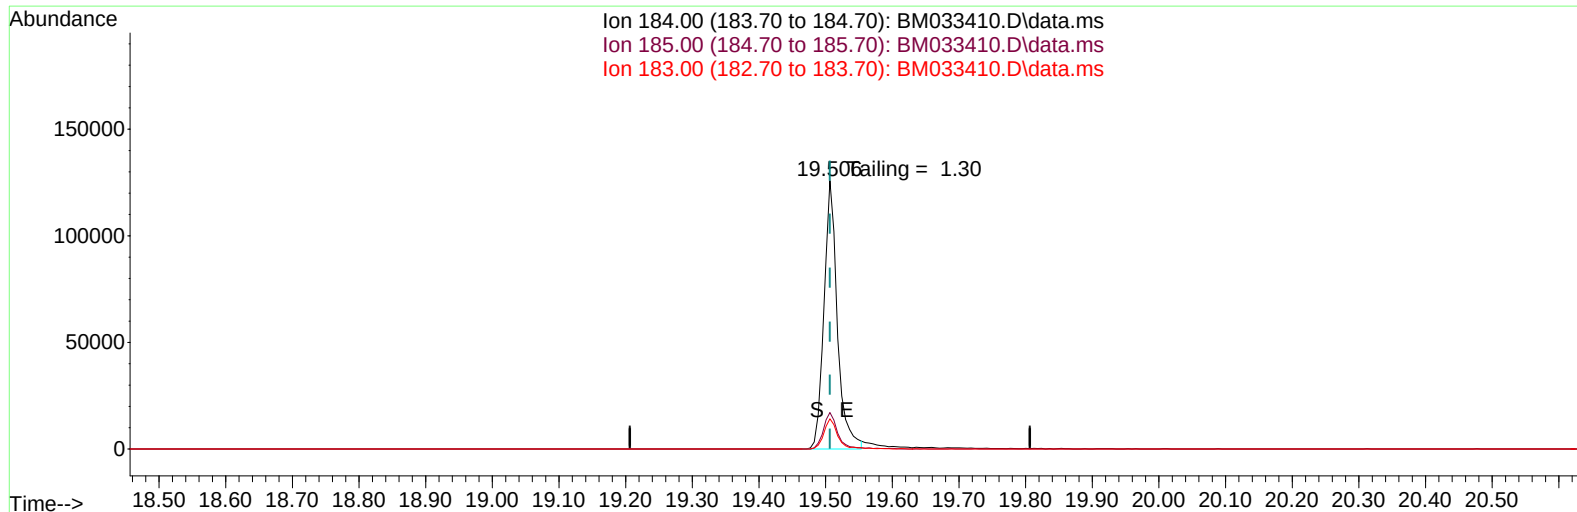

TIC: BM033410.D\data.ms

(77) Benzidine

19.506min (+ 0.000) 0.00 ng

response	182866
----------	--------

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.20	13.63
--------	-------	-------




183.00	12.10	11.27
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121121\
Data File : BM033410.D
Acq On : 11 Dec 2021 13:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 12 01:20:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 12 00:15:00 2021
Response via : Initial Calibration

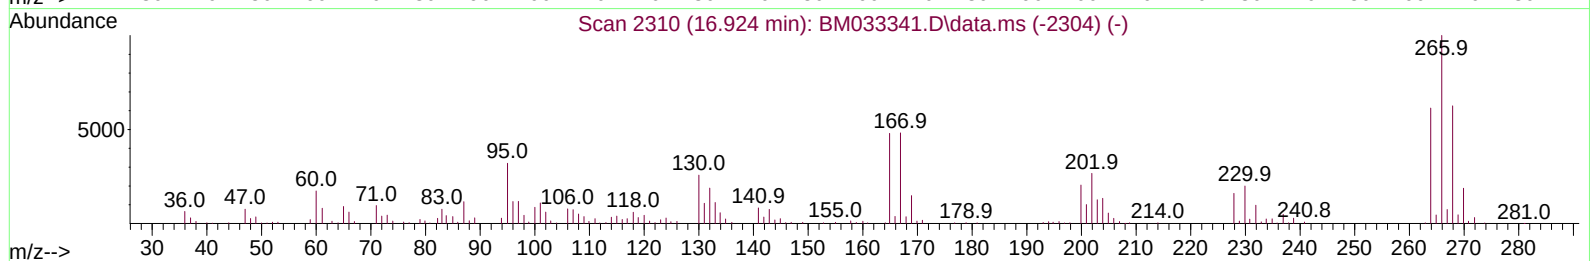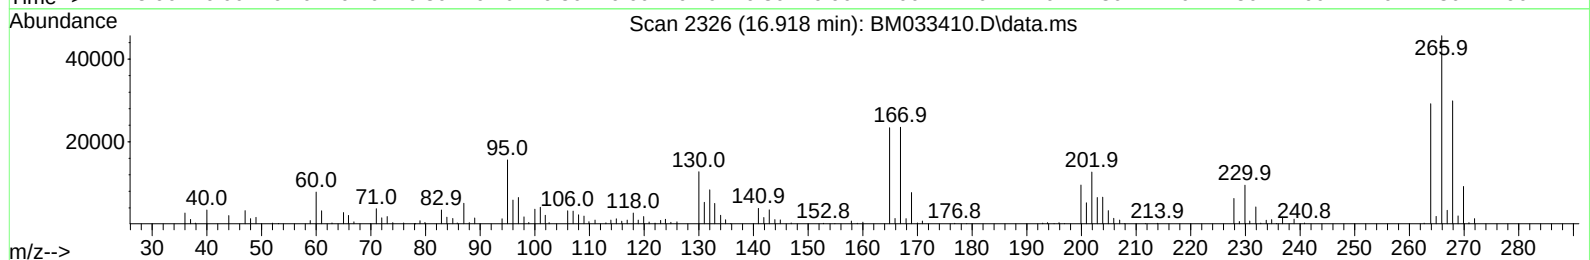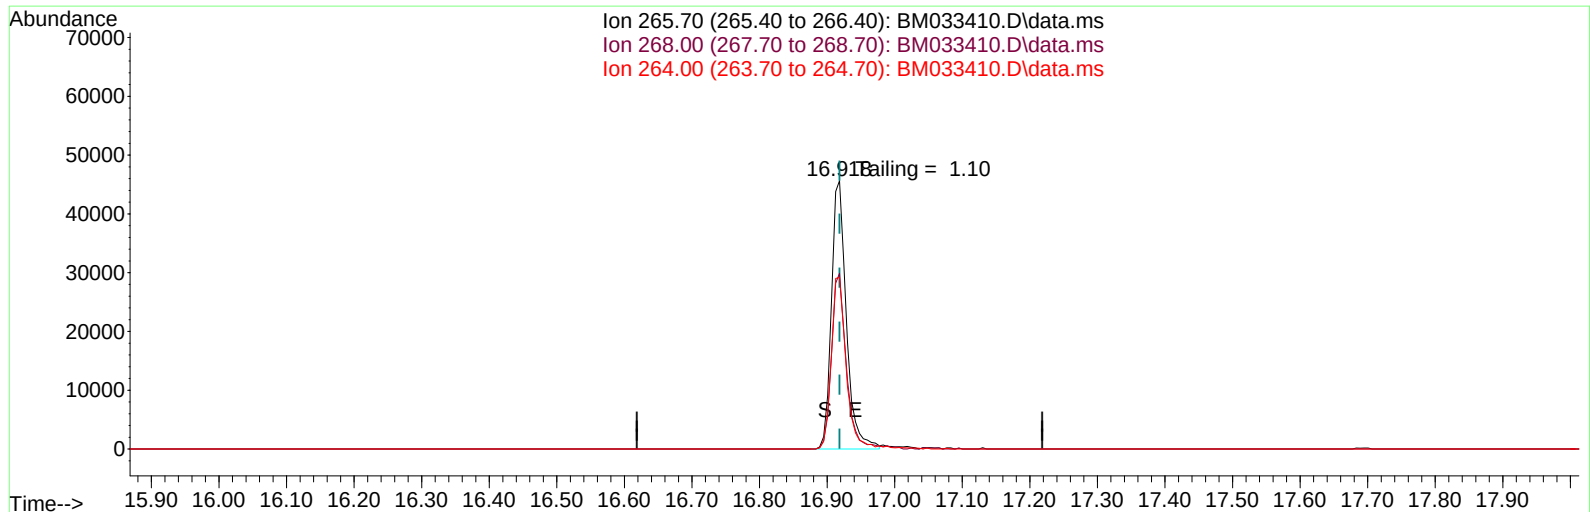

TIC: BM033410.D\data.ms

(70) Pentachlorophenol (C)

16.918min (+ 0.000) 0.00 ng

response 71231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.46
264.00	61.40	63.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2021	BNA_M	<u>BM033410.D</u>
Compound Name	Response	Retention Time
DDT	136702	20.73
DDD	1673	20.295
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1673	138375	1.21

Instrument :
BNA_M
ClientSampleId :
DFTPP