

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043232.D
 Acq On : 11 Dec 2023 18:59
 Operator : MA/JU
 Sample : PB157628BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK628

Quant Time: Dec 11 23:04:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	11649	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	36250	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	20755	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	2652326	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.953	264	29948	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	72535	4.928	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13292	0.259	ng/ul	0.00
18) Fluoranthene-d10	19.390	212	23670	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.624	166	5575	0.059	ng/ul#	12
26) Benzo(a)pyrene	23.801	252	8330	0.074	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043232.D
Acq On : 11 Dec 2023 18:59
Operator : MA/JU
Sample : PB157628BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK628

Quant Time: Dec 11 23:04:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration




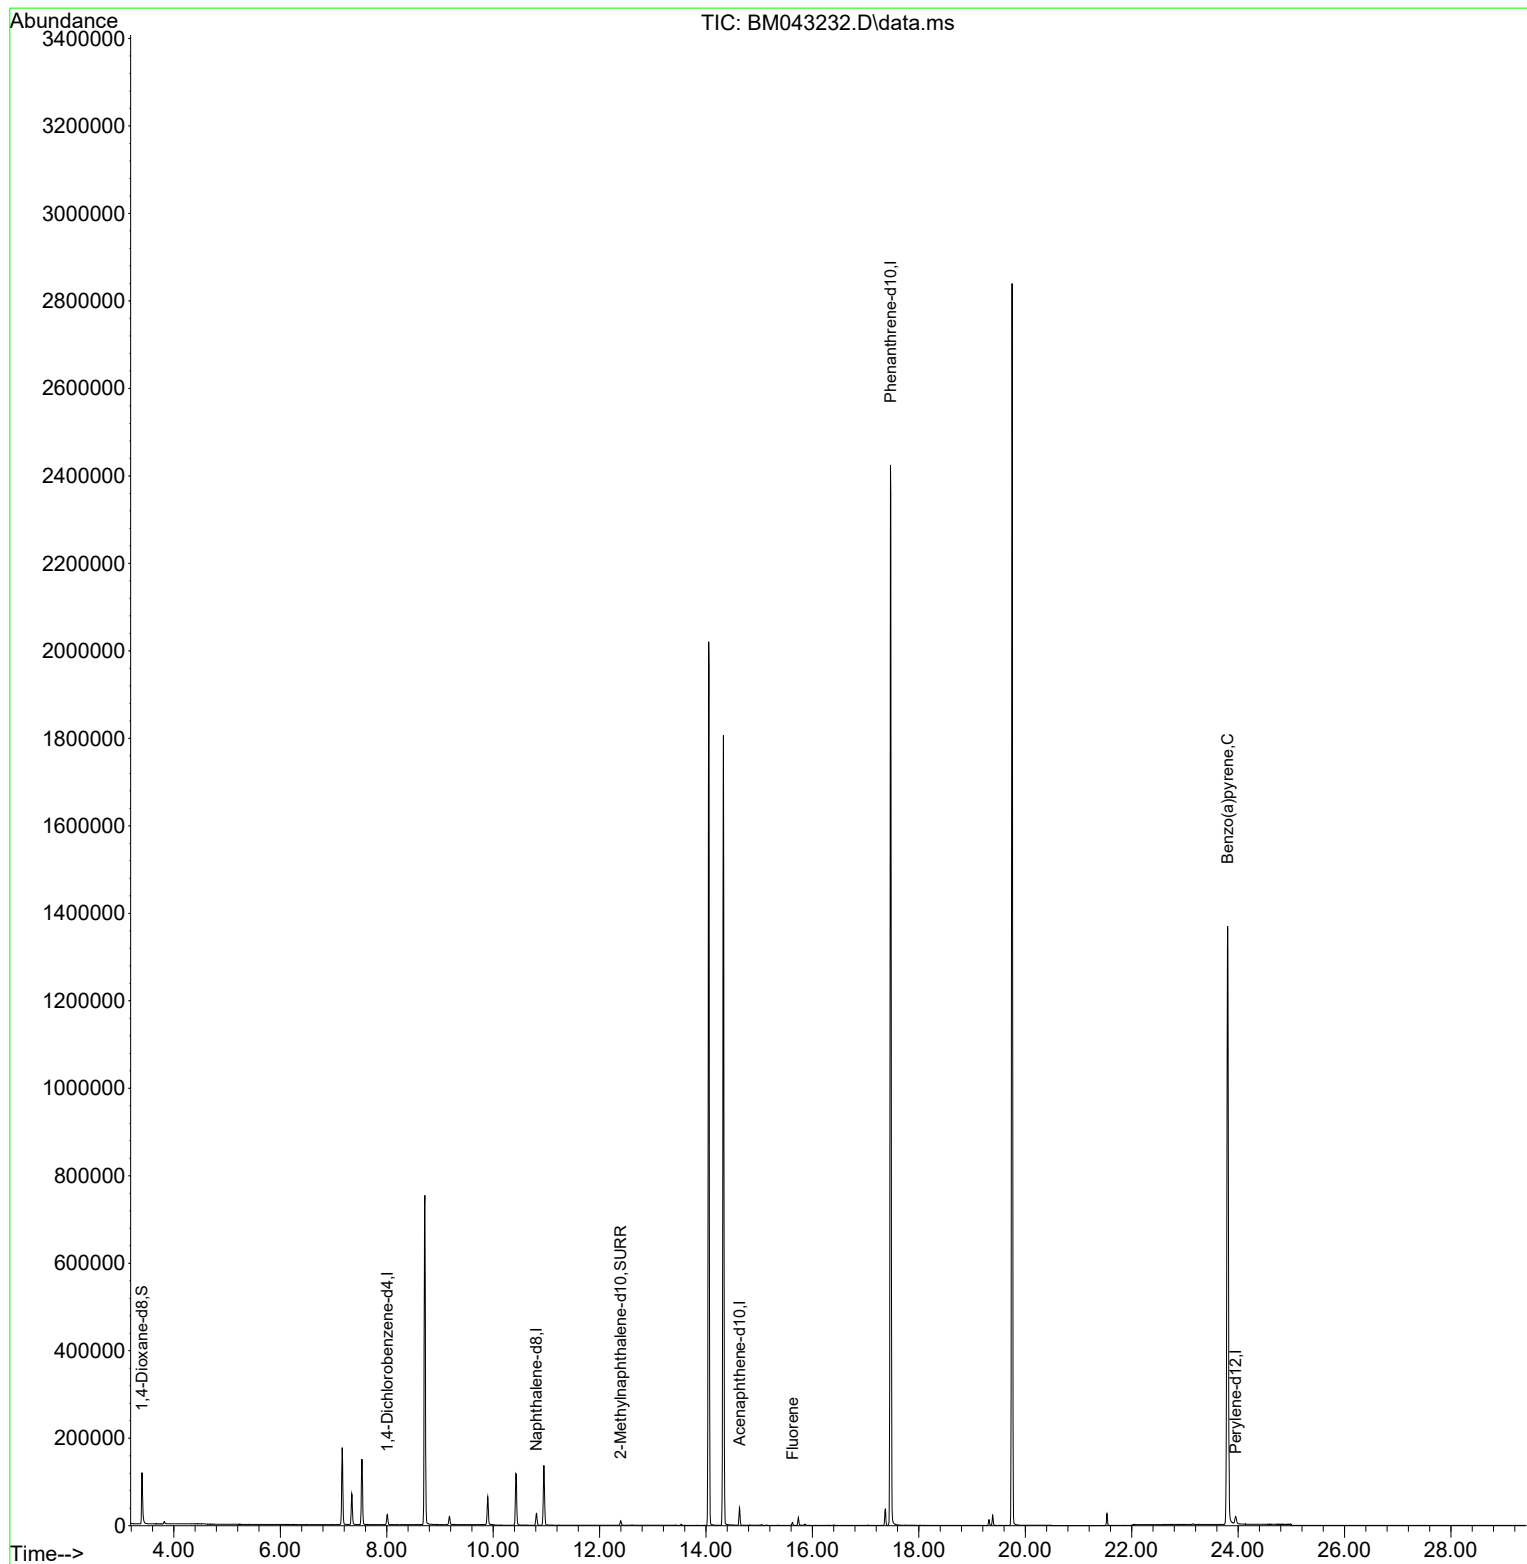


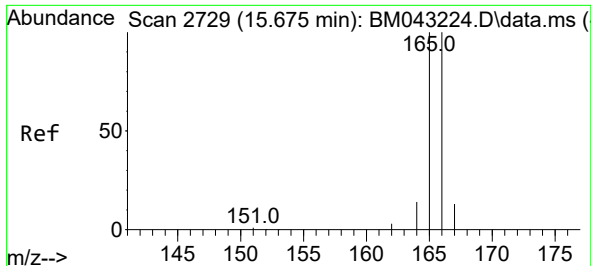

#12
Fluorene
Concen: 0.059 ng/ul
RT: 15.624 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM043232.D
Acq: 11 Dec 2023 18:59

Instrument :
BNA_M
ClientSampleId :
SBLK628

Tgt Ion:166 Resp: 5575
Ion Ratio Lower Upper
166 100
165 7.2 80.3 120.5#
167 33.9 10.8 16.2#

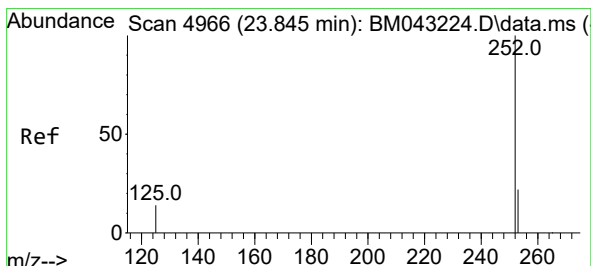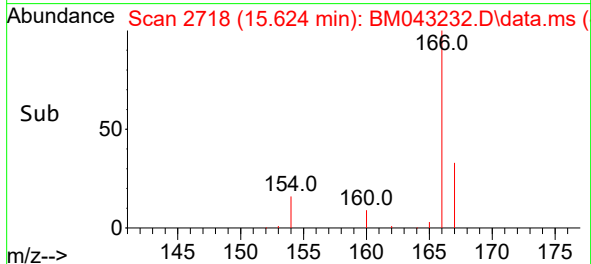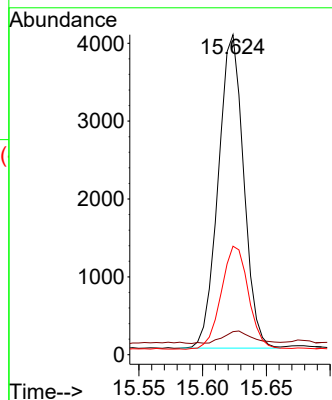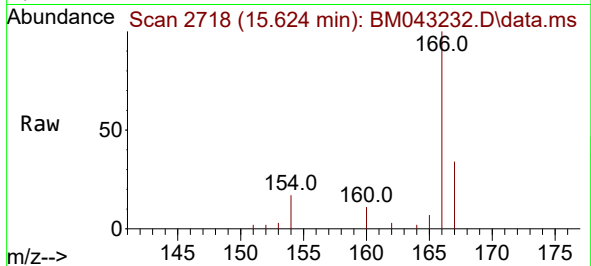

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.801 min Scan# 4951
Delta R.T. -0.044 min
Lab File: BM043232.D
Acq: 11 Dec 2023 18:59

Tgt Ion:252 Resp: 8330
Ion Ratio Lower Upper
252 100
253 39.5 20.2 30.2#
125 32.5 13.5 20.3#

