

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043233.D
 Acq On : 11 Dec 2023 19:35
 Operator : MA/JU
 Sample : PB157626BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK626

Quant Time: Dec 11 23:04:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	10615	0.400	ng/ul	0.00
4) Naphthalene-d8	10.817	136	33081	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	18945	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	2734932	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.953	264	28910	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	75036	5.595	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	13803	0.294	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	24306	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.624	166	5780	0.067	ng/ul#	12
26) Benzo(a)pyrene	23.804	252	8787	0.081	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043233.D
Acq On : 11 Dec 2023 19:35
Operator : MA/JU
Sample : PB157626BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK626

Quant Time: Dec 11 23:04:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration




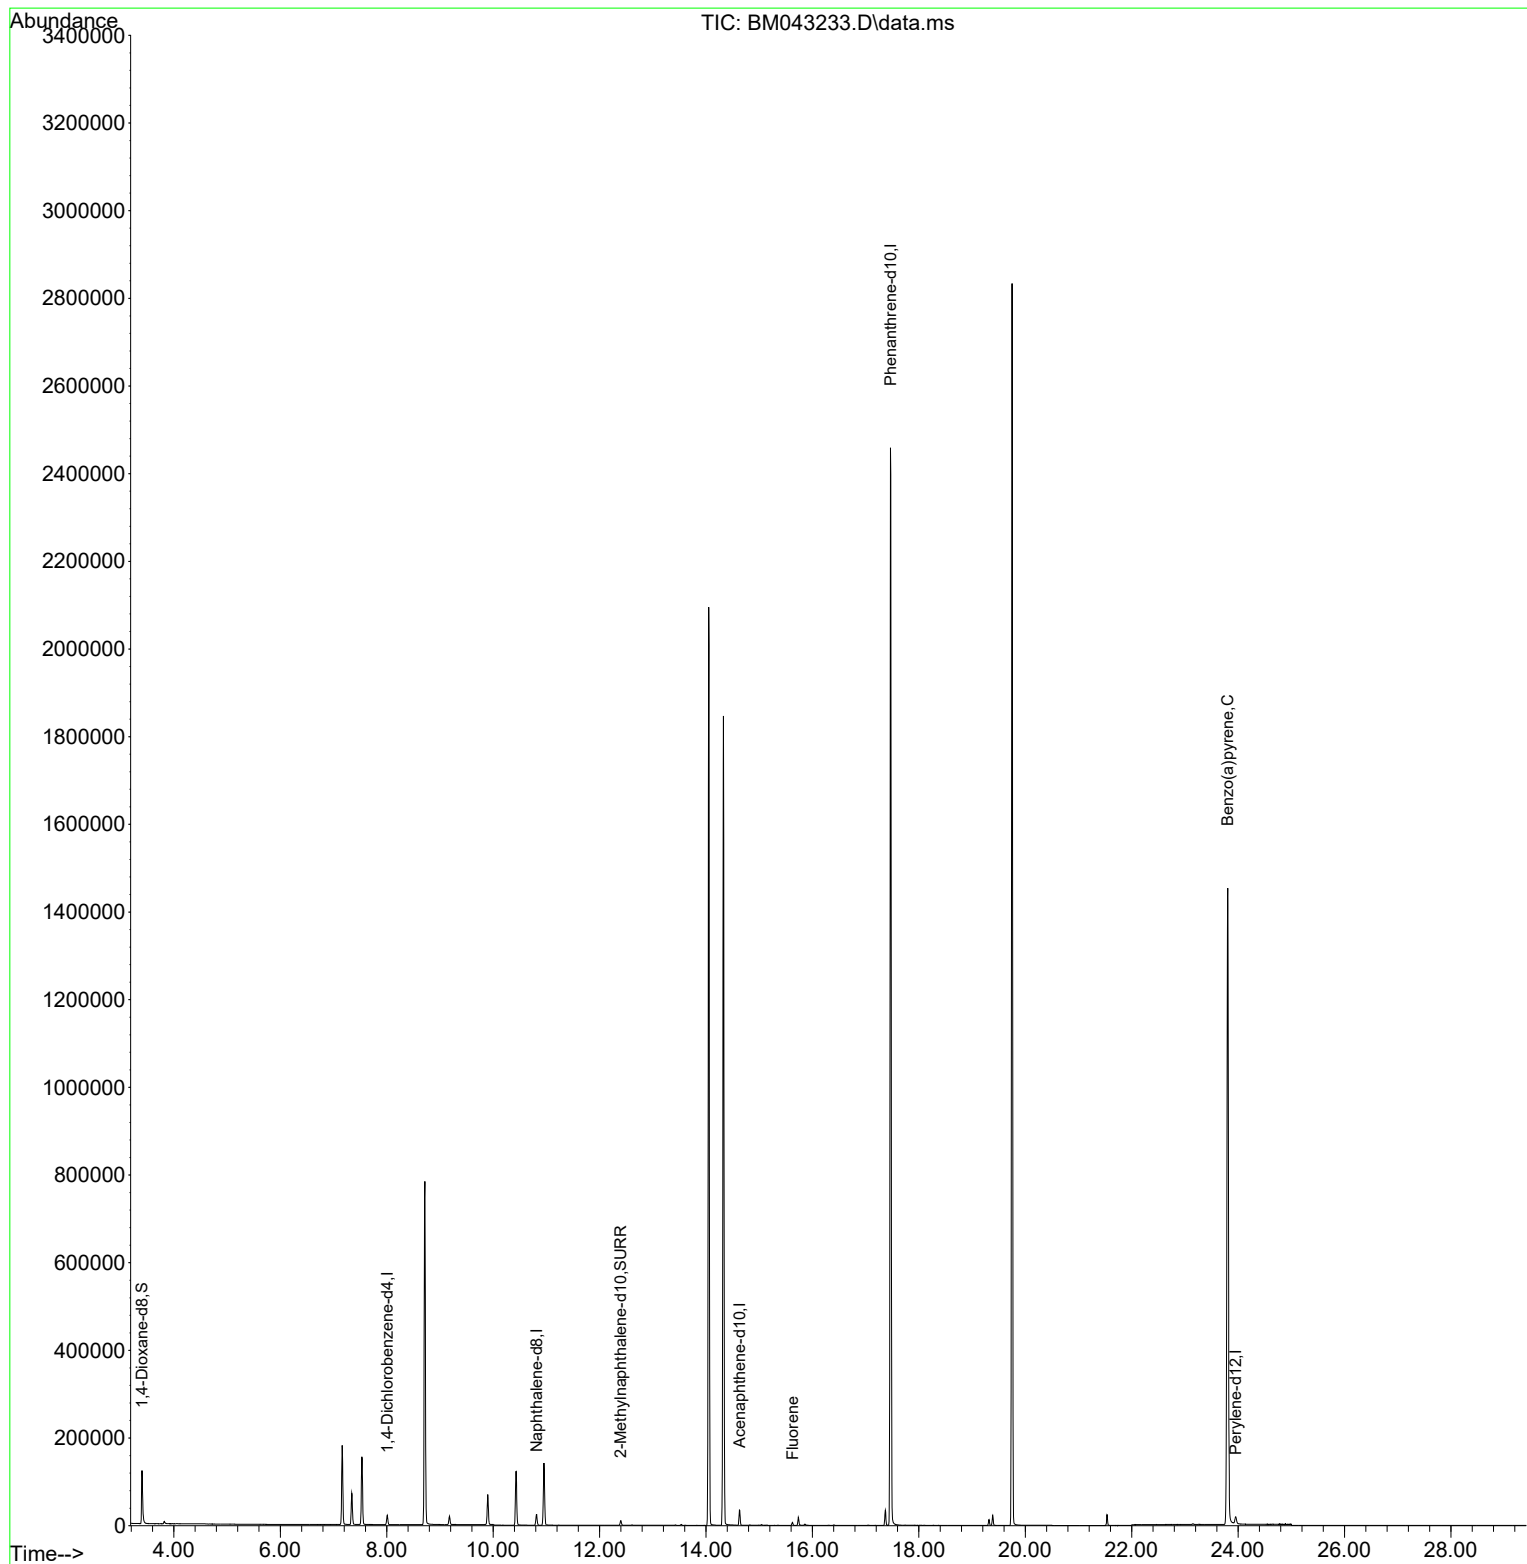


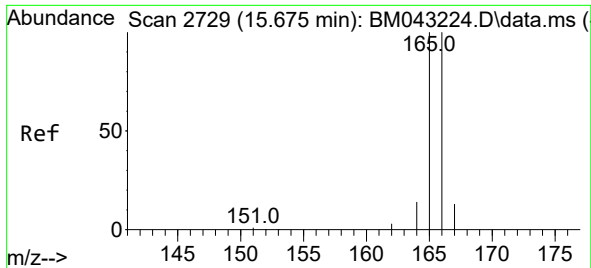

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.624 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM043233.D
Acq: 11 Dec 2023 19:35

Instrument :
BNA_M
ClientSampleId :
SBLK626

Tgt Ion:166 Resp: 5780
Ion Ratio Lower Upper
166 100
165 6.5 80.3 120.5#
167 33.3 10.8 16.2#

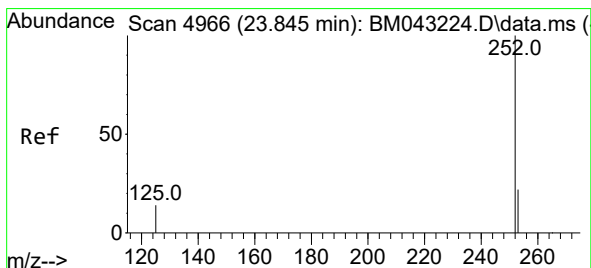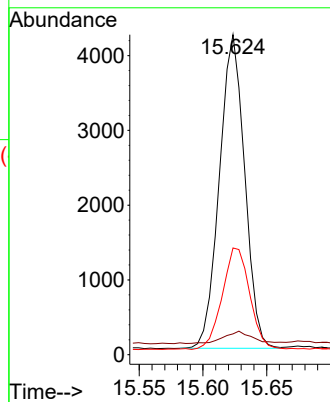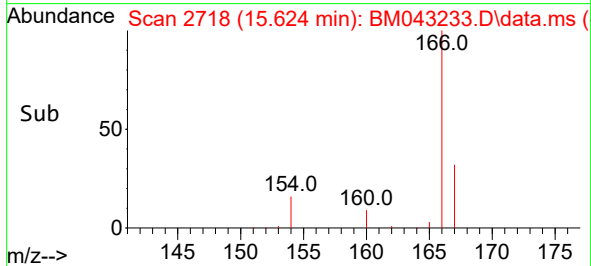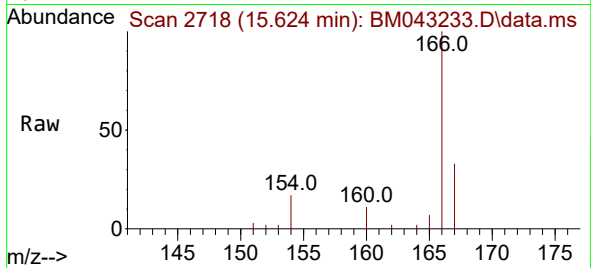

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.804 min Scan# 4952
Delta R.T. -0.041 min
Lab File: BM043233.D
Acq: 11 Dec 2023 19:35

Tgt Ion:252 Resp: 8787
Ion Ratio Lower Upper
252 100
253 37.8 20.2 30.2#
125 31.3 13.5 20.3#

