

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043274.D
 Acq On : 12 Dec 2023 21:23
 Operator : MA/JU
 Sample : 05675-22
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AD3

Quant Time: Dec 12 22:53:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	9973	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	32878	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	18236	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.468	188	3144117	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.54
23) Perylene-d12	23.953	264	27232	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	48755	3.869	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	16844	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	29787	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.435	88	38714	3.063	ng/ul#	80
5) Naphthalene	10.861	128	7339	0.074	ng/ul#	96
7) 2-Methylnaphthalene	12.467	142	1809	0.028	ng/ul	98
26) Benzo(a)pyrene	23.801	252	11105	0.109	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043274.D
Acq On : 12 Dec 2023 21:23
Operator : MA/JU
Sample : 05675-22
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AD3

Quant Time: Dec 12 22:53:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration




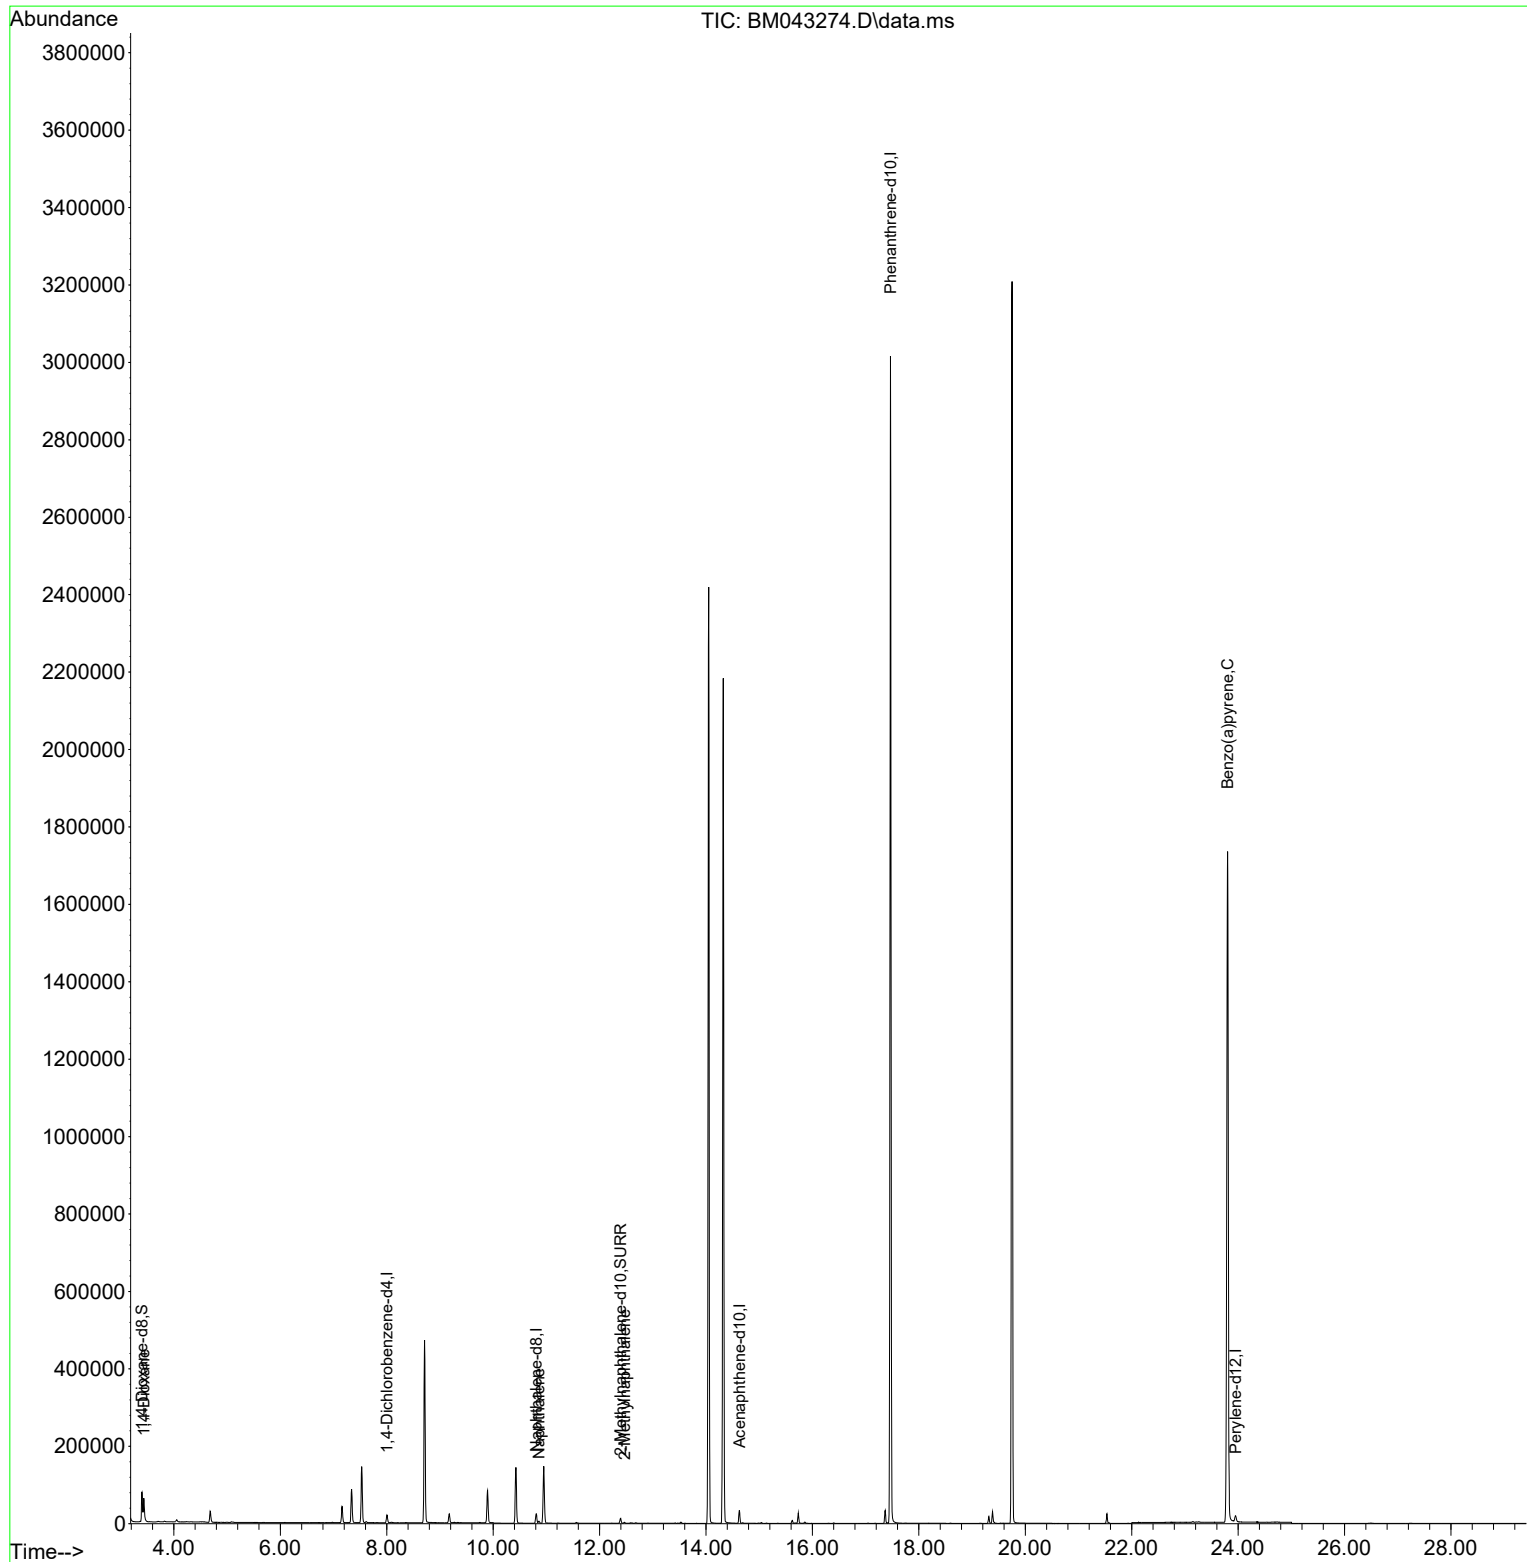


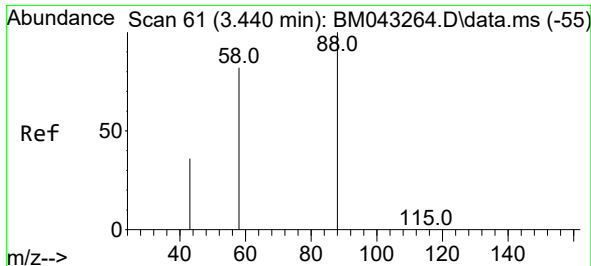

#2
1,4-Dioxane
Concen: 3.063 ng/ul
RT: 3.435 min Scan# 60
Delta R.T. -0.004 min
Lab File: BM043274.D
Acq: 12 Dec 2023 21:23




Instrument :
BNA_M
ClientSampleId :
H0AD3


Tgt Ion: 88 Resp: 38714
Ion Ratio Lower Upper
88 100
43 36.1 27.9 41.9
58 76.8 43.4 65.2#

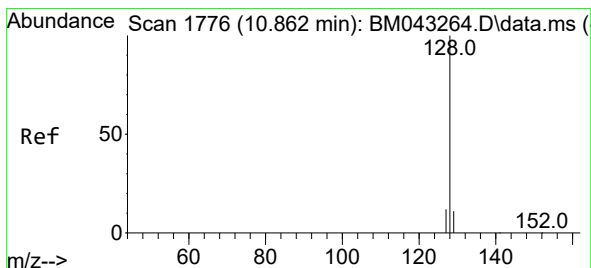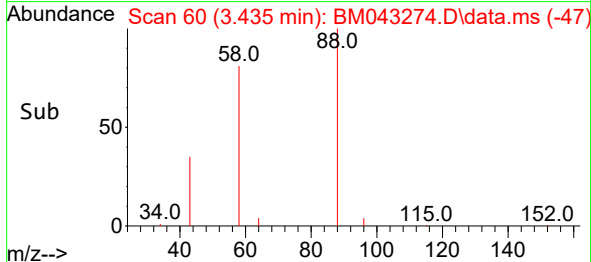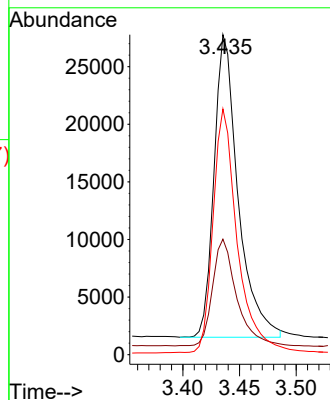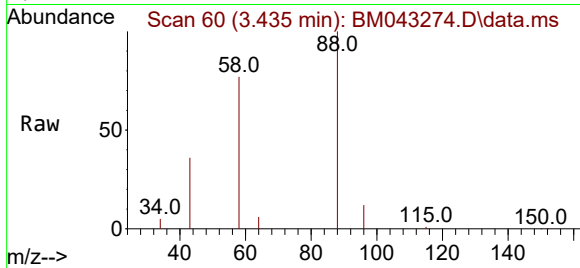

#5
Naphthalene
Concen: 0.074 ng/ul
RT: 10.861 min Scan# 1776
Delta R.T. -0.006 min
Lab File: BM043274.D
Acq: 12 Dec 2023 21:23

Tgt Ion:128 Resp: 7339
Ion Ratio Lower Upper
128 100
129 13.9 9.0 13.4#
127 13.5 10.3 15.5


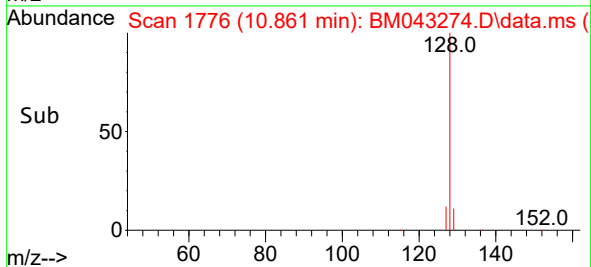
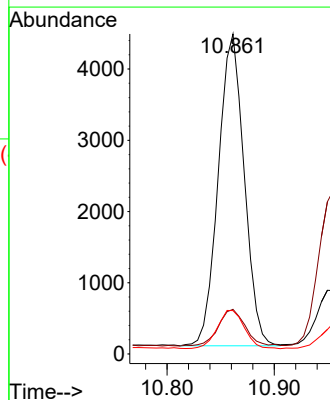
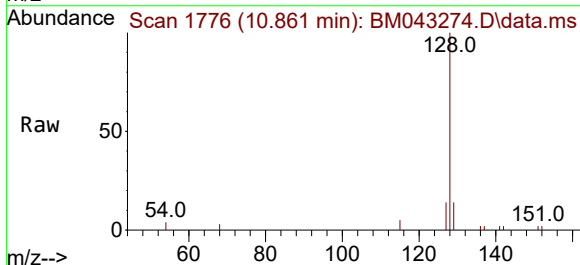


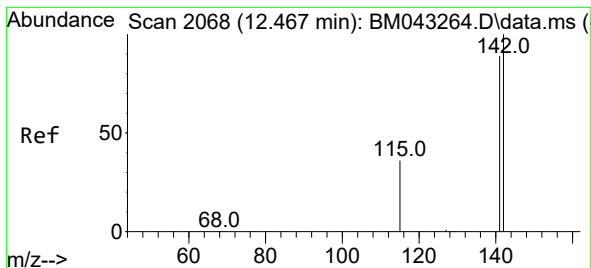

#7
2-Methylnaphthalene
Concen: 0.028 ng/ul
RT: 12.467 min Scan# 2068
Delta R.T. -0.006 min
Lab File: BM043274.D
Acq: 12 Dec 2023 21:23

Instrument :
BNA_M
ClientSampleId :
H0AD3

Tgt Ion:142 Resp: 1809
Ion Ratio Lower Upper
142 100
141 90.4 70.9 106.3

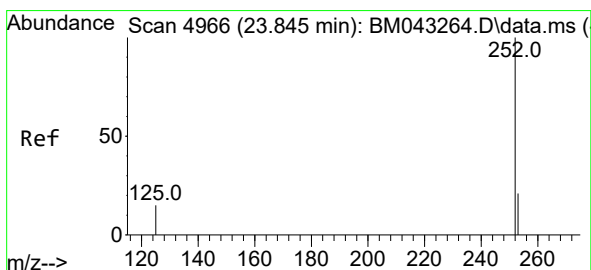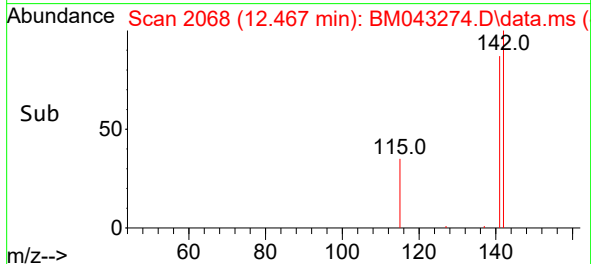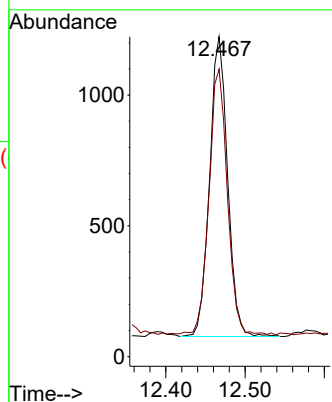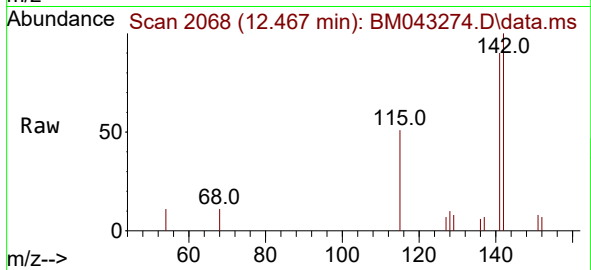

#26
Benzo(a)pyrene
Concen: 0.109 ng/ul
RT: 23.801 min Scan# 4951
Delta R.T. -0.044 min
Lab File: BM043274.D
Acq: 12 Dec 2023 21:23

Tgt Ion:252 Resp: 11105
Ion Ratio Lower Upper
252 100
253 41.3 20.2 30.2#
125 34.3 13.5 20.3#

