




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043259.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC0

Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

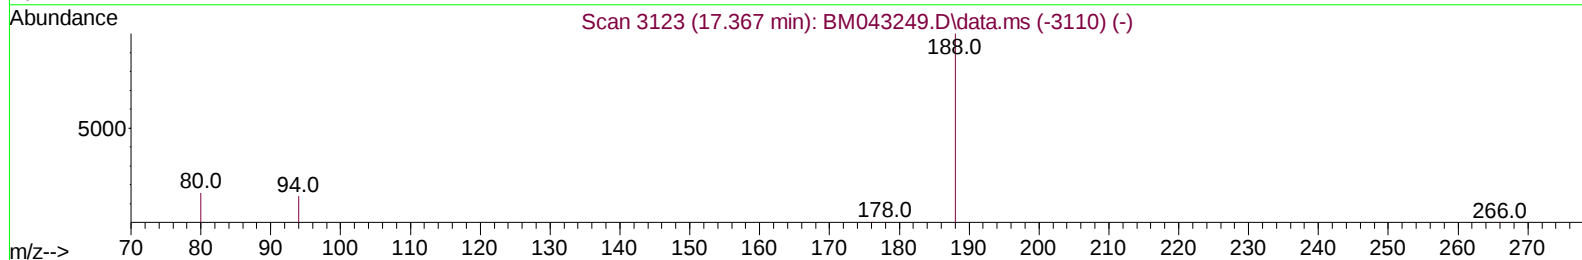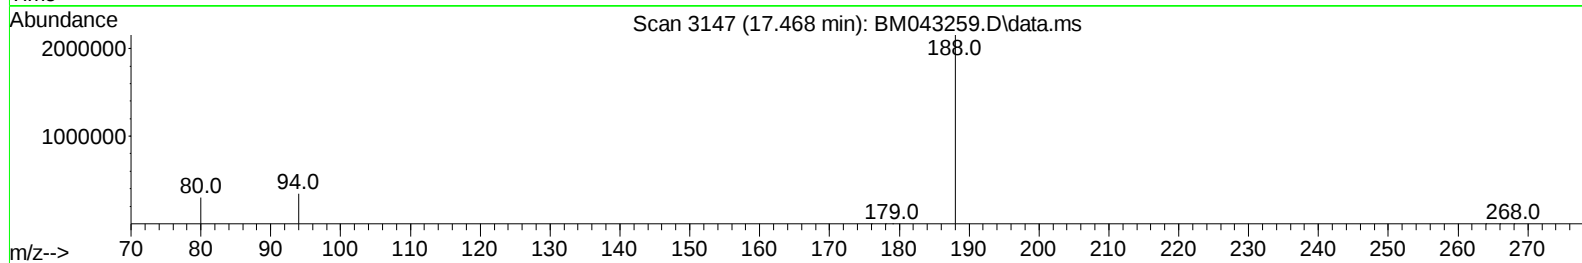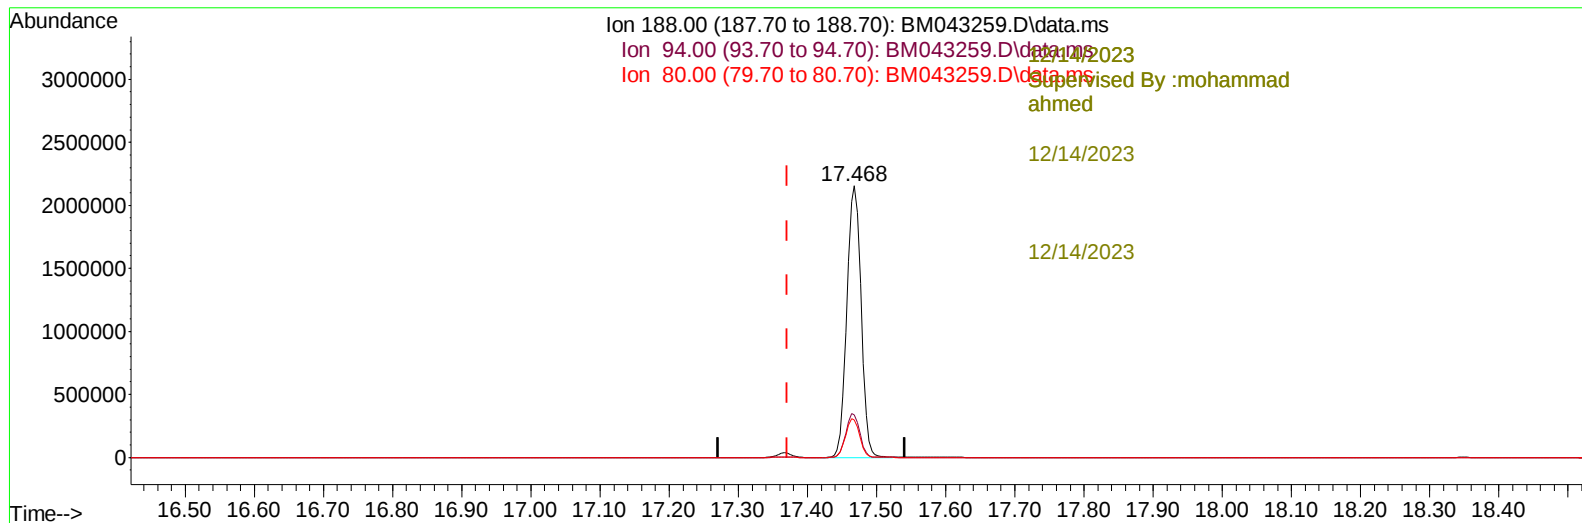

TIC: BM043259.D\data.ms

(13) Phenanthrene-d10 (I)

17.468min (+ 0.097) 0.40 ng/u1

response 3070159

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	15.80#
80.00	13.20	13.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043259.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 33 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
H0AC0

Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

12/14/2023
Supervised By :mohammad
ahmed

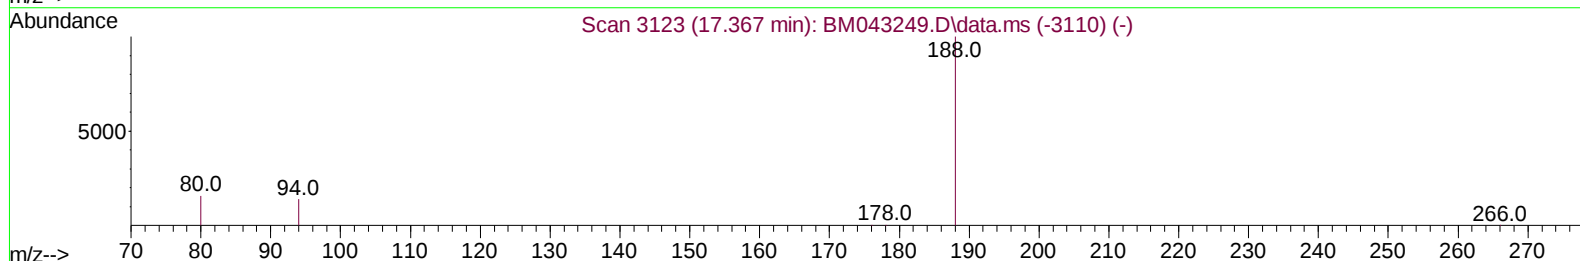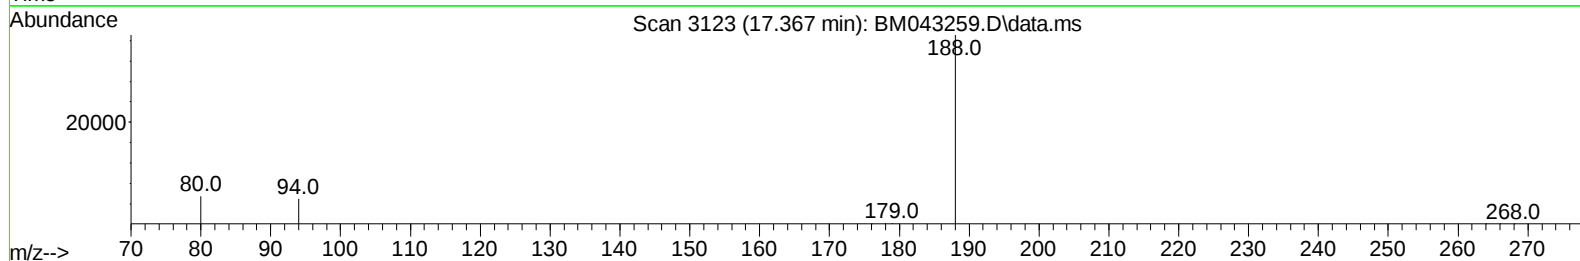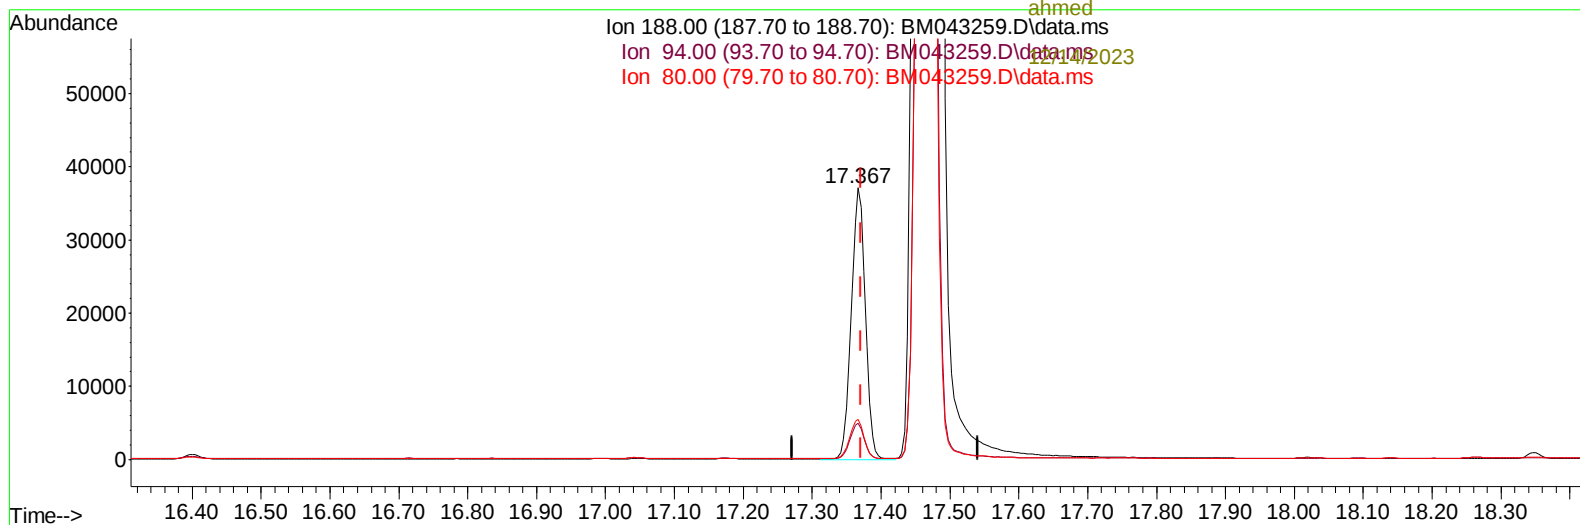

TIC: BM043259.D\data.ms

(13) Phenanthrene-d10 (I)

17.367min (-0.004) 0.40 ng/ul m

response 52482

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	13.26
80.00	13.20	14.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043259.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC0




Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

12/14/2023
 Supervised By :mohammad
 ahmed

Ion 240.00 (239.70 to 240.70): BM043259.D\data.ms
 Ion 120.00 (119.70 to 120.70): BM043259.D\data.ms
 Ion 236.00 (235.70 to 236.70): BM043259.D\data.ms

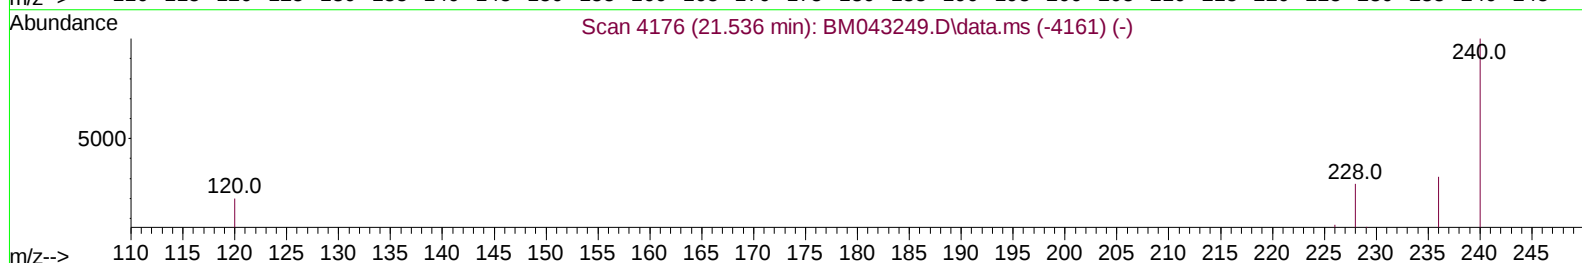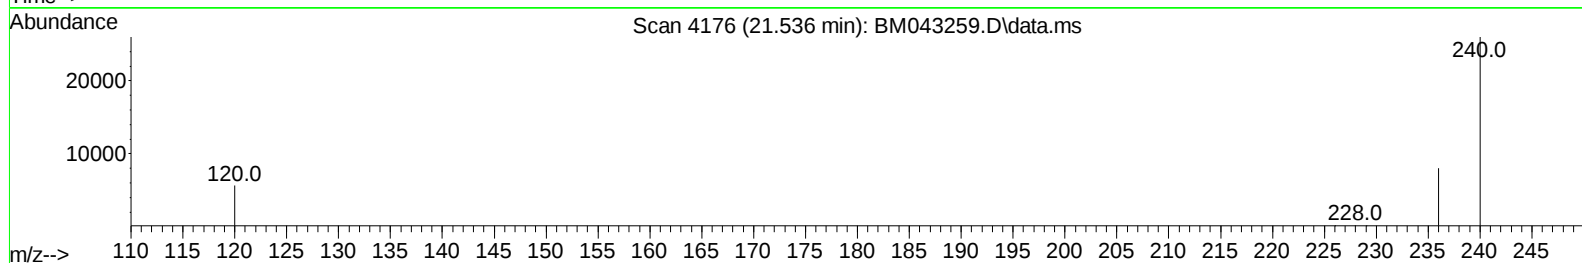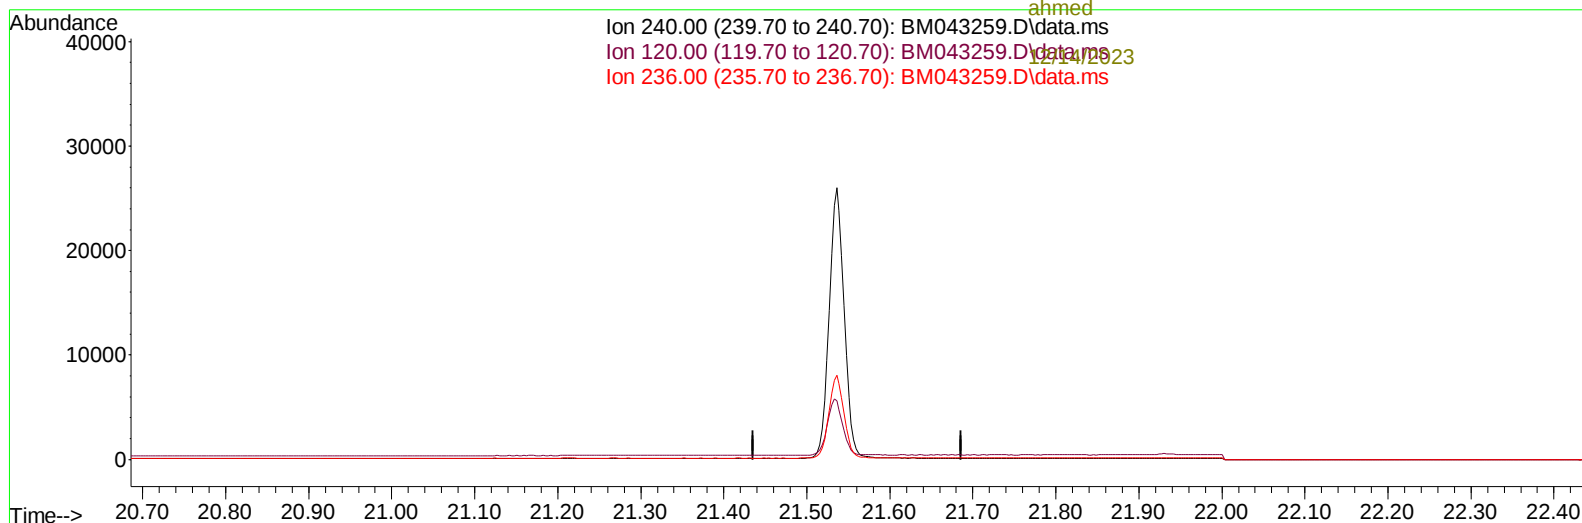

TIC: BM043259.D\data.ms

(17) Chrysene-d12

21.536min (-21.536) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	31.10	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043259.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC0




Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

12/14/2023
 Supervised By :mohammad
 ahmed

Ion 240.00 (239.70 to 240.70): BM043259.D\data.ms
 Ion 120.00 (119.70 to 120.70): BM043259.D\data.ms
 Ion 236.00 (235.70 to 236.70): BM043259.D\data.ms

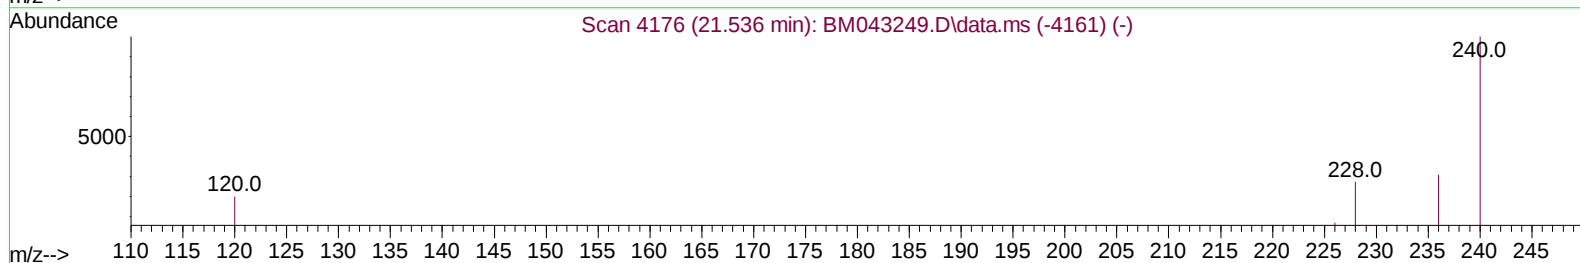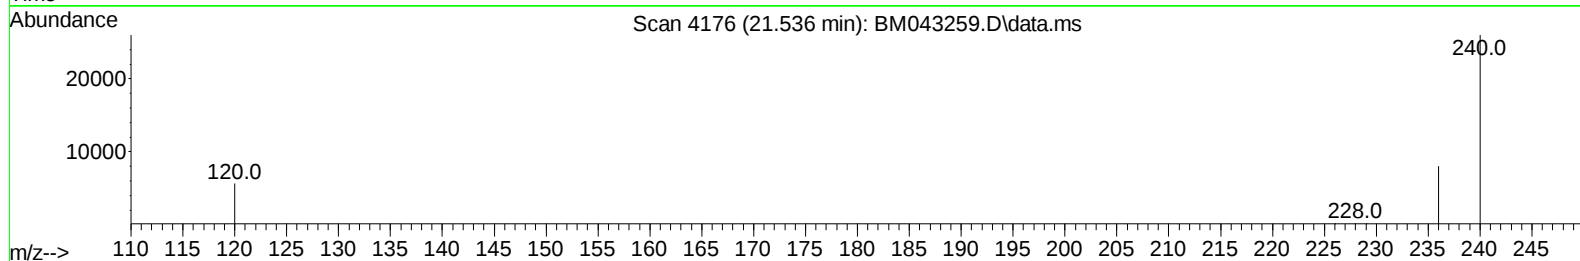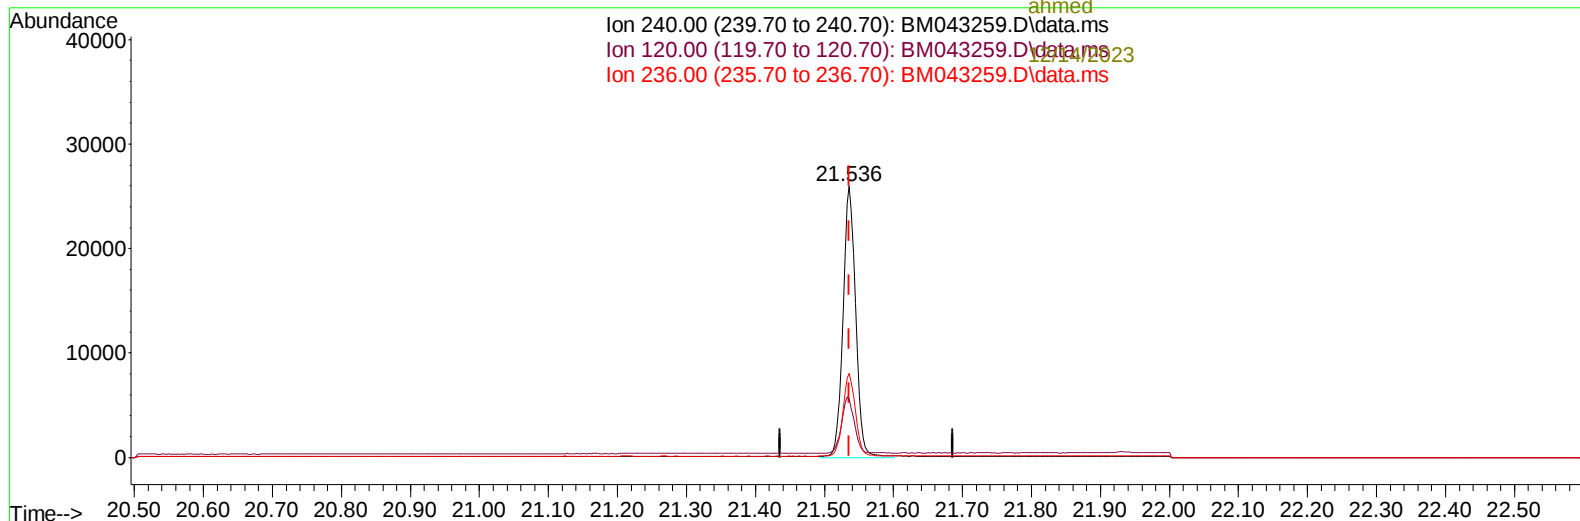

TIC: BM043259.D\data.ms

(17) Chrysene-d12

21.536min (0.000) 0.40 ng/ul m

response 33138

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	21.66
236.00	31.10	30.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043259.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 33 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
H0AC0

Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

12/14/2023
Supervised By :mohammad
ahmed

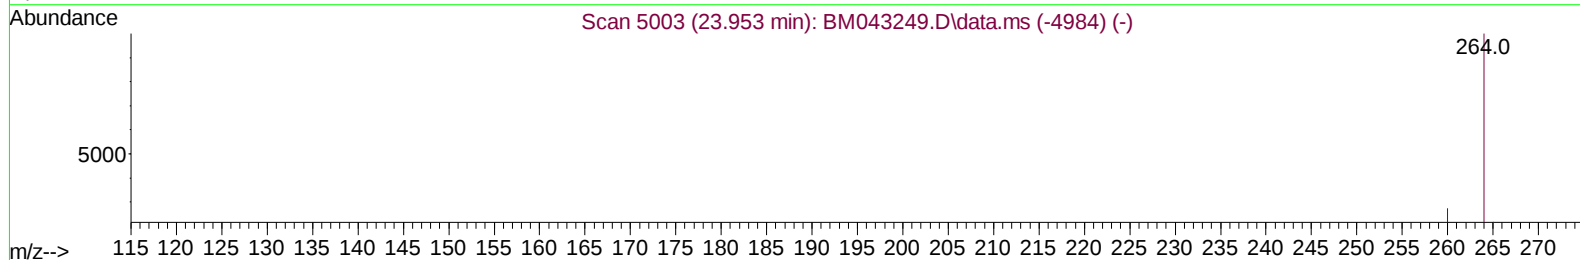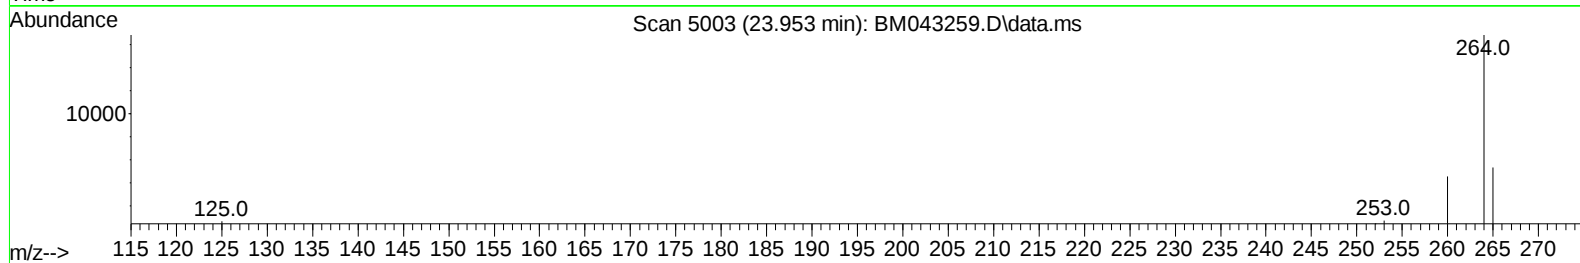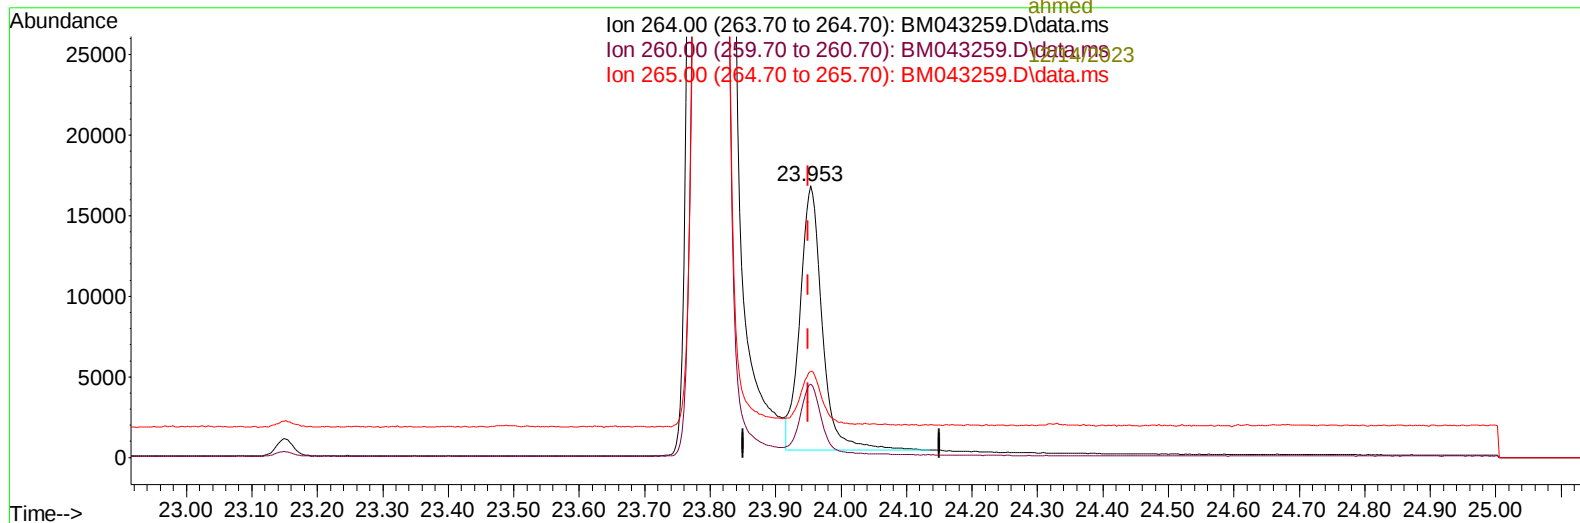

TIC: BM043259.D\data.ms

(23) Perylene-d12 (I)

23.953min (+ 0.003) 0.40 ng/u1

response 38811

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.02
265.00	39.10	31.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043259.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 H0AC0

Manual IntegrationsAPPROVED

Quant Time: Dec 12 12:31:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

12/14/2023
 Supervised By :mohammad
 ahmed

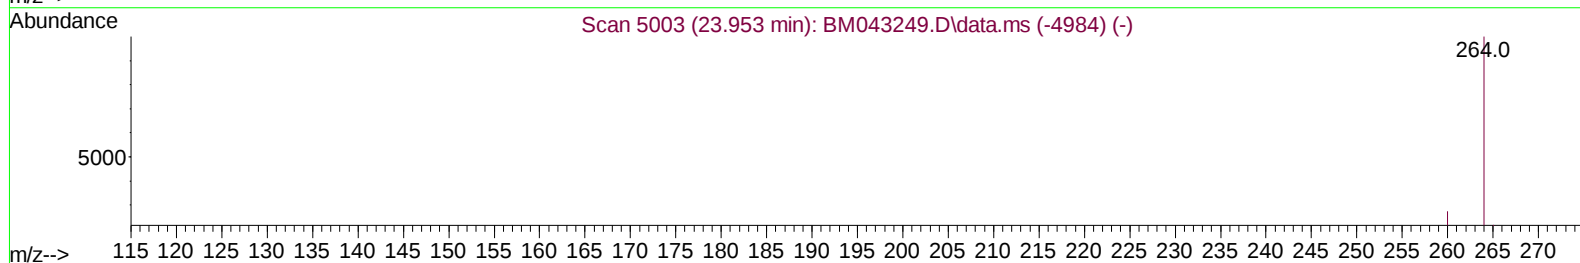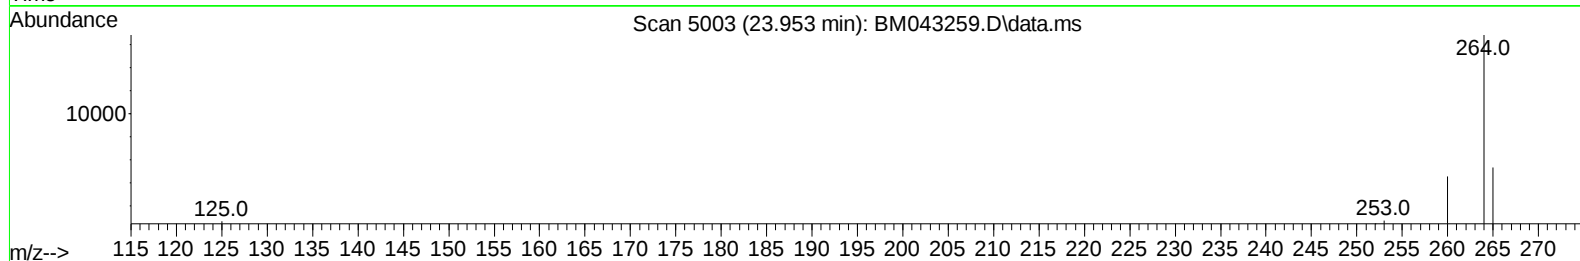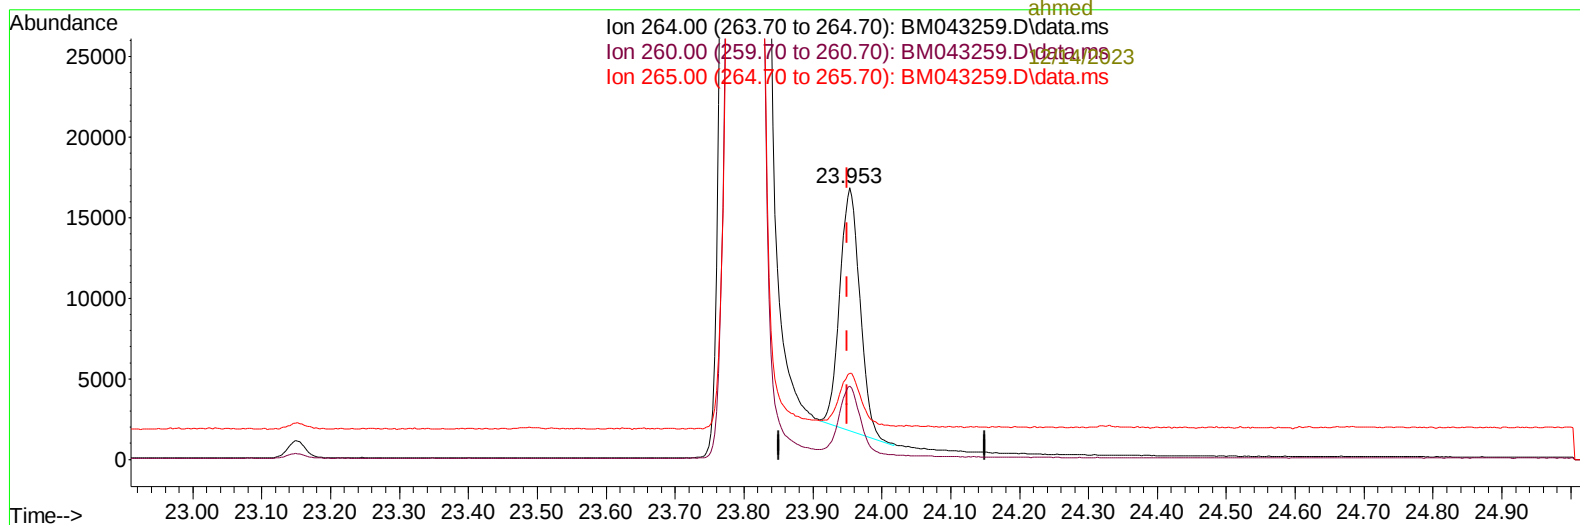

TIC: BM043259.D\data.ms

(23) Perylene-d12 (I)

23.953min (+ 0.003) 0.40 ng/ul m

response 30604

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.02
265.00	39.10	31.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043259.D
 Acq On : 12 Dec 2023 11:47
 Operator : MA/JU
 Sample : 05675-17
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0AC0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
 Patel

12/14/2023
 Supervised By :mohammad
 ahmed

Quant Time: Dec 12 12:31:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QI	Ion Response	Conc	Units	Dev(Min)
-----12/14/2023						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	13540	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	44724	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	25409	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	52482m	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	33138m	0.400	ng/ul	0.00
23) Perylene-d12	23.953	264	30604m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	45684	2.670	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	15686	0.248	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	30661	0.259	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.435	88	53162	3.098	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043259.D
Acq On : 12 Dec 2023 11:47
Operator : MA/JU
Sample : 05675-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0AC0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh
Patel

12/14/2023
Supervised By :mohammad
ahmed

12/14/2023

