

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043253.D
 Acq On : 12 Dec 2023 08:11
 Operator : MA/JU
 Sample : 05673-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHEJ2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/14/2023
 Supervised By :mohammad ahmed 12/14/2023

Quant Time: Dec 12 09:52:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	16057	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	52717	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	29441	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	60157m	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	36897m	0.400	ng/ul	0.00
23) Perylene-d12	23.950	264	34363m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	51548	2.541	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.396	152	15491	0.207	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	31160	0.236	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.861	128	5251	0.033	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043253.D
Acq On : 12 Dec 2023 08:11
Operator : MA/JU
Sample : 05673-05
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BHEJ2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :mohammad ahmed 12/14/2023


Quant Time: Dec 12 09:52:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration

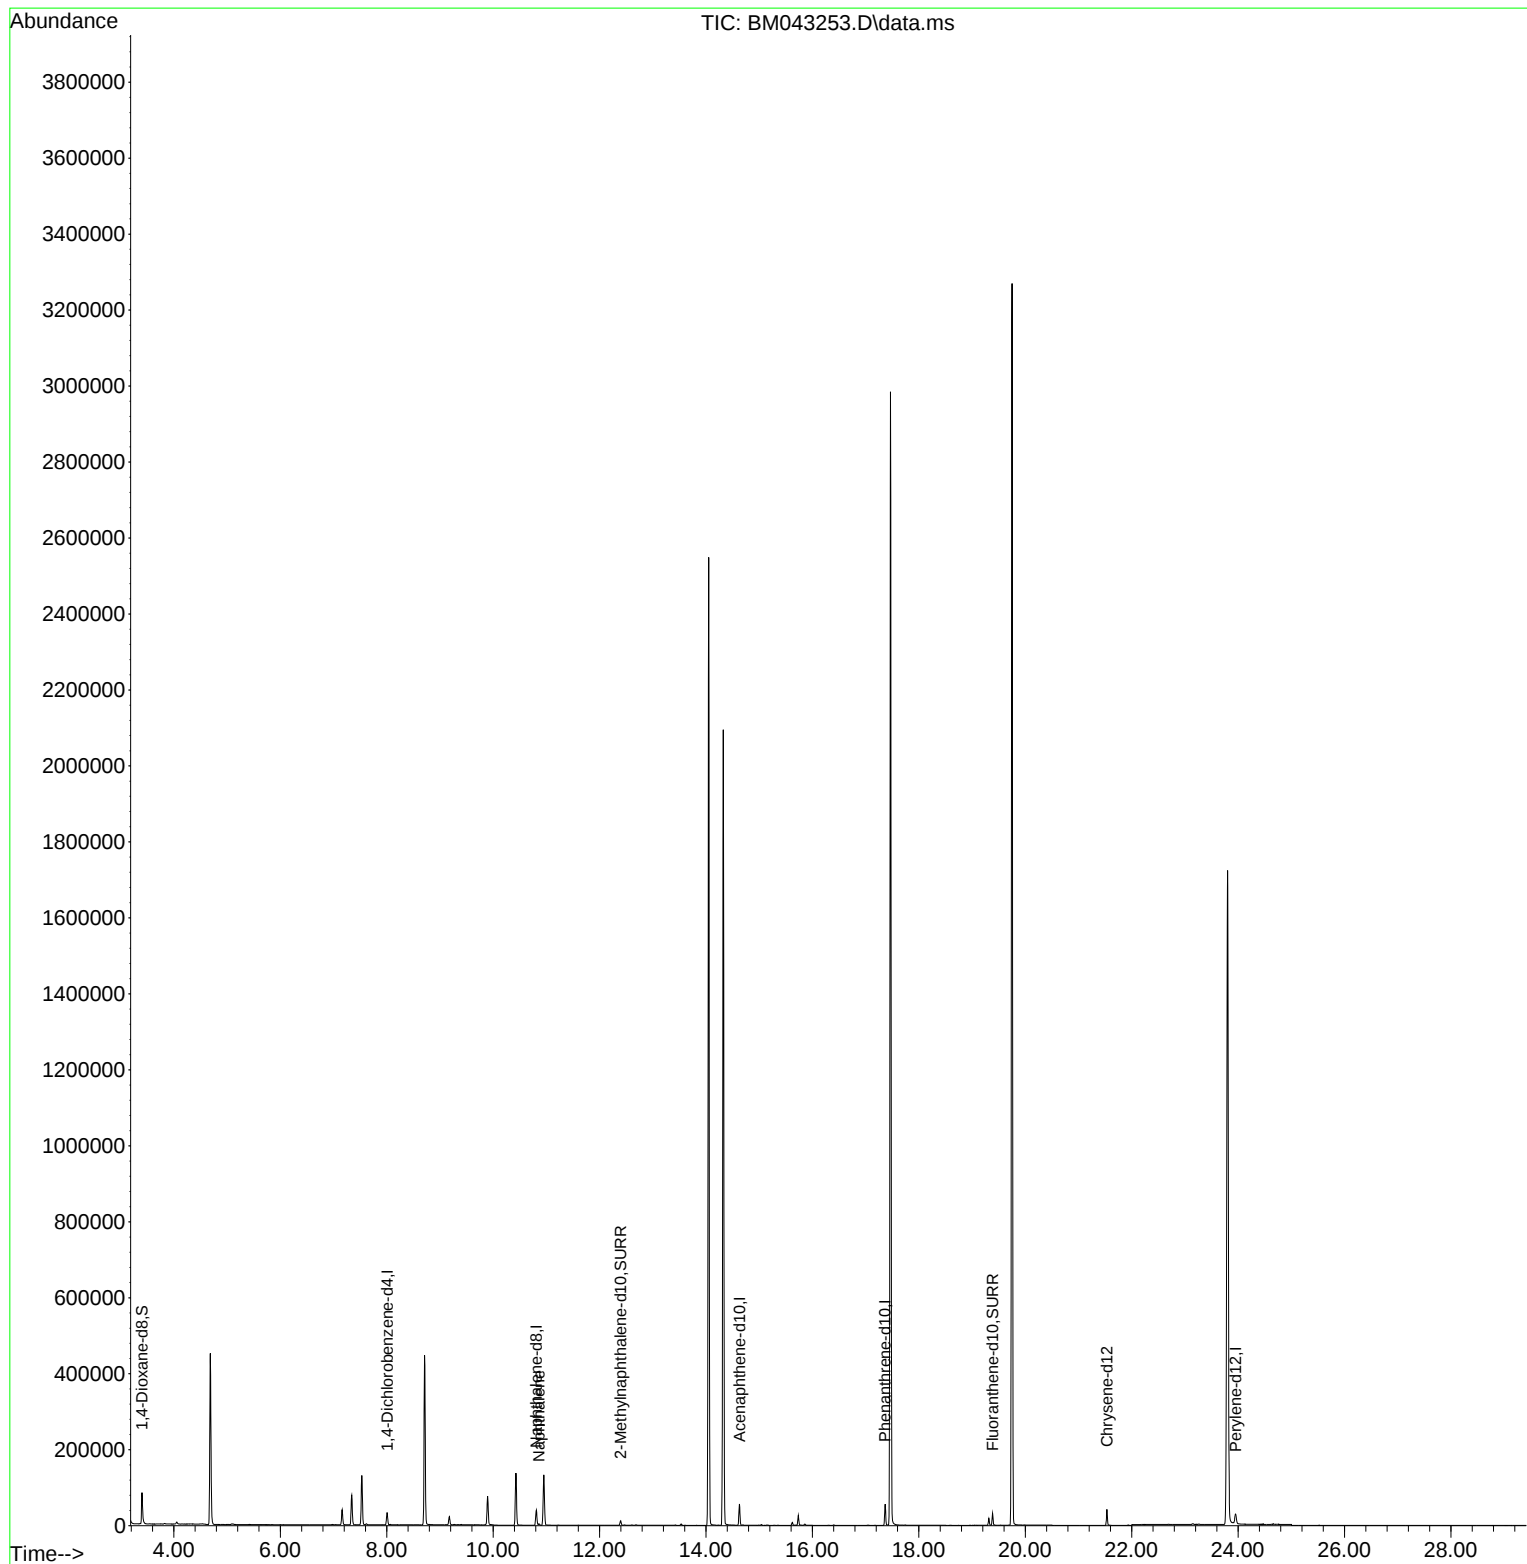

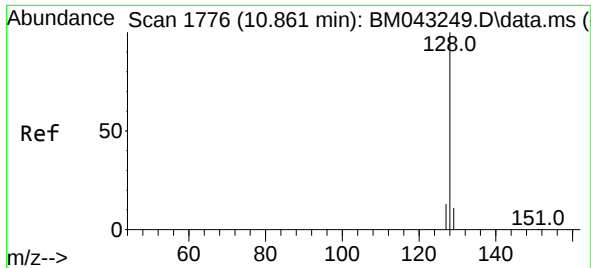

#5
Naphthalene
Concen: 0.033 ng/ul
RT: 10.861 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM043253.D
Acq: 12 Dec 2023 08:11

Instrument :
BNA_M
ClientSampleId :
BHEJ2

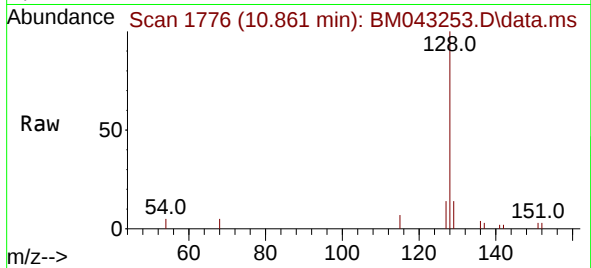

Tgt Ion:128 Resp: 525
Ion Ratio Lower Upper
128 100
129 13.7 9.0 13.4
127 14.4 10.3 15.5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/14/2023
Supervised By :mohammad ahmed 12/14/2023

