

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
 Data File : BM043277.D
 Acq On : 12 Dec 2023 23:11
 Operator : MA/JU
 Sample : 05698-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3B7

Quant Time: Dec 12 23:50:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 11 16:25:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	9764	0.400	ng/ul	0.00
4) Naphthalene-d8	10.812	136	30924	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.629	164	16358	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	33182	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	18940	0.400	ng/ul	# 0.00
23) Perylene-d12	23.950	264	19318	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.402	96	28914	2.344	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.390	152	14691	0.335	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	27271	0.403	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.436	88	9384	0.758	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121123\
Data File : BM043277.D
Acq On : 12 Dec 2023 23:11
Operator : MA/JU
Sample : 05698-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3B7

Quant Time: Dec 12 23:50:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 11 16:25:39 2023
Response via : Initial Calibration

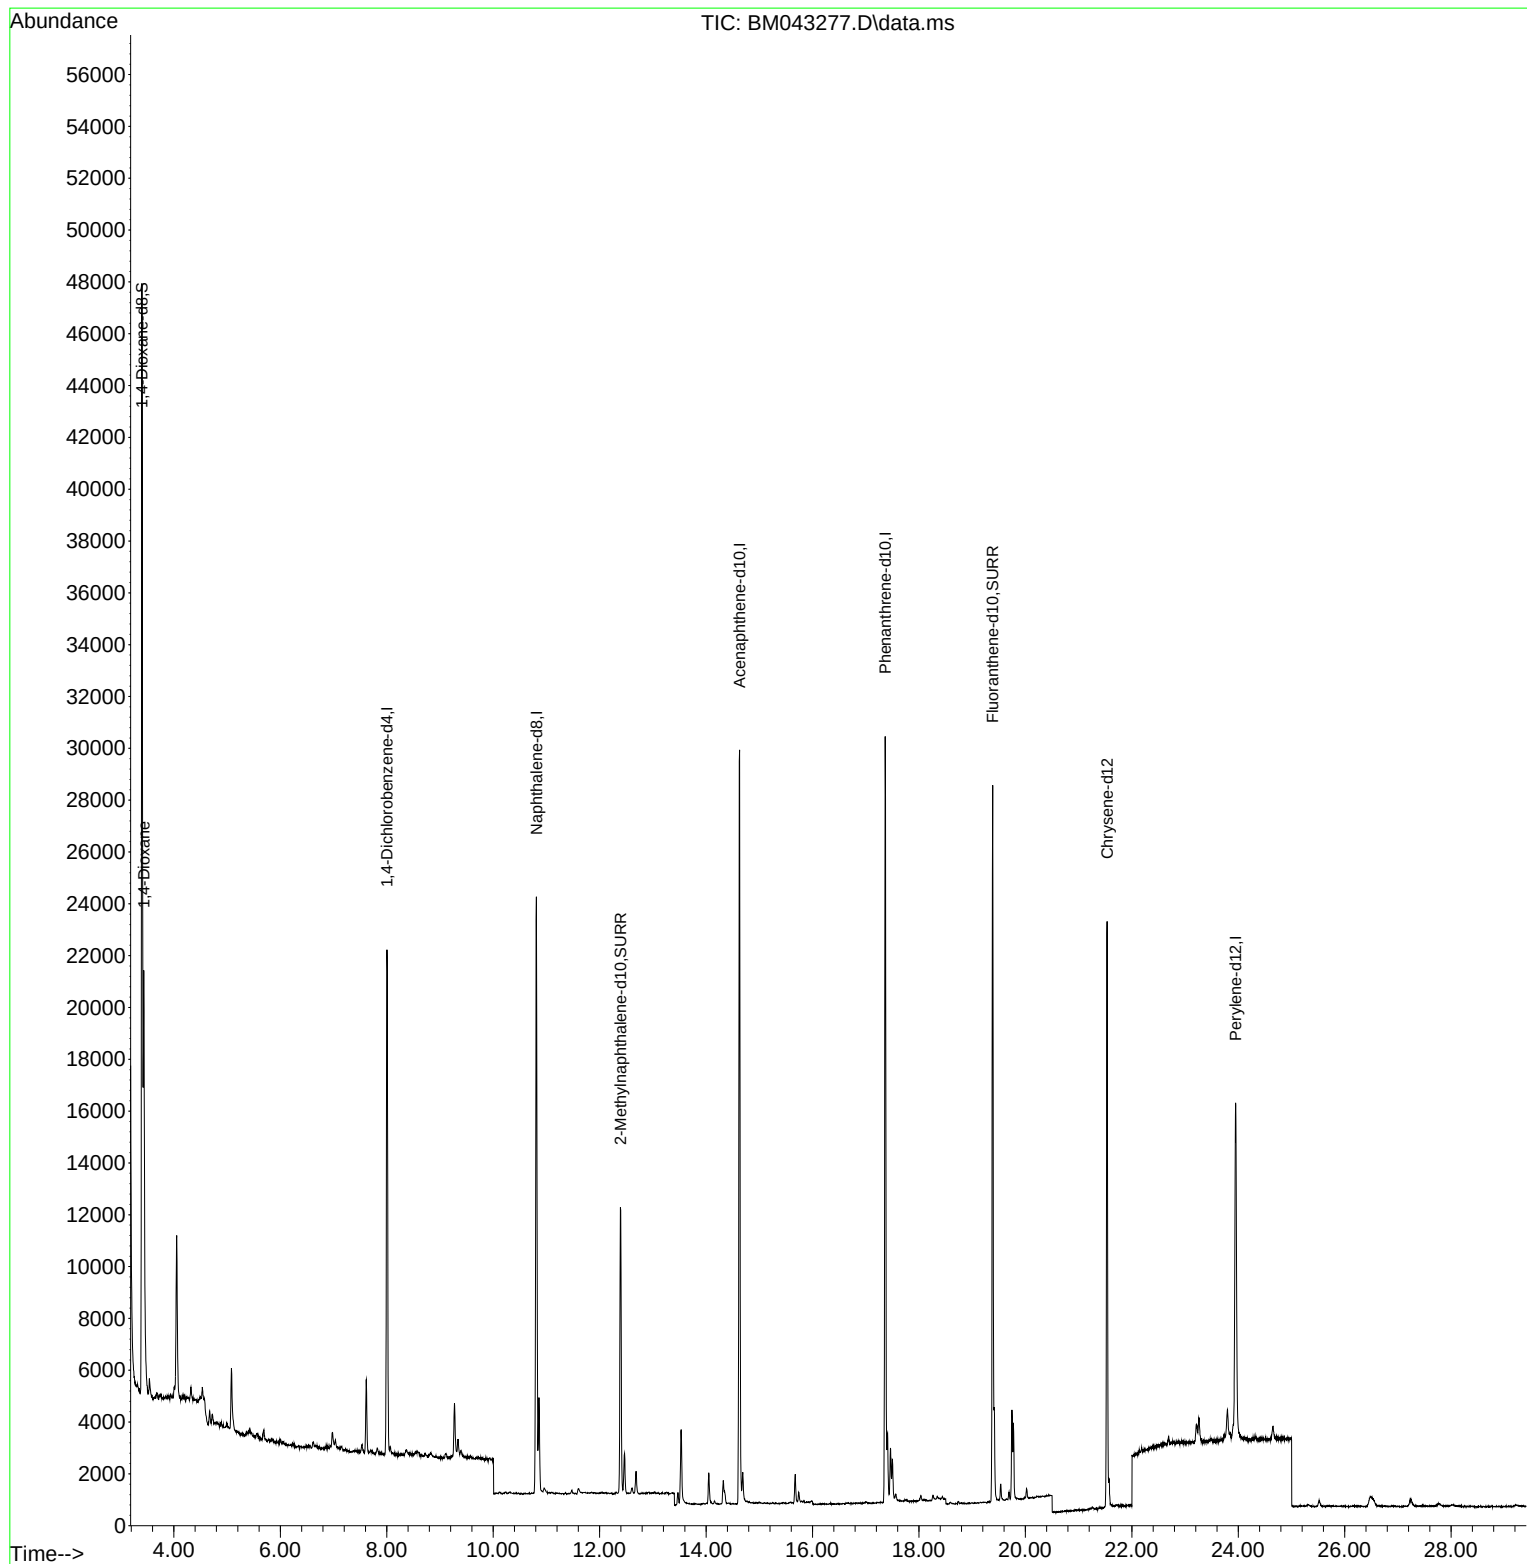

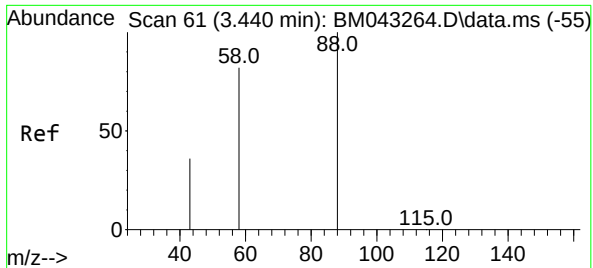

#2
 1,4-Dioxane
 Concen: 0.758 ng/ul
 RT: 3.436 min Scan# 60
 Delta R.T. -0.004 min
 Lab File: BM043277.D
 Acq: 12 Dec 2023 23:11

Instrument :
 BNA_M
 ClientSampleId :
 BH3B7

Tgt Ion:	88	Resp:	9384
Ion	Ratio	Lower	Upper
88	100		
43	40.0	27.9	41.9
58	66.4	43.4	65.2

