

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121216\
 Data File : BM008258.D
 Acq On : 12 Dec 2016 09:43
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD0.434

Quant Time: Dec 13 02:26:02 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 12 03:51:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	658	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.48	136	2215	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	1251	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	2003	0.40	ng/ul	0.00
16) Chrysene-d12	21.28	240	1825	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	1821	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.07	152	1259	0.40	ng/ul	-0.01
14) Fluoranthene-d10	19.12	212	2358	0.42	ng/ul	0.00


Target Compounds				Qvalue		
3) Naphthalene	10.52	128	2425	0.39	ng/ul	97
5) 2-Methylnaphthalene	12.14	142	1576	0.39	ng/ul	97
7) Acenaphthylene	14.04	152	2206	0.39	ng/ul	97
8) Acenaphthene	14.38	153	1629	0.38	ng/ul	93
9) Fluorene	15.39	166	1763	0.36	ng/ul	95
11) Pentachlorophenol	16.76	266	258	0.37	ng/ul	98
12) Phenanthrene	17.12	178	2543	0.41	ng/ul	95
13) Anthracene	17.21	178	2441	0.42	ng/ul	98
15) Fluoranthene	19.14	202	3184	0.40	ng/ul	94
17) Pyrene	19.51	202	3137	0.50	ng/ul	97
18) Benzo(a)anthracene	21.26	228	2621	0.47	ng/ul	99
19) Chrysene	21.31	228	2480	0.36	ng/ul	98
21) Benzo(b)fluoranthene	22.84	252	2563	0.35	ng/ul	96
22) Benzo(k)fluoranthene	22.89	252	2832	0.38	ng/ul	94
23) Benzo(a)pyrene	23.42	252	2645	0.39	ng/ul#	94
24) Indeno(1,2,3-cd)pyrene	25.77	276	3188	0.38	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.77	278	2508	0.37	ng/ul	95
26) Benzo(g,h,i)perylene	26.45	276	2753	0.37	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121216\
Data File : BM008258.D
Acq On : 12 Dec 2016 09:43
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
SSTD0.434

Quant Time: Dec 13 02:26:02 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 03:51:49 2016
Response via : Initial Calibration

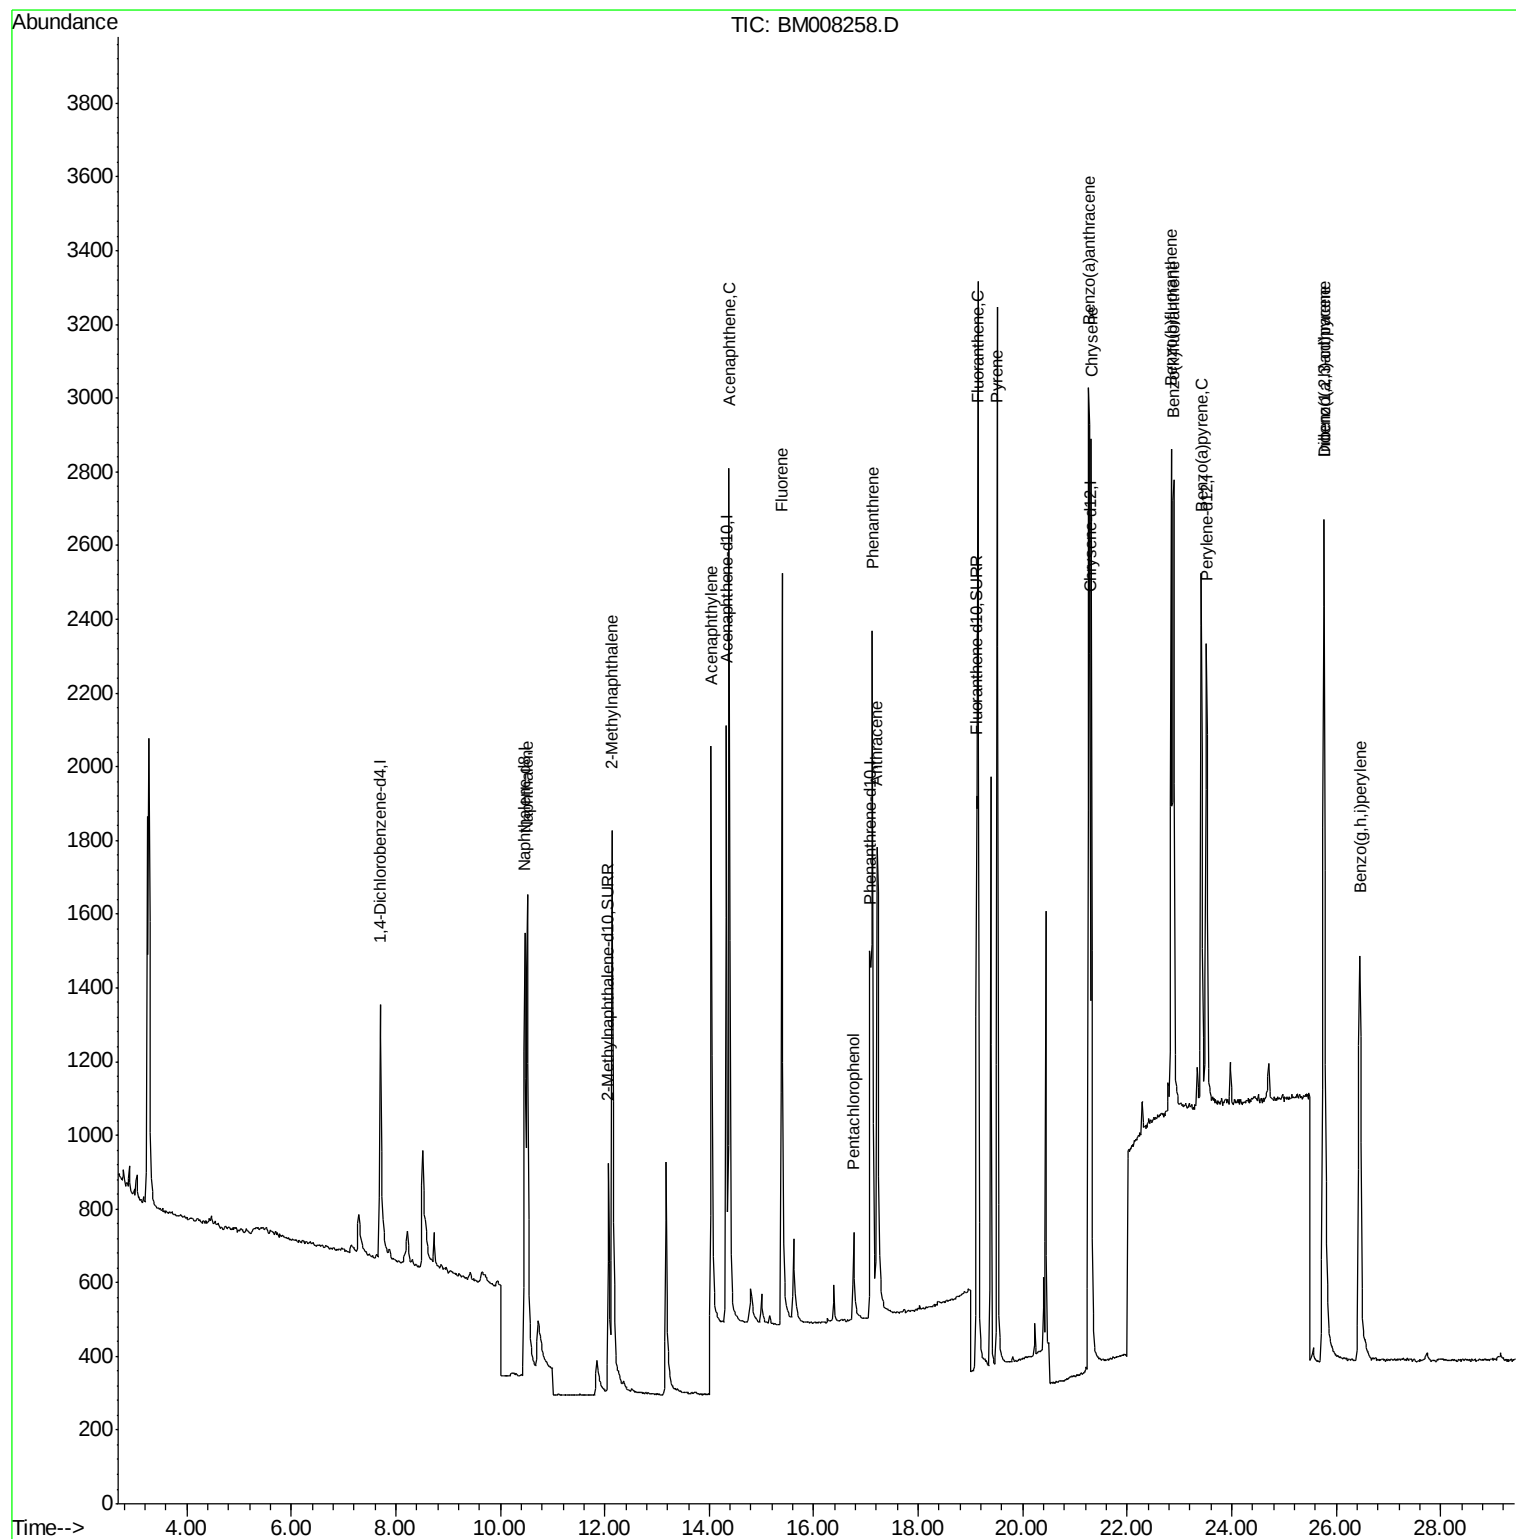

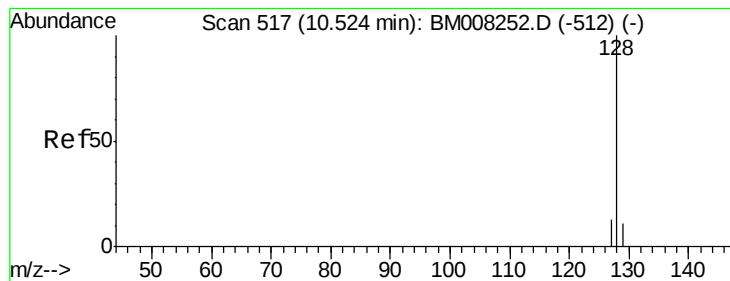

#3

Naphthalene

Concen: 0.39 ng/ul

RT: 10.52 min Scan# 517

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:128 Resp: 2425

Ion Ratio Lower Upper

128 100

129 15.2 11.3 16.9




127 17.0 12.8 19.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

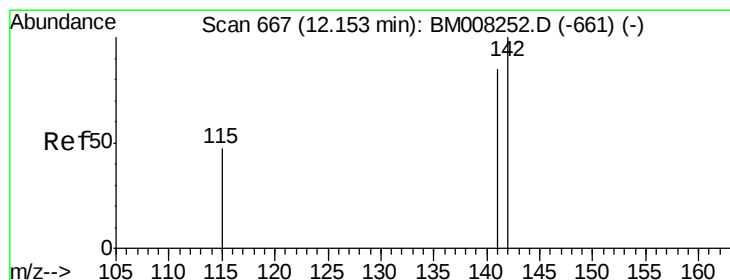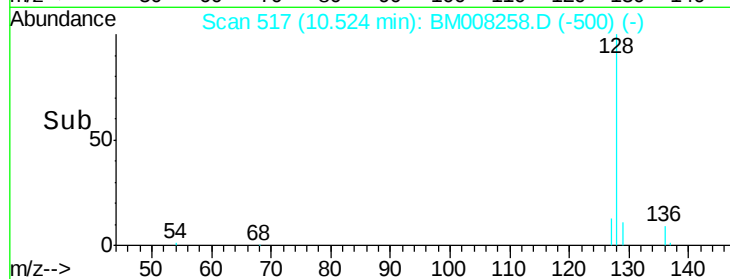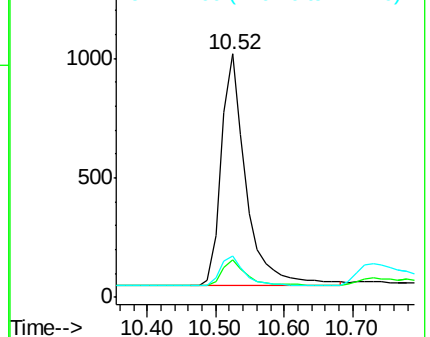

#5

2-Methylnaphthalene

Concen: 0.39 ng/ul

RT: 12.14 min Scan# 666

Delta R.T. -0.01 min

Lab File: BM008258.D


Acq: 12 Dec 2016 09:43

Tgt Ion:142 Resp: 1576

Ion Ratio Lower Upper



142 100


141 93.1 72.6 108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

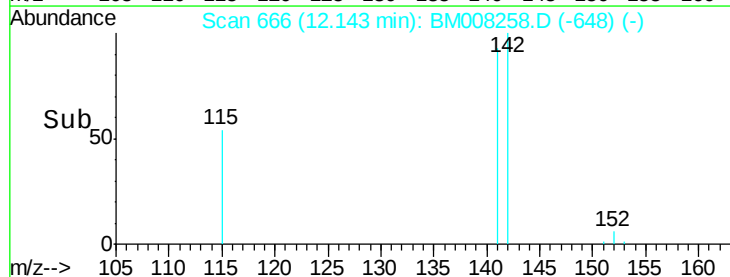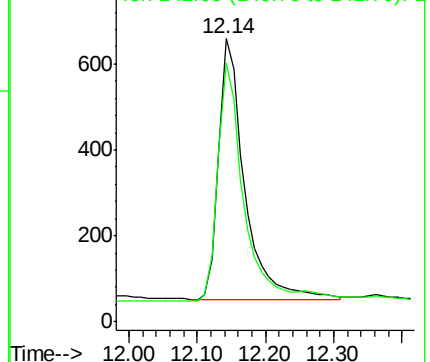

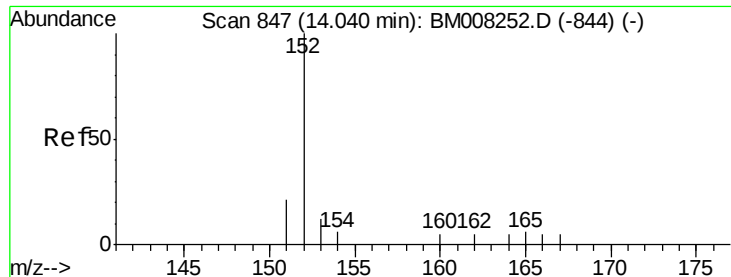

#7

Acenaphthylene

Concen: 0.39 ng/ul

RT: 14.04 min Scan# 847

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:152 Resp: 2206

Ion Ratio Lower Upper




152 100

151 23.5 17.1 25.7

153 16.2 12.8 19.2

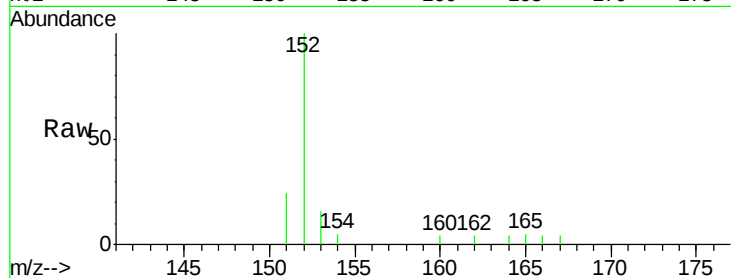

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

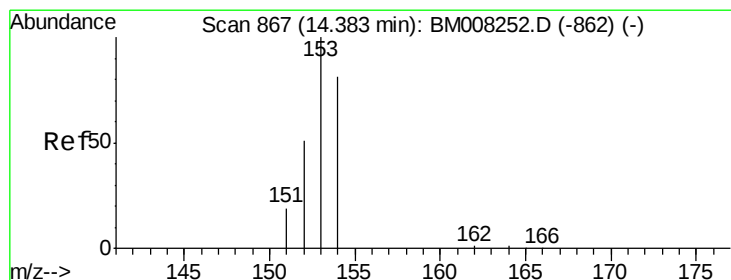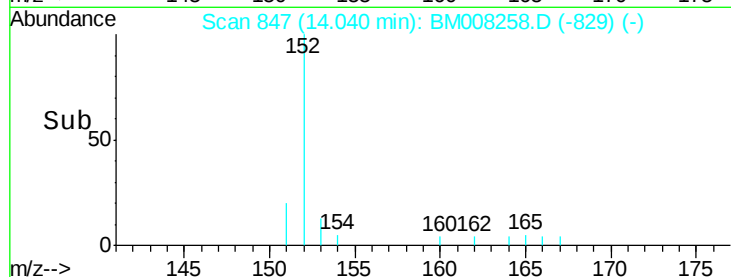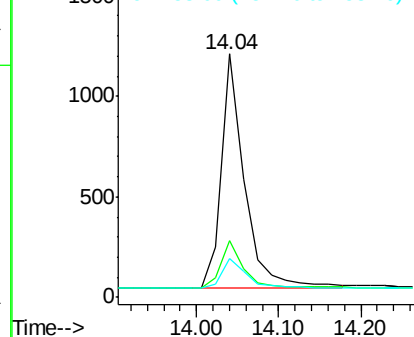

#8

Acenaphthene

Concen: 0.38 ng/ul

RT: 14.38 min Scan# 867

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion:153 Resp: 1629

Ion Ratio Lower Upper



153 100


152 54.7 40.3 60.5

154 82.7 71.4 107.2

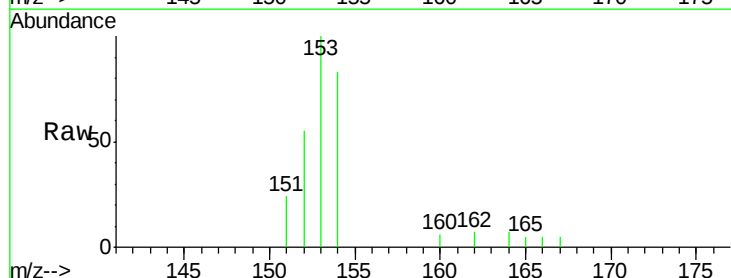

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

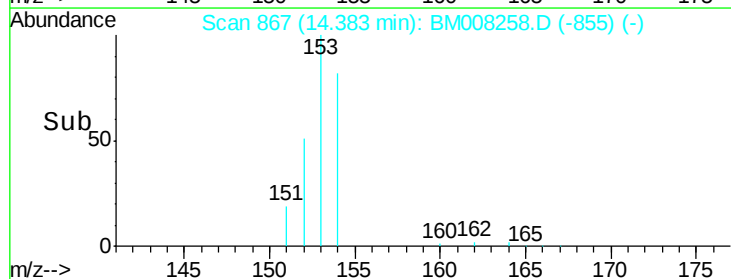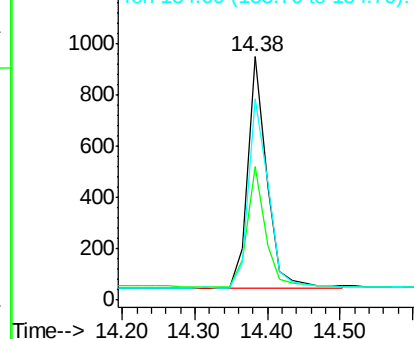

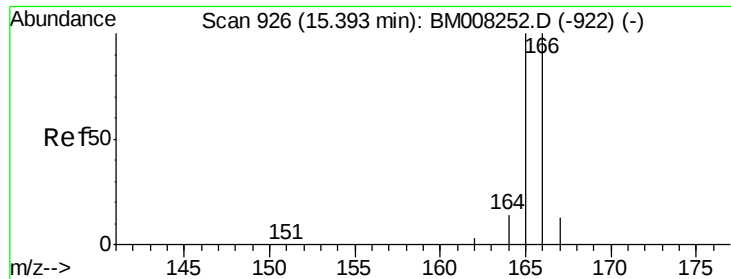

#9

Fluorene

Concen: 0.36 ng/ul

RT: 15.39 min Scan# 926

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:166 Resp: 1763

Ion Ratio Lower Upper

166 100

165 97.1 73.4 110.2




167 17.6 14.6 22.0

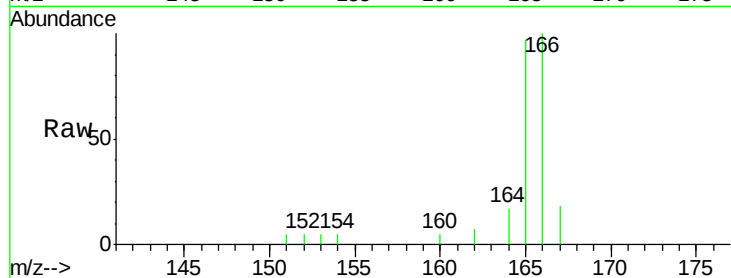

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

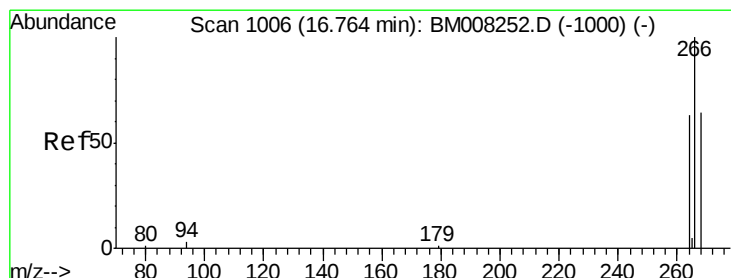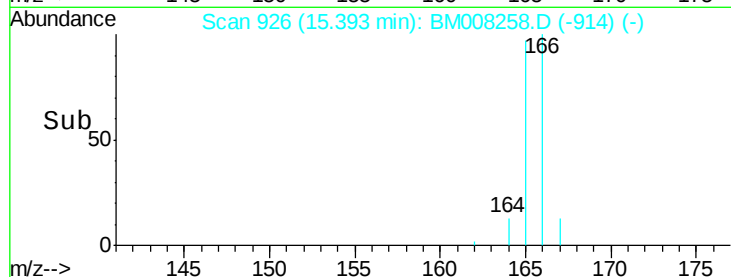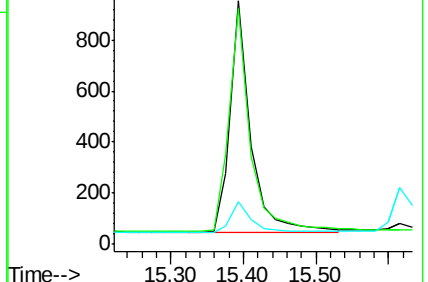

#11

Pentachlorophenol

Concen: 0.37 ng/ul

RT: 16.76 min Scan# 1006

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion:266 Resp: 258

Ion Ratio Lower Upper

266 100

264 62.4 47.9 71.9



268 63.2 49.8 74.8

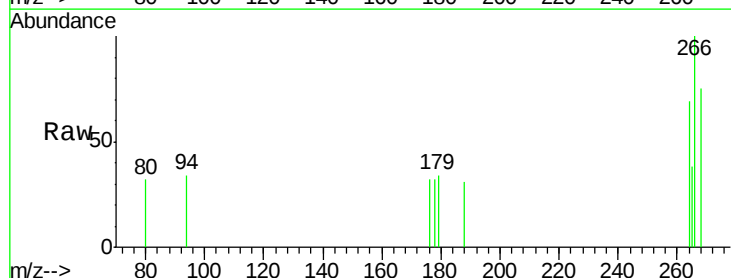


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

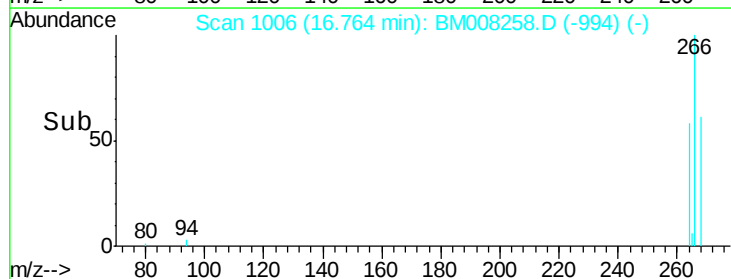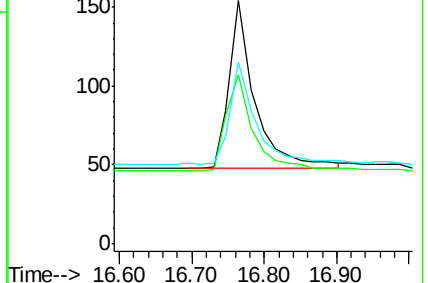

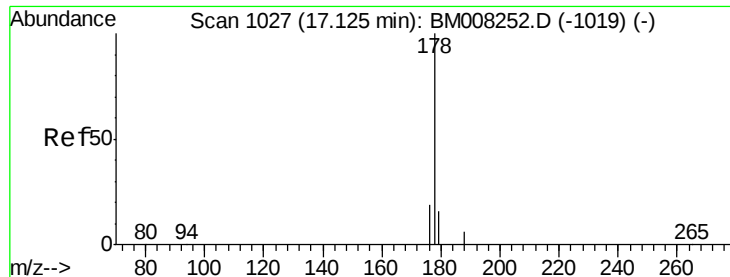

#12

Phenanthrene

Concen: 0.41 ng/ul

RT: 17.12 min Scan# 1027

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:178 Resp: 2543

Ion Ratio Lower Upper

178 100

176 20.8 18.4 27.6




179 19.1 13.6 20.4

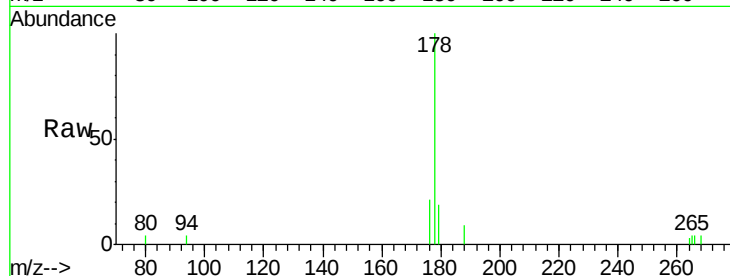

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

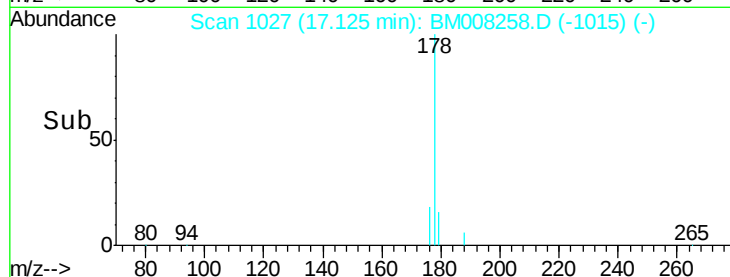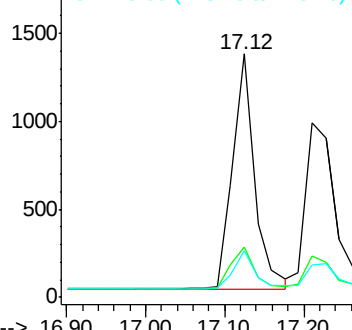

#13

Anthracene

Concen: 0.42 ng/ul

RT: 17.21 min Scan# 1032

Delta R.T. -0.02 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion:178 Resp: 2441

Ion Ratio Lower Upper

178 100

176 24.1 18.1 27.1



179 18.7 14.7 22.1




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



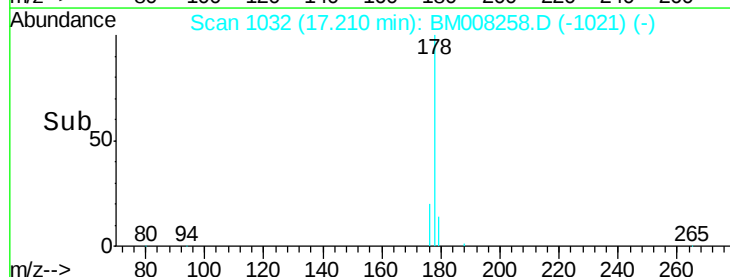
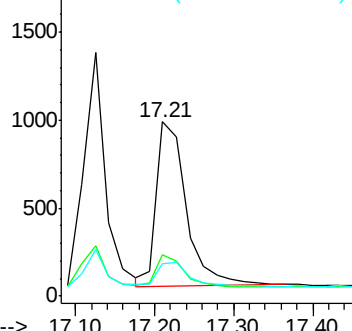


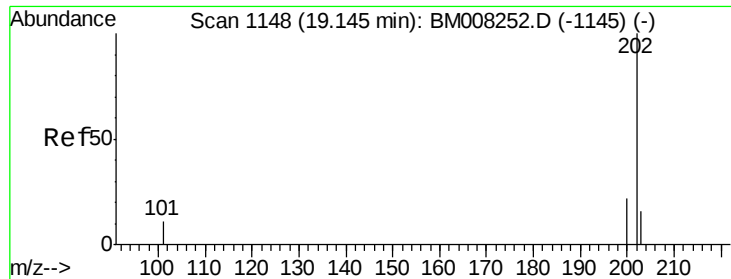

#15
Fluoranthene
 Concen: 0.40 ng/ul
 RT: 19.14 min Scan# 1148
 Delta R.T. -0.01 min
 Lab File: BM008258.D
 Acq: 12 Dec 2016 09:43




Instrument :
 BNA_M
 ClientSampleId :
 SST0.434


Tgt Ion:202 Resp: 3184
 Ion Ratio Lower Upper
 202 100
 101 15.4 0.0 30.3
 203 18.9 0.0 39.5

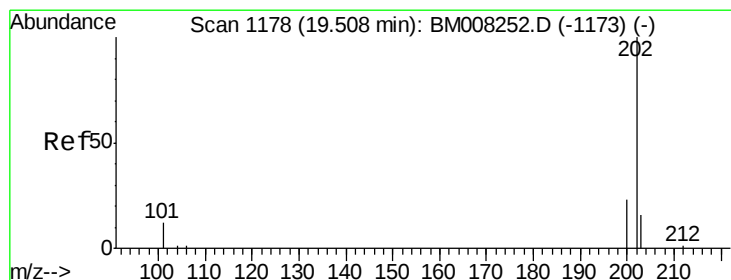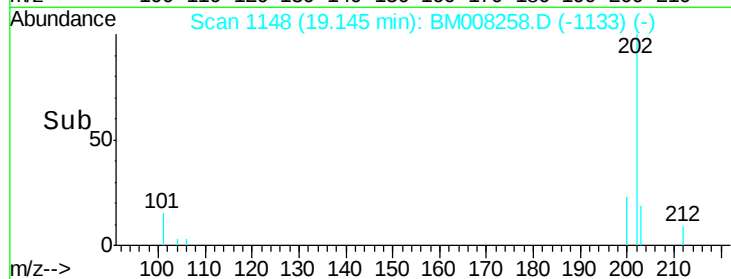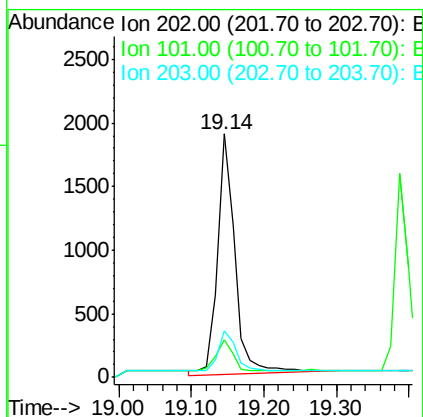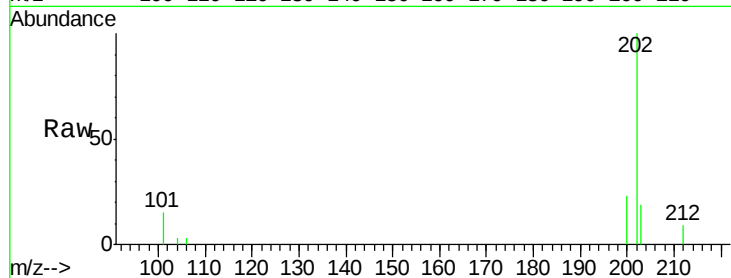

#17
Pyrene
 Concen: 0.50 ng/ul
 RT: 19.51 min Scan# 1178
 Delta R.T. -0.01 min
 Lab File: BM008258.D
 Acq: 12 Dec 2016 09:43

Tgt Ion:202 Resp: 3137
 Ion Ratio Lower Upper
 202 100
 200 24.5 18.2 27.4
 203 18.1 15.6 23.4

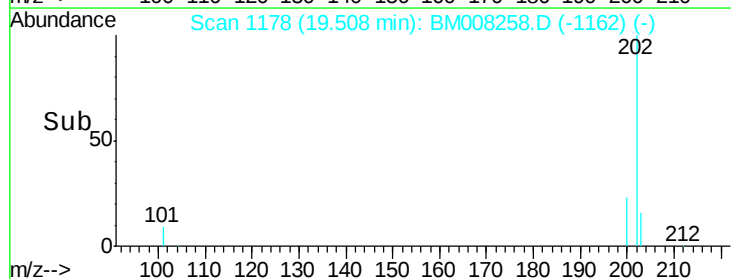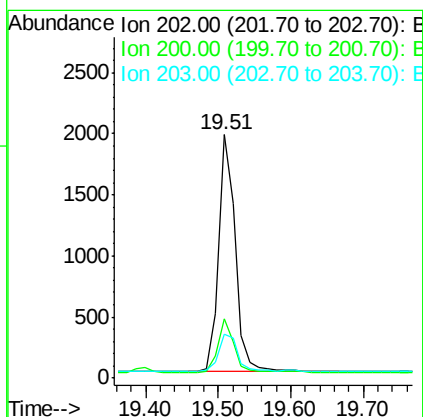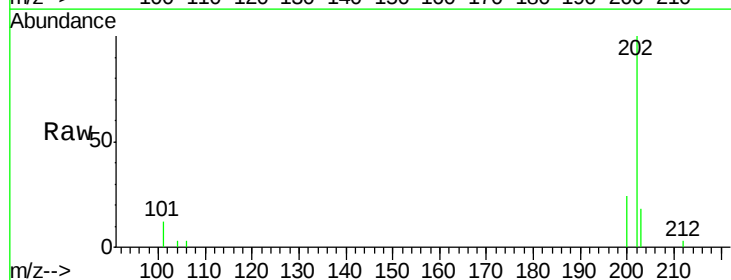

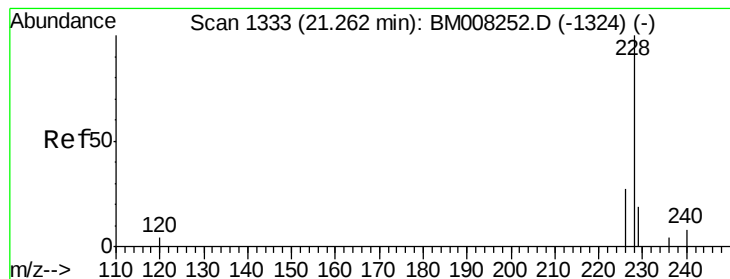

#18

Benzo(a)anthracene

Concen: 0.47 ng/ul

RT: 21.26 min Scan# 1333

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:228 Resp: 2621

Ion Ratio Lower Upper

228 100

226 29.0 22.8 34.2




229 22.3 17.0 25.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

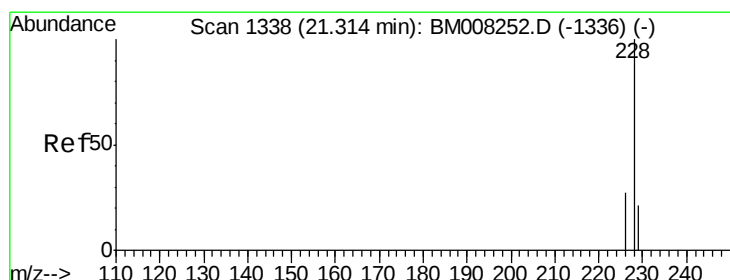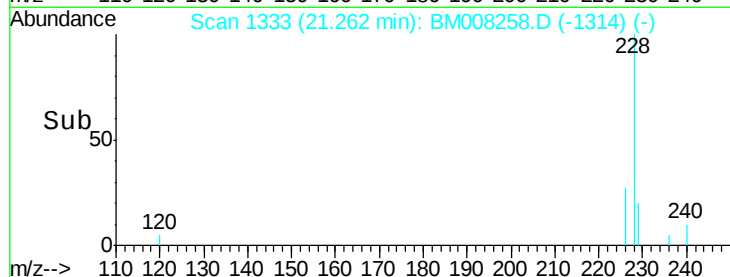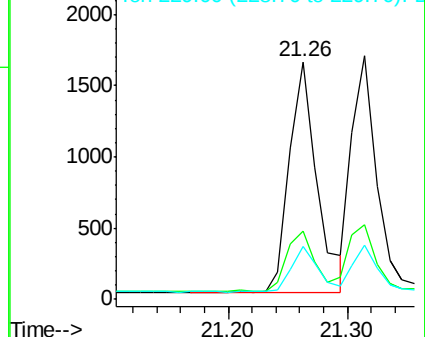

#19

Chrysene

Concen: 0.36 ng/ul

RT: 21.31 min Scan# 1338

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion:228 Resp: 2480

Ion Ratio Lower Upper

228 100

226 30.6 23.4 35.0



229 22.4 17.7 26.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

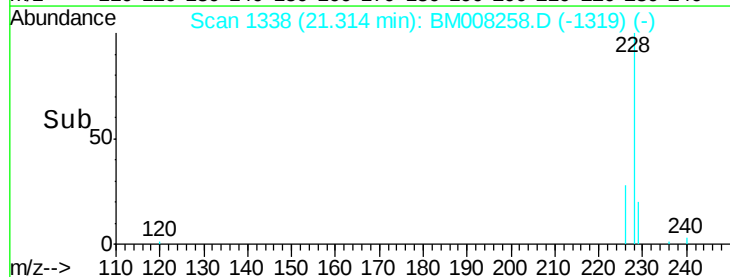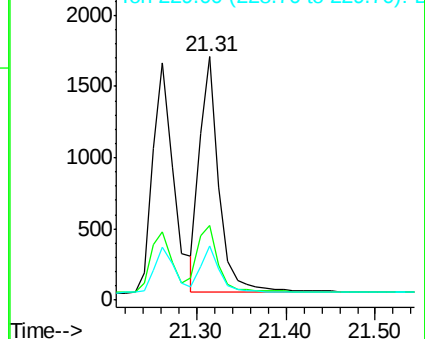

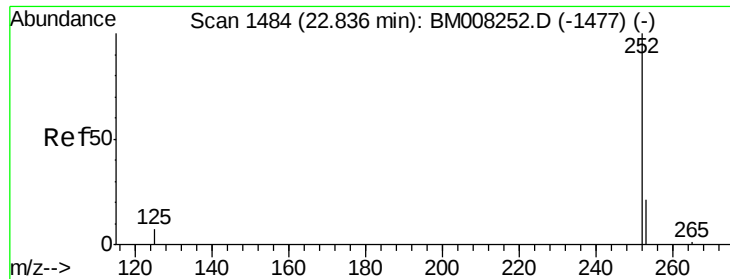

#21

Benzo(b)fluoranthene

Concen: 0.35 ng/u1

RT: 22.84 min Scan# 1484

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion:252 Resp: 2563

Ion Ratio Lower Upper




252 100

253 31.2 0.0 64.2

125 14.0 0.0 35.0



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

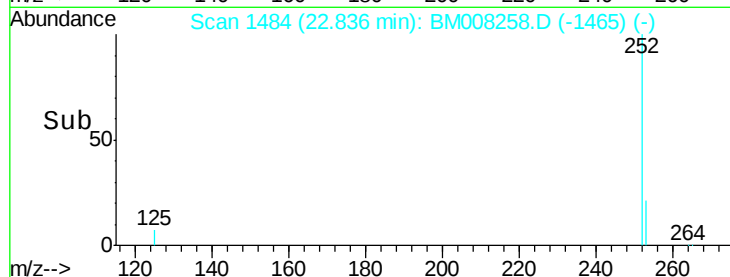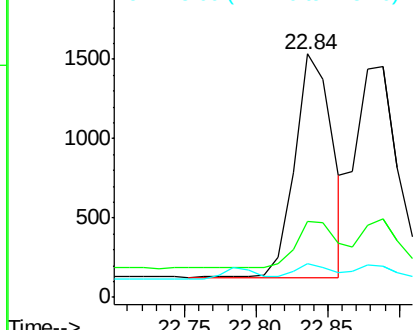

#22

Benzo(k)fluoranthene

Concen: 0.38 ng/u1

RT: 22.89 min Scan# 1489

Delta R.T. 0.01 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion:252 Resp: 2832

Ion Ratio Lower Upper



252 100


253 33.7 24.5 36.7

125 13.7 13.7 20.5



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

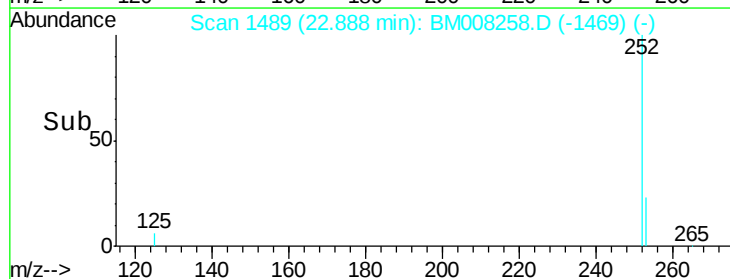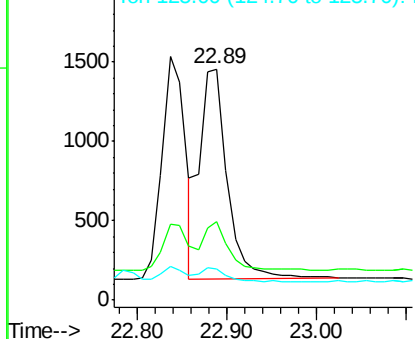

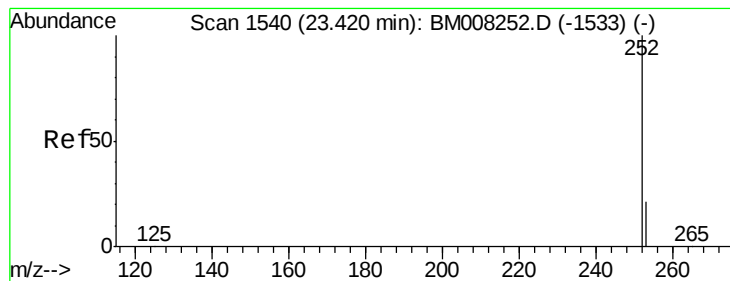

#23

Benzo(a)pyrene

Concen: 0.39 ng/ul

RT: 23.42 min Scan# 1540

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD0.434


Tgt Ion: 252 Resp: 2645

Ion Ratio Lower Upper

252 100

253 34.6 28.5 42.7




125 15.8 18.1 27.1#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

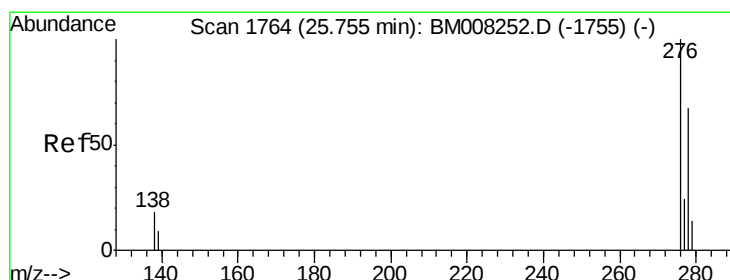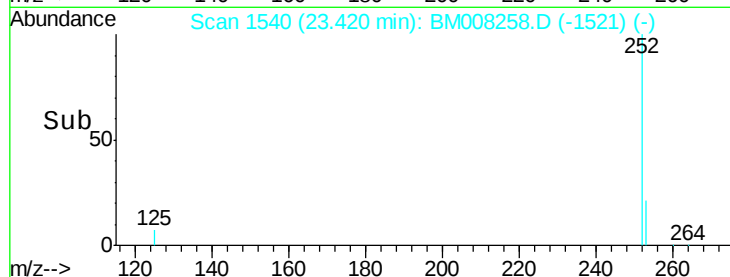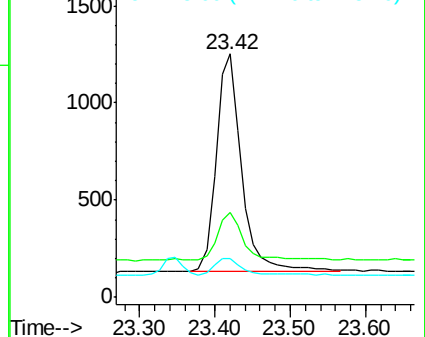

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.38 ng/ul

RT: 25.77 min Scan# 1765

Delta R.T. -0.00 min

Lab File: BM008258.D

Acq: 12 Dec 2016 09:43


Tgt Ion: 276 Resp: 3188

Ion Ratio Lower Upper

276 100

138 17.3 19.1 28.7#



277 24.7 19.6 29.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



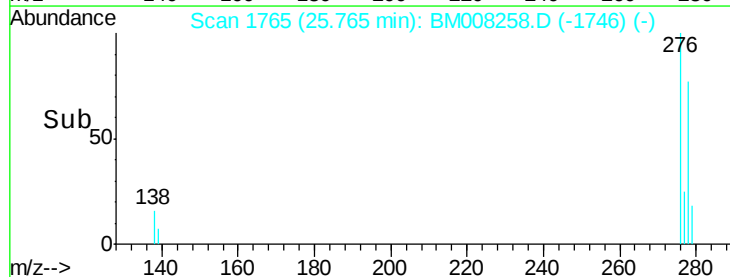
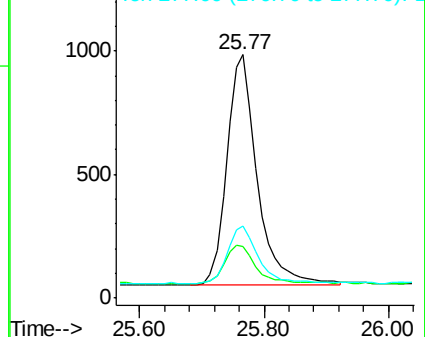


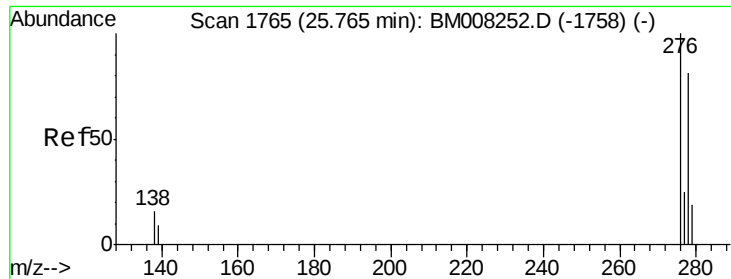

#25
Dibenzo(a,h)anthracene
Concen: 0.37 ng/ul
RT: 25.77 min Scan# 1765
Delta R.T. -0.00 min
Lab File: BM008258.D
Acq: 12 Dec 2016 09:43

Instrument :
BNA_M
ClientSampleId :
SSTD0.434

Tgt Ion:278 Resp: 2508
Ion Ratio Lower Upper
278 100
139 18.7 17.4 26.0
279 34.8 25.9 38.9

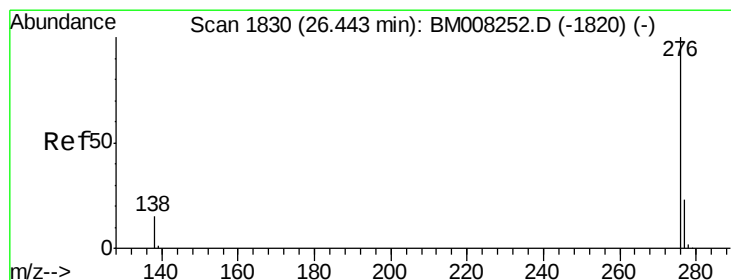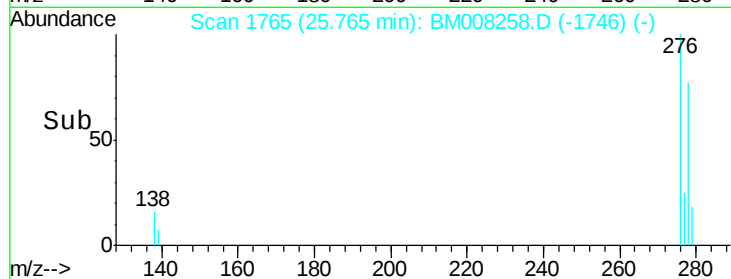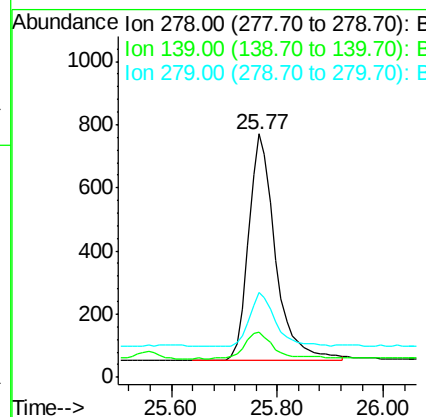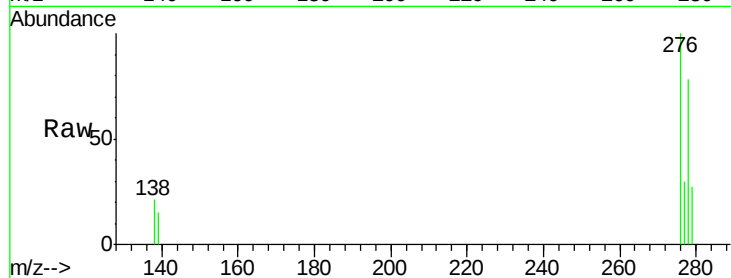

#26
Benzo(g,h,i)perylene
Concen: 0.37 ng/ul
RT: 26.45 min Scan# 1831
Delta R.T. 0.01 min
Lab File: BM008258.D
Acq: 12 Dec 2016 09:43

Tgt Ion:276 Resp: 2753
Ion Ratio Lower Upper
276 100
277 28.8 21.8 32.8
138 21.0 20.5 30.7

