


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121216\
Data File : BM008257.D
Acq On : 12 Dec 2016 09:07
Operator : UM/SJ
Sample : DFTPP65
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP65

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

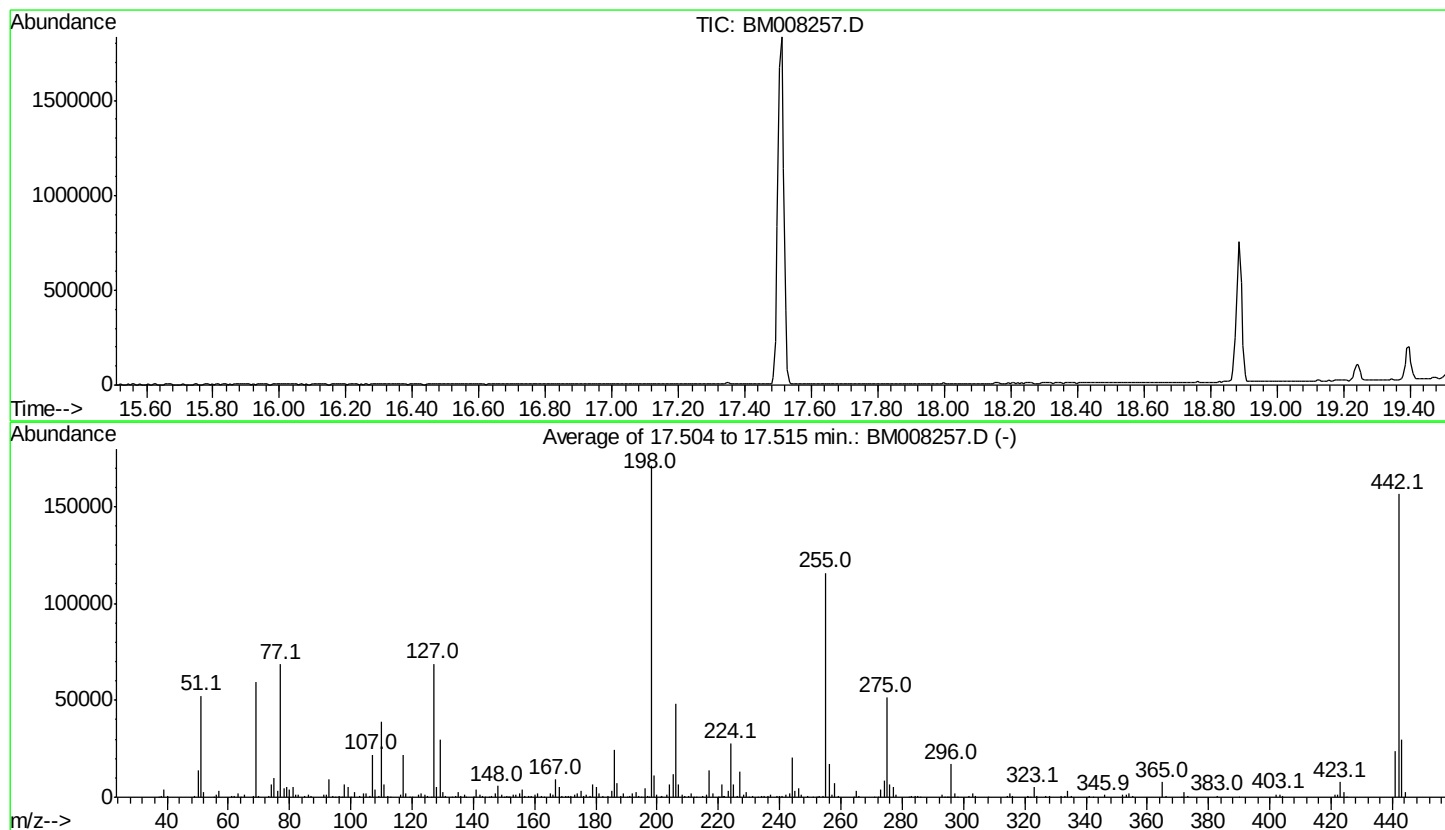

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	52482	PASS
68	69	0.00	2	1.6	974	PASS
69	198	0.00	100	34.7	59272	PASS
70	69	0.00	2	0.7	400	PASS
127	198	10	80	40.3	69010	PASS
197	198	0.00	2	0.4	753	PASS
198	198	100	100	100.0	171058	PASS
199	198	5	9	6.8	11555	PASS
275	198	10	60	29.9	51221	PASS
365	198	1	100	4.6	7813	PASS
441	443	0.01	100	78.6	23472	PASS
442	198	50	100	91.4	156352	PASS
443	442	15	24	19.1	29866	PASS

Scan 2530 (17.468 min): BM008257.D
DFTPP65

m/z	Abundance
40.00	2068.0
44.00	753.0
73.20	352.0
147.10	301.0
190.90	303.0
193.00	335.0
207.00	1376.0
208.10	398.0
281.10	886.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
37.10	382.0
38.10	679.0
39.00	4518.0
40.00	2458.0
44.00	723.0
49.00	481.0
50.10	16968.0
51.10	65504.0
52.10	3774.0
55.00	443.0
56.00	2017.0
57.00	4581.0
61.00	850.0
62.10	1038.0
63.00	2379.0
64.00	499.0
65.10	1420.0
68.10	1029.0
69.00	70488.0
70.00	559.0
73.10	981.0
74.10	8264.0
75.10	11662.0
76.00	4110.0
77.10	84552.0
78.10	5755.0
79.00	6980.0
80.00	5013.0
81.00	5862.0
82.00	1714.0
83.00	1050.0
85.10	1055.0
86.00	2076.0
87.00	856.0
91.00	1469.0
92.00	1895.0
93.00	11867.0
94.00	654.0
96.10	507.0
97.10	386.0
98.00	8246.0
99.00	7121.0
100.00	571.0
101.00	3653.0
103.00	1042.0
104.00	2469.0
105.00	2785.0
106.00	560.0
107.00	25936.0
108.00	4161.0
109.10	846.0
110.00	46360.0
111.00	7639.0
112.00	857.0
113.10	349.0
116.00	1736.0
117.00	26568.0
118.00	2232.0
119.00	472.0
120.10	531.0
122.00	1541.0
123.00	2705.0
124.00	1605.0
125.00	1163.0
126.20	559.0
127.00	80832.0
128.10	6103.0
129.00	35952.0
130.00	2965.0
131.10	575.0
134.00	996.0
135.10	2675.0
135.90	1089.0
137.00	1743.0
137.70	327.0
139.90	596.0
141.00	5295.0
142.00	1840.0
143.00	1142.0
144.00	491.0
146.00	1116.0
147.00	2836.0
148.00	7346.0
149.00	1176.0
151.00	596.0
151.70	491.0
153.00	1361.0
154.10	1283.0
155.00	2542.0
156.00	3915.0
156.90	588.0
158.00	717.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

159.10	632.0
160.00	1408.0
161.00	2301.0
162.10	569.0
165.00	2126.0
166.00	1299.0
167.00	9551.0
168.10	5481.0
169.00	1094.0
170.00	352.0
171.00	555.0
172.00	1065.0
173.10	995.0
174.00	2346.0
175.00	3725.0
176.00	872.0
177.00	1730.0
178.00	671.0
179.00	7139.0
180.00	5746.0
181.00	2148.0
182.10	332.0
184.00	442.0
185.10	3555.0
186.00	25968.0
187.10	7851.0
188.00	1254.0
189.00	1919.0
191.10	1110.0
192.00	2331.0
193.10	2662.0
194.00	529.0
196.00	5704.0
197.00	1053.0
198.00	187136.0
199.00	12634.0
199.90	1229.0
201.50	769.0
203.00	1537.0
204.10	7060.0
205.10	12245.0
206.10	52480.0
207.10	7880.0
208.00	1918.0
209.10	1133.0
210.10	938.0
211.10	2121.0
212.90	341.0
215.10	506.0
216.00	1304.0
217.00	14916.0
218.00	2087.0
221.00	7598.0
221.70	1767.0
223.00	3282.0
224.10	30560.0
225.10	8028.0
226.00	746.0
227.00	12735.0
228.10	1562.0
229.00	2728.0
230.90	1085.0
232.80	317.0
234.00	802.0
234.90	1122.0
236.10	833.0
236.90	1364.0
238.90	561.0
240.10	412.0
241.00	522.0
242.00	1674.0
243.00	1850.0
244.10	20952.0
245.00	3355.0
246.00	5031.0
247.00	1235.0
249.00	672.0
253.00	738.0
254.20	963.0
255.00	119864.0
256.00	18272.0
257.10	1327.0
258.00	7197.0
259.00	1058.0
265.10	3005.0
266.00	463.0
271.00	343.0
272.20	549.0
273.00	3769.0
274.00	8659.0
275.00	51400.0
276.00	6518.0
277.00	5493.0
278.00	1372.0
281.00	479.0
283.00	640.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

284.10	551.0
285.10	958.0
286.00	360.0
292.90	1034.0
296.00	16592.0
297.00	2302.0
298.20	328.0
301.90	489.0
303.00	2168.0
304.00	592.0
307.90	386.0
314.00	907.0
315.00	1964.0
316.00	984.0
320.90	682.0
323.10	5137.0
324.00	929.0
327.00	1110.0
328.00	471.0
332.00	388.0
332.90	576.0
334.00	3189.0
335.10	925.0
341.00	636.0
345.90	1007.0
352.00	1466.0
352.90	1045.0
354.00	1732.0
355.00	370.0
365.00	7341.0
366.10	892.0
370.90	349.0
372.00	2496.0
373.10	626.0
383.00	795.0
402.10	935.0
403.10	1388.0
404.10	487.0
421.00	934.0
422.00	1188.0
423.10	6815.0
424.10	2043.0
441.00	20688.0
442.10	132992.0
443.10	27328.0
444.10	2314.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
38.00	665.0
39.10	4169.0
40.00	2718.0
44.00	848.0
49.10	495.0
50.10	15478.0
51.10	60176.0
52.10	3197.0
55.10	361.0
56.00	1989.0
57.00	3987.0
61.00	1114.0
62.00	1153.0
63.00	2922.0
64.10	551.0
65.10	1219.0
68.00	1094.0
69.00	70344.0
70.00	341.0
73.10	1345.0
74.10	7665.0
75.00	12375.0
76.10	4159.0
77.10	78528.0
78.10	5623.0
79.00	5920.0
80.00	4148.0
81.10	5766.0
82.10	1815.0
83.00	1219.0
85.00	1381.0
85.90	1526.0
87.00	797.0
91.00	1292.0
92.10	1613.0
93.00	10114.0
94.00	914.0
96.10	459.0
98.00	7894.0
99.00	5943.0
100.00	396.0
101.10	3394.0
103.00	1228.0
104.10	1811.0
105.10	2041.0
106.10	543.0
107.00	26656.0
108.00	4628.0
109.00	816.0
110.00	44752.0
111.00	7449.0
112.00	776.0
116.10	1953.0
117.00	26216.0
118.00	1631.0
122.10	1781.0
123.00	2238.0
124.00	1223.0
125.00	966.0
127.00	79824.0
128.00	6094.0
129.00	34864.0
130.00	2832.0
131.00	372.0
133.00	368.0
134.00	1255.0
135.00	2880.0
136.00	1187.0
137.00	1883.0
140.10	535.0
141.00	4425.0
142.00	1833.0
142.90	996.0
144.00	316.0
144.90	321.0
145.90	785.0
147.00	2947.0
148.00	6739.0
149.10	1241.0
150.00	415.0
150.90	635.0
152.00	444.0
153.00	1584.0
154.00	1066.0
155.00	2874.0
156.00	4870.0
156.90	493.0
158.00	1527.0
159.00	588.0
160.00	1749.0
161.00	2749.0
162.00	665.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

162.90	373.0
165.00	2235.0
166.00	1394.0
167.00	10854.0
168.00	5710.0
169.00	821.0
170.00	522.0
171.00	670.0
172.00	829.0
173.00	1456.0
174.00	1873.0
175.00	3931.0
176.00	1216.0
176.90	1828.0
178.00	891.0
179.00	7719.0
180.00	6315.0
181.00	1861.0
182.00	390.0
184.10	635.0
185.00	4436.0
186.00	29192.0
187.00	8841.0
188.00	1094.0
188.90	2395.0
190.00	425.0
190.90	989.0
192.10	2420.0
193.00	3438.0
194.10	682.0
194.90	541.0
196.00	5593.0
196.80	1207.0
198.00	205184.0
199.00	13614.0
200.00	1105.0
201.50	893.0
202.90	1939.0
204.00	7557.0
205.00	14250.0
206.10	57032.0
207.10	9045.0
208.00	2528.0
208.90	926.0
210.10	955.0
211.00	2149.0
211.90	351.0
213.00	304.0
214.90	707.0
216.10	1708.0
217.00	16536.0
218.00	1651.0
220.30	419.0
221.00	7616.0
221.90	1696.0
223.00	3971.0
224.10	33408.0
225.00	8129.0
226.10	803.0
227.00	16050.0
228.00	2295.0
229.00	3452.0
230.00	314.0
231.00	1247.0
234.00	966.0
235.00	965.0
236.00	657.0
237.00	1518.0
239.00	504.0
240.00	489.0
240.90	945.0
242.00	1849.0
243.10	2132.0
244.10	24280.0
245.10	3859.0
246.00	5547.0
247.00	1005.0
249.00	1134.0
250.90	315.0
252.00	429.0
253.00	602.0
254.00	879.0
255.00	139648.0
256.00	20560.0
257.00	2049.0
258.00	8316.0
259.00	1017.0
264.00	319.0
265.00	3437.0
265.90	497.0
273.10	4523.0
274.00	10606.0
275.00	61000.0
276.00	9158.0
277.00	6656.0
278.00	1143.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

281.00	584.0
282.10	320.0
283.00	658.0
284.00	641.0
285.00	786.0
292.90	1230.0
294.00	447.0
294.80	471.0
296.00	21584.0
297.00	2612.0
298.10	345.0
302.00	575.0
303.00	2283.0
304.00	684.0
314.10	949.0
315.00	2349.0
316.00	1346.0
320.90	713.0
321.90	353.0
323.10	5840.0
324.00	1139.0
327.00	1309.0
327.90	511.0
332.00	435.0
333.00	828.0
334.00	3800.0
335.00	1024.0
341.00	984.0
342.10	324.0
346.00	1273.0
352.10	1880.0
353.00	1437.0
354.00	1945.0
355.10	352.0
365.00	9290.0
366.00	1153.0
372.10	3116.0
373.00	792.0
383.00	1076.0
390.10	338.0
402.00	1196.0
403.10	1445.0
404.00	559.0
421.00	1756.0
422.00	1223.0
423.10	9467.0
424.10	3135.0
425.00	449.0
441.00	26680.0
442.10	187392.0
443.10	36256.0
444.00	3446.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
39.10	2399.0
40.00	2753.0
44.00	423.0
49.10	401.0
50.10	8303.0
51.10	31768.0
52.10	1531.0
56.10	953.0
57.00	2316.0
61.00	385.0
62.00	477.0
63.00	1400.0
65.10	713.0
68.10	800.0
69.00	36984.0
70.00	300.0
73.10	957.0
74.10	4540.0
75.00	6110.0
76.00	2332.0
77.10	42192.0
78.10	3293.0
79.00	3288.0
80.00	2314.0
81.00	3311.0
82.00	813.0
83.00	785.0
85.10	609.0
86.00	1047.0
86.90	443.0
91.00	810.0
92.00	761.0
93.00	5979.0
94.00	389.0
95.00	371.0
95.90	331.0
98.00	4302.0
99.00	3752.0
101.00	1850.0
103.00	599.0
104.10	1451.0
105.00	1298.0
106.10	505.0
107.00	13423.0
108.00	2406.0
109.20	407.0
110.00	25584.0
111.00	4115.0
112.00	520.0
116.10	693.0
117.00	13586.0
118.10	1223.0
122.00	1108.0
123.00	1674.0
124.00	739.0
125.00	584.0
127.00	46376.0
128.10	3670.0
129.00	19328.0
130.10	1893.0
131.00	354.0
133.00	373.0
134.00	606.0
135.00	1846.0
136.00	630.0
137.00	919.0
141.10	3144.0
141.90	803.0
143.00	530.0
146.00	606.0
147.00	1653.0
148.00	3673.0
149.00	785.0
151.20	425.0
151.90	323.0
152.90	1023.0
154.00	971.0
155.00	1476.0
156.00	2983.0
157.00	530.0
158.10	634.0
159.00	437.0
160.00	851.0
161.00	1338.0
162.00	577.0
164.90	1362.0
166.00	606.0
167.00	6647.0
168.00	4138.0
168.90	588.0
169.90	338.0
171.90	605.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

173.00	709.0
174.00	1269.0
175.00	2414.0
175.90	773.0
177.00	1422.0
177.90	457.0
178.90	4675.0
179.90	2886.0
181.00	1410.0
182.00	422.0
184.00	430.0
185.10	2303.0
186.10	17264.0
187.10	5016.0
188.10	564.0
188.90	940.0
190.90	671.0
192.00	1617.0
193.00	2223.0
194.10	635.0
195.90	3255.0
197.10	777.0
198.00	120856.0
199.00	8418.0
199.90	744.0
201.10	428.0
201.50	445.0
203.00	908.0
204.00	5058.0
205.00	8482.0
206.10	34952.0
207.10	6570.0
208.00	1668.0
209.00	603.0
210.00	599.0
211.00	1370.0
215.00	461.0
215.90	1058.0
217.00	9867.0
218.00	1318.0
220.00	316.0
221.10	4129.0
222.00	1211.0
223.10	1822.0
224.00	19032.0
225.00	4629.0
226.10	415.0
227.00	10033.0
228.00	1141.0
229.00	2342.0
231.00	682.0
234.00	900.0
235.00	624.0
235.90	389.0
237.10	841.0
238.90	547.0
239.90	334.0
241.00	599.0
242.10	1283.0
243.00	1344.0
244.00	16856.0
245.00	1820.0
246.00	3993.0
246.90	978.0
248.90	607.0
253.00	362.0
254.10	575.0
255.00	88144.0
256.00	12966.0
257.00	1102.0
258.00	5678.0
258.90	756.0
265.00	2653.0
266.10	412.0
273.00	2915.0
274.00	6981.0
275.00	41264.0
276.00	4749.0
277.00	4246.0
278.00	719.0
281.00	411.0
283.10	570.0
285.00	859.0
293.00	844.0
295.10	379.0
296.00	13045.0
297.00	1345.0
301.90	340.0
303.00	1645.0
304.10	340.0
308.00	343.0
314.20	530.0
315.00	1598.0
316.00	583.0
321.10	327.0
323.00	4409.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

323.90	890.0
326.90	519.0
328.00	456.0
332.00	469.0
333.10	307.0
334.10	2812.0
335.00	638.0
341.00	402.0
346.00	911.0
352.00	1201.0
353.00	938.0
354.00	1605.0
355.20	335.0
365.00	6808.0
366.00	791.0
372.10	2157.0
373.10	501.0
383.00	788.0
402.00	1016.0
403.10	1599.0
404.00	552.0
421.10	1169.0
422.00	1021.0
423.10	7359.0
424.10	2175.0
441.10	23048.0
442.10	148672.0
443.10	26016.0
444.10	2926.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65