


Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
Data File : BM013346.D
Acq On : 12 Dec 2017 19:25
Operator : SJ/JU
Sample : I6775-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
F9A07

Manual Integrations
APPROVED

Sohil
12/13/2017 12:05:43 PM

Quant Time: Dec 13 03:01:53 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 01:37:55 2017
Response via : Initial Calibration

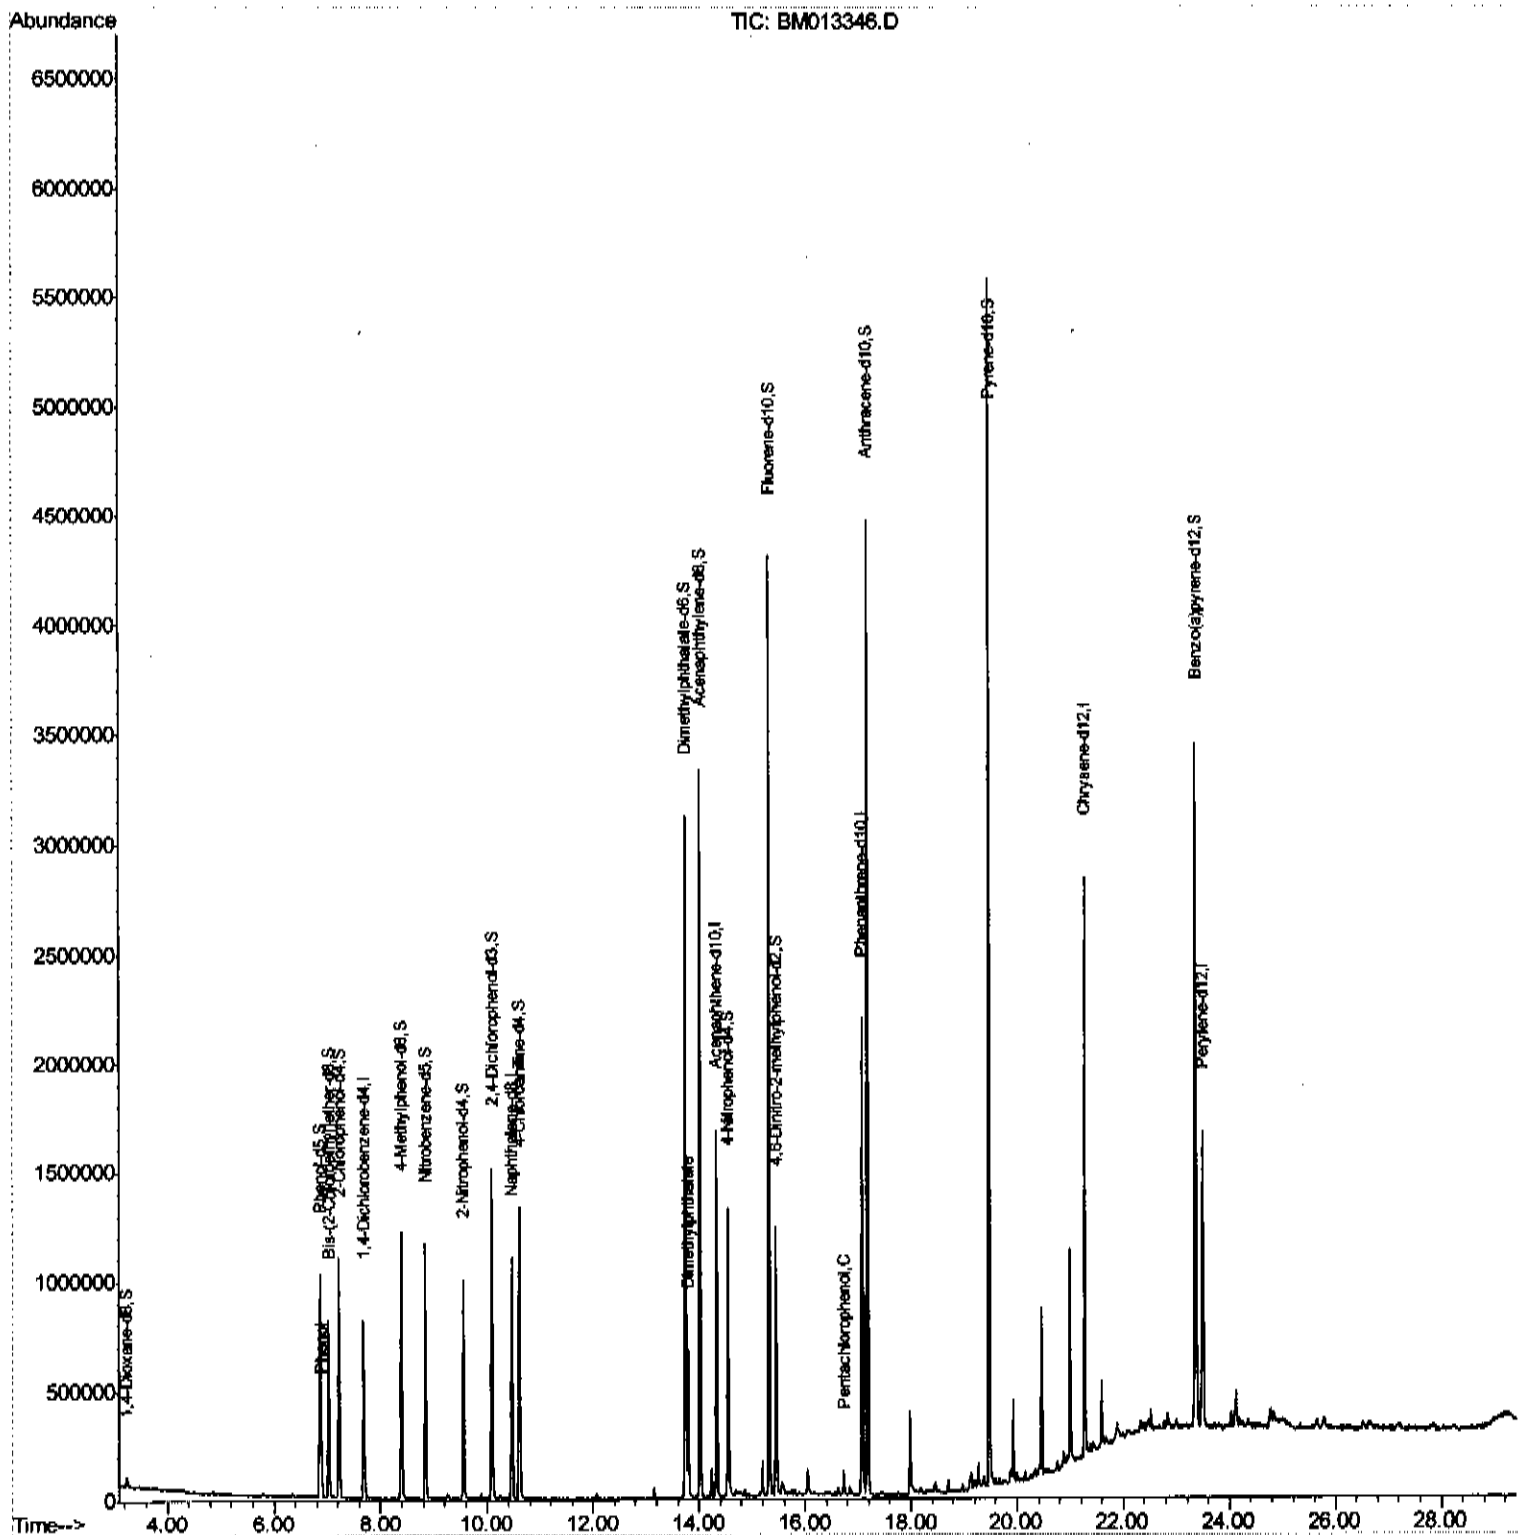




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013346.D
 Acq On : 12 Dec 2017 19:25
 Operator : SJ/JU
 Sample : I6775-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A07

Manual Integrations
 APPROVED

Sohil
 12/13/2017 12:05:43 PM

Quant Time: Dec 13 01:44:46 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 01:37:55 2017
 Response via : Initial Calibration

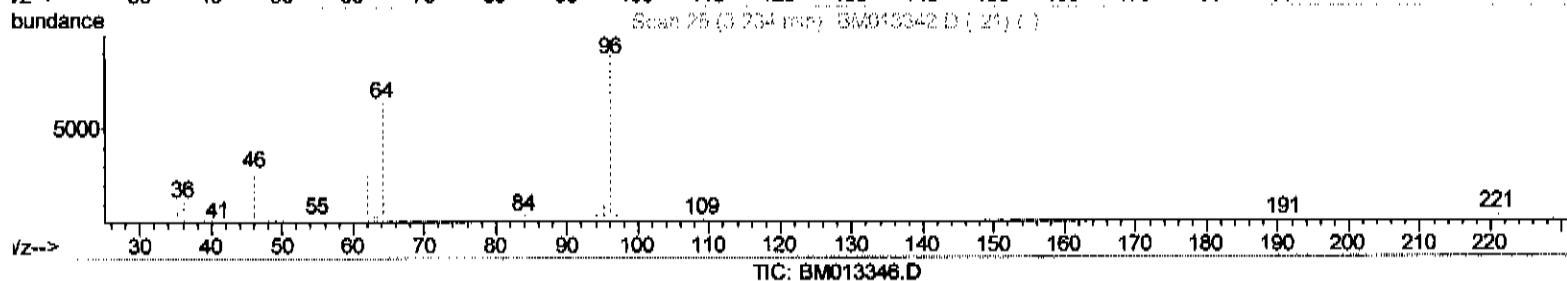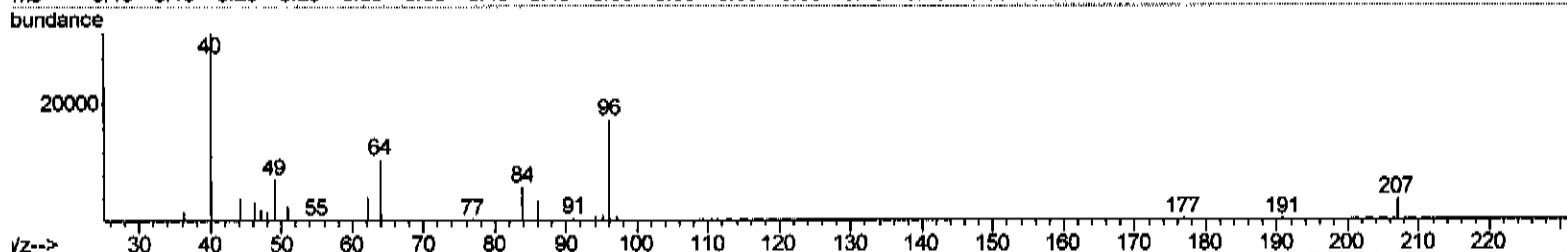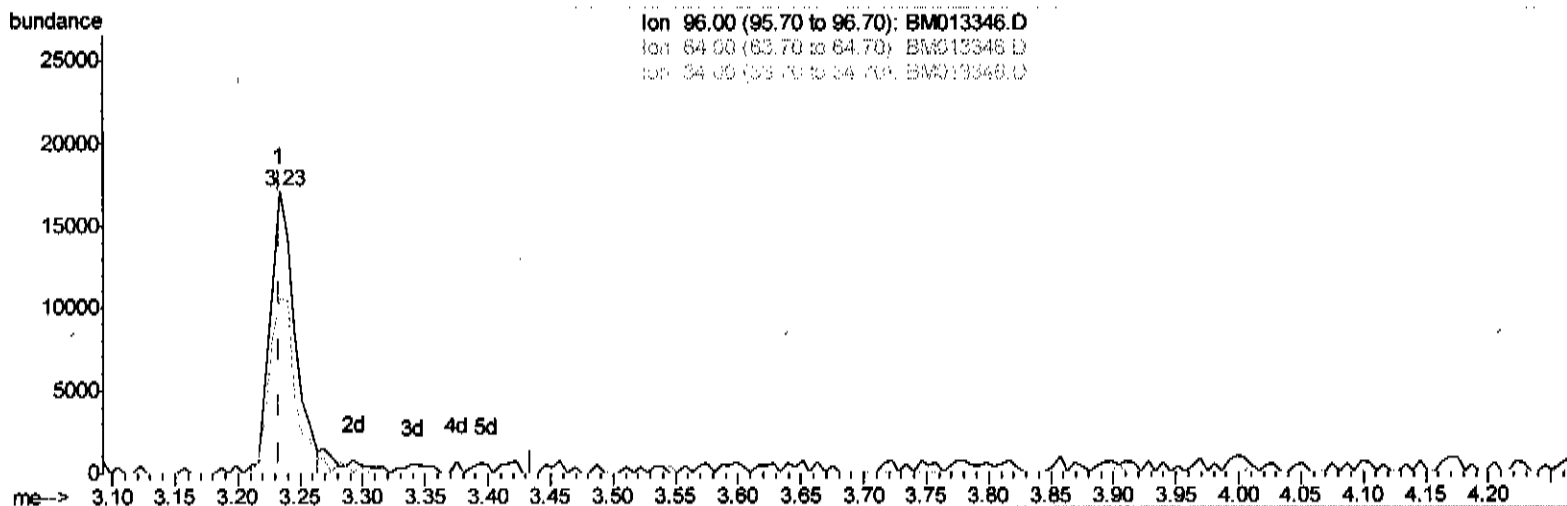

(3) 1,4-Dioxane-d8 (S)

3.234min (-0.000) 5.67ng/uL

response 23209

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	67.34
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013346.D
 Acq On : 12 Dec 2017 19:25
 Operator : SJ/JU
 Sample : I6775-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A07

Manual Integrations
 APPROVED

Sohil
 12/13/2017 12:05:43 PM

Quant Time: Dec 13 01:44:46 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 OLast Update : Wed Dec 13 01:37:55 2017
 Response via : Initial Calibration

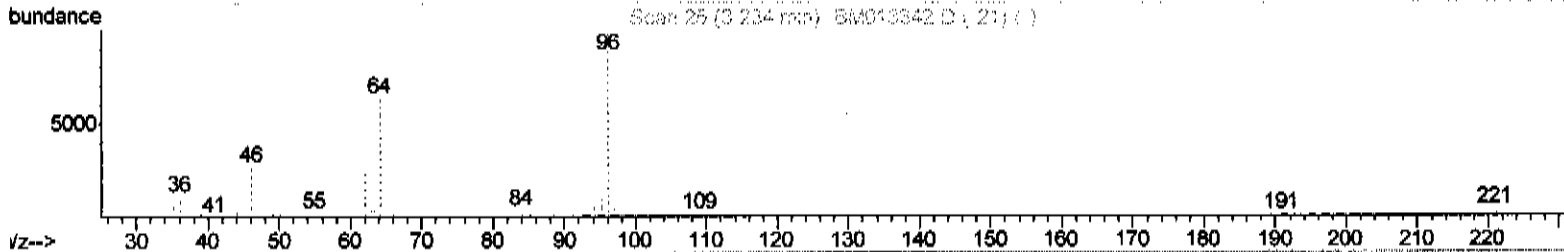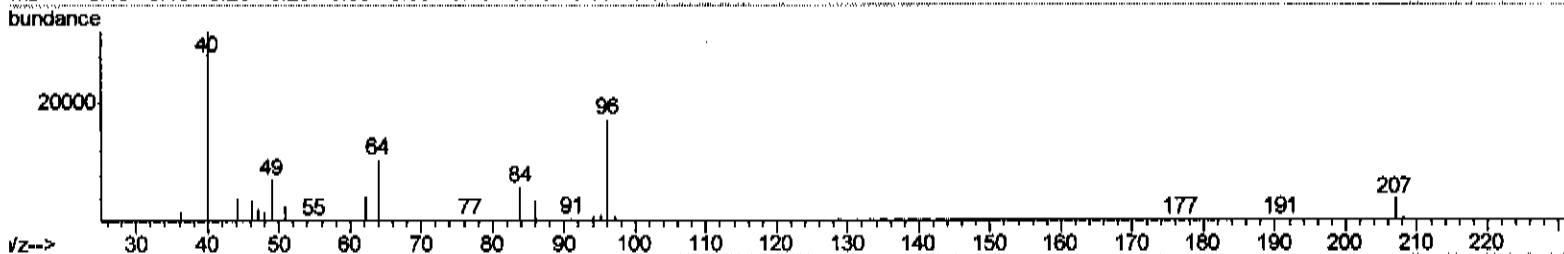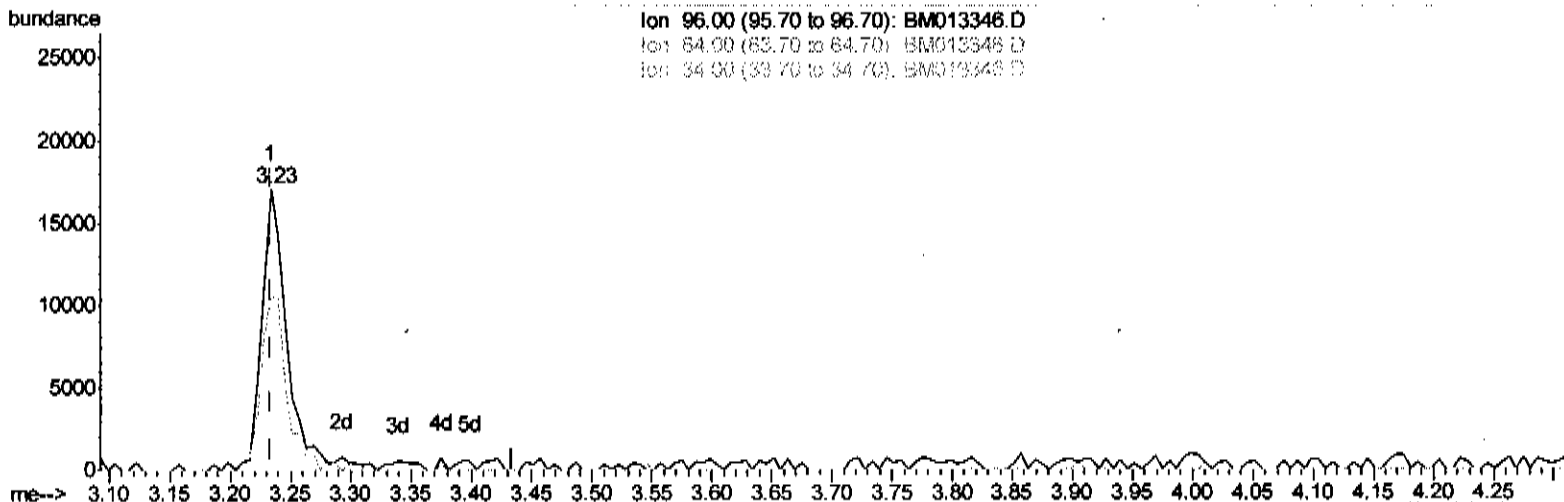

TIC: BM013346.D

(3) 1,4-Dioxane-d8 (S)

3.234min (-0.000) 6.16ng/uL

response 25243

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	61.91
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013346.D
 Acq On : 12 Dec 2017 19:25
 Operator : SJ/JU
 Sample : I6775-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 F9A07

Manual Integrations
 APPROVED

Sohil
 12/13/2017 12:05:43 PM

Quant Time: Dec 13 03:01:53 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 01:37:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	202807	20.00	ng/ul	0.00
18) Naphthalene-d8	10.47	136	863145	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	531013	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	1234805	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1203940	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	991862	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	25243m	6.16	ng/uL	0.00
5) Phenol-d5	6.87	99	533045	30.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	334421	33.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	441108	32.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	411682	27.46	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	246788	36.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	274643	37.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	510187	33.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	629255	45.35	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1864575	39.46	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	2234478	38.32	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	286739	34.93	ng/ul	0.00
57) Fluorene-d10	15.33	176	1567933	38.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	242534	31.22	ng/ul	0.00
70) Anthracene-d10	17.18	188	2488361	40.24	ng/ul	0.00
76) Pvrene-d10	19.47	212	2784604	46.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	2111759	41.80	ng/ul	0.00

JUL 12/18/17

Target Compounds

				Ovalue	
6) Phenol	6.89	94	78845	4.545	ng/ul# 86
44) Dimethylphthalate	13.79	163	379764	8.403	ng/ul 99
68) Pentachlorophenol	16.73	266	19288	2.083	ng/ul 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed