

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013348.D
 Acq On : 12 Dec 2017 20:37
 Operator : SJ/JU
 Sample : I6776-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A40

Quant Time: Dec 13 03:28:49 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 01:37:55 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	177732	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	782942	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	482240	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1132190	20.00	ng/ul	0.00
75) Chrysene-d12	21.27	240	1255493	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	1079195	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	7684	2.14	ng/uL	0.00
5) Phenol-d5	6.86	99	244398	15.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.03	67	143883	16.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	190469	15.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	228470	17.39	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	106717	17.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	115661	17.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	236023	17.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	265771	21.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	856958	19.97	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1019725	19.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	119929	16.08	ng/ul	0.00
57) Fluorene-d10	15.32	176	726339	19.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	92268	12.95	ng/ul	0.00
70) Anthracene-d10	17.17	188	1154364	20.36	ng/ul	0.00
76) Pyrene-d10	19.47	212	1391024	22.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.36	264	1172596	21.33	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	6.89	94	41264	2.714	ng/ul#	77
44) Dimethylphthalate	13.79	163	150882	3.676	ng/ul	99
74) Fluoranthene	19.14	202	108846	1.381	ng/ul#	94
77) Pyrene	19.50	202	123649	1.621	ng/ul#	94
85) Benzo(b)fluoranthene	22.83	252	137865	1.895	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
Data File : BM013348.D
Acq On : 12 Dec 2017 20:37
Operator : SJ/JU
Sample : I6776-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A40

Quant Time: Dec 13 03:28:49 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 01:37:55 2017
Response via : Initial Calibration

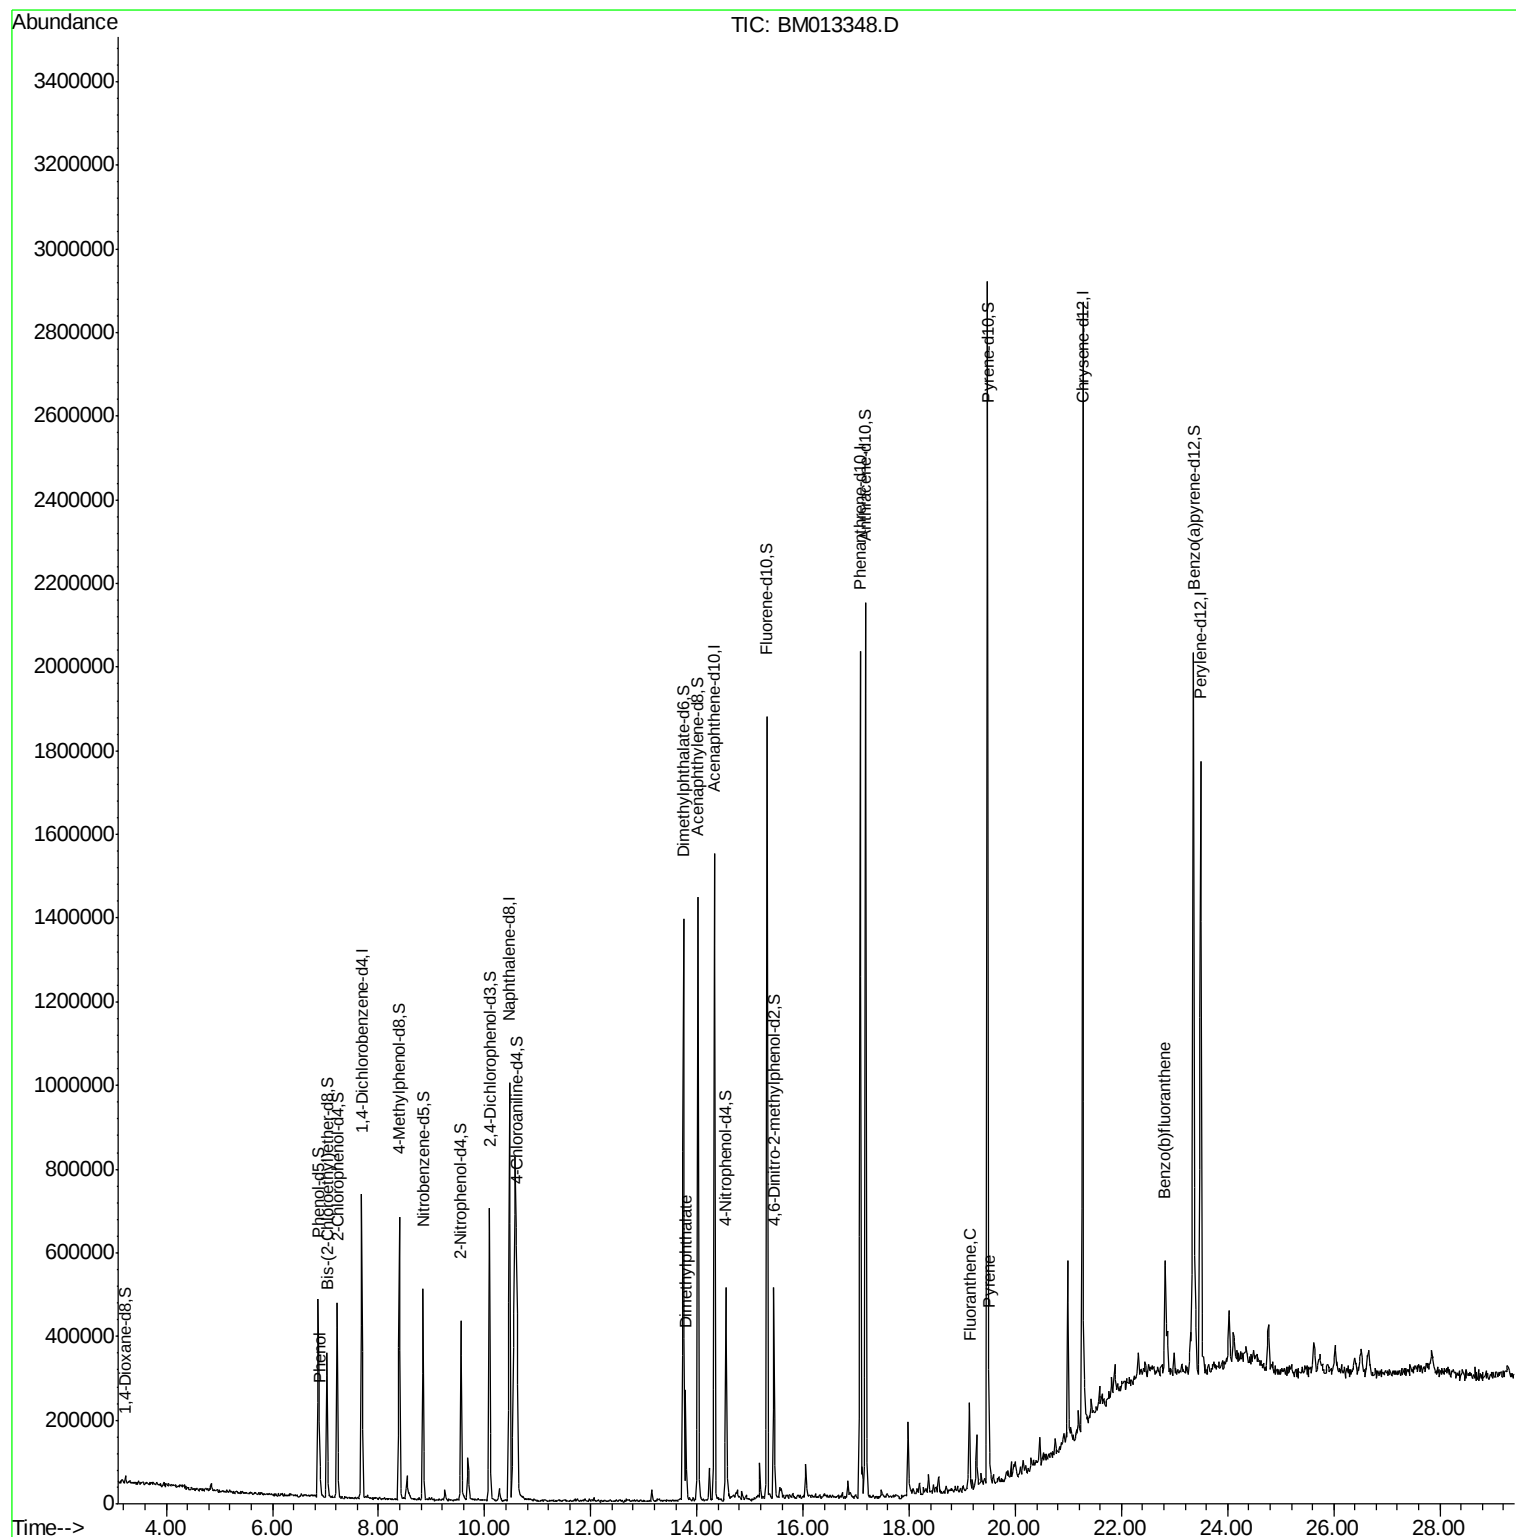

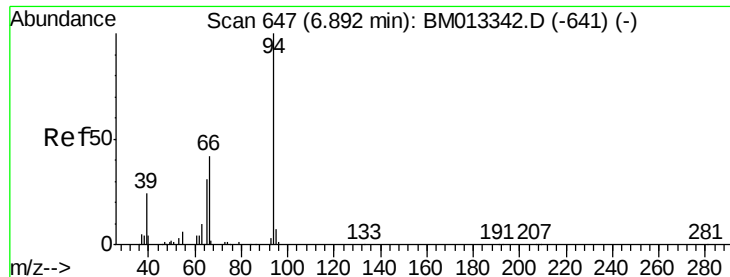





#6

Phenol

Concen: 2.714 ng/ul
 RT: 6.89 min Scan# 647
 Delta R.T. 0.00 min
 Lab File: BM013348.D
 Acq: 12 Dec 2017 20:37

Instrument :
 BNA_M
 ClientSampleId :
 F9A40

Tot Ion	Ratio	Lower	Upper
94	100		
65	27.4	28.2	42.4#
66	37.7	47.2	70.8#

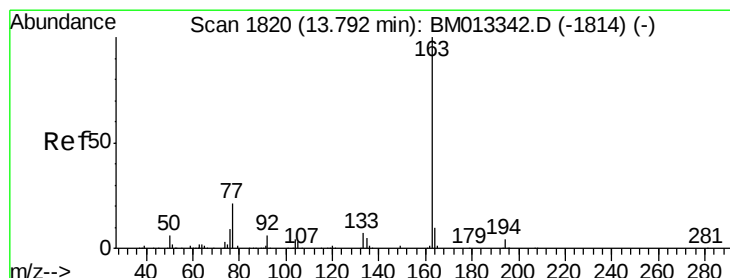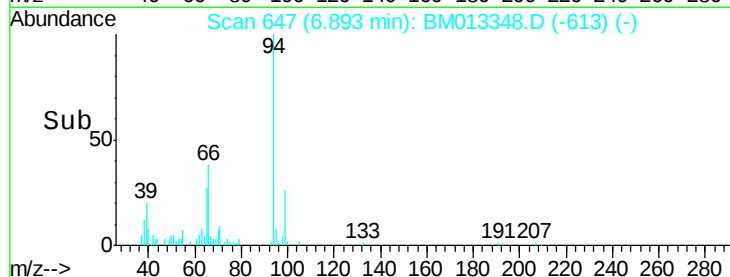
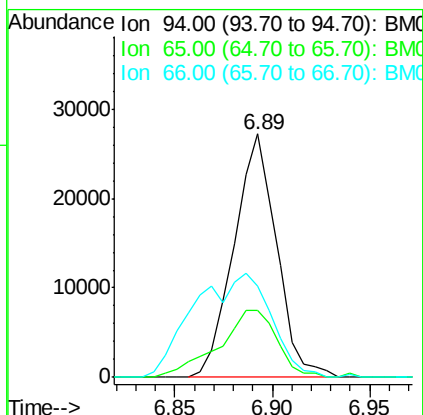
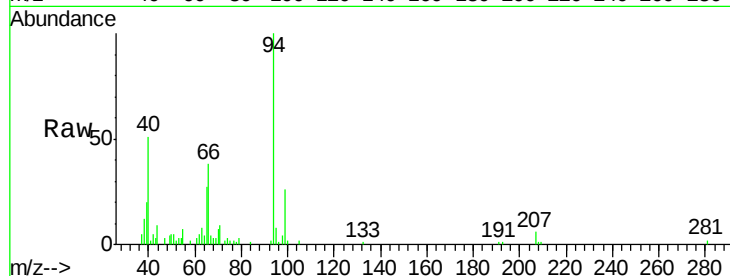



#44

Dimethylphthalate

Concen: 3.676 ng/ul
 RT: 13.79 min Scan# 1820
 Delta R.T. 0.00 min
 Lab File: BM013348.D
 Acq: 12 Dec 2017 20:37

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.5	5.3
164	9.7	8.2	12.4


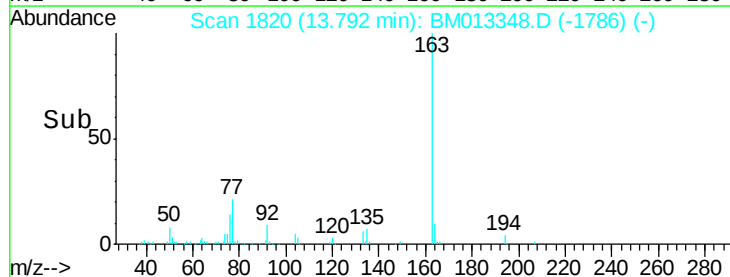
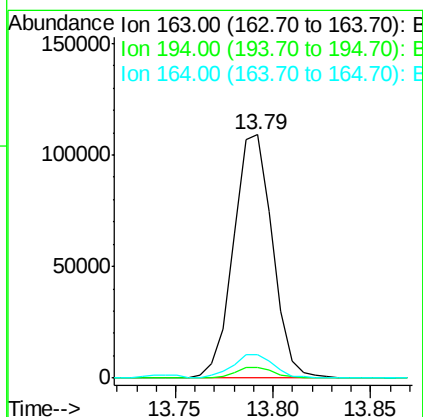
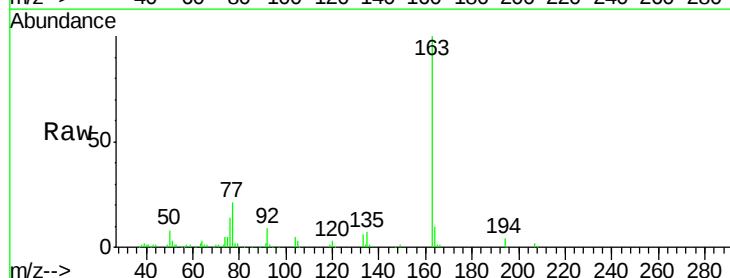


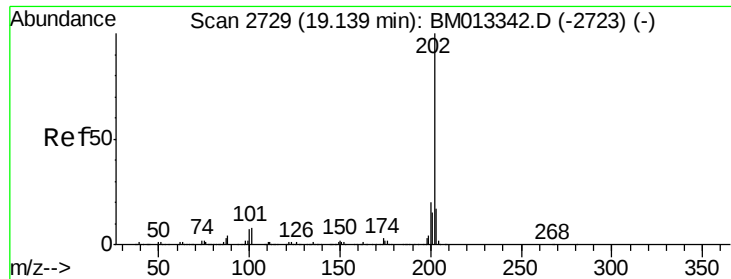

#74
 Fluoranthene
 Concen: 1.381 ng/ul
 RT: 19.14 min Scan# 2729
 Delta R.T. 0.00 min
 Lab File: BM013348.D
 Acq: 12 Dec 2017 20:37




Instrument :
 BNA_M
 ClientSampleId :
 F9A40


Tot Ion	Ratio	Lower	Upper
202	100		
101	7.0	4.6	7.0#
100	7.1	3.4	5.2#

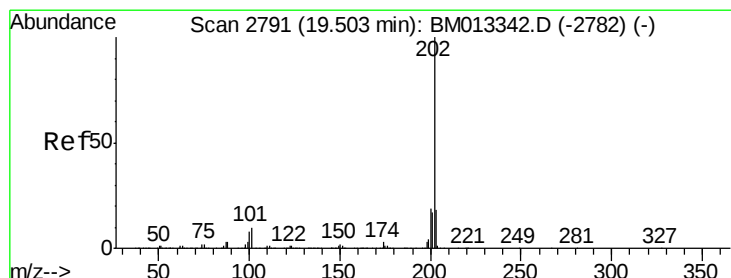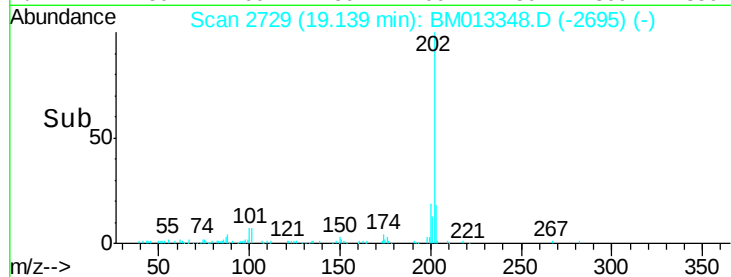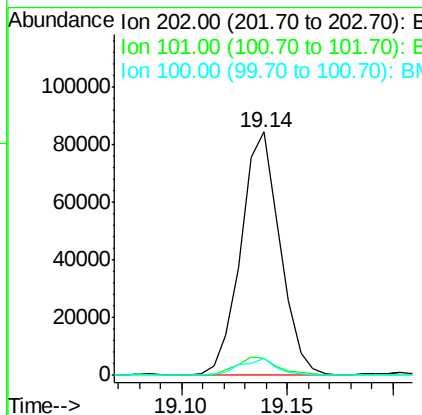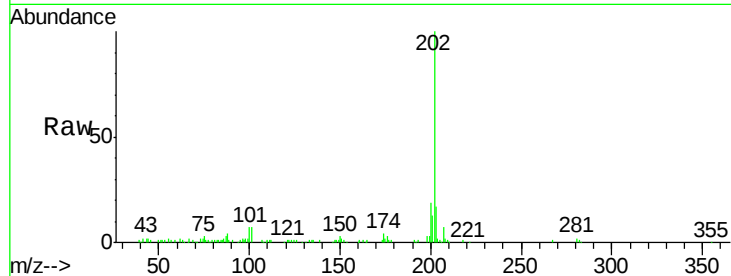

#77
 Pyrene
 Concen: 1.621 ng/ul
 RT: 19.50 min Scan# 2791
 Delta R.T. 0.00 min
 Lab File: BM013348.D
 Acq: 12 Dec 2017 20:37

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.8	5.1	7.7#
100	7.8	4.9	7.3#

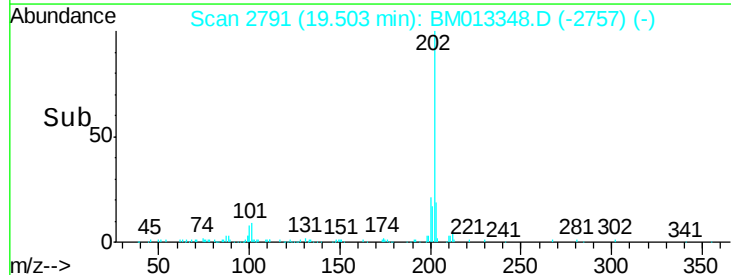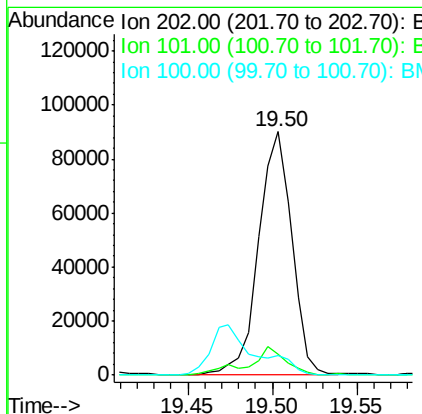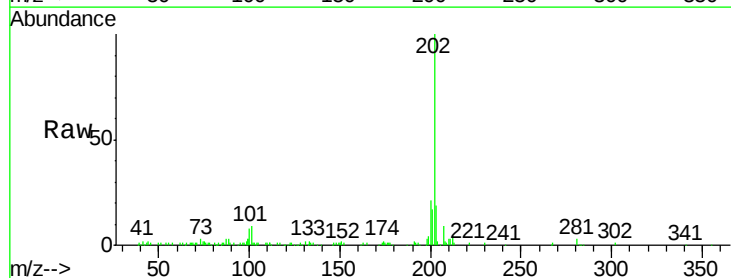

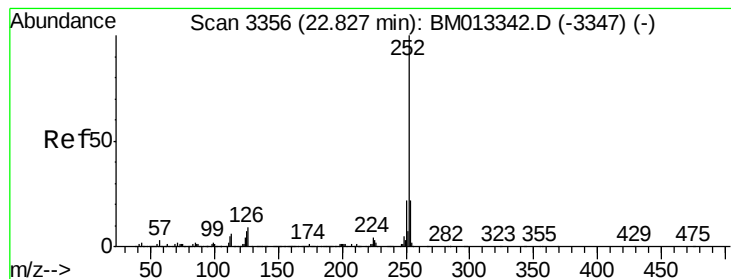

#85

Benzo(b)fluoranthene

Concen: 1.895 ng/ul

RT: 22.83 min Scan# 3356

Delta R.T. 0.00 min

Lab File: BM013348.D

Acq: 12 Dec 2017 20:37

Instrument :

BNA_M

ClientSampleId :

F9A40

Tot Ion:252 Resp: 137865

Ion Ratio Lower Upper

252 100

253 21.4 17.9 26.9

125 7.9 3.6 5.4#

