

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013356.D
 Acq On : 13 Dec 2017 01:22
 Operator : SJ/JU
 Sample : I6775-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.863	635	642	656	rVB2	395089	777905	19.88%	1.902%
2	7.028	664	670	678	rVB	305401	479601	12.26%	1.173%
3	7.222	696	703	710	rVB	410214	666009	17.02%	1.628%
4	7.687	774	782	791	rBV	536918	875759	22.38%	2.141%
5	8.392	895	902	910	rBV	499964	824666	21.08%	2.016%
6	8.839	971	978	989	rBV	421500	711347	18.18%	1.739%
7	9.251	1042	1048	1052	rVB3	37716	58155	1.49%	0.142%
8	9.551	1092	1099	1108	rBV	371893	617044	15.77%	1.509%
9	10.092	1184	1191	1200	rBV	531731	926036	23.67%	2.264%
10	10.463	1247	1254	1261	rBV	795827	1293461	33.06%	3.163%
11	10.604	1271	1278	1288	rBV	439916	779950	19.93%	1.907%
12	13.739	1805	1811	1816	rBV	1143484	1606239	41.05%	3.927%
13	13.786	1816	1819	1827	rVB	237006	332459	8.50%	0.813%
14	14.016	1852	1858	1870	rVB	1212179	1906201	48.72%	4.661%
15	14.233	1890	1895	1900	rBV	38589	53238	1.36%	0.130%
16	14.327	1904	1911	1919	rBV2	1227595	1883925	48.15%	4.606%
17	14.539	1941	1947	1959	rBV	382326	712450	18.21%	1.742%
18	15.133	2044	2048	2053	rBV4	39642	59712	1.53%	0.146%
19	15.186	2053	2057	2063	rVB2	52348	74412	1.90%	0.182%
20	15.321	2070	2080	2087	rBV	1664806	2314162	59.14%	5.658%
21	15.451	2097	2102	2115	rVB	441600	649252	16.59%	1.587%
22	15.568	2115	2122	2124	rBV6	25471	45223	1.16%	0.111%
23	16.051	2199	2204	2212	rBV6	66631	136268	3.48%	0.333%
24	16.733	2316	2320	2325	rVB4	26162	44827	1.15%	0.110%
25	16.845	2335	2339	2343	rBV2	46140	62294	1.59%	0.152%
26	16.892	2343	2347	2354	rVB7	33097	53222	1.36%	0.130%
27	17.074	2372	2378	2383	rBV2	1775026	2543930	65.01%	6.220%
28	17.115	2383	2385	2389	rVB	177336	198861	5.08%	0.486%
29	17.174	2389	2395	2400	rBV	1970634	2790602	71.32%	6.823%
30	17.486	2445	2448	2456	rVB3	22341	44308	1.13%	0.108%
31	17.580	2461	2464	2468	rBV4	48340	56935	1.46%	0.139%
32	17.757	2490	2494	2497	rBV4	43810	55333	1.41%	0.135%
33	17.980	2527	2532	2541	rVB3	168200	245952	6.29%	0.601%
34	18.151	2556	2561	2564	rBV6	34353	64042	1.64%	0.157%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
 Data File : BM013356.D
 Acq On : 13 Dec 2017 01:22
 Operator : SJ/JU
 Sample : I6775-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9A52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Title : SVOA CALIBRATION

35	18.274	2578	2582	2586	rBV4	51395	68403	1.75%	0.167%
36	18.933	2692	2694	2697	rVB3	45298	45599	1.17%	0.111%
37	19.009	2704	2707	2712	rBV4	27717	45254	1.16%	0.111%
38	19.139	2721	2729	2734	rBV	352136	507429	12.97%	1.241%
39	19.262	2746	2750	2759	rBV6	128545	217189	5.55%	0.531%
40	19.474	2780	2786	2794	rBV	2514532	3912943	100.00%	9.567%
41	19.586	2801	2805	2808	rBV6	27337	40564	1.04%	0.099%
42	19.668	2816	2819	2825	rBV7	32622	69208	1.77%	0.169%
43	19.868	2850	2853	2856	rBV3	52982	60645	1.55%	0.148%
44	19.921	2858	2862	2866	rBV	142085	173920	4.44%	0.425%
45	20.139	2895	2899	2900	rBV4	40894	45989	1.18%	0.112%
46	20.456	2950	2953	2958	rVB	171638	223263	5.71%	0.546%
47	20.509	2959	2962	2967	rBV7	40631	80199	2.05%	0.196%
48	20.745	3000	3002	3008	rVB2	69706	95384	2.44%	0.233%
49	20.903	3027	3029	3034	rVB3	41322	55781	1.43%	0.136%
50	20.950	3034	3037	3039	rBV4	75206	76910	1.97%	0.188%
51	20.986	3039	3043	3048	rVB3	192429	261006	6.67%	0.638%
52	21.186	3075	3077	3081	rVB2	47021	42806	1.09%	0.105%
53	21.262	3084	3090	3095	rBV	2721832	3793873	96.96%	9.276%
54	22.827	3351	3356	3361	rBV2	280534	562423	14.37%	1.375%
55	23.350	3439	3445	3458	rVB	1816846	3664340	93.65%	8.959%
56	23.491	3462	3469	3477	rVV	1571678	2912466	74.43%	7.121%


Sum of corrected areas: 40899374

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121217\
Data File : BM013356.D
Acq On : 13 Dec 2017 01:22
Operator : SJ/JU
Sample : I6775-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A52

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

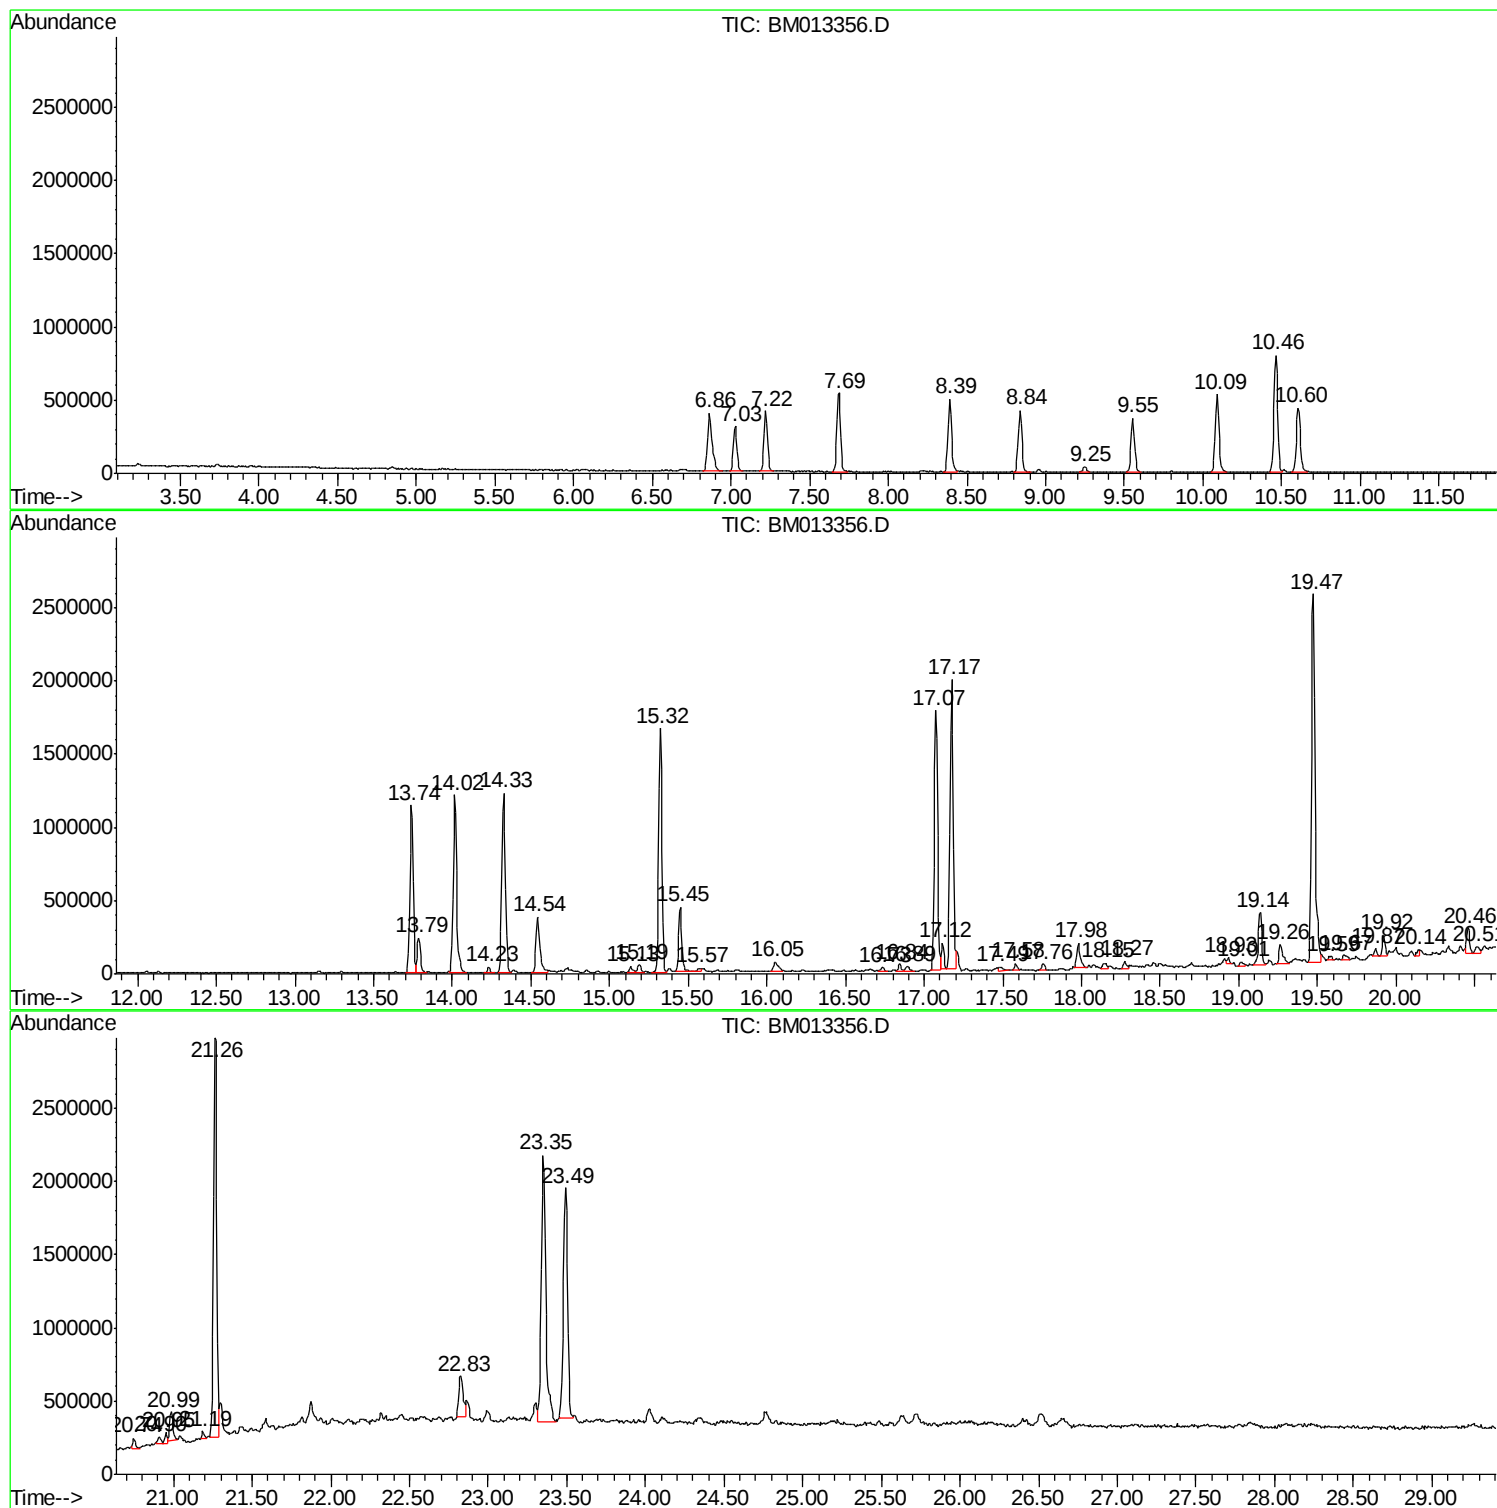

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121217\
Data File : BM013356.D
Acq On : 13 Dec 2017 01:22
Operator : SJ/JU
Sample : I6775-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A52

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121217\
Data File : BM013356.D
Acq On : 13 Dec 2017 01:22
Operator : SJ/JU
Sample : I6775-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9A52

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc