
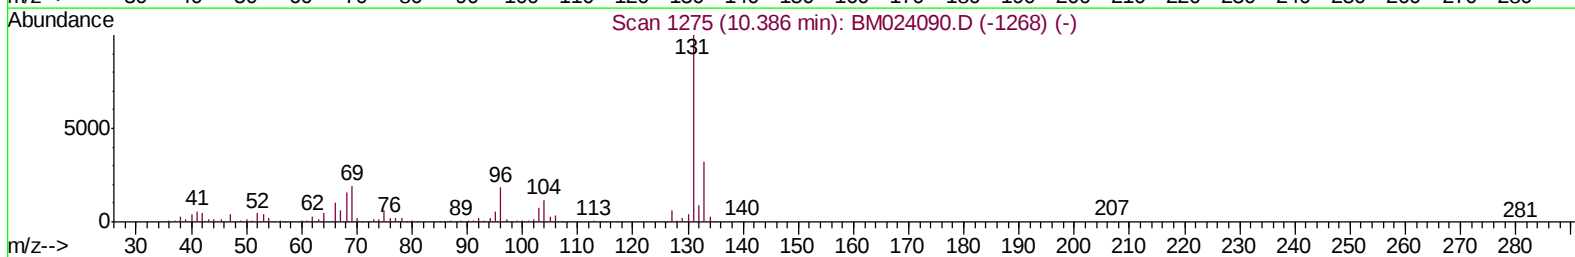
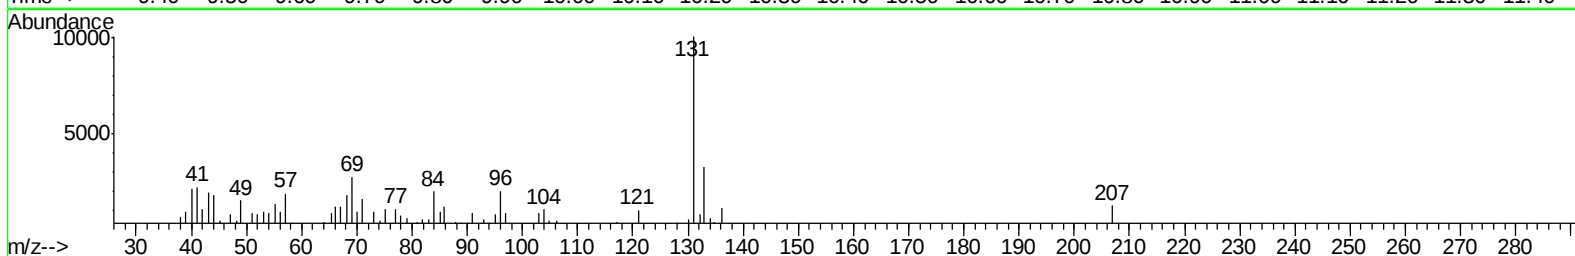


Data File : BM024098.D
Acq On : 13 Dec 2019 19:00
Operator : JU
Sample : K6167-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 14 00:30:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 14 00:26:31 2019
Response via : Initial Calibration

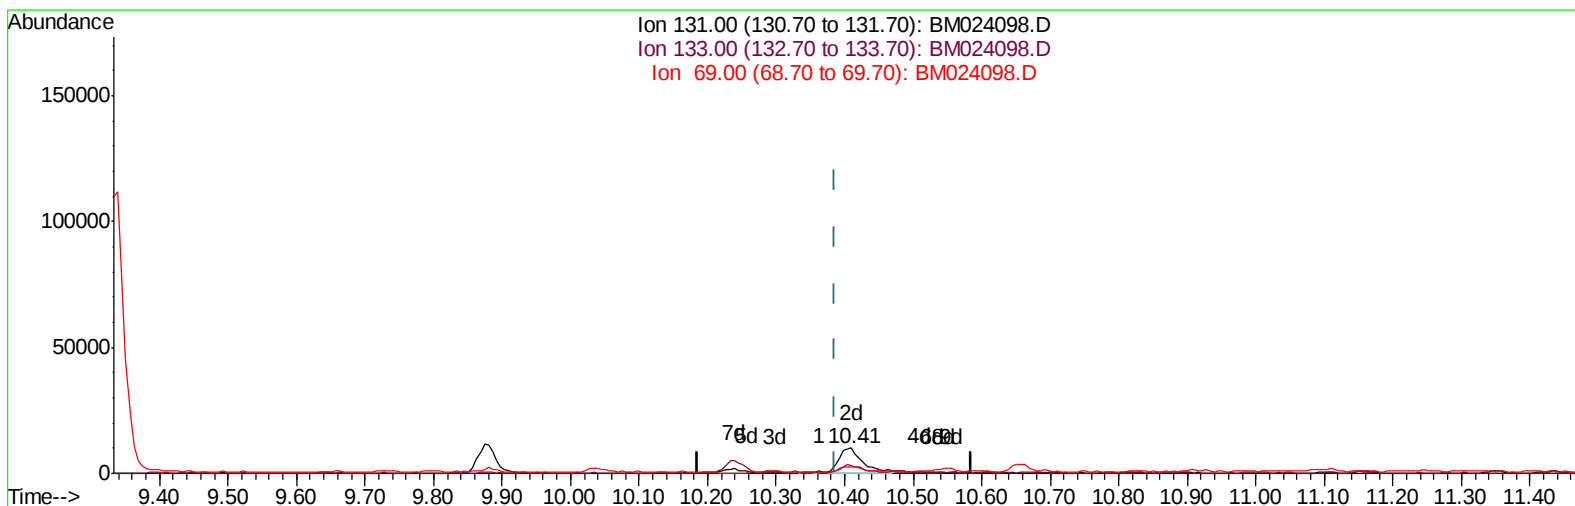

TIC: BM024098.D

(29) 4-Chloroaniline-d4 (S)

10.410min (+0.023) 1.07ng/ul m

response 25728

Ion	Exp%	Act%
131.00	100	100
133.00	32.30	32.52
69.00	18.80	27.10#
0.00	0.00	0.00