

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
 Data File : BM024055.D
 Acq On : 12 Dec 2019 12:59
 Operator : JU
 Sample : K6088-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 13 00:59:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 07 04:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	431458	20.00	ng/ul	0.00
18) Naphthalene-d8	10.24	136	1854293	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.13	164	1199744	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	2484239	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	1848845	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1913664	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	27790	2.87	ng/uL	0.00
5) Phenol-d5	6.66	99	542918	14.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	373048	16.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	443447	15.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	431218	14.45	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	219828	15.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	227834	13.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	425936	13.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	549402	16.16	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1570662	16.85	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1753034	16.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	144562	9.22	ng/ul	0.00
58) Fluorene-d10	15.13	176	1330598	16.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.28	200	175376	11.25	ng/ul	0.00
71) Anthracene-d10	16.99	188	2111621	17.80	ng/ul	0.00
79) Pyrene-d10	19.29	212	2243016	23.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	1962561	19.40	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.60	163	241133	2.642	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
Data File : BM024055.D
Acq On : 12 Dec 2019 12:59
Operator : JU
Sample : K6088-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 13 00:59:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 07 04:26:57 2019
Response via : Initial Calibration

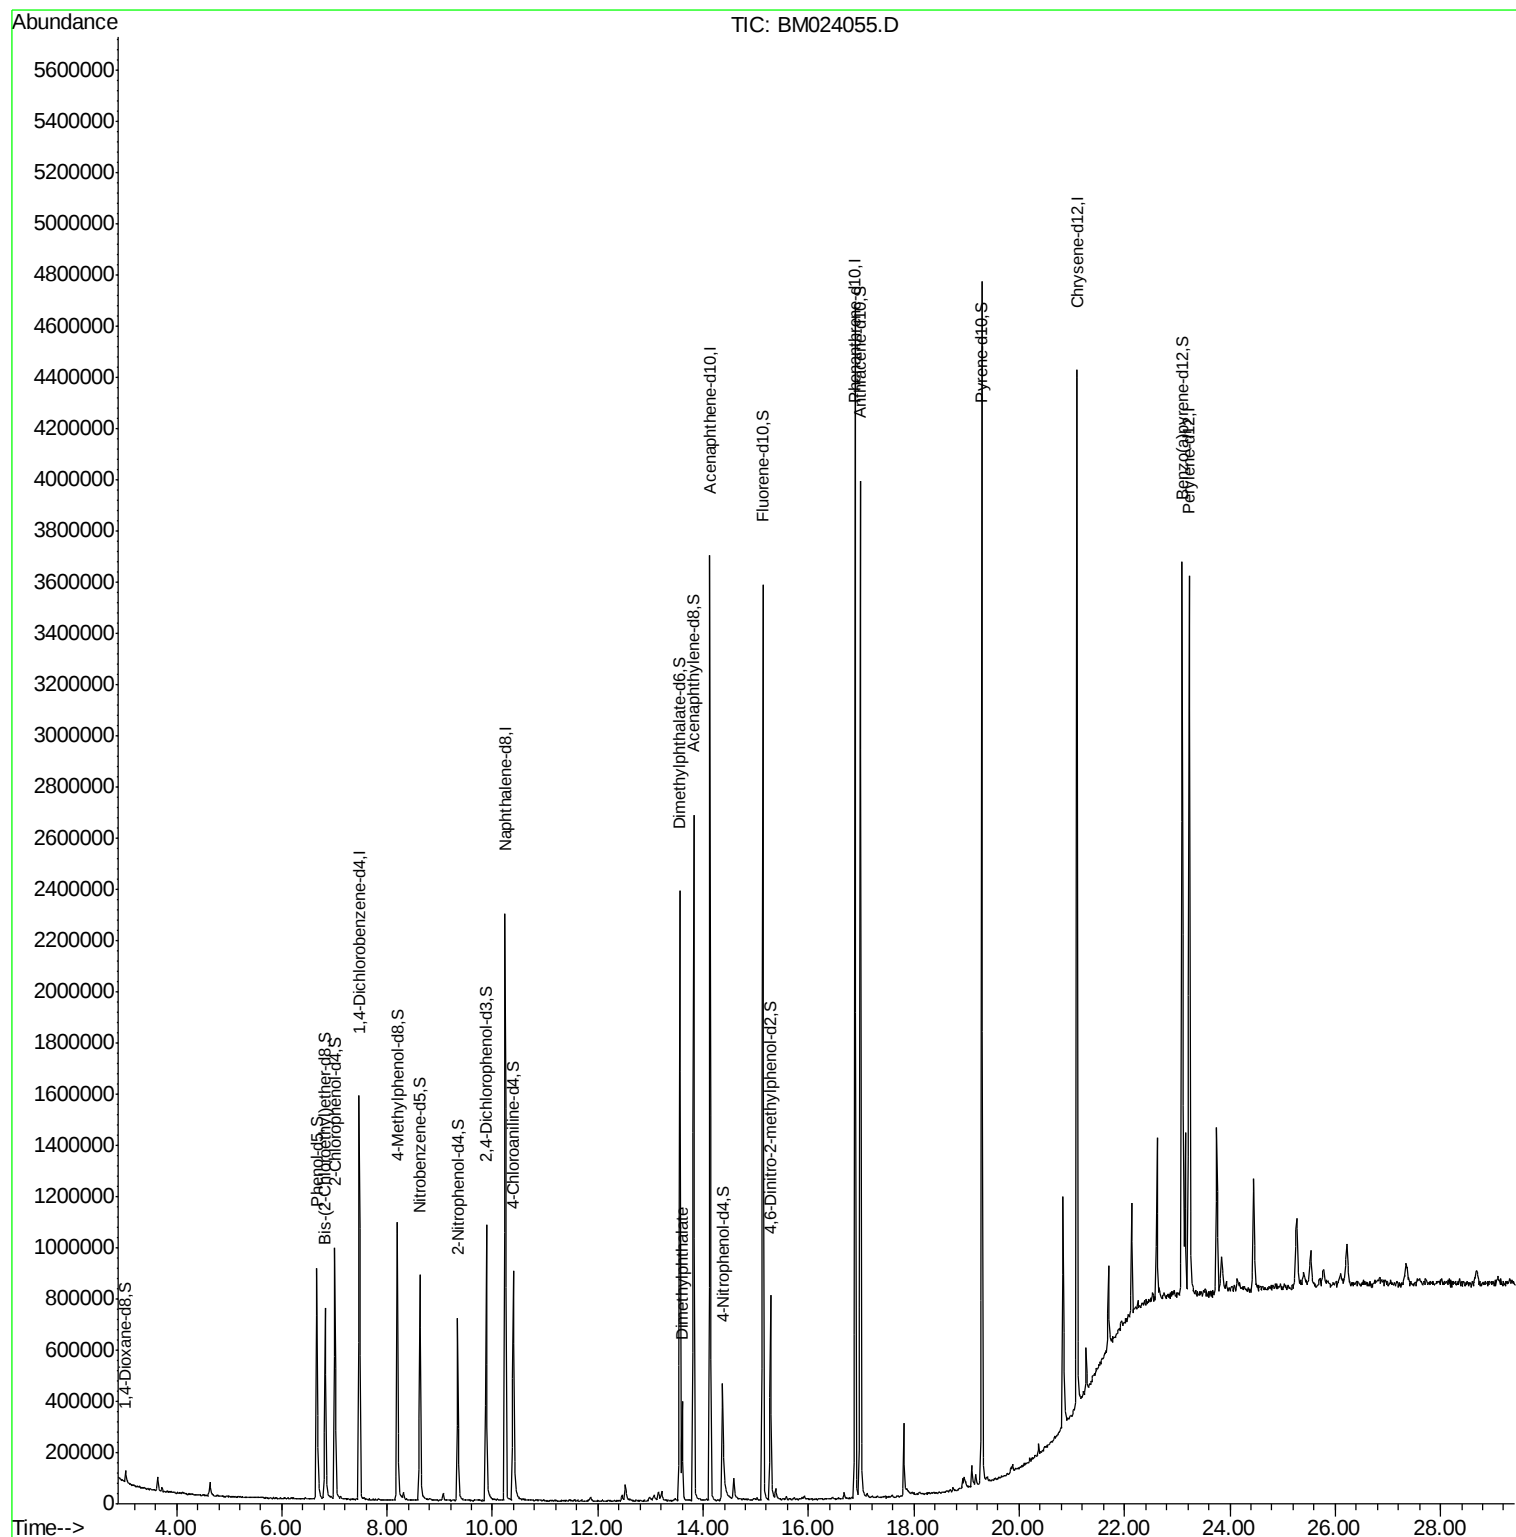

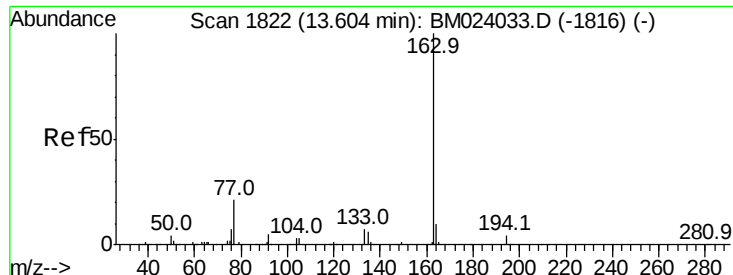

#45

Dimethylphthalate

Concen: 2.642 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM024055.D

Acq: 12 Dec 2019 12:59

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 241133

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.1 7.9 11.9

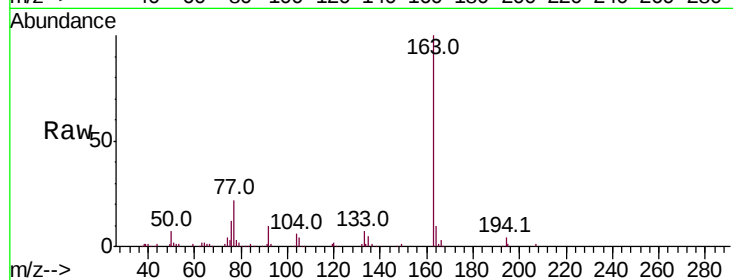

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

