

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121219\
 Data File : BM024086.D
 Acq On : 13 Dec 2019 11:31
 Operator : JU
 Sample : K6132-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQR2

Quant Time: Dec 13 13:52:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 07 04:26:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	434733	20.00	ng/ul	0.00
18) Naphthalene-d8	10.24	136	1735729	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.13	164	987425	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.89	188	1876353	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1586769	20.00	ng/ul	-0.01
86) Perylene-d12	23.23	264	1875451	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	55139	5.64	ng/uL	0.00
5) Phenol-d5	6.66	99	336479	8.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	688369	31.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	750857	25.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	516063	17.17	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	421249	31.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	477178	31.16	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	832670	28.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	75096	2.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.55	166	2574821	33.56	ng/ul	-0.01
47) Acenaphthylene-d8	13.82	160	3116982	34.66	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.38	143	81195	6.29	ng/ul	0.01
58) Fluorene-d10	15.13	176	2145406	33.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	342506	29.08	ng/ul	0.00
71) Anthracene-d10	16.98	188	3085092	34.43	ng/ul	-0.01
79) Pyrene-d10	19.29	212	3057731	37.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	3445299	34.75	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.60	163	122799	1.635	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121219\
Data File : BM024086.D
Acq On : 13 Dec 2019 11:31
Operator : JU
Sample : K6132-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQR2

Quant Time: Dec 13 13:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 07 04:26:57 2019
Response via : Initial Calibration

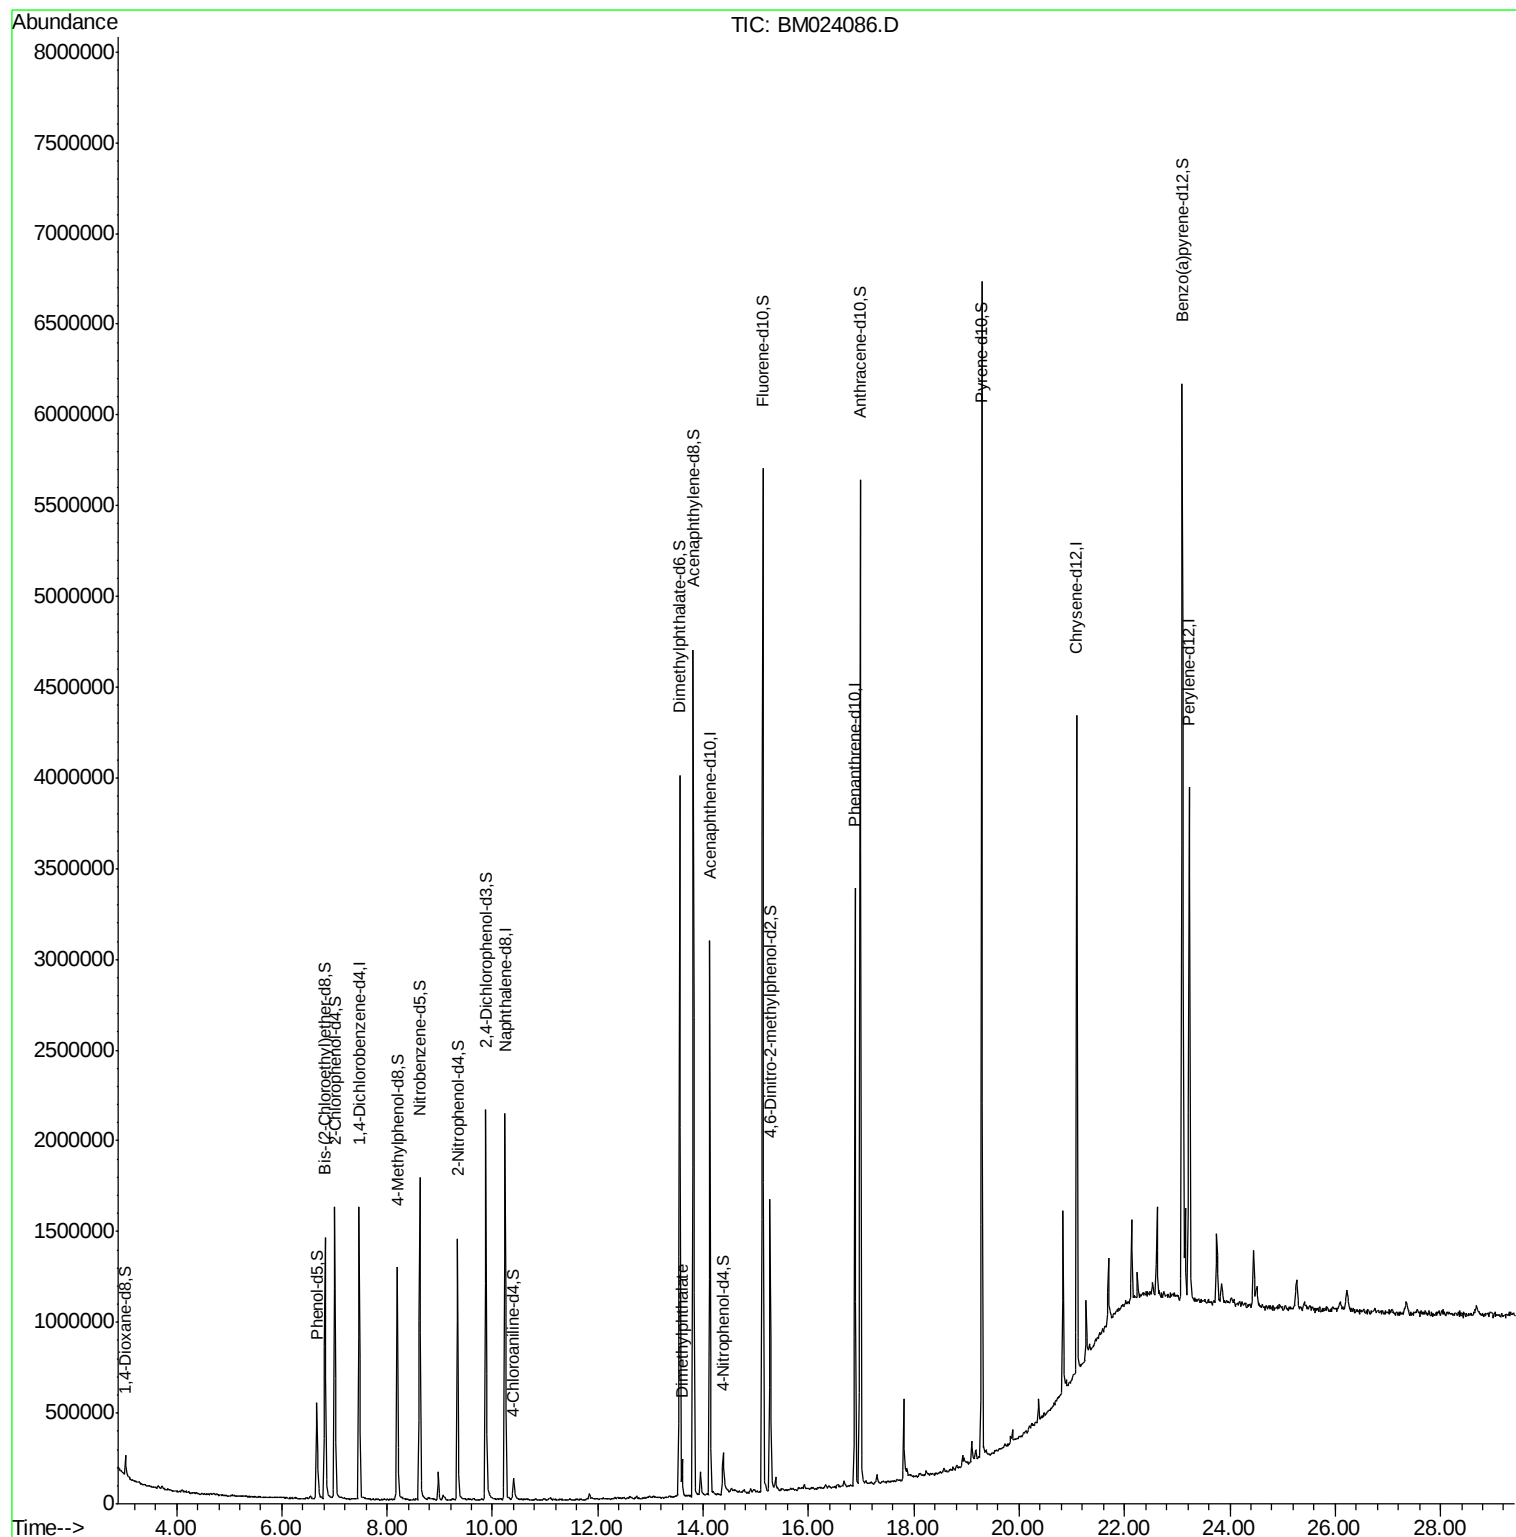

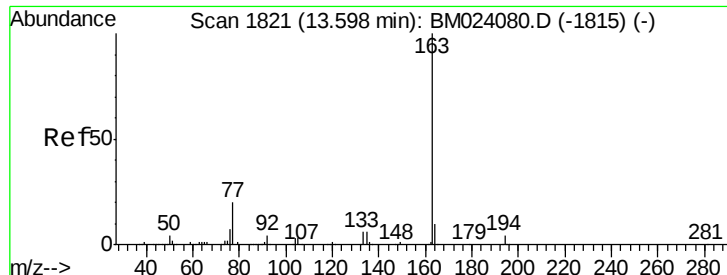

#45

Dimethylphthalate

Concen: 1.635 ng/ul

RT: 13.60 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM024086.D

Acq: 13 Dec 2019 11:31

Instrument :

BNA_M

ClientSampleId :

BFQR2


Tgt Ion:163 Resp: 122799

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.2 7.9 11.9

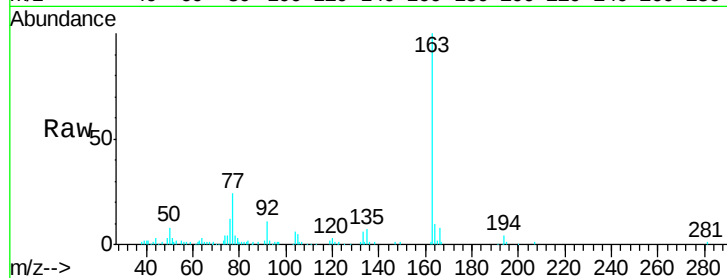

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

