

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
 Data File : BM024100.D
 Acq On : 13 Dec 2019 20:12
 Operator : JU
 Sample : K6167-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQS8

Quant Time: Dec 14 00:31:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 14 00:26:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	316825	20.00	ng/ul	0.00
18) Naphthalene-d8	10.24	136	1322873	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	807171	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	1685759	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1619799	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1954630	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	39256	5.51	ng/uL	0.00
5) Phenol-d5	6.67	99	204940	7.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	446728	27.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	504187	23.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	367594	16.78	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	277664	27.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	321221	27.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	588623	26.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	67356	2.78	ng/ul	0.02
44) Dimethylphthalate-d6	13.55	166	1874282	29.88	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	2265273	30.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	59957	5.69	ng/ul	0.02
58) Fluorene-d10	15.13	176	1643352	31.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	260040	24.57	ng/ul	0.00
71) Anthracene-d10	16.98	188	2462442	30.58	ng/ul	0.00
79) Pyrene-d10	19.29	212	2671407	31.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	3208076	31.05	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.60	163	95145	1.550	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
Data File : BM024100.D
Acq On : 13 Dec 2019 20:12
Operator : JU
Sample : K6167-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQS8

Quant Time: Dec 14 00:31:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 14 00:26:31 2019
Response via : Initial Calibration

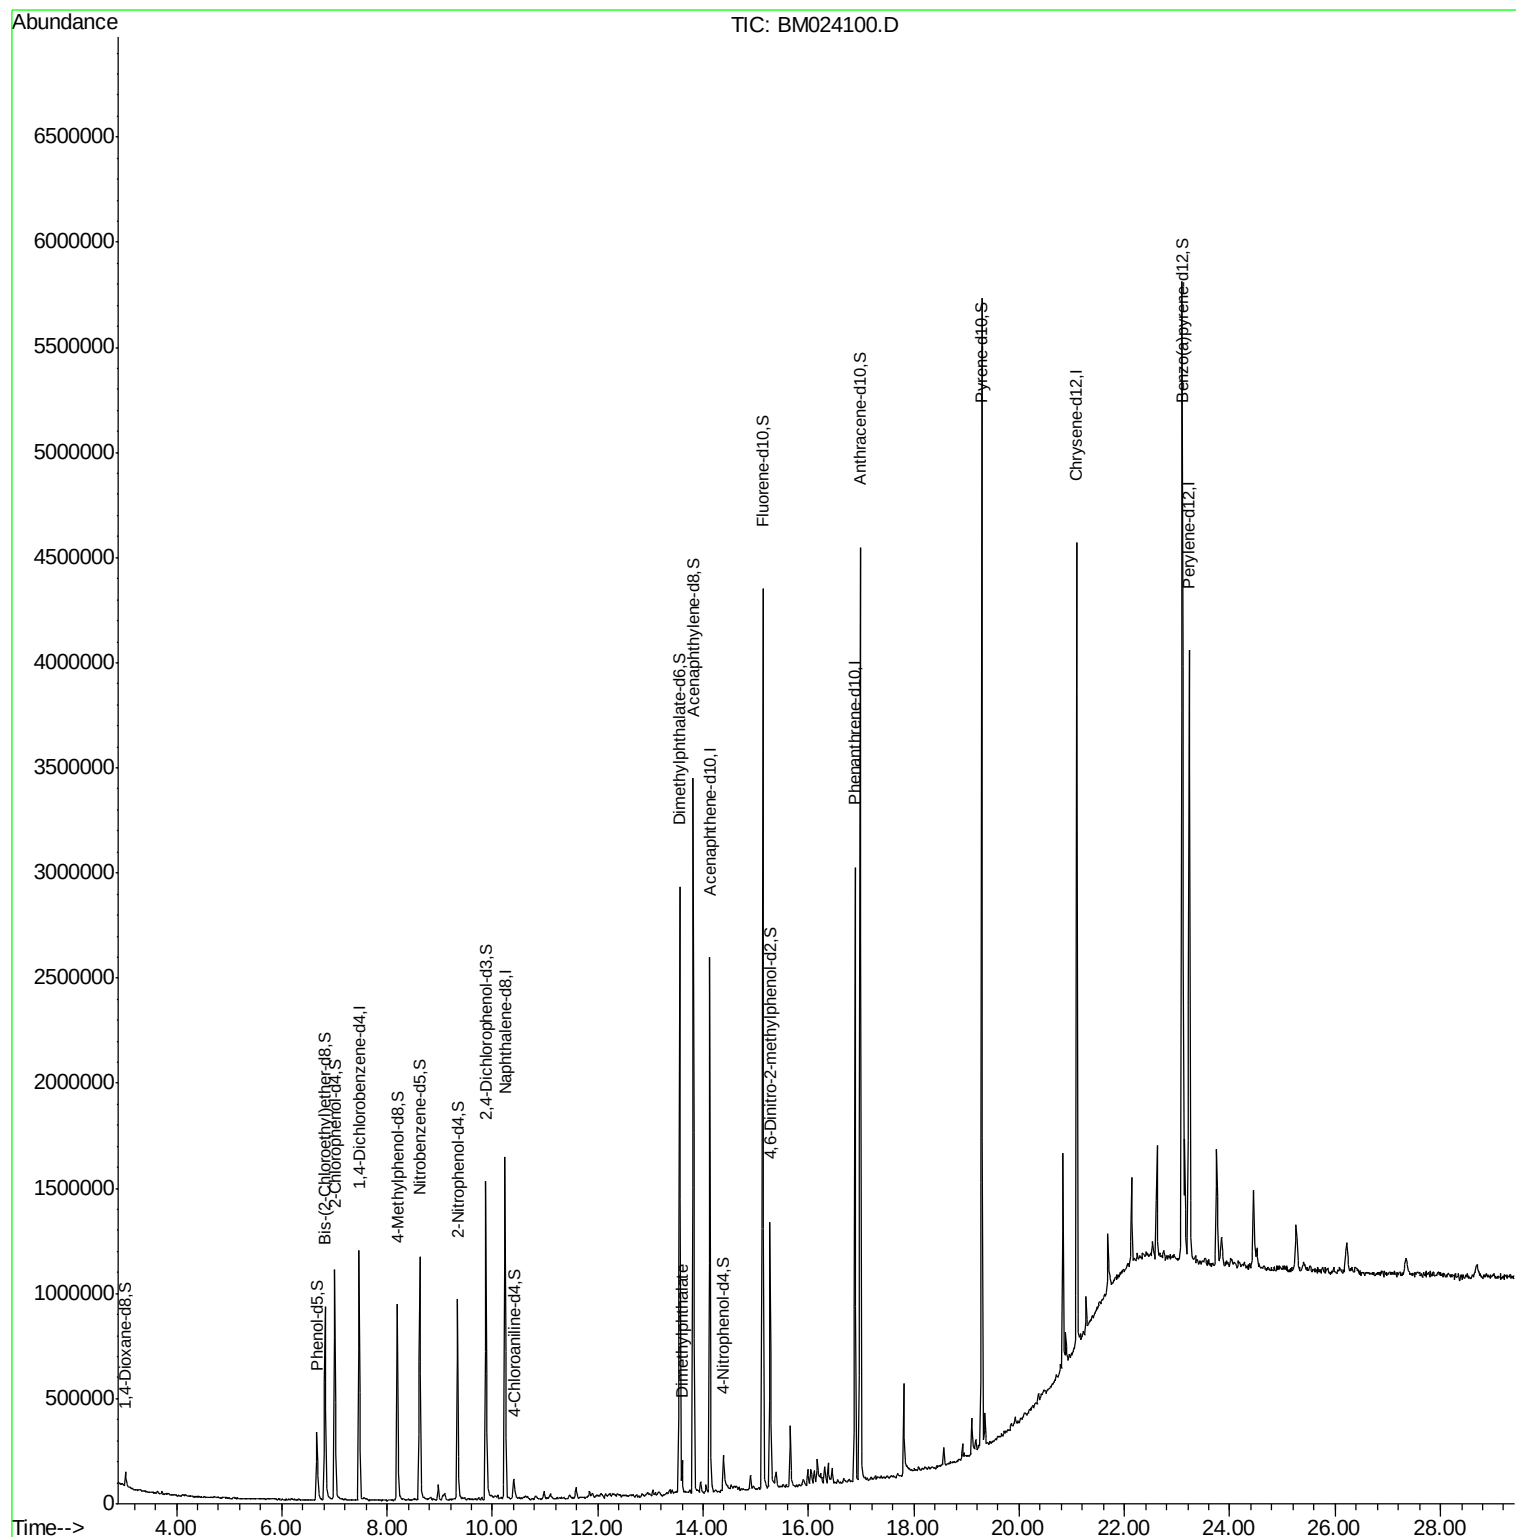

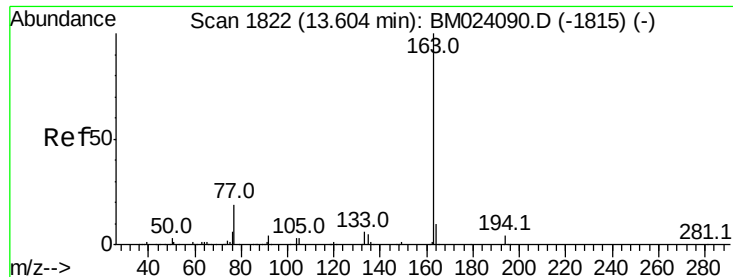

#45

Dimethylphthalate

Concen: 1.550 ng/ul

RT: 13.60 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM024100.D

Acq: 13 Dec 2019 20:12

Instrument :

BNA_M

ClientSampleId :

BFQS8


Tot Ion:163 Resp: 95145

Ion Ratio Lower Upper

163 100

194 3.4 3.3 4.9

164 9.1 7.9 11.9

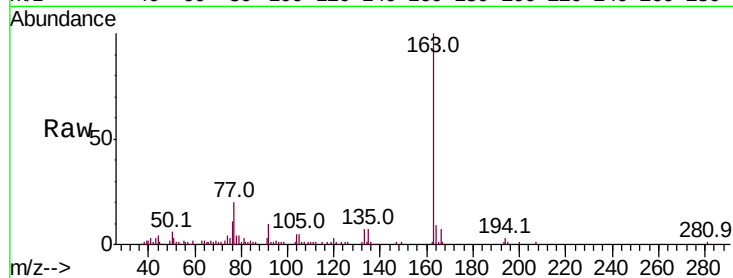

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

