

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
 Data File : BM024103.D
 Acq On : 13 Dec 2019 22:00
 Operator : JU
 Sample : K6167-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQT4

Quant Time: Dec 14 00:31:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 14 00:26:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	312043	20.00	ng/ul	0.00
18) Naphthalene-d8	10.24	136	1305639	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	788490	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	1663866	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1628539	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1988980	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.03	96	33302	4.75	ng/uL	0.00
5) Phenol-d5	6.67	99	177228	6.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	411488	25.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	451760	21.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	329718	15.28	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	262238	25.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	290616	25.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	531598	24.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	29033	1.21	ng/ul	0.03
44) Dimethylphthalate-d6	13.55	166	1776189	28.99	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	2153619	29.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	52564	5.10	ng/ul	0.02
58) Fluorene-d10	15.13	176	1553869	30.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	236903	22.68	ng/ul	0.00
71) Anthracene-d10	16.98	188	2381014	29.96	ng/ul	0.00
79) Pyrene-d10	19.29	212	2576619	30.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	3139497	29.86	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.60	163	106346	1.773	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
Data File : BM024103.D
Acq On : 13 Dec 2019 22:00
Operator : JU
Sample : K6167-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQT4

Quant Time: Dec 14 00:31:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 14 00:26:31 2019
Response via : Initial Calibration

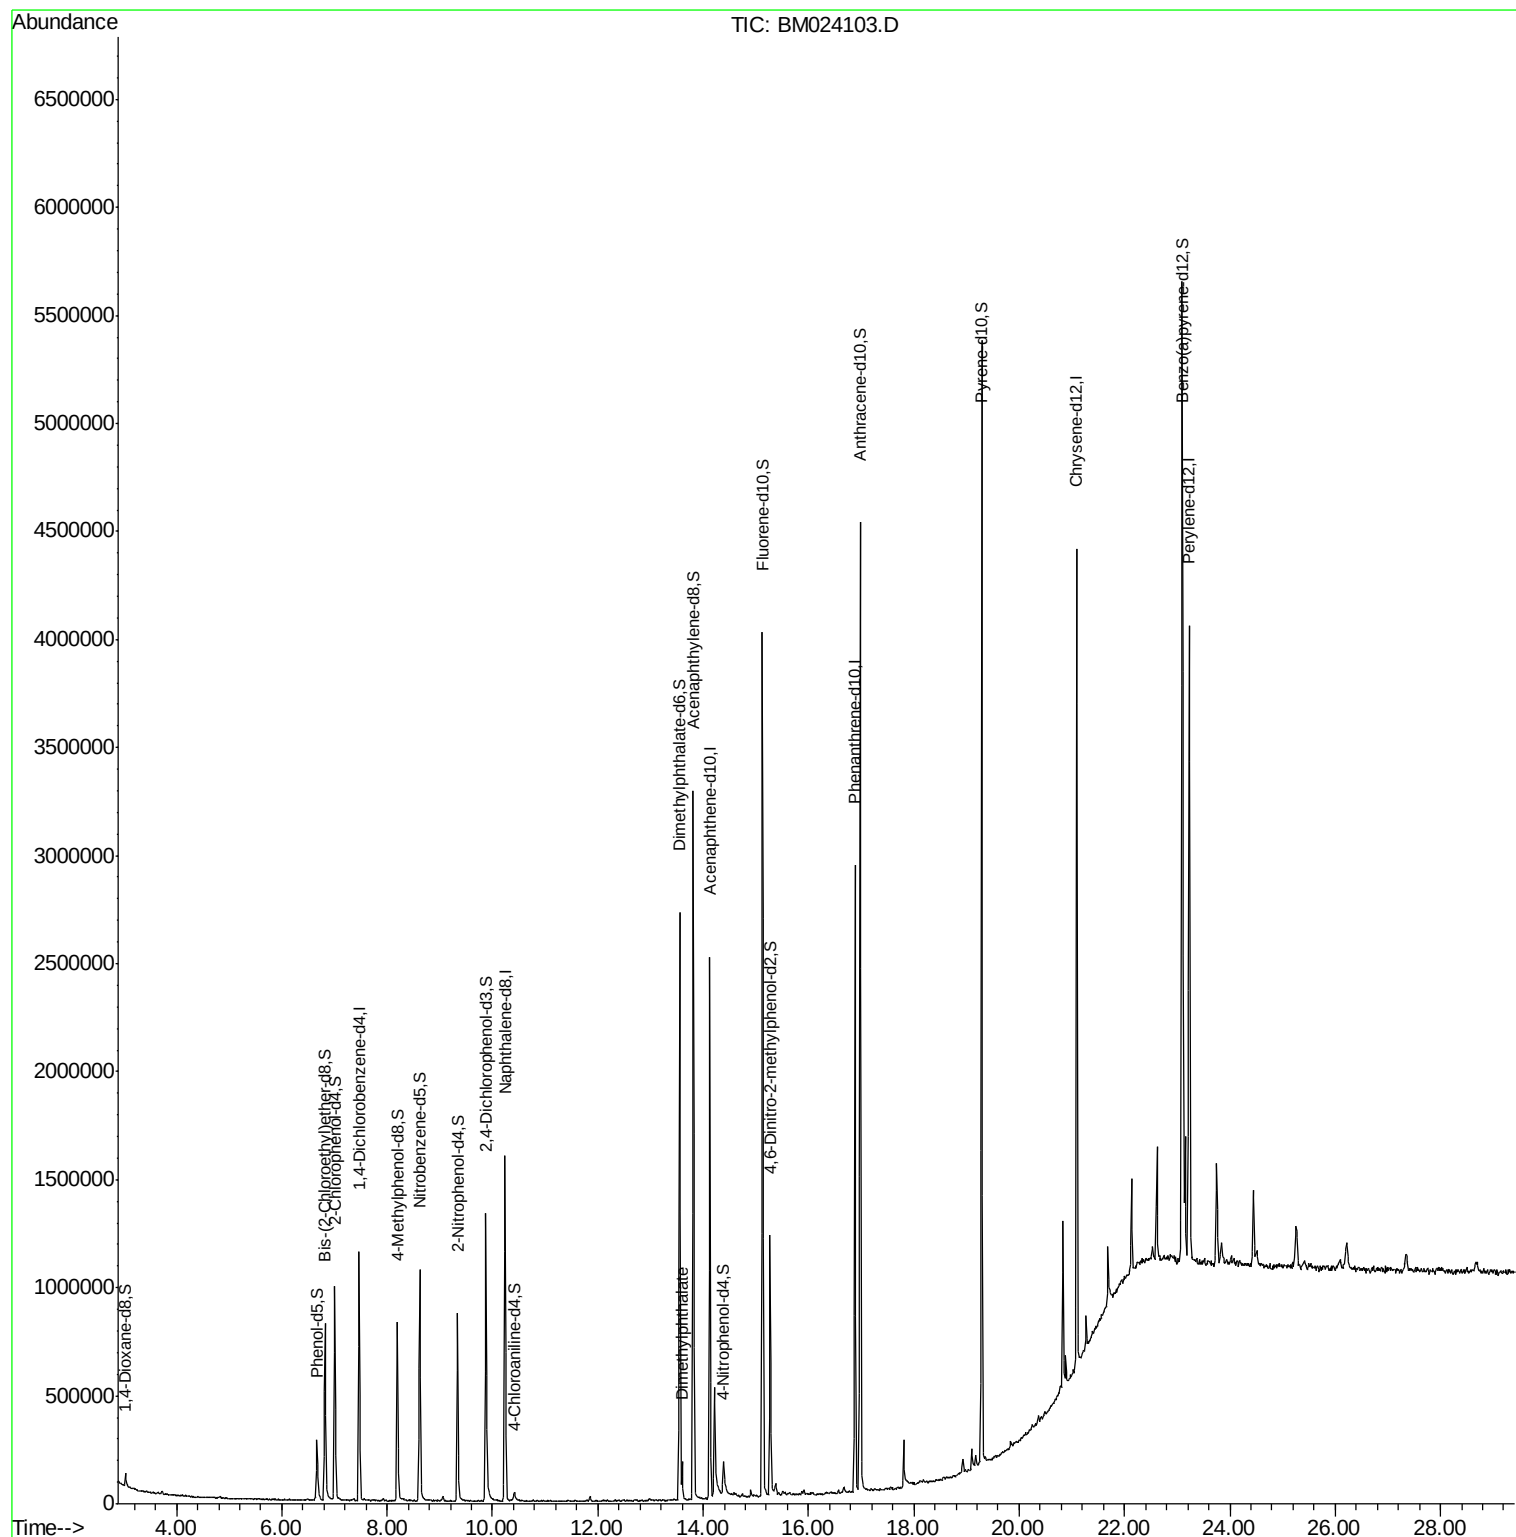

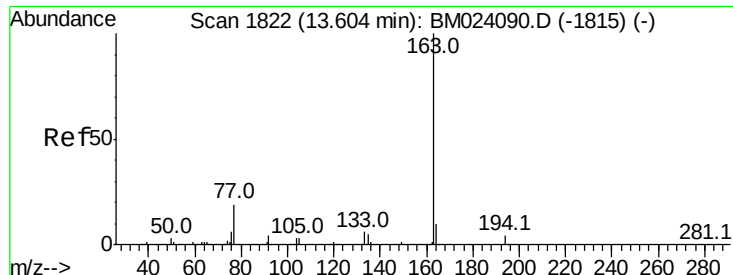

#45

Dimethylphthalate

Concen: 1.773 ng/ul

RT: 13.60 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM024103.D

Acq: 13 Dec 2019 22:00

Instrument :

BNA_M

ClientSampleId :

BFQT4


Tot Ion:163 Resp: 106346

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.8 7.9 11.9

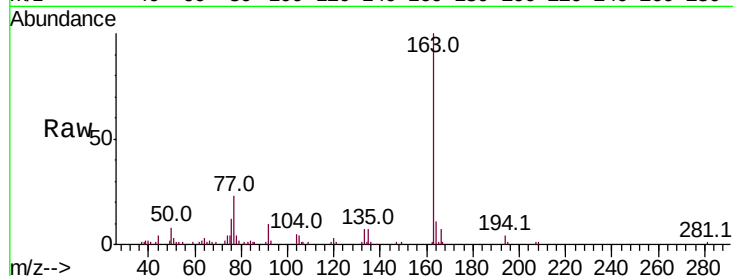

Abundance Ion 163.00 (162.70 to 163.70): E

100000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

