

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
 Data File : BM024106.D
 Acq On : 13 Dec 2019 23:48
 Operator : JU
 Sample : K6167-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQW8

Quant Time: Dec 14 00:32:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Dec 14 00:26:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	302257	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	1288133	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	779181	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	1597505	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1601508	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1941531	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	38259	5.63	ng/uL	0.00
5) Phenol-d5	6.67	99	155996	5.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.82	67	388872	25.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.01	132	416870	20.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	300213	14.36	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	237169	23.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.34	143	262211	23.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	497884	23.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	36068	1.53	ng/ul	0.02
44) Dimethylphthalate-d6	13.55	166	1708061	28.21	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1963198	27.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.39	143	56321	5.53	ng/ul	0.02
58) Fluorene-d10	15.13	176	1472791	28.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	242816	24.21	ng/ul	0.00
71) Anthracene-d10	16.98	188	2378042	31.17	ng/ul	0.00
79) Pyrene-d10	19.29	212	2609180	31.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	3222088	31.40	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.60	163	118183	1.994	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121219\
Data File : BM024106.D
Acq On : 13 Dec 2019 23:48
Operator : JU
Sample : K6167-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFQW8

Quant Time: Dec 14 00:32:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Dec 14 00:26:31 2019
Response via : Initial Calibration

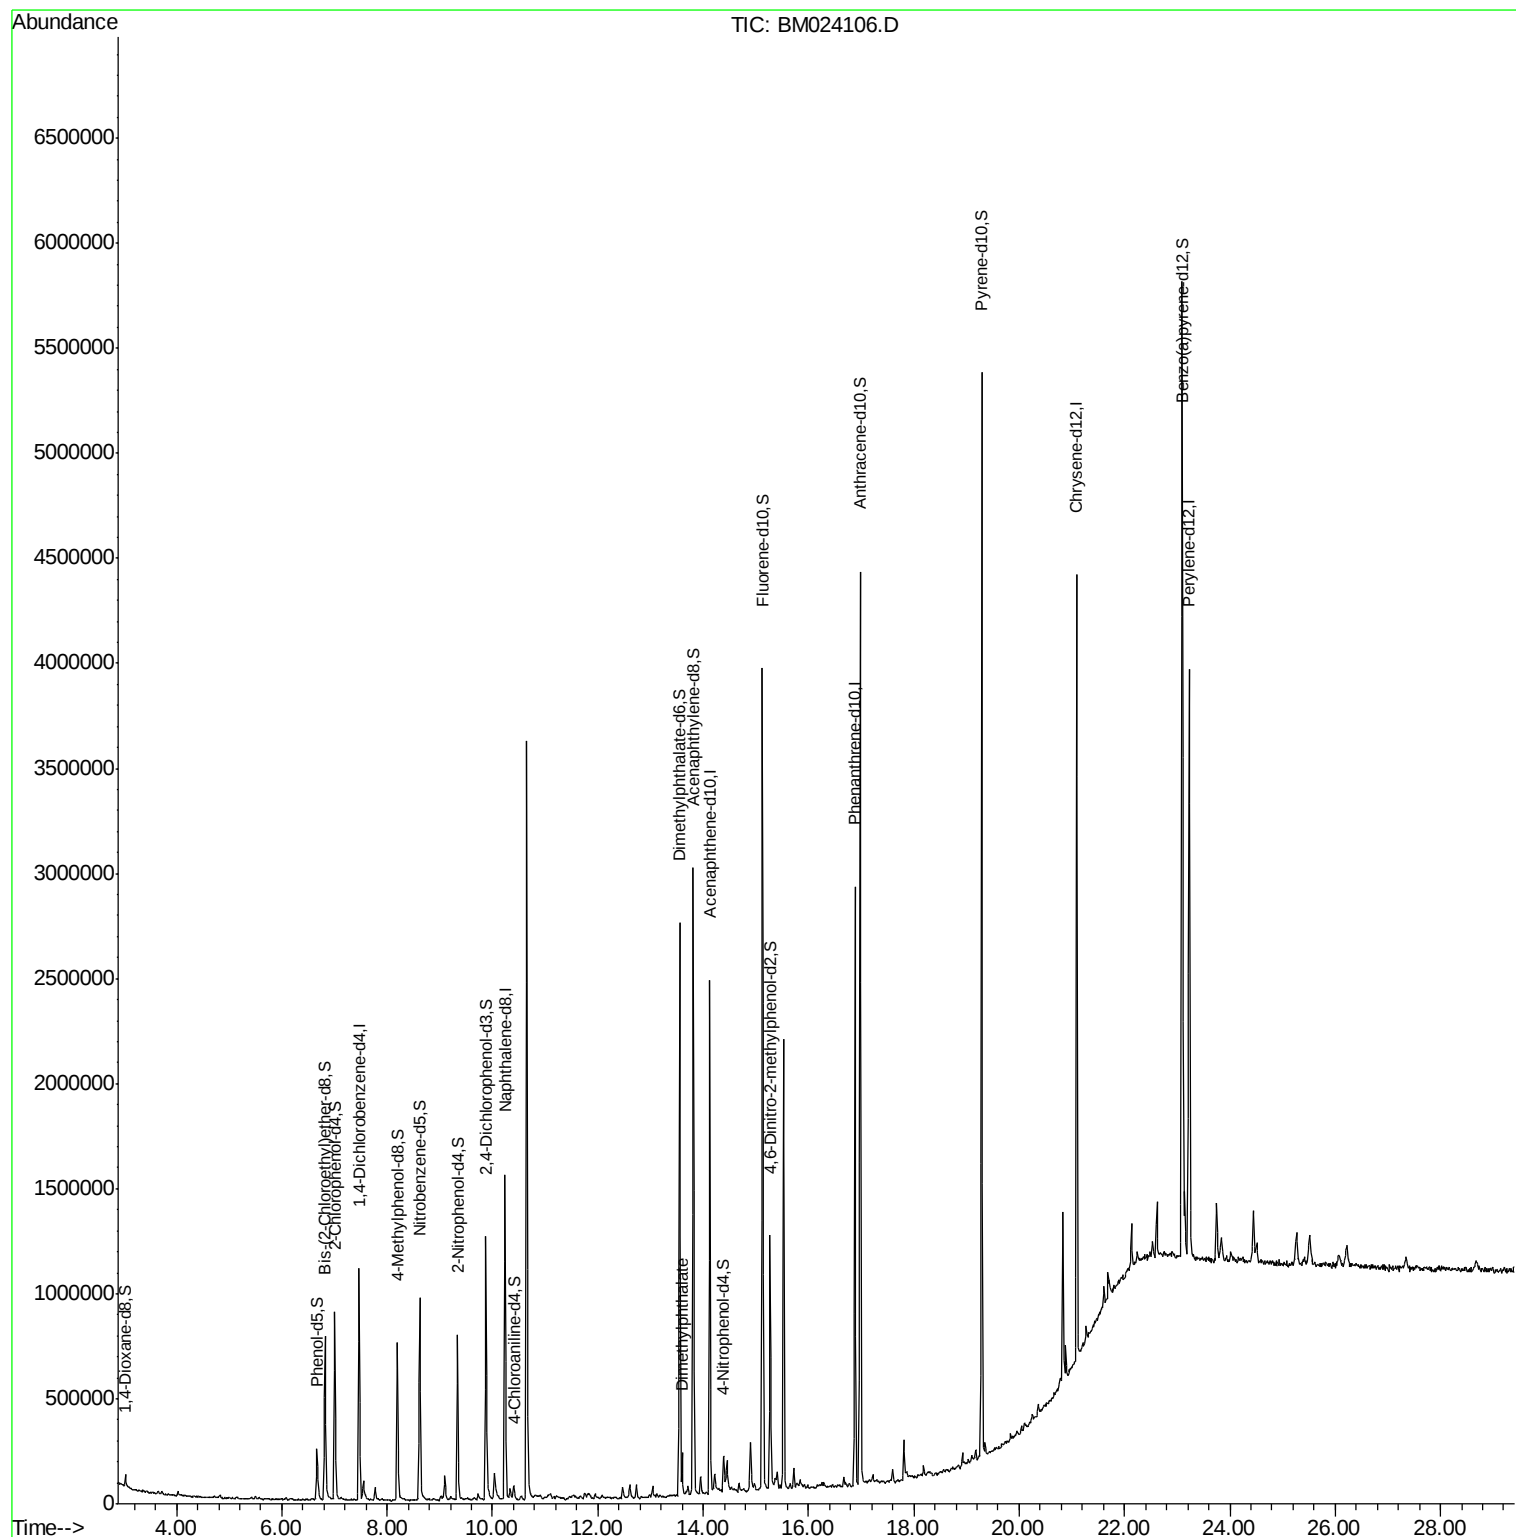

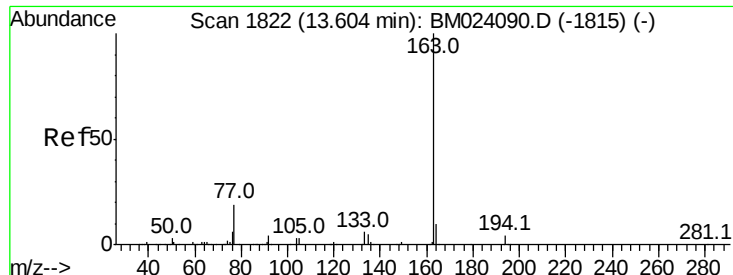

#45

Dimethylphthalate

Concen: 1.994 ng/ul

RT: 13.60 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM024106.D

Acq: 13 Dec 2019 23:48

Instrument :

BNA_M

ClientSampleId :

BFQW8

Tot Ion:163 Resp: 118183

Ion Ratio Lower Upper

163 100

194 4.7 3.3 4.9

164 9.6 7.9 11.9

