

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037967.D
 Acq On : 12 Dec 2022 15:46
 Operator : CG/JU
 Sample : PB149528BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK528

Quant Time: Dec 13 00:57:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	176160	20.000	ng/ul	0.00
20) Naphthalene-d8	10.892	136	709869	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.704	164	397060	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	698674	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	567109	20.000	ng/ul	0.00
88) Perylene-d12	24.097	264	595063	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	22745	5.862	ng/uL	0.00
4) Pyridine-d5	3.852	84	344114	29.899	ng/ul	0.00
7) Phenol-d5	7.228	99	451500	31.541	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	271621	31.161	ng/ul	0.00
11) 2-Chlorophenol-d4	7.604	132	383198	32.632	ng/ul	0.00
15) 4-Methylphenol-d8	8.786	113	351958	31.498	ng/ul	0.00
21) Nitrobenzene-d5	9.245	128	190087	33.821	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.975	143	198093	33.632	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	353140	31.566	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.033	131	471096	30.506	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	950424	33.575	ng/ul	-0.01
49) Acenaphthylene-d8	14.404	160	1147457	33.166	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	103376	21.428	ng/ul	0.00
60) Fluorene-d10	15.692	176	827190	32.799	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	71441	19.125	ng/ul	0.00
73) Anthracene-d10	17.545	188	1146255	35.153	ng/ul	0.00
81) Pyrene-d10	19.827	212	1169964	34.344	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.938	264	1084730	36.496	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.786	70	8359	1.010 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037967.D
Acq On : 12 Dec 2022 15:46
Operator : CG/JU
Sample : PB149528BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK528


Quant Time: Dec 13 00:57:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

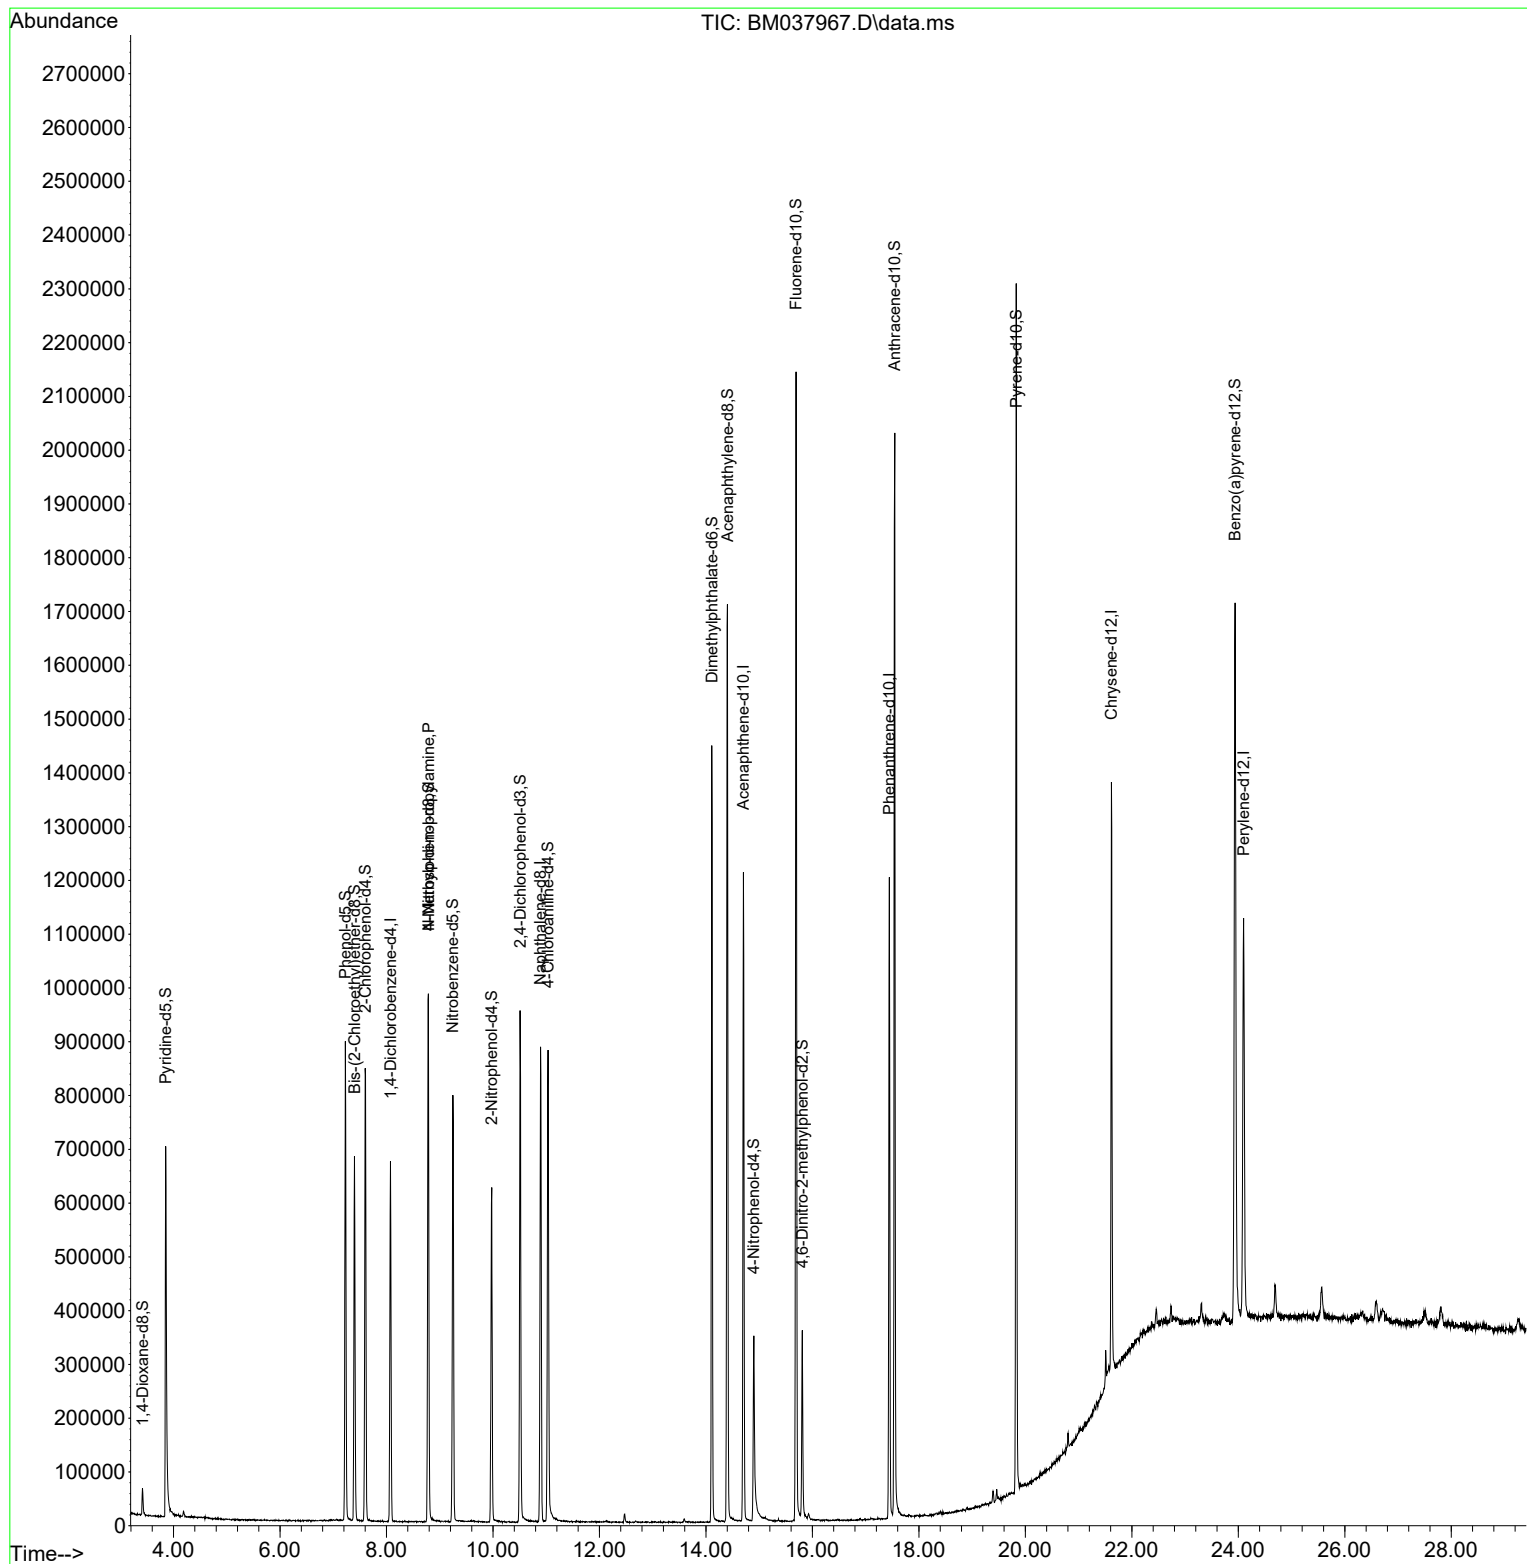

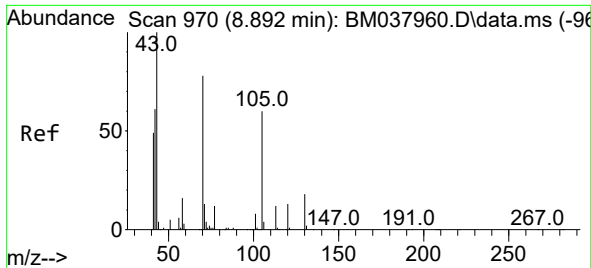

#17
N-Nitroso-di-n-propylamine
Concen: 1.010 ng/ul
RT: 8.786 min Scan# 91
Delta R.T. -0.112 min
Lab File: BM037967.D
Acq: 12 Dec 2022 15:46

Instrument :
BNA_M
ClientSampleId :
SBLK528

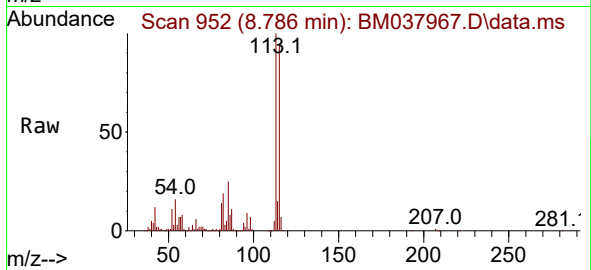

Tgt Ion:	70	Resp:	8359
Ion	Ratio	Lower	Upper
70	100		
42	484.2	62.3	93.5#
101	0.0	8.0	12.0#
130	0.0	17.6	26.4#

