

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037969.D
 Acq On : 12 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5948-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB6

Quant Time: Dec 13 00:57:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	179500	20.000	ng/u1	0.00
20) Naphthalene-d8	10.892	136	721089	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.704	164	409769	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	729228	20.000	ng/u1	0.00
79) Chrysene-d12	21.615	240	615963	20.000	ng/u1	# 0.00
88) Perylene-d12	24.091	264	672543	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	16555	4.188	ng/uL	0.00
4) Pyridine-d5	3.875	84	16385	1.397	ng/u1	0.02
7) Phenol-d5	7.228	99	84455	5.790	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	243091	27.369	ng/u1	0.00
11) 2-Chlorophenol-d4	7.598	132	278408	23.267	ng/u1	-0.01
15) 4-Methylphenol-d8	8.781	113	154460	13.566	ng/u1	-0.01
21) Nitrobenzene-d5	9.245	128	176378	30.893	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.975	143	175365	29.310	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	294151	25.884	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.033	131	87124	5.554	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	911876	31.214	ng/u1	-0.01
49) Acenaphthylene-d8	14.398	160	1104803	30.943	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.904	143	13022	2.616	ng/u1	0.00
60) Fluorene-d10	15.692	176	798485	30.679	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	72322	18.550	ng/u1	0.00
73) Anthracene-d10	17.545	188	1113380	32.714	ng/u1	0.00
81) Pyrene-d10	19.827	212	1170224	31.627	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.933	264	1117918	33.279	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	14179	3.419	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037969.D
Acq On : 12 Dec 2022 17:01
Operator : CG/JU
Sample : N5948-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB6

Quant Time: Dec 13 00:57:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

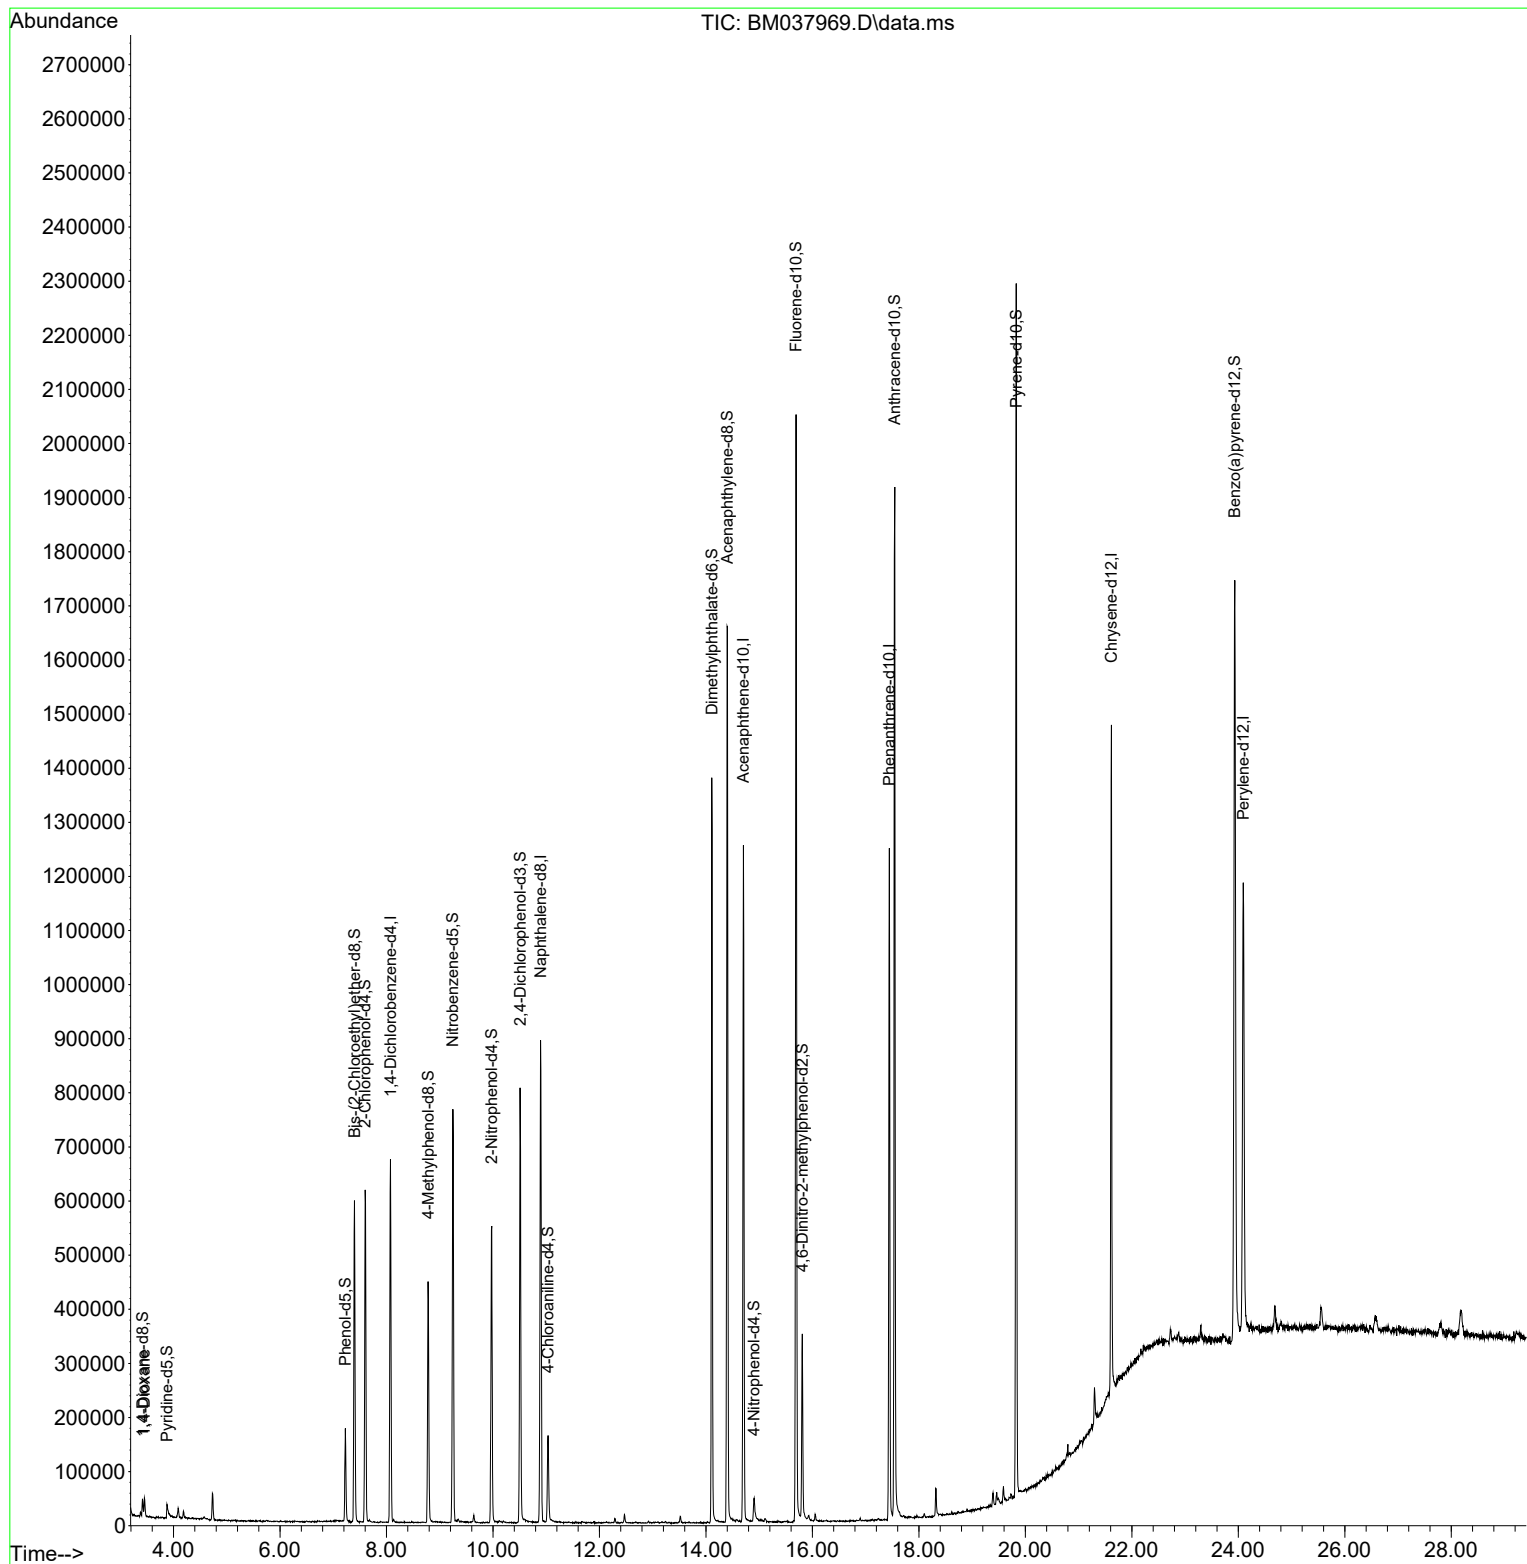

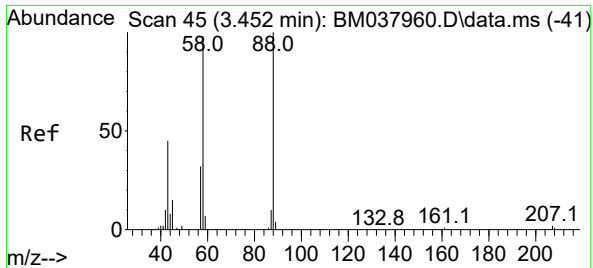

#2
 1,4-Dioxane
 Concen: 3.419 ng/uL
 RT: 3.452 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BM037969.D
 Acq: 12 Dec 2022 17:01

Instrument :
 BNA_M
 ClientSampleId :
 EXZB6

Tgt Ion:	88	Resp:	14179
Ion	Ratio	Lower	Upper
88	100		
43	47.9	32.8	49.2
58	89.7	64.6	97.0

