

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037978.D
 Acq On : 12 Dec 2022 22:31
 Operator : CG/JU
 Sample : PB149528BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS528

Quant Time: Dec 13 00:58:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	177419	20.000	ng/u1	0.00
20) Naphthalene-d8	10.892	136	771498	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.704	164	498657	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	946122	20.000	ng/u1	0.00
79) Chrysene-d12	21.615	240	757754	20.000	ng/u1	0.00
88) Perylene-d12	24.091	264	798733	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	23157	5.926	ng/uL	0.00
4) Pyridine-d5	3.852	84	333193	28.745	ng/u1	0.00
7) Phenol-d5	7.228	99	444111	30.804	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	263723	30.041	ng/u1	0.00
11) 2-Chlorophenol-d4	7.604	132	377990	31.960	ng/u1	0.00
15) 4-Methylphenol-d8	8.787	113	349529	31.058	ng/u1	0.00
21) Nitrobenzene-d5	9.245	128	194967	31.918	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.975	143	204942	32.015	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	403364	33.175	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.033	131	484258	28.853	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	1127999	31.729	ng/u1	-0.01
49) Acenaphthylene-d8	14.398	160	1372979	31.599	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.898	143	160589	26.505	ng/u1	0.00
60) Fluorene-d10	15.692	176	1034420	32.659	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	141102	27.895	ng/u1	0.00
73) Anthracene-d10	17.545	188	1453161	32.909	ng/u1	0.00
81) Pyrene-d10	19.827	212	1438754	31.608	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.933	264	1352468	33.901	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	42570	10.385	ng/uL	96
5) Pyridine	3.869	79	315662	27.098	ng/u1	94
6) Benzaldehyde	7.210	77	231034	42.845	ng/u1	94
8) Phenol	7.257	94	420800	29.102	ng/u1	93
10) Bis(2-Chloroethyl)ether	7.493	93	335717	28.275	ng/u1	99
12) 2-Chlorophenol	7.634	128	375212	31.021	ng/u1	99
13) 2-Methylphenol	8.516	108	327281	29.577	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.610	45	618847	28.864	ng/u1	98
16) Acetophenone	8.910	105	541130	30.573	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.898	70	259456	31.118	ng/u1	98
18) 4-Methylphenol	8.851	108	356227	29.760	ng/u1	99
19) Hexachloroethane	9.163	117	149590	30.935	ng/u1	96
22) Nitrobenzene	9.292	77	399441	30.391	ng/u1	100
23) Isophorone	9.822	82	721932	29.975	ng/u1	97
25) 2-Nitrophenol	10.004	139	209990	31.290	ng/u1	93
26) 2,4-Dimethylphenol	10.057	107	378777	29.186	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.298	93	460267	28.748	ng/u1	98
29) 2,4-Dichlorophenol	10.539	162	380943	31.934	ng/u1	98
30) Naphthalene	10.945	128	1256398	30.177	ng/u1	99
32) 4-Chloroaniline	11.057	127	460262	27.500	ng/u1	97
33) Hexachlorobutadiene	11.222	225	263952	33.635	ng/u1	98
34) Caprolactam	11.851	113	96592	31.566	ng/u1	88
35) 4-Chloro-3-methylphenol	12.169	107	349761	32.211	ng/u1	99
36) 2-Methylnaphthalene	12.545	142	864266	32.005	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037978.D
 Acq On : 12 Dec 2022 22:31
 Operator : CG/JU
 Sample : PB149528BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS528

Quant Time: Dec 13 00:58:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.763	142	872700	31.606	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.904	216	498140	30.574	ng/ul	99
40) Hexachlorocyclopentadiene	12.880	237	133933	14.370	ng/ul	100
41) 2,4,6-Trichlorophenol	13.145	196	302283	30.458	ng/ul	97
42) 2,4,5-Trichlorophenol	13.216	196	320118	30.928	ng/ul	97
43) 1,1'-Biphenyl	13.545	154	1159811	28.936	ng/ul	98
44) 2-Chloronaphthalene	13.586	162	912983	29.526	ng/ul	98
45) 2-Nitroaniline	13.792	65	230195	30.897	ng/ul	99
47) Dimethylphthalate	14.163	163	1092768	31.155	ng/ul	99
48) 2,6-Dinitrotoluene	14.286	165	213815	31.383	ng/ul	96
50) Acenaphthylene	14.427	152	1432657	29.987	ng/ul	99
51) 3-Nitroaniline	14.616	138	210728	31.001	ng/ul	99
52) Acenaphthene	14.769	153	1009818	30.558	ng/ul	98
53) 2,4-Dinitrophenol	14.816	184	79430	23.759	ng/ul	92
55) 4-Nitrophenol	14.916	109	115713	28.960	ng/ul	91
56) Dibenzofuran	15.104	168	1366561	30.290	ng/ul	100
57) 2,4-Dinitrotoluene	15.068	165	293639	31.825	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.327	232	279104	32.057	ng/ul	98
59) Diethylphthalate	15.516	149	1119371	32.035	ng/ul	99
61) Fluorene	15.751	166	1158159	31.477	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.739	204	583077	32.427	ng/ul	98
63) 4-Nitroaniline	15.774	138	201991	32.772	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.827	198	136060	27.784	ng/ul	96
67) N-Nitrosodiphenylamine	15.951	169	921869	32.301	ng/ul	99
68) 4-Bromophenyl-phenylether	16.633	248	341378	32.916	ng/ul	97
69) Hexachlorobenzene	16.751	284	410040	33.121	ng/ul	98
70) Atrazine	16.898	200	294410	30.187	ng/ul	99
71) Pentachlorophenol	17.092	266	195851	28.454	ng/ul	97
72) Phenanthrene	17.486	178	1612105	31.201	ng/ul	100
74) Anthracene	17.580	178	1616013	30.777	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.510	216	490484	32.067	ng/uL	98
76) Pentachlorobenzene	15.021	250	488897	32.267	ng/uL	96
77) Carbazole	17.851	167	1328690	29.208	ng/ul	100
78) Di-n-butylphthalate	18.398	149	1789831	33.100	ng/ul	99
80) Fluoranthene	19.492	202	1648090	30.679	ng/ul	98
82) Pyrene	19.856	202	1716135	30.695	ng/ul	98
83) Butylbenzylphthalate	20.733	149	621537	29.897	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.527	252	450422	30.039	ng/ul	98
85) Benzo(a)anthracene	21.597	228	1606260	31.486	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.503	149	902264	29.833	ng/ul	99
87) Chrysene	21.650	228	1480446	30.930	ng/ul	99
89) Di-n-octyl phthalate	22.450	149	1477201	28.863	ng/ul	100
90) Benzo(b)fluoranthene	23.333	252	1571104	31.728	ng/ul	100
91) Benzo(k)fluoranthene	23.380	252	1561230	32.532	ng/ul	99
93) Benzo(a)pyrene	23.980	252	1376129	31.602	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.685	276	1541214	27.482	ng/ul	97
95) Dibenzo(a,h)anthracene	26.697	278	1390623	29.414	ng/ul	99
96) Benzo(g,h,i)perylene	27.485	276	1276511	28.509	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037978.D
 Acq On : 12 Dec 2022 22:31
 Operator : CG/JU
 Sample : PB149528BS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS528

Quant Time: Dec 13 00:58:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration




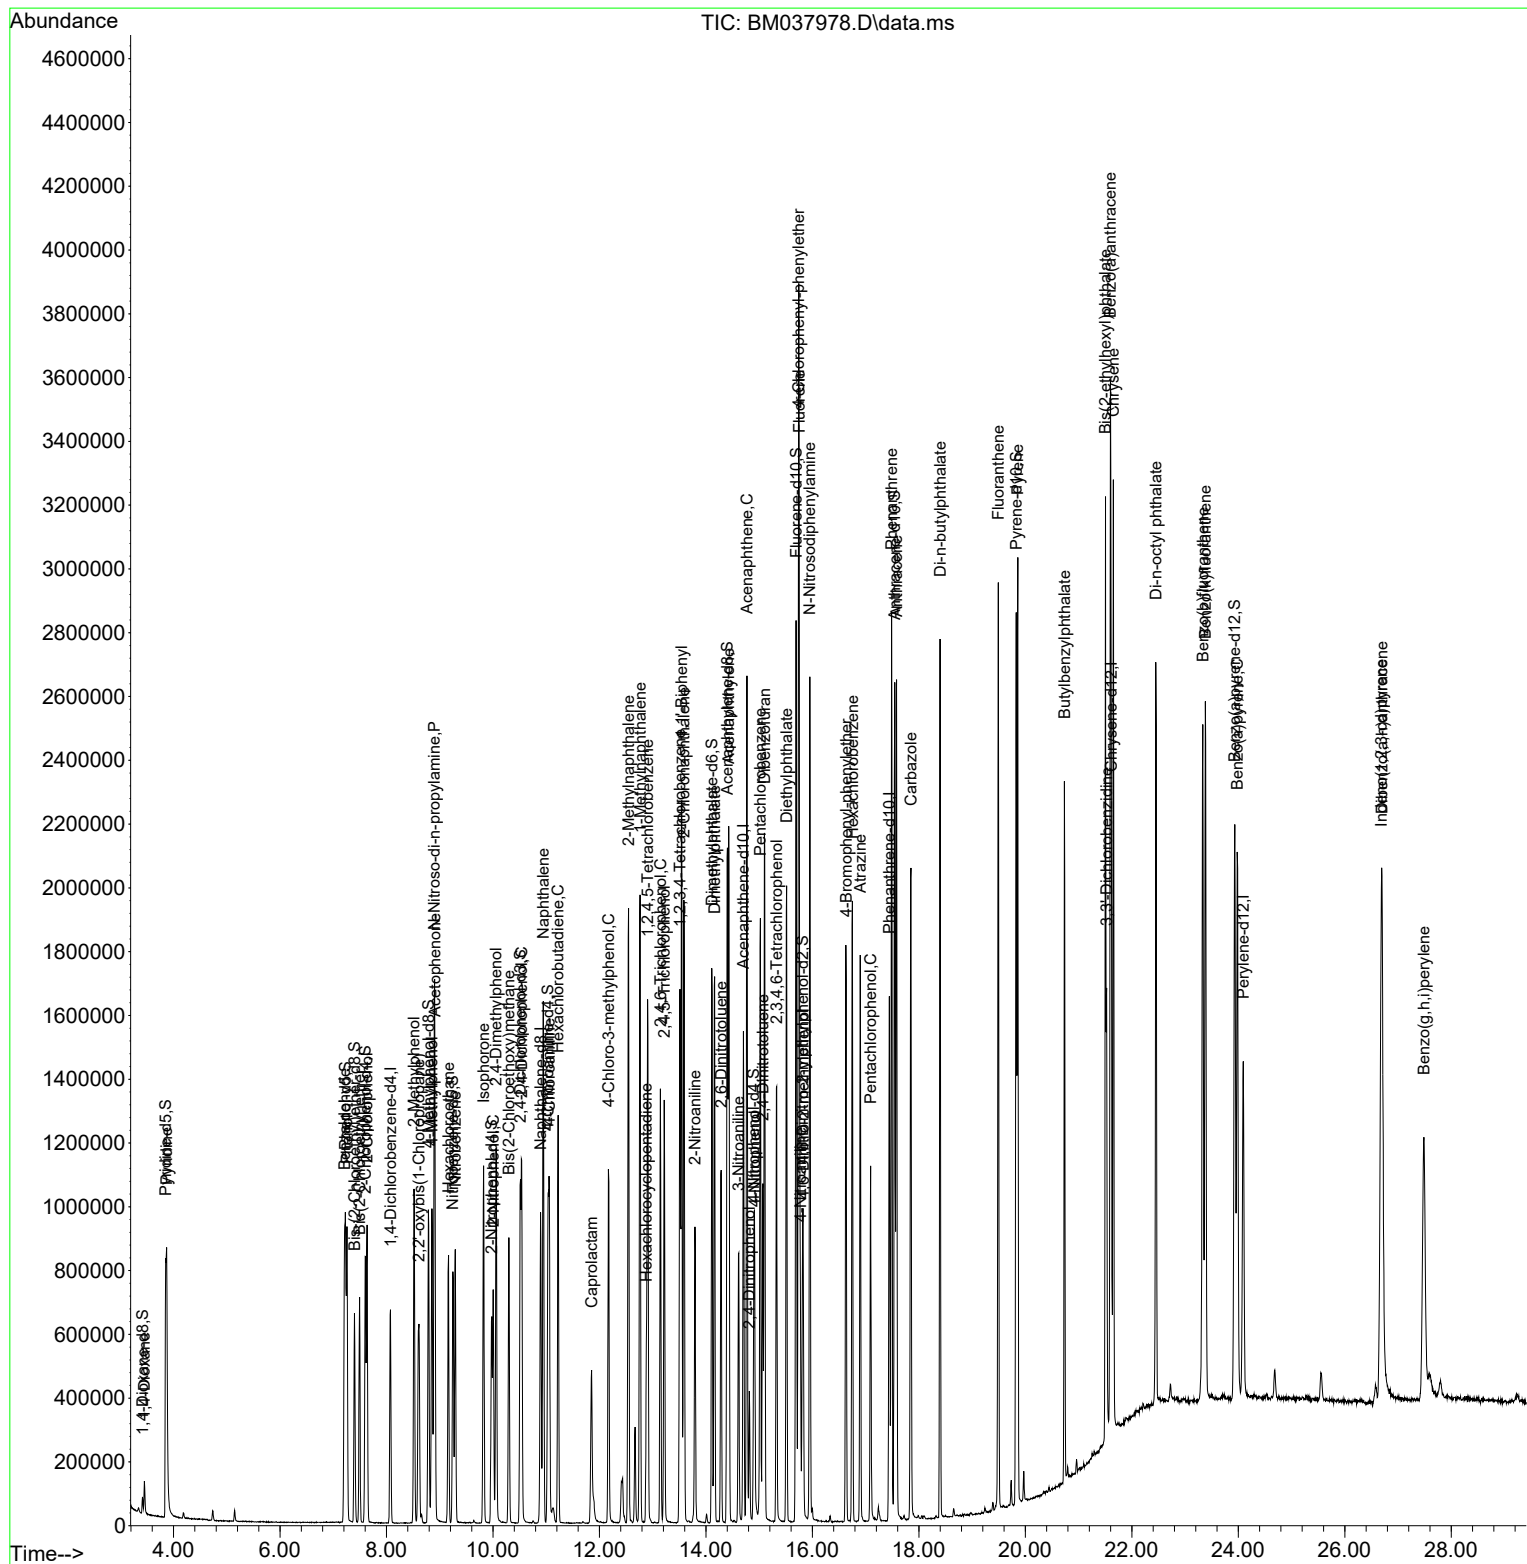




#2
1,4-Dioxane
Concen: 10.385 ng/uL
RT: 3.452 min Scan# 41
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion: 88 Resp: 42570
Ion Ratio Lower Upper
88 100
43 39.6 32.8 49.2
58 85.5 64.6 97.0



#5
Pyridine
Concen: 27.098 ng/uL
RT: 3.869 min Scan# 116
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion: 79 Resp: 315662
Ion Ratio Lower Upper
79 100
52 103.2 78.1 117.1
51 50.8 37.2 55.8



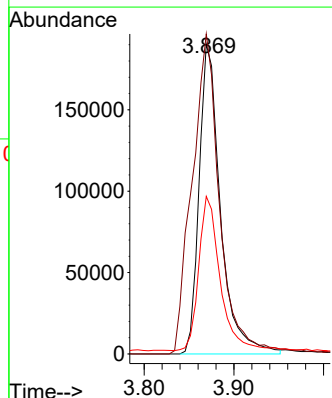





#6
Benzaldehyde
Concen: 42.845 ng/ul
RT: 7.210 min Scan# 684
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion: 77 Resp: 231034
Ion Ratio Lower Upper
77 100
105 98.7 82.5 123.7
106 94.4 81.8 122.6

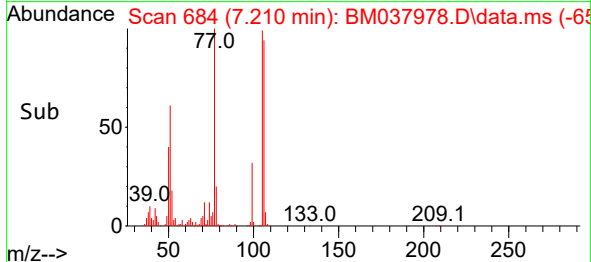

#8
Phenol
Concen: 29.102 ng/ul
RT: 7.257 min Scan# 692
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion: 94 Resp: 420800
Ion Ratio Lower Upper
94 100
65 30.5 22.2 33.4
66 39.0 27.3 40.9




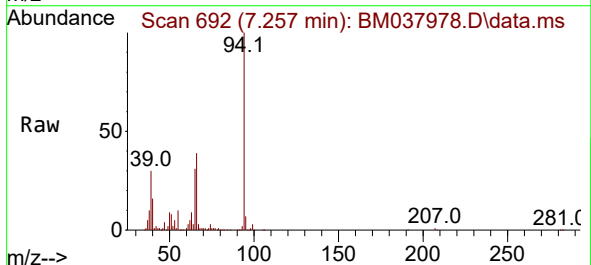




#10
Bis(2-Chloroethyl)ether
Concen: 28.275 ng/ul
RT: 7.493 min Scan# 732
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion: 93 Resp: 335717
Ion Ratio Lower Upper
93 100
63 83.5 66.3 99.5
95 33.3 25.7 38.5

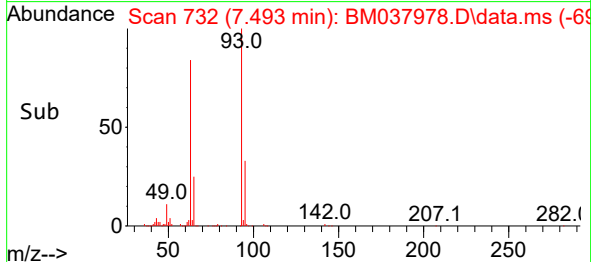

#12
2-Chlorophenol
Concen: 31.021 ng/ul
RT: 7.634 min Scan# 756
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:128 Resp: 375212
Ion Ratio Lower Upper
128 100
64 44.7 35.2 52.8
130 33.2 25.9 38.9

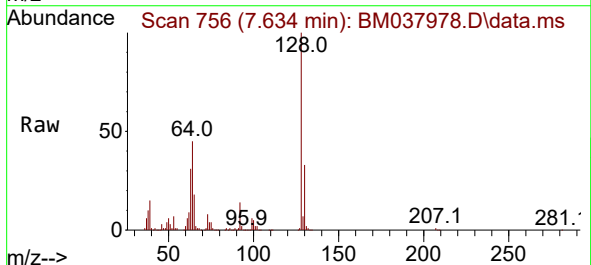



#13

2-Methylphenol

Concen: 29.577 ng/ul

RT: 8.516 min Scan# 906

Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :





SLCS528

Tgt Ion:108 Resp: 327281

Ion Ratio Lower Upper

108 100

107 88.7 71.9 107.9

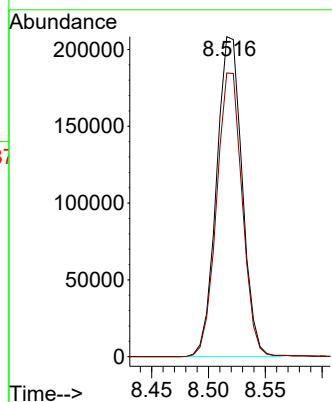

#14

2,2'-oxybis(1-Chloropropane)

Concen: 28.864 ng/ul

RT: 8.610 min Scan# 922

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion: 45 Resp: 618847


Ion Ratio Lower Upper

45 100

77 10.6 9.0 13.4

79 8.7 6.2 9.4









#16
Acetophenone
Concen: 30.573 ng/ul
RT: 8.910 min Scan# 91
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:105 Resp: 541130
Ion Ratio Lower Upper
105 100
77 70.8 59.7 89.5
51 33.5 27.2 40.8



#17
N-Nitroso-di-n-propylamine
Concen: 31.118 ng/ul
RT: 8.898 min Scan# 971
Delta R.T. -0.000 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion: 70 Resp: 259456
Ion Ratio Lower Upper
70 100
42 79.9 62.3 93.5
101 10.2 8.0 12.0
130 23.3 17.6 26.4





#18

4-Methylphenol

Concen: 29.760 ng/ul

RT: 8.851 min Scan# 9

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :





SLCS528

Tgt Ion:108 Resp: 356227

Ion Ratio Lower Upper

108 100

107 111.6 88.1 132.1



#19

Hexachloroethane

Concen: 30.935 ng/ul

RT: 9.163 min Scan# 1016

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:117 Resp: 149590


Ion Ratio Lower Upper

117 100

201 110.3 87.3 130.9

199 71.6 50.9 76.3







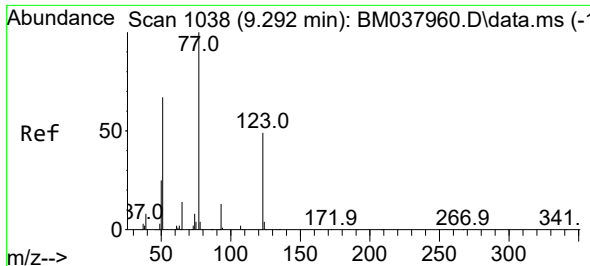

#22
Nitrobenzene
Concen: 30.391 ng/ul
RT: 9.292 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion: 77 Resp: 399441
Ion Ratio Lower Upper
77 100
123 47.2 37.8 56.6
65 13.8 11.1 16.7

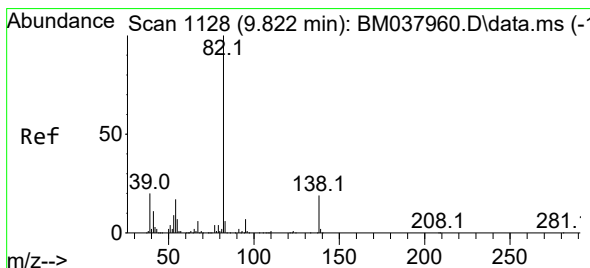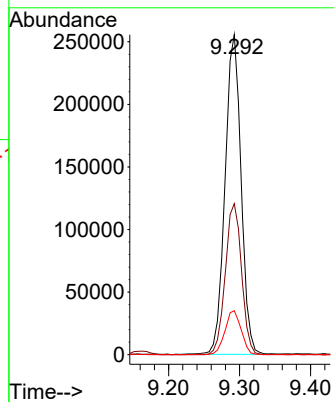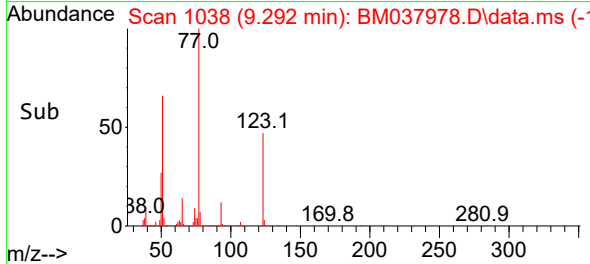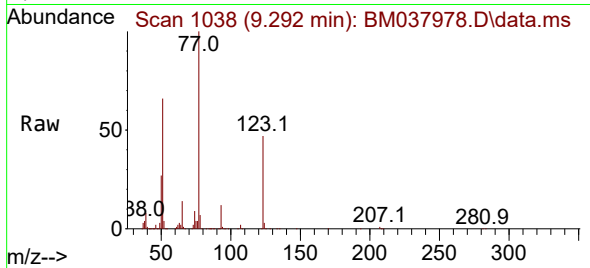

#23
Isophorone
Concen: 29.975 ng/ul
RT: 9.822 min Scan# 1128
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion: 82 Resp: 721932
Ion Ratio Lower Upper
82 100
95 7.1 5.2 7.8
138 20.0 14.9 22.3


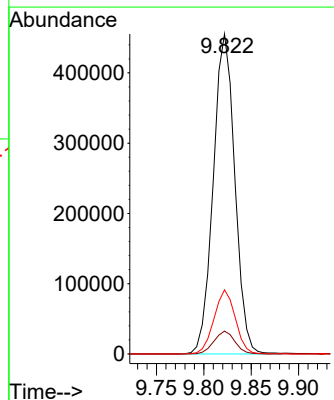
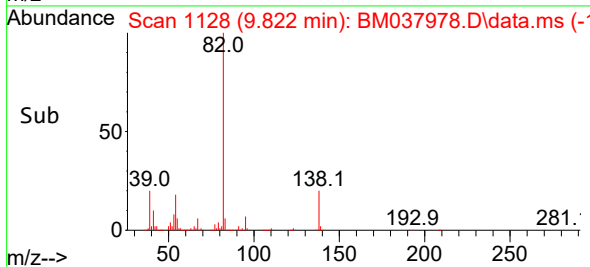
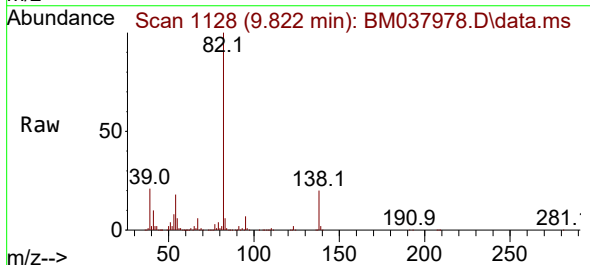


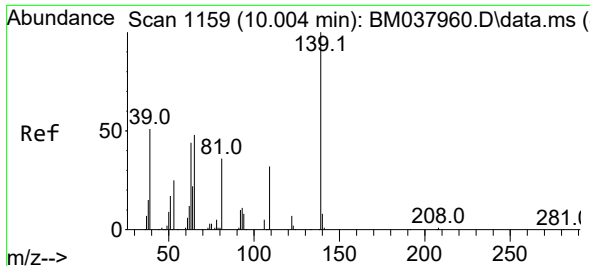

#25
2-Nitrophenol
Concen: 31.290 ng/ul
RT: 10.004 min Scan# 1159
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:139 Resp: 209990
Ion Ratio Lower Upper
139 100
65 49.6 36.2 54.4
109 28.0 19.7 29.5

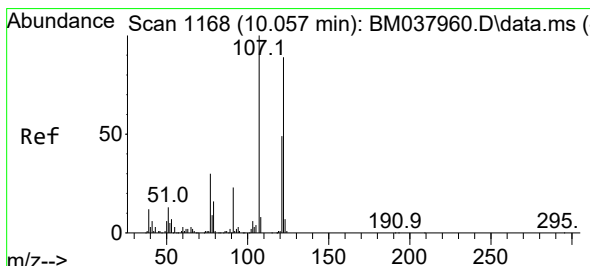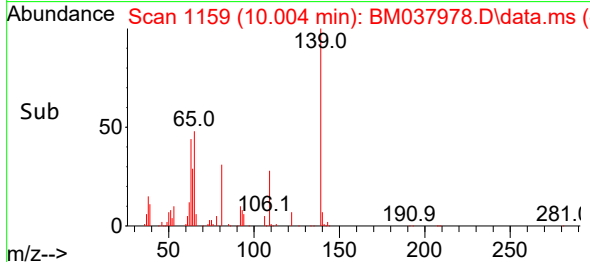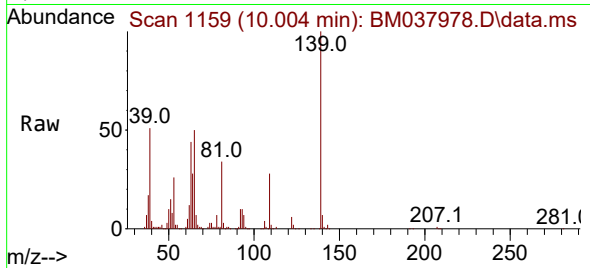

#26
2,4-Dimethylphenol
Concen: 29.186 ng/ul
RT: 10.057 min Scan# 1168
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:107 Resp: 378777
Ion Ratio Lower Upper
107 100
121 51.5 42.0 63.0
122 90.6 71.4 107.2

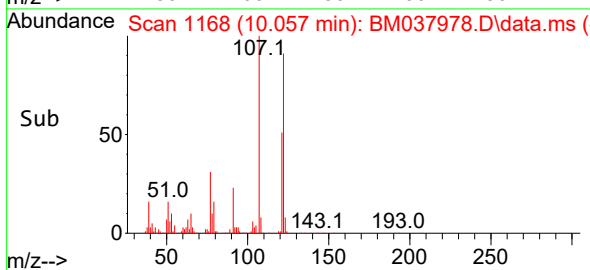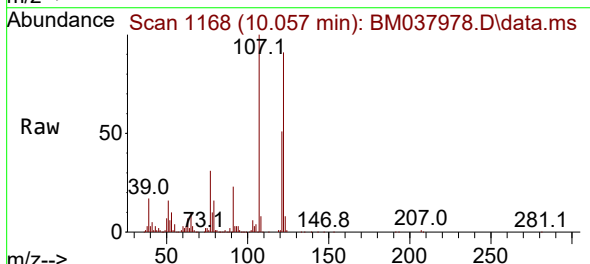



#27

Bis(2-Chloroethoxy)methane

Concen: 28.748 ng/ul

RT: 10.298 min Scan# 11

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion: 93 Resp: 460267

Ion Ratio Lower Upper

93 100

95 33.2 25.5 38.3

123 12.1 9.4 14.2

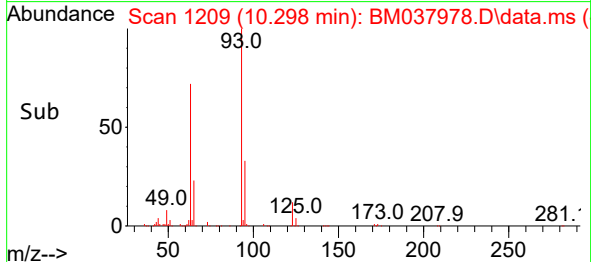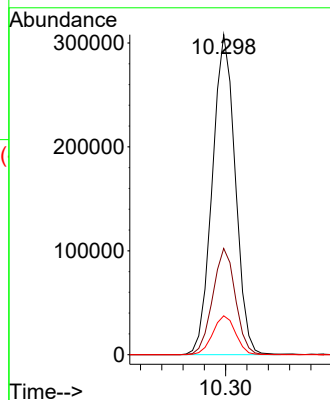

#29

2,4-Dichlorophenol

Concen: 31.934 ng/ul

RT: 10.539 min Scan# 1250

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:162 Resp: 380943


Ion Ratio Lower Upper

162 100

164 65.5 51.4 77.2

98 31.3 26.1 39.1


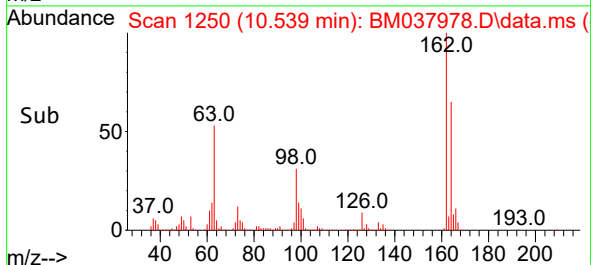
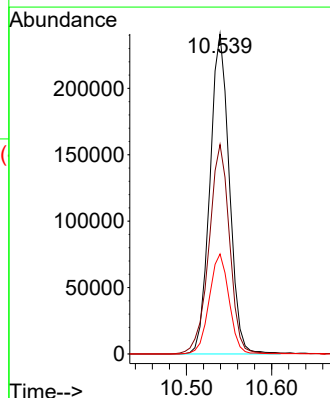
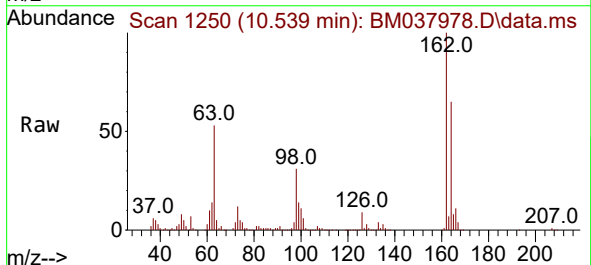




#30
Naphthalene
Concen: 30.177 ng/ul
RT: 10.945 min Scan# 1319
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:128 Resp: 1256398
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.4
127 12.5 10.4 15.6

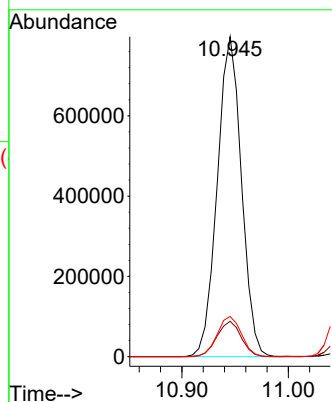

#32
4-Chloroaniline
Concen: 27.500 ng/ul
RT: 11.057 min Scan# 1338
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:127 Resp: 460262
Ion Ratio Lower Upper
127 100
129 33.1 25.3 37.9









#33
Hexachlorobutadiene
Concen: 33.635 ng/ul
RT: 11.222 min Scan# 11
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:225 Resp: 263952
Ion Ratio Lower Upper
225 100
223 61.3 50.8 76.2
227 64.3 50.5 75.7

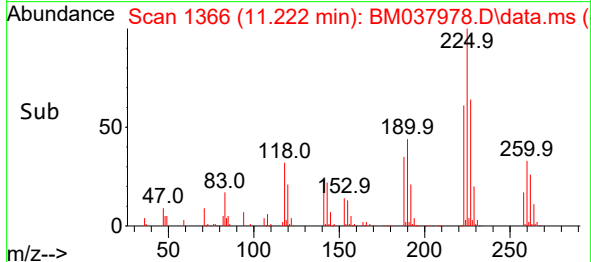

#34
Caprolactam
Concen: 31.566 ng/ul
RT: 11.851 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:113 Resp: 96592
Ion Ratio Lower Upper
113 100
55 192.1 172.2 258.2
56 139.2 120.7 181.1




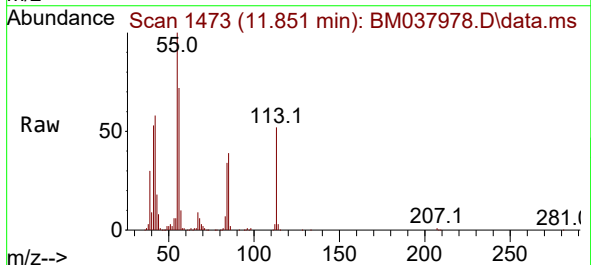




#35
 4-Chloro-3-methylphenol
 Concen: 32.211 ng/ul
 RT: 12.169 min Scan# 1527
 Delta R.T. -0.006 min
 Lab File: BM037978.D
 Acq: 12 Dec 2022 22:31




Instrument :
 BNA_M
 ClientSampleId :
 SLCS528


Tgt Ion:107 Resp: 349761
 Ion Ratio Lower Upper
 107 100
 144 29.1 23.4 35.0
 142 87.1 71.0 106.4

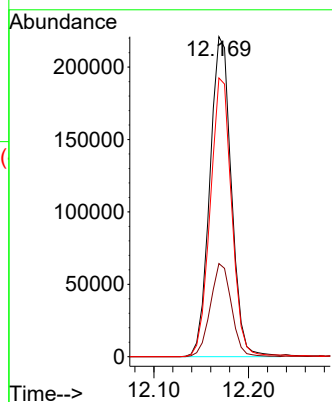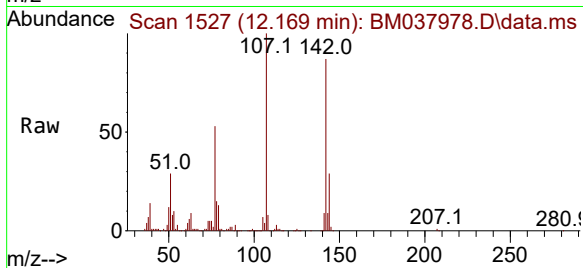

#36
 2-Methylnaphthalene
 Concen: 32.005 ng/ul
 RT: 12.545 min Scan# 1591
 Delta R.T. -0.006 min
 Lab File: BM037978.D
 Acq: 12 Dec 2022 22:31

Tgt Ion:142 Resp: 864266
 Ion Ratio Lower Upper
 142 100
 141 89.2 69.4 104.0


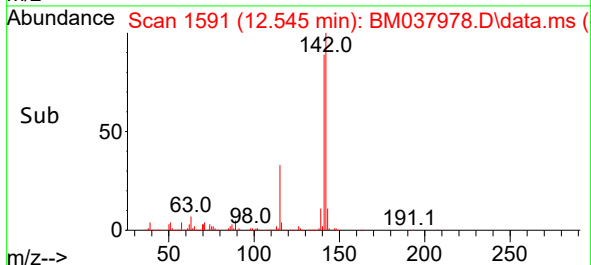

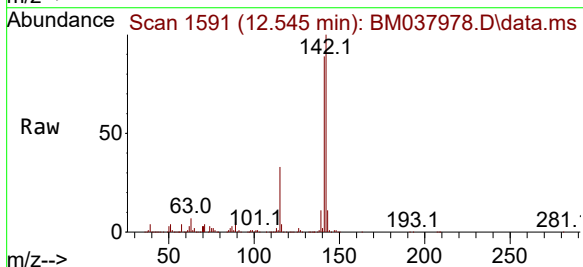




#37
1-Methylnaphthalene
Concen: 31.606 ng/ul
RT: 12.763 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:142 Resp: 872700
Ion Ratio Lower Upper
142 100
141 91.7 72.4 108.6
116 3.7 2.9 4.3

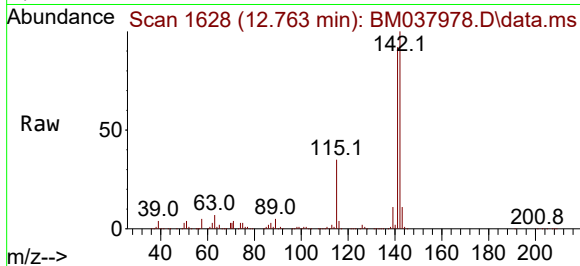

#39
1,2,4,5-Tetrachlorobenzene
Concen: 30.574 ng/ul
RT: 12.904 min Scan# 1652
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:216 Resp: 498140
Ion Ratio Lower Upper
216 100
214 79.9 64.2 96.4
179 18.6 15.4 23.2
108 16.5 12.7 19.1




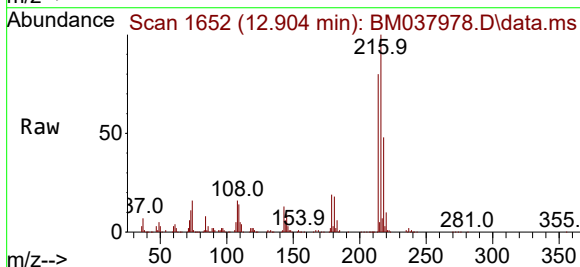




#40
Hexachlorocyclopentadiene
Concen: 14.370 ng/ul
RT: 12.880 min Scan# 1648
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:237 Resp: 133933
Ion Ratio Lower Upper
237 100
235 63.1 50.4 75.6
272 14.0 10.6 16.0

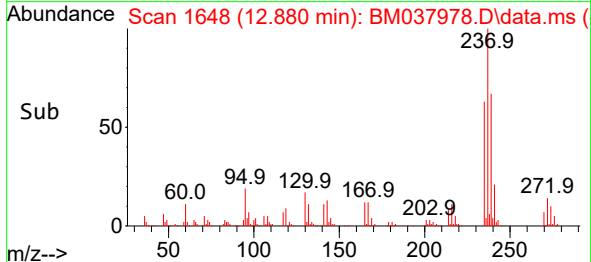

#41
2,4,6-Trichlorophenol
Concen: 30.458 ng/ul
RT: 13.145 min Scan# 1693
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:196 Resp: 302283
Ion Ratio Lower Upper
196 100
198 96.0 75.0 112.6
200 32.7 24.5 36.7




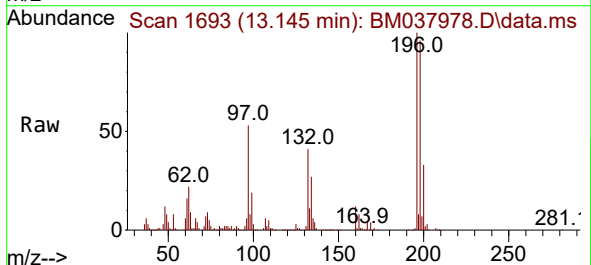




#42
2,4,5-Trichlorophenol
Concen: 30.928 ng/ul
RT: 13.216 min Scan# 1705
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:196 Resp: 320118
Ion Ratio Lower Upper
196 100
198 98.8 76.5 114.7
200 30.1 24.9 37.3

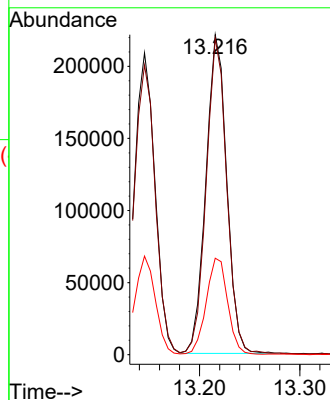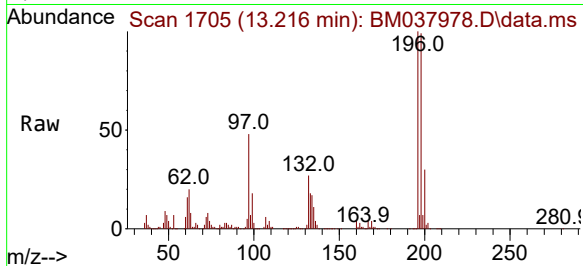

#43
1,1'-Biphenyl
Concen: 28.936 ng/ul
RT: 13.545 min Scan# 1761
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:154 Resp: 1159811
Ion Ratio Lower Upper
154 100
153 38.4 31.2 46.8
76 10.3 9.3 13.9



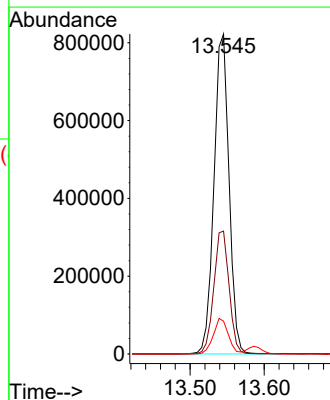
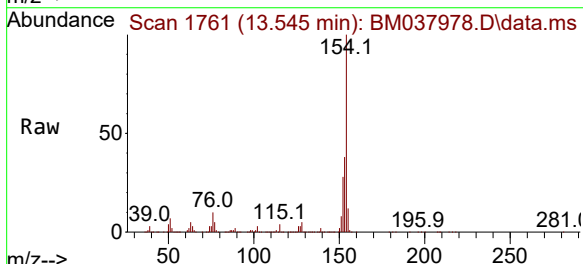


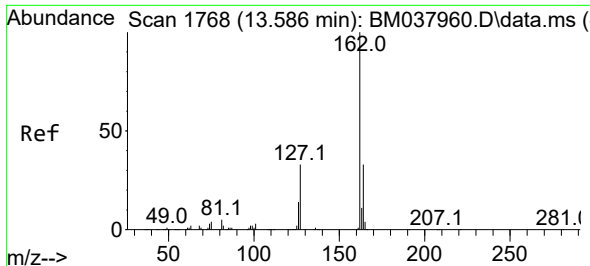

#44
2-Chloronaphthalene
Concen: 29.526 ng/ul
RT: 13.586 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:162 Resp: 912983
Ion Ratio Lower Upper
162 100
164 32.6 27.3 40.9
127 37.0 29.4 44.0

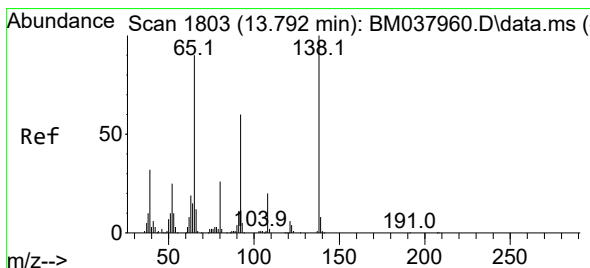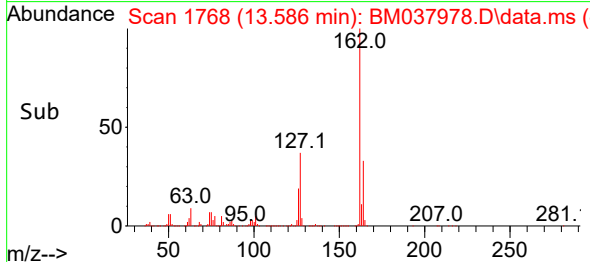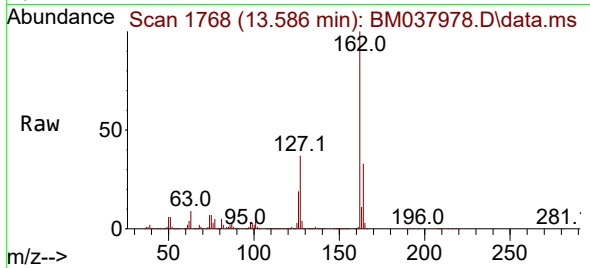

#45
2-Nitroaniline
Concen: 30.897 ng/ul
RT: 13.792 min Scan# 1803
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion: 65 Resp: 230195
Ion Ratio Lower Upper
65 100
92 67.0 53.5 80.3
138 111.9 91.3 136.9

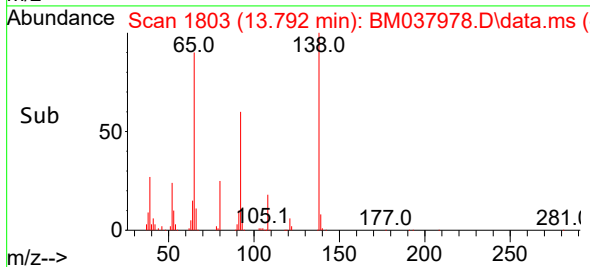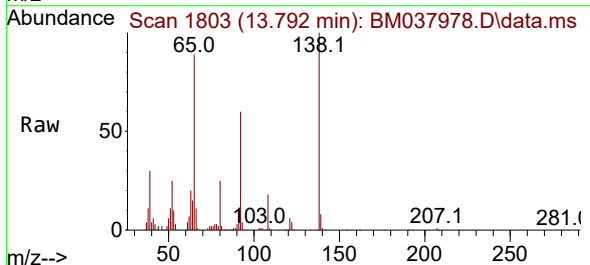



#47

Dimethylphthalate

Concen: 31.155 ng/ul

RT: 14.163 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:163 Resp: 1092768

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6

164 9.9 8.2 12.4

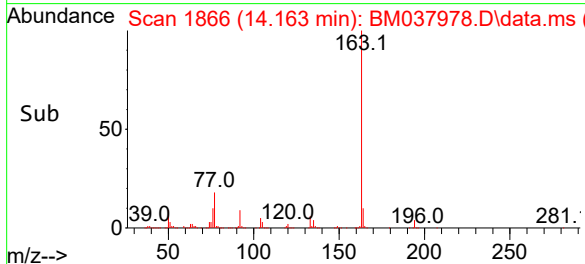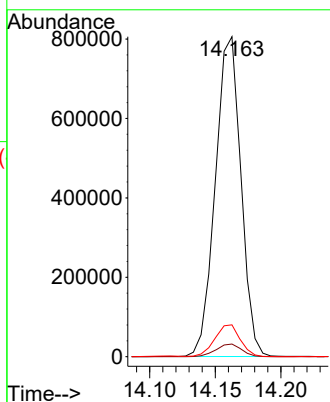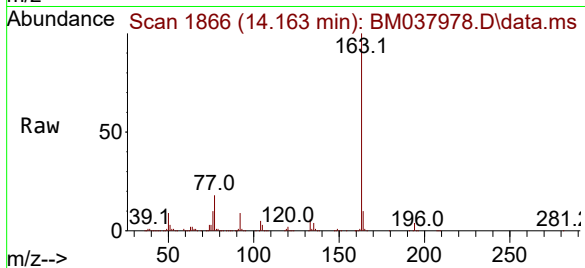

#48

2,6-Dinitrotoluene

Concen: 31.383 ng/ul

RT: 14.286 min Scan# 1887

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:165 Resp: 213815


Ion Ratio Lower Upper

165 100

89 54.6 41.1 61.7

121 20.1 17.4 26.2


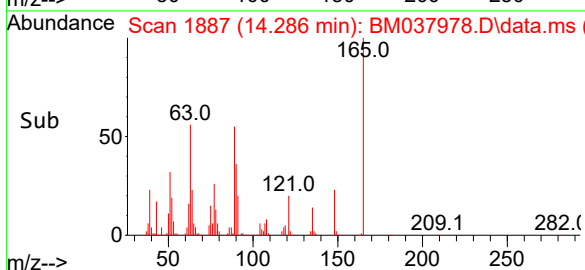
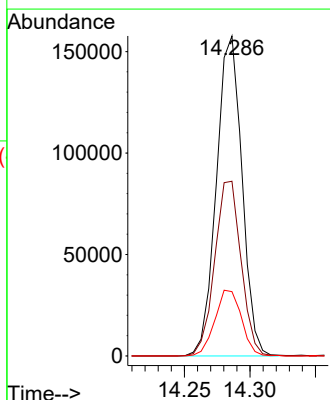
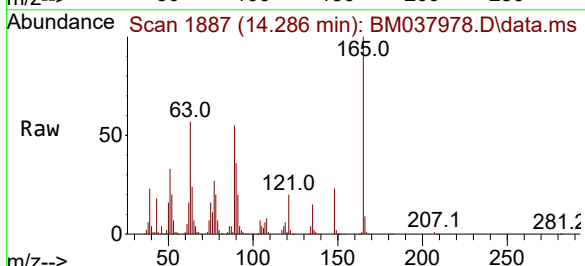




#50
Acenaphthylene
Concen: 29.987 ng/ul
RT: 14.427 min Scan# 1911
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:152 Resp: 1432657
Ion Ratio Lower Upper
152 100
151 20.0 15.3 22.9
153 13.1 10.2 15.4

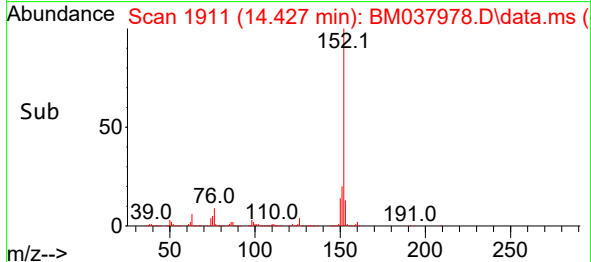

#51
3-Nitroaniline
Concen: 31.001 ng/ul
RT: 14.616 min Scan# 1943
Delta R.T. -0.000 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:138 Resp: 210728
Ion Ratio Lower Upper
138 100
108 9.2 7.9 11.9
92 103.1 83.4 125.0




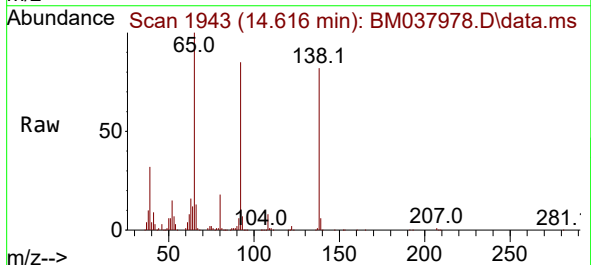




#52
Acenaphthene
Concen: 30.558 ng/ul
RT: 14.769 min Scan# 1969
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:153 Resp: 1009818
Ion Ratio Lower Upper
153 100
152 46.5 38.2 57.4
154 88.0 71.4 107.0

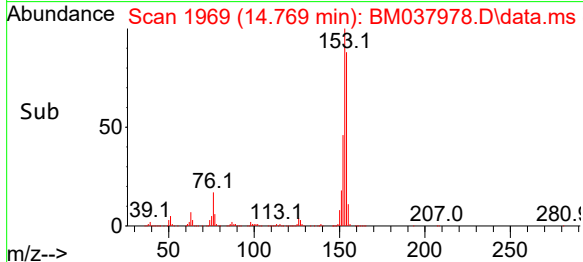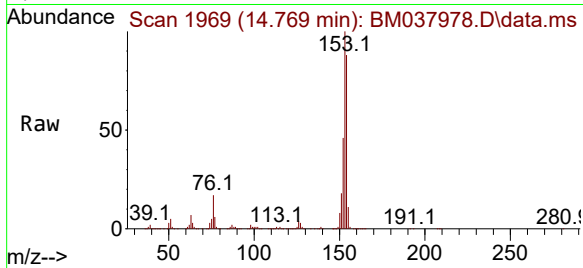

#53
2,4-Dinitrophenol
Concen: 23.759 ng/ul
RT: 14.816 min Scan# 1977
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:184 Resp: 79430
Ion Ratio Lower Upper
184 100
63 67.5 46.2 69.4
154 58.8 45.5 68.3




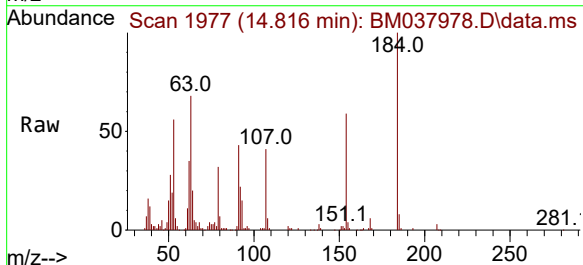




#55
4-Nitrophenol
Concen: 28.960 ng/ul
RT: 14.916 min Scan# 1994
Delta R.T. -0.000 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:109 Resp: 115713
Ion Ratio Lower Upper
109 100
139 135.8 119.2 178.8
65 128.0 108.7 163.1



#56
Dibenzofuran
Concen: 30.290 ng/ul
RT: 15.104 min Scan# 2026
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:168 Resp: 1366561
Ion Ratio Lower Upper
168 100
139 35.0 28.1 42.1





#57

2,4-Dinitrotoluene

Concen: 31.825 ng/ul

RT: 15.068 min Scan# 2019

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:165 Resp: 293639

Ion Ratio Lower Upper

165 100

63 44.1 34.9 52.3

182 2.4 2.2 3.2

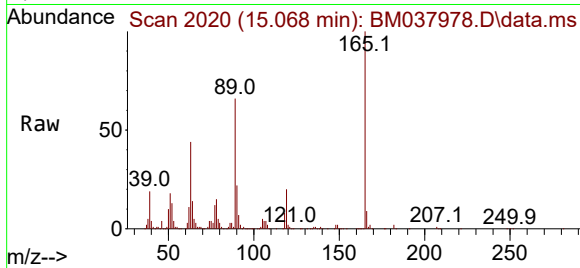

#58

2,3,4,6-Tetrachlorophenol

Concen: 32.057 ng/ul

RT: 15.327 min Scan# 2064

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Tgt Ion:232 Resp: 279104




Ion Ratio Lower Upper


232 100

131 40.7 32.8 49.2

130 2.3 2.0 3.0

166 27.2 23.2 34.8



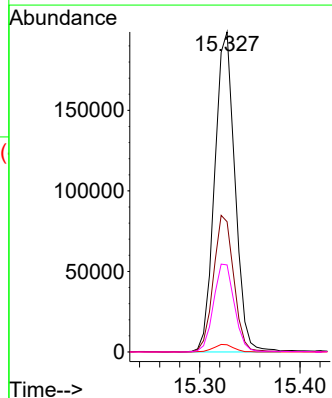
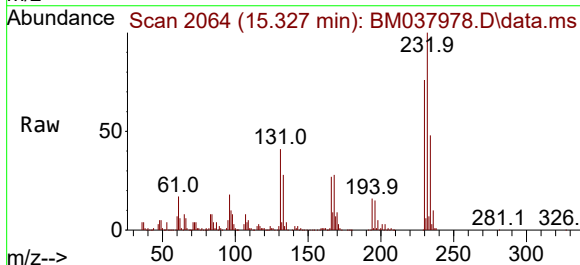




#59
Diethylphthalate
Concen: 32.035 ng/ul
RT: 15.516 min Scan# 2096
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:149 Resp: 1119371
Ion Ratio Lower Upper
149 100
177 22.5 18.5 27.7
150 11.6 9.5 14.3

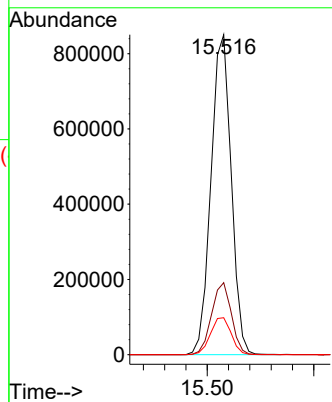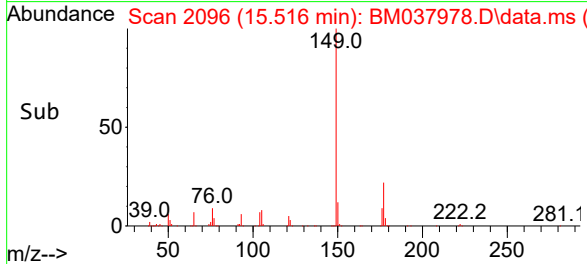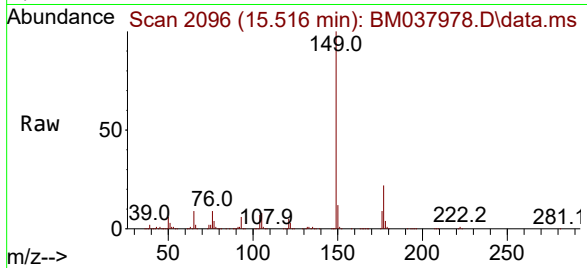

#61
Fluorene
Concen: 31.477 ng/ul
RT: 15.751 min Scan# 2136
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:166 Resp: 1158159
Ion Ratio Lower Upper
166 100
165 99.2 77.2 115.8
167 13.5 10.4 15.6



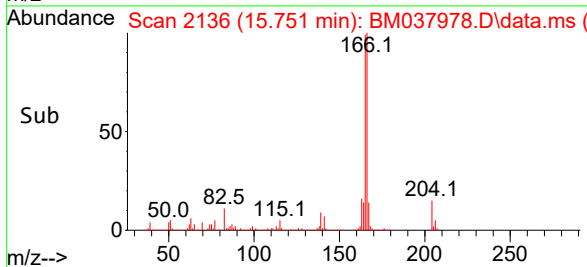
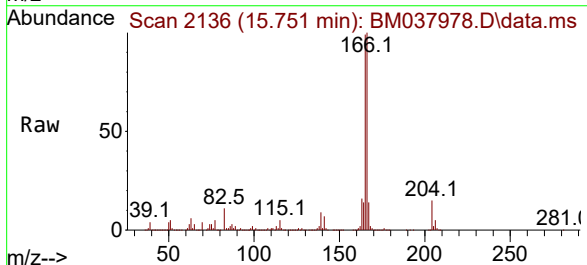




#62
4-Chlorophenyl-phenylether
Concen: 32.427 ng/ul
RT: 15.739 min Scan# 2134
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:204 Resp: 583077
Ion Ratio Lower Upper
204 100
206 32.8 25.5 38.3
141 55.5 42.8 64.2

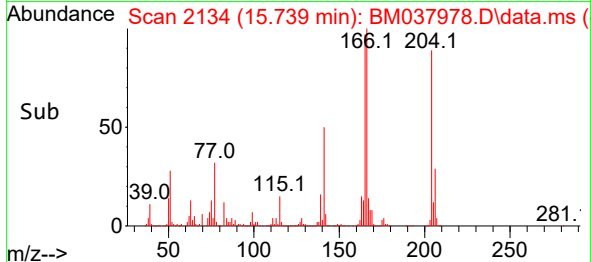

#63
4-Nitroaniline
Concen: 32.772 ng/ul
RT: 15.774 min Scan# 2140
Delta R.T. -0.000 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:138 Resp: 201991
Ion Ratio Lower Upper
138 100
92 45.7 36.1 54.1
108 73.3 51.6 77.4




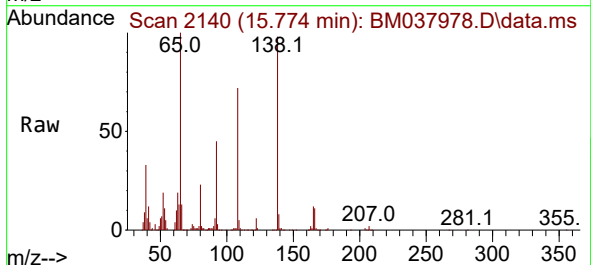




#66
4,6-Dinitro-2-methylphenol
Concen: 27.784 ng/ul
RT: 15.827 min Scan# 2148
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:198 Resp: 136060
Ion Ratio Lower Upper
198 100
182 4.1 3.8 5.8
77 22.1 19.3 28.9

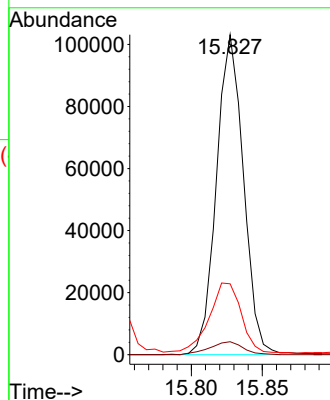

#67
N-Nitrosodiphenylamine
Concen: 32.301 ng/ul
RT: 15.951 min Scan# 2170
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:169 Resp: 921869
Ion Ratio Lower Upper
169 100
168 66.5 53.8 80.8
167 36.6 29.3 43.9



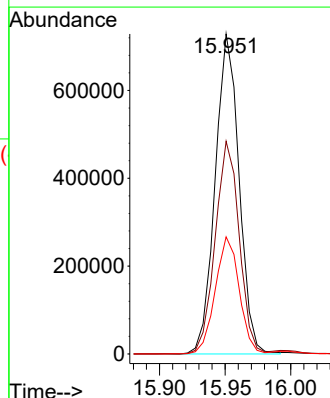





#68
4-Bromophenyl-phenylether
Concen: 32.916 ng/ul
RT: 16.633 min Scan# 2286
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:248 Resp: 341378
Ion Ratio Lower Upper
248 100
250 97.1 78.7 118.1
141 61.5 52.7 79.1



#69
Hexachlorobenzene
Concen: 33.121 ng/ul
RT: 16.751 min Scan# 2306
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:284 Resp: 410040
Ion Ratio Lower Upper
284 100
142 30.5 23.1 34.7
249 28.5 23.3 34.9





#70

Atrazine

Concen: 30.187 ng/ul

RT: 16.898 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:200 Resp: 294410

Ion Ratio Lower Upper

200 100

173 26.0 20.5 30.7

215 49.4 40.1 60.1

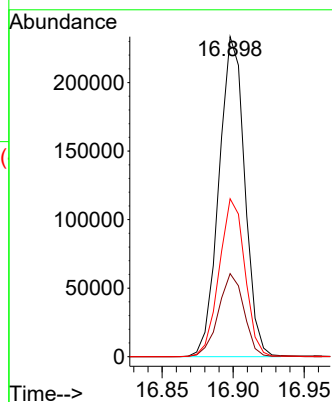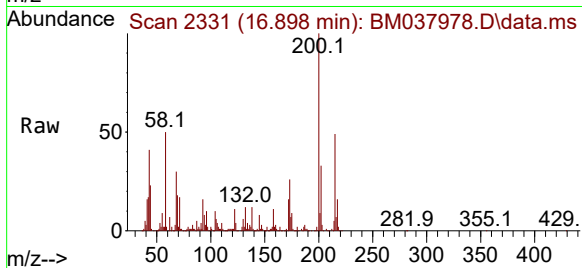

#71

Pentachlorophenol

Concen: 28.454 ng/ul

RT: 17.092 min Scan# 2364

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:266 Resp: 195851


Ion Ratio Lower Upper

266 100

264 64.8 50.1 75.1

268 65.6 50.6 75.8




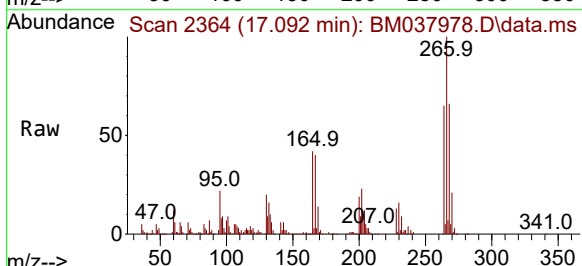




#72
Phenanthrene
Concen: 31.201 ng/ul
RT: 17.486 min Scan# 2431
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:178 Resp: 1612105
Ion Ratio Lower Upper
178 100
179 15.2 12.2 18.2
176 19.0 15.4 23.0



#74
Anthracene
Concen: 30.777 ng/ul
RT: 17.580 min Scan# 2447
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:178 Resp: 1616013
Ion Ratio Lower Upper
178 100
179 15.4 11.8 17.8
176 18.6 15.0 22.6





#75

1,2,3,4-Tetrachlorobenzene

Concen: 32.067 ng/uL

RT: 13.510 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:216 Resp: 490484

Ion Ratio Lower Upper

216 100

214 76.7 62.6 93.8

218 46.7 38.3 57.5



#76

Pentachlorobenzene

Concen: 32.267 ng/uL

RT: 15.021 min Scan# 2012

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:250 Resp: 488897


Ion Ratio Lower Upper

250 100

248 60.8 51.0 76.4

252 61.9 51.8 77.6









#77
 Carbazole
 Concen: 29.208 ng/ul
 RT: 17.851 min Scan# 2493
 Delta R.T. -0.006 min
 Lab File: BM037978.D
 Acq: 12 Dec 2022 22:31




Instrument :
 BNA_M
 ClientSampleId :
 SLCS528


Tgt Ion:167 Resp: 1328690
 Ion Ratio Lower Upper
 167 100
 166 20.9 16.7 25.1
 139 12.6 9.8 14.6

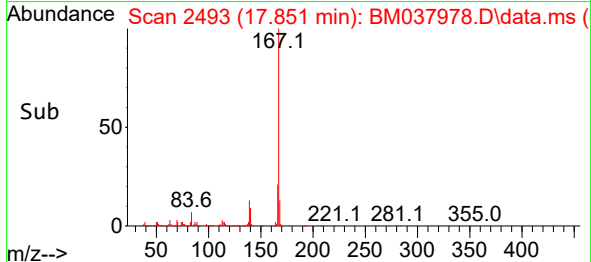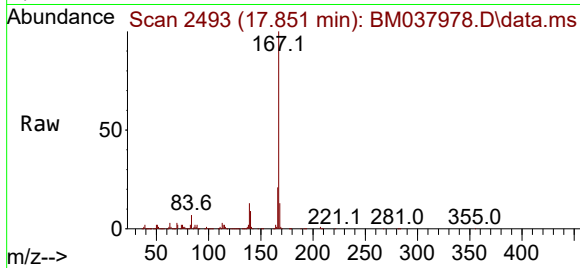

#78
 Di-n-butylphthalate
 Concen: 33.100 ng/ul
 RT: 18.398 min Scan# 2586
 Delta R.T. -0.006 min
 Lab File: BM037978.D
 Acq: 12 Dec 2022 22:31

Tgt Ion:149 Resp: 1789831
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.3 10.9
 104 4.9 3.4 5.2

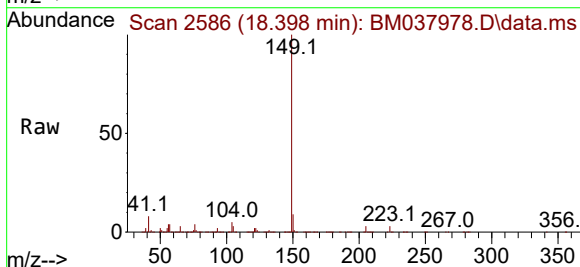



#80

Fluoranthene

Concen: 30.679 ng/ul

RT: 19.492 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:202 Resp: 1648090

Ion Ratio Lower Upper

202 100

101 10.0 8.6 13.0

100 7.8 6.6 10.0



#82

Pyrene

Concen: 30.695 ng/ul

RT: 19.856 min Scan# 2834

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:202 Resp: 1716135


Ion Ratio Lower Upper

202 100

101 11.4 10.0 15.0

100 9.8 7.9 11.9









#83
Butylbenzylphthalate
Concen: 29.897 ng/ul
RT: 20.733 min Scan# 2983
Delta R.T. -0.012 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31




Instrument :
BNA_M
ClientSampleId :
SLCS528


Tgt Ion:149 Resp: 621537
Ion Ratio Lower Upper
149 100
91 69.2 54.5 81.7
206 19.8 15.8 23.8

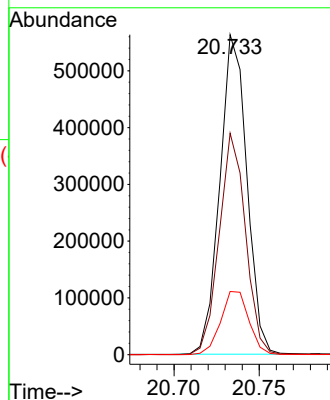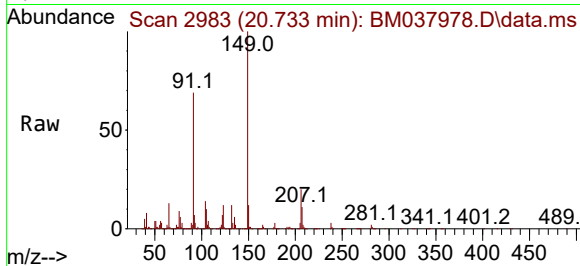

#84
3,3'-Dichlorobenzidine
Concen: 30.039 ng/ul
RT: 21.527 min Scan# 3118
Delta R.T. -0.006 min
Lab File: BM037978.D
Acq: 12 Dec 2022 22:31

Tgt Ion:252 Resp: 450422
Ion Ratio Lower Upper
252 100
254 64.6 53.2 79.8
126 10.1 7.8 11.8

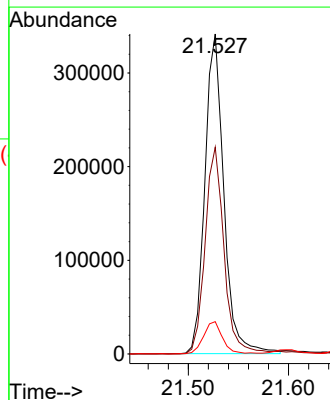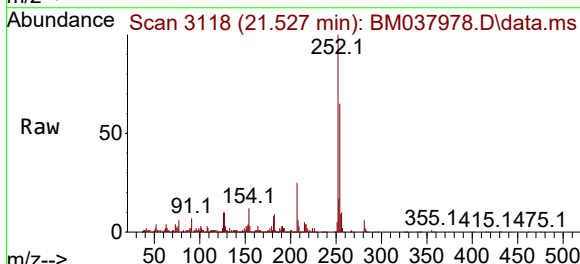



#85

Benzo(a)anthracene

Concen: 31.486 ng/ul

RT: 21.597 min Scan# 31

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:228 Resp: 1606260

Ion Ratio Lower Upper

228 100

229 19.8 15.5 23.3

226 27.1 21.8 32.8

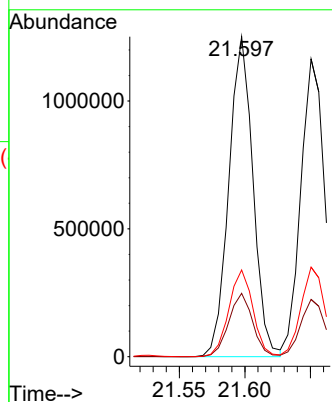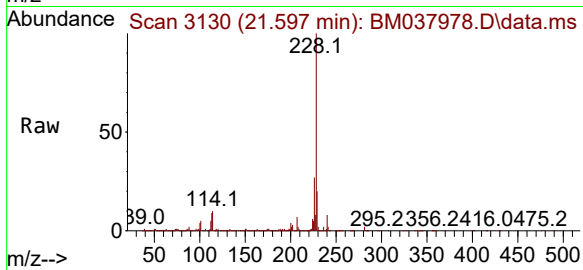

#86

Bis(2-ethylhexyl)phthalate

Concen: 29.833 ng/ul

RT: 21.503 min Scan# 3114

Delta R.T. -0.006 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:149 Resp: 902264


Ion Ratio Lower Upper

149 100

167 27.5 21.5 32.3

279 4.0 3.2 4.8

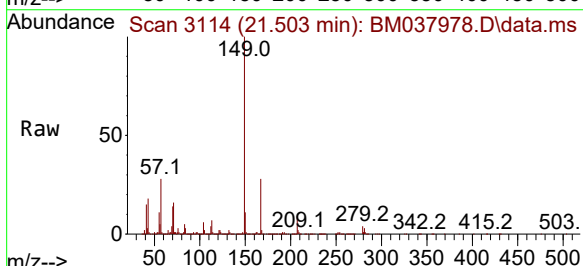



#87

Chrysene

Concen: 30.930 ng/ul

RT: 21.650 min Scan# 31

Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:228 Resp: 1480446

Ion Ratio Lower Upper

228 100

226 30.1 24.3 36.5

229 19.3 15.6 23.4

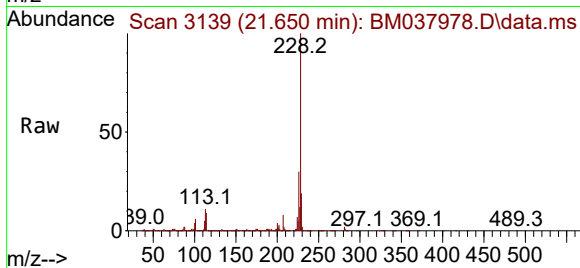

#89

Di-n-octyl phthalate

Concen: 28.863 ng/ul




RT: 22.450 min Scan# 3275


Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Tgt Ion:149 Resp: 1477201

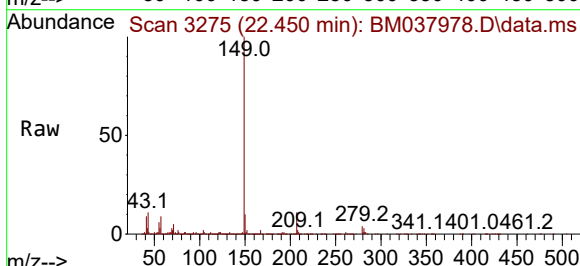

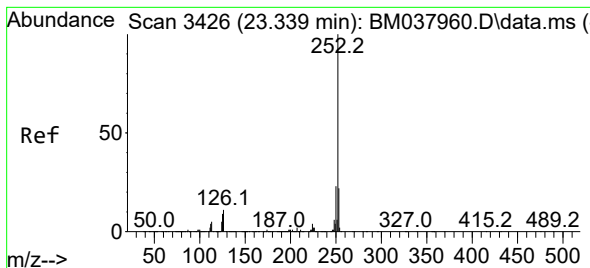

#90

Benzo(b)fluoranthene

Concen: 31.728 ng/ul

RT: 23.333 min Scan# 3426

Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:252 Resp: 1571104

Ion Ratio Lower Upper

252 100

253 21.9 17.6 26.4

125 9.7 8.0 12.0

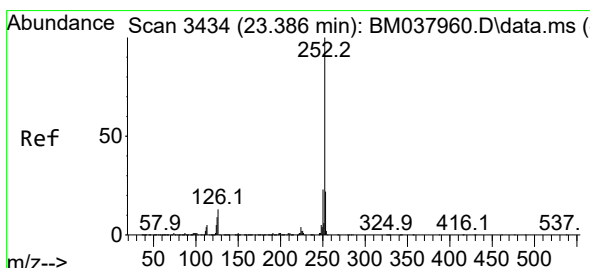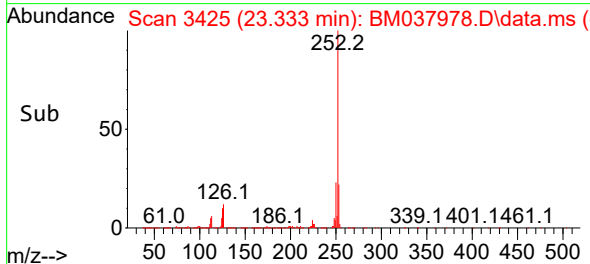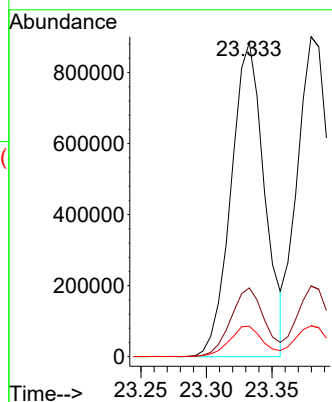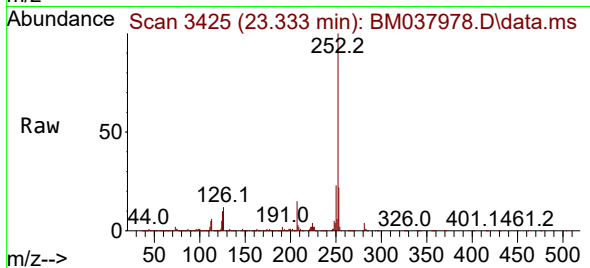

#91

Benzo(k)fluoranthene

Concen: 32.532 ng/ul

RT: 23.380 min Scan# 3433

Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:252 Resp: 1561230


Ion Ratio Lower Upper

252 100

253 22.1 17.4 26.2

125 9.7 8.1 12.1

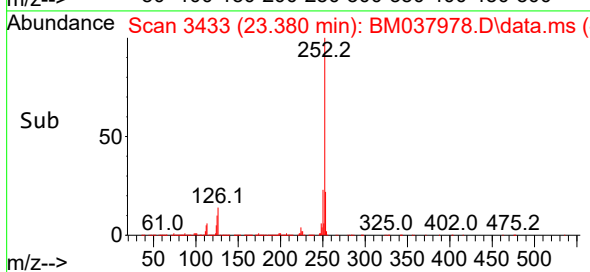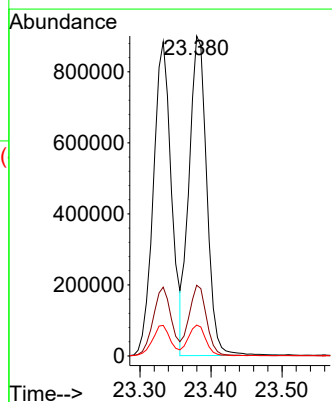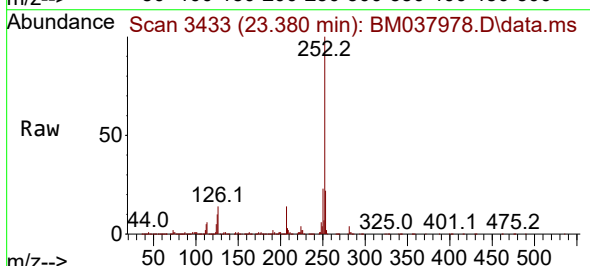



#93

Benzo(a)pyrene

Concen: 31.602 ng/ul

RT: 23.980 min Scan# 3

Delta R.T. -0.012 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:252 Resp: 1376129

Ion Ratio Lower Upper

252 100

253 21.9 17.4 26.0

125 10.9 9.4 14.0

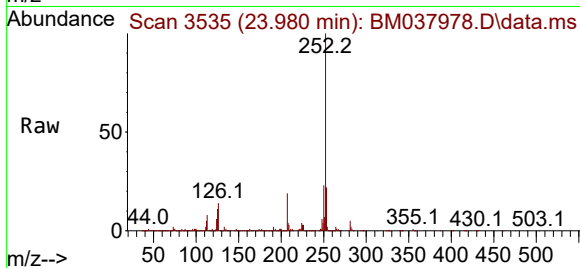

#94

Indeno(1,2,3-cd)pyrene

Concen: 27.482 ng/ul

RT: 26.685 min Scan# 3995

Delta R.T. -0.018 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31




Tgt Ion:276 Resp: 1541214


Ion Ratio Lower Upper

276 100

138 22.0 19.3 28.9

277 25.3 19.8 29.8

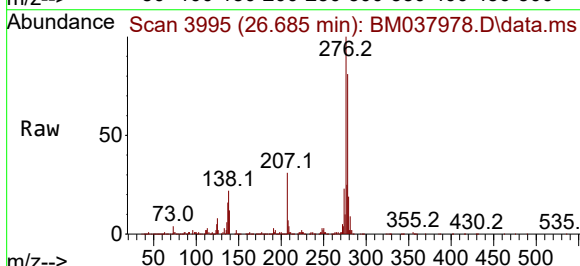



#95

Dibenzo(a,h)anthracene

Concen: 29.414 ng/ul

RT: 26.697 min Scan# 3999

Delta R.T. -0.018 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Instrument :

BNA_M

ClientSampleId :

SLCS528





Tgt Ion:278 Resp: 1390623

Ion Ratio Lower Upper

278 100

139 14.7 12.4 18.6

279 24.3 19.8 29.6



#96

Benzo(g,h,i)perylene

Concen: 28.509 ng/ul

RT: 27.485 min Scan# 4131

Delta R.T. -0.018 min

Lab File: BM037978.D

Acq: 12 Dec 2022 22:31

Tgt Ion:276 Resp: 1276511

Ion Ratio Lower Upper

276 100

138 20.4 17.1 25.7

277 24.7 18.2 27.4

