

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037980.D
 Acq On : 12 Dec 2022 23:45
 Operator : CG/JU
 Sample : SSTDCC020
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076

Quant Time: Dec 13 01:00:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	230458	20.000	ng/u1	0.00
20) Naphthalene-d8	10.892	136	980372	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.704	164	596052	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1120309	20.000	ng/u1	0.00
79) Chrysene-d12	21.615	240	818987	20.000	ng/u1	0.00
88) Perylene-d12	24.091	264	852665	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	36598	7.211	ng/uL	0.00
4) Pyridine-d5	3.852	84	281407	18.690	ng/u1	0.00
7) Phenol-d5	7.228	99	350372	18.709	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	210011	18.417	ng/u1	0.00
11) 2-Chlorophenol-d4	7.598	132	299071	19.468	ng/u1	-0.01
15) 4-Methylphenol-d8	8.786	113	280428	19.183	ng/u1	0.00
21) Nitrobenzene-d5	9.245	128	149570	19.269	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.969	143	160911	19.781	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.510	165	312361	20.217	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.033	131	394011	18.474	ng/u1	0.00
46) Dimethylphthalate-d6	14.110	166	841394	19.800	ng/u1	-0.01
49) Acenaphthylene-d8	14.398	160	1004565	19.342	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.898	143	107423	14.833	ng/u1	0.00
60) Fluorene-d10	15.692	176	734826	19.409	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	93758	15.653	ng/u1	0.00
73) Anthracene-d10	17.539	188	1005017	19.222	ng/u1	-0.01
81) Pyrene-d10	19.827	212	977649	19.872	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.927	264	851469	19.993	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.452	88	37269	7.000	ng/uL	95
5) Pyridine	3.869	79	280101	18.511	ng/u1	96
6) Benzaldehyde	7.204	77	129981	18.557	ng/u1	97
8) Phenol	7.257	94	350289	18.650	ng/u1	95
10) Bis(2-Chloroethyl)ether	7.492	93	279987	18.154	ng/u1	98
12) 2-Chlorophenol	7.634	128	305920	19.471	ng/u1	98
13) 2-Methylphenol	8.516	108	270322	18.807	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.610	45	498713	17.908	ng/u1	99
16) Acetophenone	8.904	105	446594	19.425	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.892	70	214335	19.790	ng/u1	98
18) 4-Methylphenol	8.845	108	293136	18.853	ng/u1	96
19) Hexachloroethane	9.157	117	119198	18.977	ng/u1	96
22) Nitrobenzene	9.292	77	327754	19.624	ng/u1	98
23) Isophorone	9.816	82	584402	19.095	ng/u1	98
25) 2-Nitrophenol	10.004	139	168563	19.766	ng/u1	95
26) 2,4-Dimethylphenol	10.057	107	327528	19.860	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.298	93	382594	18.806	ng/u1	99
29) 2,4-Dichlorophenol	10.539	162	298232	19.674	ng/u1	98
30) Naphthalene	10.945	128	1021396	19.306	ng/u1	99
32) 4-Chloroaniline	11.057	127	392344	18.448	ng/u1	99
33) Hexachlorobutadiene	11.222	225	201657	20.222	ng/u1	99
34) Caprolactam	11.845	113	75163	19.330	ng/u1	90
35) 4-Chloro-3-methylphenol	12.169	107	277706	20.126	ng/u1	96
36) 2-Methylnaphthalene	12.539	142	681642	19.864	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037980.D
 Acq On : 12 Dec 2022 23:45
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076

Quant Time: Dec 13 01:00:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.763	142	699729	19.942	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.904	216	376523	19.333	ng/ul	100
40) Hexachlorocyclopentadiene	12.880	237	101081	9.073	ng/ul	99
41) 2,4,6-Trichlorophenol	13.145	196	233448	19.679	ng/ul	97
42) 2,4,5-Trichlorophenol	13.216	196	243357	19.670	ng/ul	99
43) 1,1'-Biphenyl	13.539	154	918852	19.178	ng/ul	100
44) 2-Chloronaphthalene	13.586	162	711494	19.250	ng/ul	99
45) 2-Nitroaniline	13.792	65	174554	19.601	ng/ul	97
47) Dimethylphthalate	14.157	163	834350	19.901	ng/ul	100
48) 2,6-Dinitrotoluene	14.280	165	165745	20.352	ng/ul	95
50) Acenaphthylene	14.427	152	1113260	19.494	ng/ul	100
51) 3-Nitroaniline	14.610	138	137099	16.873	ng/ul	98
52) Acenaphthene	14.768	153	763919	19.340	ng/ul	98
53) 2,4-Dinitrophenol	14.815	184	50630	12.670	ng/ul	91
55) 4-Nitrophenol	14.910	109	81921	17.153	ng/ul	98
56) Dibenzofuran	15.098	168	1050468	19.479	ng/ul	99
57) 2,4-Dinitrotoluene	15.063	165	215422	19.533	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.321	232	203600	19.564	ng/ul	98
59) Diethylphthalate	15.510	149	833743	19.962	ng/ul	99
61) Fluorene	15.745	166	864356	19.653	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.733	204	435515	20.263	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.827	198	89877	15.500	ng/ul#	96
67) N-Nitrosodiphenylamine	15.951	169	679163	20.097	ng/ul	99
68) 4-Bromophenyl-phenylether	16.627	248	250310	20.382	ng/ul	96
69) Hexachlorobenzene	16.745	284	298933	20.392	ng/ul	93
70) Atrazine	16.898	200	224307	19.423	ng/ul	100
71) Pentachlorophenol	17.092	266	139897	17.165	ng/ul	98
72) Phenanthrene	17.486	178	1169264	19.112	ng/ul	99
74) Anthracene	17.574	178	1197119	19.254	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.510	216	368006	20.319	ng/uL	97
76) Pentachlorobenzene	15.015	250	374714	20.886	ng/uL	97
77) Carbazole	17.845	167	949763	17.632	ng/ul	100
78) Di-n-butylphthalate	18.398	149	1308103	20.430	ng/ul	99
80) Fluoranthene	19.492	202	1152658	19.852	ng/ul	99
82) Pyrene	19.850	202	1195892	19.791	ng/ul	99
83) Butylbenzylphthalate	20.733	149	430627	19.165	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.527	252	285631	17.625	ng/ul	98
85) Benzo(a)anthracene	21.597	228	1079392	19.577	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.503	149	664046	20.315	ng/ul	99
87) Chrysene	21.650	228	1008693	19.498	ng/ul	99
89) Di-n-octyl phthalate	22.450	149	1020021	18.670	ng/ul	100
90) Benzo(b)fluoranthene	23.327	252	1072282	20.285	ng/ul	100
91) Benzo(k)fluoranthene	23.380	252	1040669	20.313	ng/ul	98
93) Benzo(a)pyrene	23.980	252	922219	19.839	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.685	276	1126953	18.824	ng/ul	98
95) Dibenzo(a,h)anthracene	26.697	278	953164	18.886	ng/ul	98
96) Benzo(g,h,i)perylene	27.479	276	921865	19.286	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037980.D
 Acq On : 12 Dec 2022 23:45
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076

Quant Time: Dec 13 01:00:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration









#2
1,4-Dioxane
Concen: 7.000 ng/uL
RT: 3.452 min Scan# 41
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion: 88 Resp: 37269
Ion Ratio Lower Upper
88 100
43 41.0 32.8 49.2
58 87.4 64.6 97.0



#5
Pyridine
Concen: 18.511 ng/uL
RT: 3.869 min Scan# 116
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion: 79 Resp: 280101
Ion Ratio Lower Upper
79 100
52 101.4 78.1 117.1
51 49.4 37.2 55.8









#6
Benzaldehyde
Concen: 18.557 ng/ul
RT: 7.204 min Scan# 684
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion: 77 Resp: 129981
Ion Ratio Lower Upper
77 100
105 103.5 82.5 123.7
106 96.7 81.8 122.6



#8
Phenol
Concen: 18.650 ng/ul
RT: 7.257 min Scan# 692
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion: 94 Resp: 350289
Ion Ratio Lower Upper
94 100
65 29.5 22.2 33.4
66 38.0 27.3 40.9









#10
Bis(2-Chloroethyl)ether
Concen: 18.154 ng/ul
RT: 7.492 min Scan# 71
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion: 93 Resp: 279987
Ion Ratio Lower Upper
93 100
63 84.2 66.3 99.5
95 34.2 25.7 38.5



#12
2-Chlorophenol
Concen: 19.471 ng/ul
RT: 7.634 min Scan# 756
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:128 Resp: 305920
Ion Ratio Lower Upper
128 100
64 45.0 35.2 52.8
130 33.4 25.9 38.9





#13

2-Methylphenol

Concen: 18.807 ng/ul

RT: 8.516 min Scan# 906

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :





SSTD020076

Tgt Ion:108 Resp: 270322

Ion Ratio Lower Upper

108 100

107 91.2 71.9 107.9



#14

2,2'-oxybis(1-Chloropropane)

Concen: 17.908 ng/ul

RT: 8.610 min Scan# 922

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion: 45 Resp: 498713


Ion Ratio Lower Upper

45 100

77 10.8 9.0 13.4

79 8.5 6.2 9.4









#16
Acetophenone
Concen: 19.425 ng/ul
RT: 8.904 min Scan# 91
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:105 Resp: 446594
Ion Ratio Lower Upper
105 100
77 76.3 59.7 89.5
51 34.1 27.2 40.8



#17
N-Nitroso-di-n-propylamine
Concen: 19.790 ng/ul
RT: 8.892 min Scan# 970
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion: 70 Resp: 214335
Ion Ratio Lower Upper
70 100
42 80.2 62.3 93.5
101 10.8 8.0 12.0
130 22.1 17.6 26.4









#18
4-Methylphenol
Concen: 18.853 ng/ul
RT: 8.845 min Scan# 90
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:108 Resp: 293136
Ion Ratio Lower Upper
108 100
107 114.2 88.1 132.1



#19
Hexachloroethane
Concen: 18.977 ng/ul
RT: 9.157 min Scan# 1015
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:117 Resp: 119198
Ion Ratio Lower Upper
117 100
201 103.0 87.3 130.9
199 62.5 50.9 76.3







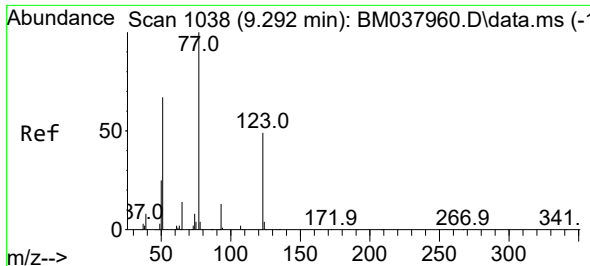

#22
Nitrobenzene
Concen: 19.624 ng/ul
RT: 9.292 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion: 77 Resp: 327754
Ion Ratio Lower Upper
77 100
123 48.8 37.8 56.6
65 14.1 11.1 16.7



#23
Isophorone
Concen: 19.095 ng/ul
RT: 9.816 min Scan# 1127
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion: 82 Resp: 584402
Ion Ratio Lower Upper
82 100
95 7.3 5.2 7.8
138 19.2 14.9 22.3







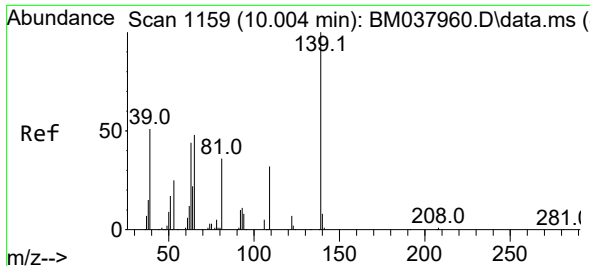

#25
2-Nitrophenol
Concen: 19.766 ng/ul
RT: 10.004 min Scan# 1159
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:139 Resp: 168563
Ion Ratio Lower Upper
139 100
65 47.9 36.2 54.4
109 28.4 19.7 29.5

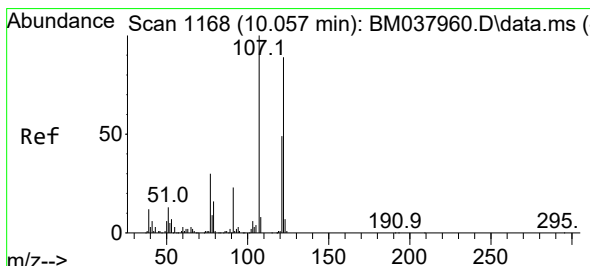

#26
2,4-Dimethylphenol
Concen: 19.860 ng/ul
RT: 10.057 min Scan# 1168
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:107 Resp: 327528
Ion Ratio Lower Upper
107 100
121 49.0 42.0 63.0
122 89.3 71.4 107.2









#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.806 ng/ul
 RT: 10.298 min Scan# 1209
 Delta R.T. -0.006 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076


Tgt Ion: 93 Resp: 382594
 Ion Ratio Lower Upper
 93 100
 95 32.6 25.5 38.3
 123 12.0 9.4 14.2



#29
 2,4-Dichlorophenol
 Concen: 19.674 ng/ul
 RT: 10.539 min Scan# 1250
 Delta R.T. -0.006 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45

Tgt Ion:162 Resp: 298232
 Ion Ratio Lower Upper
 162 100
 164 66.0 51.4 77.2
 98 32.8 26.1 39.1









#30
Naphthalene
Concen: 19.306 ng/ul
RT: 10.945 min Scan# 1319
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:128 Resp: 1021396
Ion Ratio Lower Upper
128 100
129 10.7 9.0 13.4
127 12.9 10.4 15.6



#32
4-Chloroaniline
Concen: 18.448 ng/ul
RT: 11.057 min Scan# 1338
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:127 Resp: 392344
Ion Ratio Lower Upper
127 100
129 31.3 25.3 37.9









#33
Hexachlorobutadiene
Concen: 20.222 ng/ul
RT: 11.222 min Scan# 11
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:225 Resp: 201657
Ion Ratio Lower Upper
225 100
223 63.3 50.8 76.2
227 64.3 50.5 75.7



#34
Caprolactam
Concen: 19.330 ng/ul
RT: 11.845 min Scan# 1472
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:113 Resp: 75163
Ion Ratio Lower Upper
113 100
55 194.1 172.2 258.2
56 144.1 120.7 181.1









#35
4-Chloro-3-methylphenol
Concen: 20.126 ng/ul
RT: 12.169 min Scan# 1527
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:107 Resp: 277706
Ion Ratio Lower Upper
107 100
144 27.0 23.4 35.0
142 85.1 71.0 106.4



#36
2-Methylnaphthalene
Concen: 19.864 ng/ul
RT: 12.539 min Scan# 1590
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:142 Resp: 681642
Ion Ratio Lower Upper
142 100
141 89.0 69.4 104.0





#37

1-Methylnaphthalene

Concen: 19.942 ng/ul

RT: 12.763 min Scan# 1

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:142 Resp: 699729

Ion Ratio Lower Upper

142 100

141 90.5 72.4 108.6

116 3.4 2.9 4.3



#39

1,2,4,5-Tetrachlorobenzene

Concen: 19.333 ng/ul

RT: 12.904 min Scan# 1652

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Tgt Ion:216 Resp: 376523




Ion Ratio Lower Upper


216 100

214 80.6 64.2 96.4

179 19.1 15.4 23.2

108 15.9 12.7 19.1









#40
Hexachlorocyclopentadiene
Concen: 9.073 ng/ul
RT: 12.880 min Scan# 1648
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:237 Resp: 101081
Ion Ratio Lower Upper
237 100
235 62.6 50.4 75.6
272 13.0 10.6 16.0



#41
2,4,6-Trichlorophenol
Concen: 19.679 ng/ul
RT: 13.145 min Scan# 1693
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:196 Resp: 233448
Ion Ratio Lower Upper
196 100
198 97.2 75.0 112.6
200 31.1 24.5 36.7









#42
2,4,5-Trichlorophenol
Concen: 19.670 ng/ul
RT: 13.216 min Scan# 1705
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:196 Resp: 243357
Ion Ratio Lower Upper
196 100
198 95.1 76.5 114.7
200 30.3 24.9 37.3



#43
1,1'-Biphenyl
Concen: 19.178 ng/ul
RT: 13.539 min Scan# 1760
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:154 Resp: 918852
Ion Ratio Lower Upper
154 100
153 38.9 31.2 46.8
76 11.7 9.3 13.9









#44
2-Chloronaphthalene
Concen: 19.250 ng/ul
RT: 13.586 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:162 Resp: 711494
Ion Ratio Lower Upper
162 100
164 32.8 27.3 40.9
127 37.1 29.4 44.0



#45
2-Nitroaniline
Concen: 19.601 ng/ul
RT: 13.792 min Scan# 1803
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion: 65 Resp: 174554
Ion Ratio Lower Upper
65 100
92 67.4 53.5 80.3
138 118.5 91.3 136.9









#47
Dimethylphthalate
Concen: 19.901 ng/ul
RT: 14.157 min Scan# 1865
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:163 Resp: 834350
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 10.2 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 20.352 ng/ul
RT: 14.280 min Scan# 1886
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:165 Resp: 165745
Ion Ratio Lower Upper
165 100
89 56.5 41.1 61.7
121 21.9 17.4 26.2









#50
Acenaphthylene
Concen: 19.494 ng/ul
RT: 14.427 min Scan# 1911
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:152 Resp: 1113260
Ion Ratio Lower Upper
152 100
151 19.2 15.3 22.9
153 12.8 10.2 15.4



#51
3-Nitroaniline
Concen: 16.873 ng/ul
RT: 14.610 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:138 Resp: 137099
Ion Ratio Lower Upper
138 100
108 10.1 7.9 11.9
92 106.3 83.4 125.0









#52
Acenaphthene
Concen: 19.340 ng/ul
RT: 14.768 min Scan# 1969
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:153 Resp: 763919
Ion Ratio Lower Upper
153 100
152 46.6 38.2 57.4
154 87.5 71.4 107.0



#53
2,4-Dinitrophenol
Concen: 12.670 ng/ul
RT: 14.815 min Scan# 1977
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:184 Resp: 50630
Ion Ratio Lower Upper
184 100
63 67.3 46.2 69.4
154 61.2 45.5 68.3









#55
4-Nitrophenol
Concen: 17.153 ng/ul
RT: 14.910 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:109 Resp: 81921
Ion Ratio Lower Upper
109 100
139 147.1 119.2 178.8
65 139.2 108.7 163.1



#56
Dibenzofuran
Concen: 19.479 ng/ul
RT: 15.098 min Scan# 2025
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:168 Resp: 1050468
Ion Ratio Lower Upper
168 100
139 35.8 28.1 42.1









#57
2,4-Dinitrotoluene
Concen: 19.533 ng/ul
RT: 15.063 min Scan# 2019
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:165 Resp: 215422
Ion Ratio Lower Upper
165 100
63 46.0 34.9 52.3
182 2.6 2.2 3.2



#58
2,3,4,6-Tetrachlorophenol
Concen: 19.564 ng/ul
RT: 15.321 min Scan# 2063
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:232 Resp: 203600
Ion Ratio Lower Upper
232 100
131 43.1 32.8 49.2
130 2.2 2.0 3.0
166 29.0 23.2 34.8





#59

Diethylphthalate

Concen: 19.962 ng/ul

RT: 15.510 min Scan# 2095

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:149 Resp: 833743

Ion Ratio Lower Upper

149 100

177 22.3 18.5 27.7

150 11.8 9.5 14.3



#61

Fluorene

Concen: 19.653 ng/ul

RT: 15.745 min Scan# 2135

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:166 Resp: 864356


Ion Ratio Lower Upper

166 100

165 96.8 77.2 115.8

167 13.5 10.4 15.6









#62
4-Chlorophenyl-phenylether
Concen: 20.263 ng/ul
RT: 15.733 min Scan# 2133
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:204 Resp: 435515
Ion Ratio Lower Upper
204 100
206 32.2 25.5 38.3
141 56.5 42.8 64.2



#66
4,6-Dinitro-2-methylphenol
Concen: 15.500 ng/ul
RT: 15.827 min Scan# 2149
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:198 Resp: 89877
Ion Ratio Lower Upper
198 100
182 3.6 3.8 5.8#
77 22.2 19.3 28.9





#67

N-Nitrosodiphenylamine

Concen: 20.097 ng/ul

RT: 15.951 min Scan# 2170

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:169 Resp: 679163

Ion Ratio Lower Upper

169 100

168 66.8 53.8 80.8

167 36.4 29.3 43.9



#68

4-Bromophenyl-phenylether

Concen: 20.382 ng/ul

RT: 16.627 min Scan# 2285

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:248 Resp: 250310


Ion Ratio Lower Upper

248 100

250 101.2 78.7 118.1

141 71.2 52.7 79.1









#69
Hexachlorobenzene
Concen: 20.392 ng/ul
RT: 16.745 min Scan# 21
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:284 Resp: 298933
Ion Ratio Lower Upper
284 100
142 34.5 23.1 34.7
249 30.9 23.3 34.9



#70
Atrazine
Concen: 19.423 ng/ul
RT: 16.898 min Scan# 2331
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:200 Resp: 224307
Ion Ratio Lower Upper
200 100
173 25.6 20.5 30.7
215 49.9 40.1 60.1





#71

Pentachlorophenol

Concen: 17.165 ng/ul

RT: 17.092 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:266 Resp: 139897

Ion Ratio Lower Upper

266 100

264 59.7 50.1 75.1

268 63.4 50.6 75.8



#72

Phenanthrene

Concen: 19.112 ng/ul

RT: 17.486 min Scan# 2431

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:178 Resp: 1169264


Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.2

176 19.4 15.4 23.0





#74

Anthracene

Concen: 19.254 ng/uI

RT: 17.574 min Scan# 2447

Delta R.T. -0.012 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:178 Resp: 1197119

Ion Ratio Lower Upper

178 100

179 15.3 11.8 17.8

176 18.8 15.0 22.6



#75

1,2,3,4-Tetrachlorobenzene

Concen: 20.319 ng/uI

RT: 13.510 min Scan# 1755

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:216 Resp: 368006


Ion Ratio Lower Upper

216 100

214 80.9 62.6 93.8

218 49.5 38.3 57.5









#76
 Pentachlorobenzene
 Concen: 20.886 ng/uL
 RT: 15.015 min Scan# 2011
 Delta R.T. -0.012 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45




Instrument :
 BNA_M
 ClientSampleId :
 SST020076


Tgt Ion:250 Resp: 374714
 Ion Ratio Lower Upper
 250 100
 248 60.7 51.0 76.4
 252 63.3 51.8 77.6



#77
 Carbazole
 Concen: 17.632 ng/uL
 RT: 17.845 min Scan# 2492
 Delta R.T. -0.012 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45

Tgt Ion:167 Resp: 949763
 Ion Ratio Lower Upper
 167 100
 166 20.7 16.7 25.1
 139 12.4 9.8 14.6





#78

Di-n-butylphthalate

Concen: 20.430 ng/ul

RT: 18.398 min Scan# 2

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:149 Resp: 1308103

Ion Ratio Lower Upper

149 100

150 9.1 7.3 10.9

104 4.9 3.4 5.2



#80

Fluoranthene

Concen: 19.852 ng/ul

RT: 19.492 min Scan# 2772

Delta R.T. -0.006 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:202 Resp: 1152658


Ion Ratio Lower Upper

202 100

101 10.5 8.6 13.0

100 7.8 6.6 10.0









#82
 Pyrene
 Concen: 19.791 ng/ul
 RT: 19.850 min Scan# 2834
 Delta R.T. -0.012 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076


Tgt Ion:202 Resp: 1195892
 Ion Ratio Lower Upper
 202 100
 101 12.0 10.0 15.0
 100 9.9 7.9 11.9



#83
 Butylbenzylphthalate
 Concen: 19.165 ng/ul
 RT: 20.733 min Scan# 2983
 Delta R.T. -0.012 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45

Tgt Ion:149 Resp: 430627
 Ion Ratio Lower Upper
 149 100
 91 68.6 54.5 81.7
 206 21.0 15.8 23.8









#84
3,3'-Dichlorobenzidine
Concen: 17.625 ng/ul
RT: 21.527 min Scan# 3118
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:252 Resp: 285631
Ion Ratio Lower Upper
252 100
254 64.8 53.2 79.8
126 10.0 7.8 11.8



#85
Benzo(a)anthracene
Concen: 19.577 ng/ul
RT: 21.597 min Scan# 3130
Delta R.T. -0.006 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:228 Resp: 1079392
Ion Ratio Lower Upper
228 100
229 19.4 15.5 23.3
226 27.0 21.8 32.8









#86
 Bis(2-ethylhexyl)phthalate
 Concen: 20.315 ng/ul
 RT: 21.503 min Scan# 3115
 Delta R.T. -0.006 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076


Tgt Ion:149 Resp: 664046
 Ion Ratio Lower Upper
 149 100
 167 27.5 21.5 32.3
 279 4.4 3.2 4.8



#87
 Chrysene
 Concen: 19.498 ng/ul
 RT: 21.650 min Scan# 3139
 Delta R.T. -0.012 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45

Tgt Ion:228 Resp: 1008693
 Ion Ratio Lower Upper
 228 100
 226 29.3 24.3 36.5
 229 19.7 15.6 23.4









#89
Di-n-octyl phthalate
Concen: 18.670 ng/ul
RT: 22.450 min Scan# 31
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Instrument :
BNA_M
ClientSampleId :
SSTD020076




Tgt Ion:149 Resp: 1020021




#90
Benzo(b)fluoranthene
Concen: 20.285 ng/ul
RT: 23.327 min Scan# 3424
Delta R.T. -0.018 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:252 Resp: 1072282

Ion	Ratio	Lower	Upper
252	100		
253	22.0	17.6	26.4
125	9.9	8.0	12.0









#91
Benzo(k)fluoranthene
Concen: 20.313 ng/ul
RT: 23.380 min Scan# 34
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45




Instrument :
BNA_M
ClientSampleId :
SSTD020076


Tgt Ion:252 Resp: 1040669
Ion Ratio Lower Upper
252 100
253 21.0 17.4 26.2
125 9.3 8.1 12.1



#93
Benzo(a)pyrene
Concen: 19.839 ng/ul
RT: 23.980 min Scan# 3535
Delta R.T. -0.012 min
Lab File: BM037980.D
Acq: 12 Dec 2022 23:45

Tgt Ion:252 Resp: 922219
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.0
125 10.4 9.4 14.0





#94

Indeno(1,2,3-cd)pyrene

Concen: 18.824 ng/ul

RT: 26.685 min Scan# 3995

Delta R.T. -0.018 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45

Instrument :

BNA_M

ClientSampleId :

SSTD020076





Tgt Ion:276 Resp: 1126953

Ion Ratio Lower Upper

276 100

138 22.5 19.3 28.9

277 24.8 19.8 29.8



#95

Dibenzo(a,h)anthracene

Concen: 18.886 ng/ul

RT: 26.697 min Scan# 3997

Delta R.T. -0.018 min

Lab File: BM037980.D

Acq: 12 Dec 2022 23:45




Tgt Ion:278 Resp: 953164


Ion Ratio Lower Upper

278 100

139 14.0 12.4 18.6

279 23.8 19.8 29.6





#96
 Benzo(g,h,i)perylene
 Concen: 19.286 ng/ul
 RT: 27.479 min Scan# 41
 Delta R.T. -0.024 min
 Lab File: BM037980.D
 Acq: 12 Dec 2022 23:45

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020076

Tgt Ion:276 Resp: 921865
 Ion Ratio Lower Upper
 276 100
 138 20.1 17.1 25.7
 277 23.9 18.2 27.4

