




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037963.D
 Acq On : 12 Dec 2022 13:19
 Operator : CG/JU
 Sample : N5948-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ94

Manual IntegrationsAPPROVED

Quant Time: Dec 13 00:55:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/13/2022
 Supervised By :mohammad ahmed 12/14/2022

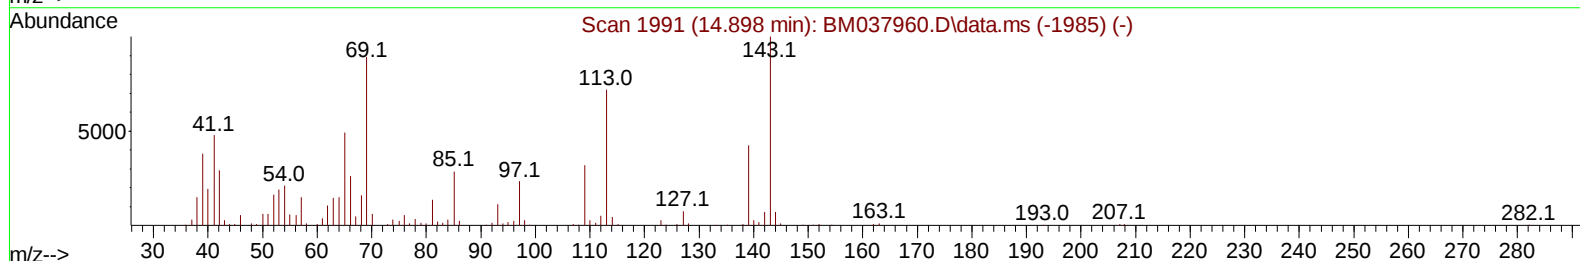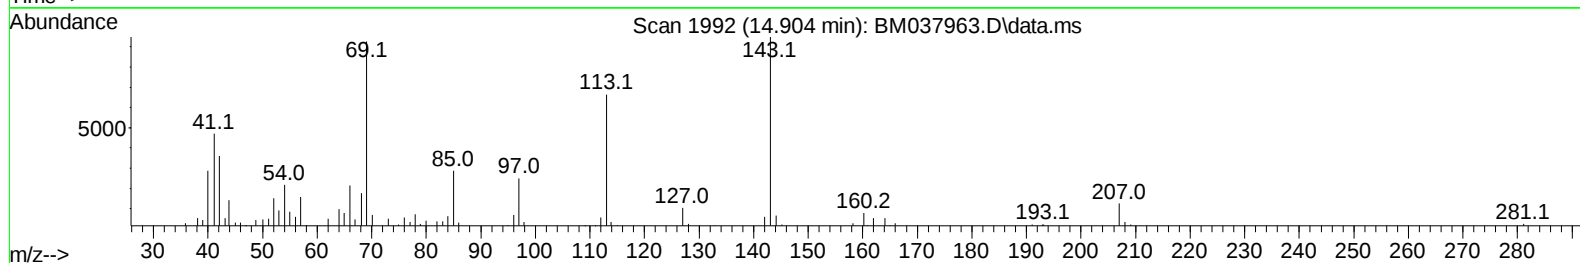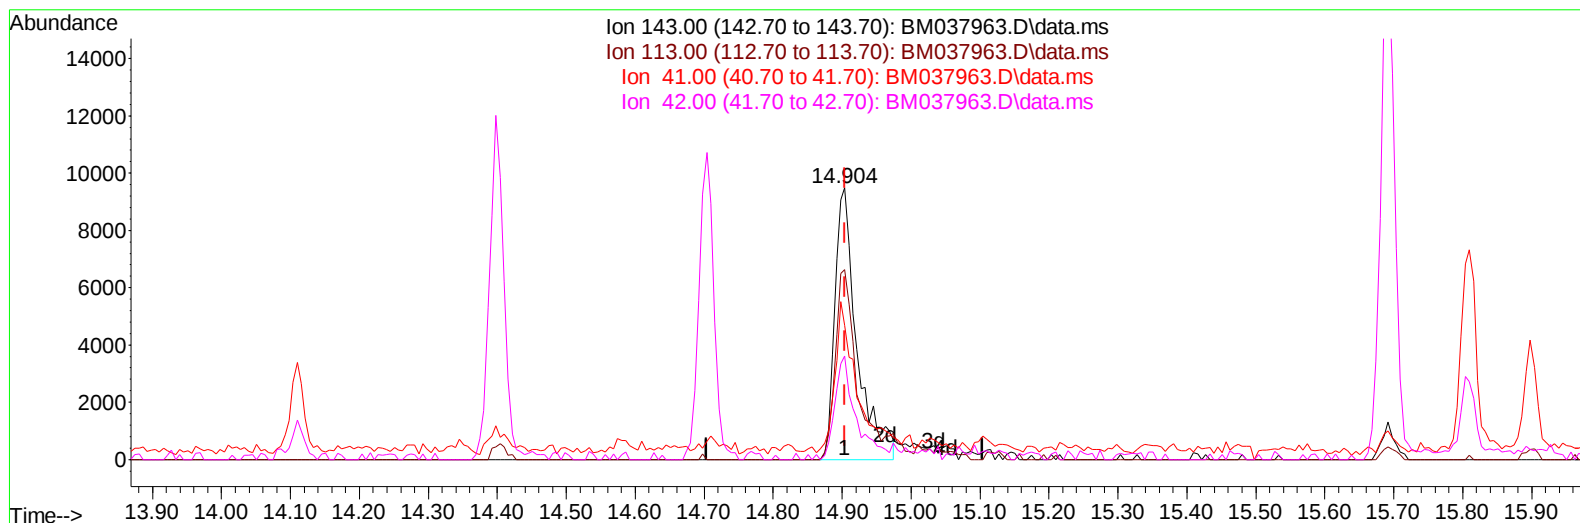

TIC: BM037963.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.904min (-0.000) 3.59 ng/ul m

response 21101

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	60.30	70.01
41.00	43.90	49.51
42.00	30.30	38.00#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037963.D
 Acq On : 12 Dec 2022 13:19
 Operator : CG/JU
 Sample : N5948-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ94

Manual IntegrationsAPPROVED

Quant Time: Dec 13 00:55:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/13/2022
 Supervised By :mohammad ahmed 12/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	208662	20.000	ng/ul	0.00
20) Naphthalene-d8	10.892	136	845429	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.704	164	483262	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	867340	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	693018	20.000	ng/ul	0.00
88) Perylene-d12	24.091	264	756938	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	17700	3.852	ng/uL	0.00
4) Pyridine-d5	3.863	84	55111	4.043	ng/ul	0.00
7) Phenol-d5	7.228	99	102543	6.048	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	280544	27.172	ng/ul	0.00
11) 2-Chlorophenol-d4	7.598	132	282377	20.301	ng/ul	-0.01
15) 4-Methylphenol-d8	8.781	113	174460	13.181	ng/ul	-0.01
21) Nitrobenzene-d5	9.245	128	202784	30.295	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.975	143	191066	27.238	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	312580	23.460	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.033	131	264180	14.364	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	1069362	31.038	ng/ul	-0.01
49) Acenaphthylene-d8	14.398	160	1258649	29.891	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.904	143	21101m	3.594	ng/ul	0.00
60) Fluorene-d10	15.692	176	915825	29.836	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	100537	21.681	ng/ul	0.00
73) Anthracene-d10	17.545	188	1343877	33.199	ng/ul	0.00
81) Pyrene-d10	19.827	212	1392261	33.444	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	1301124	34.414	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037963.D
Acq On : 12 Dec 2022 13:19
Operator : CG/JU
Sample : N5948-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ94

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

Quant Time: Dec 13 00:55:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

