




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Manual IntegrationsAPPROVED

Quant Time: Dec 13 00:58:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

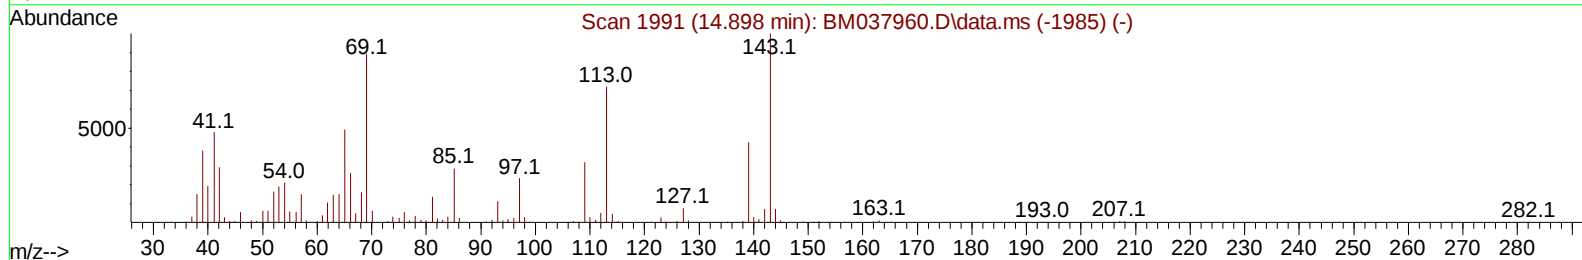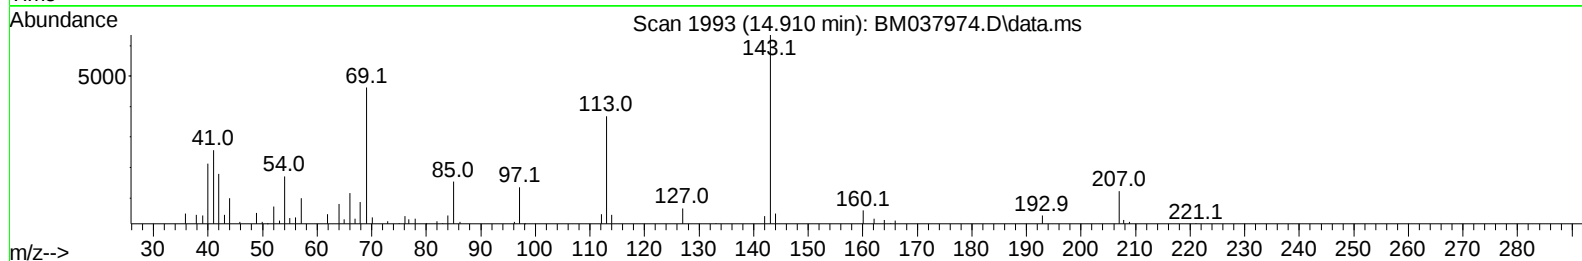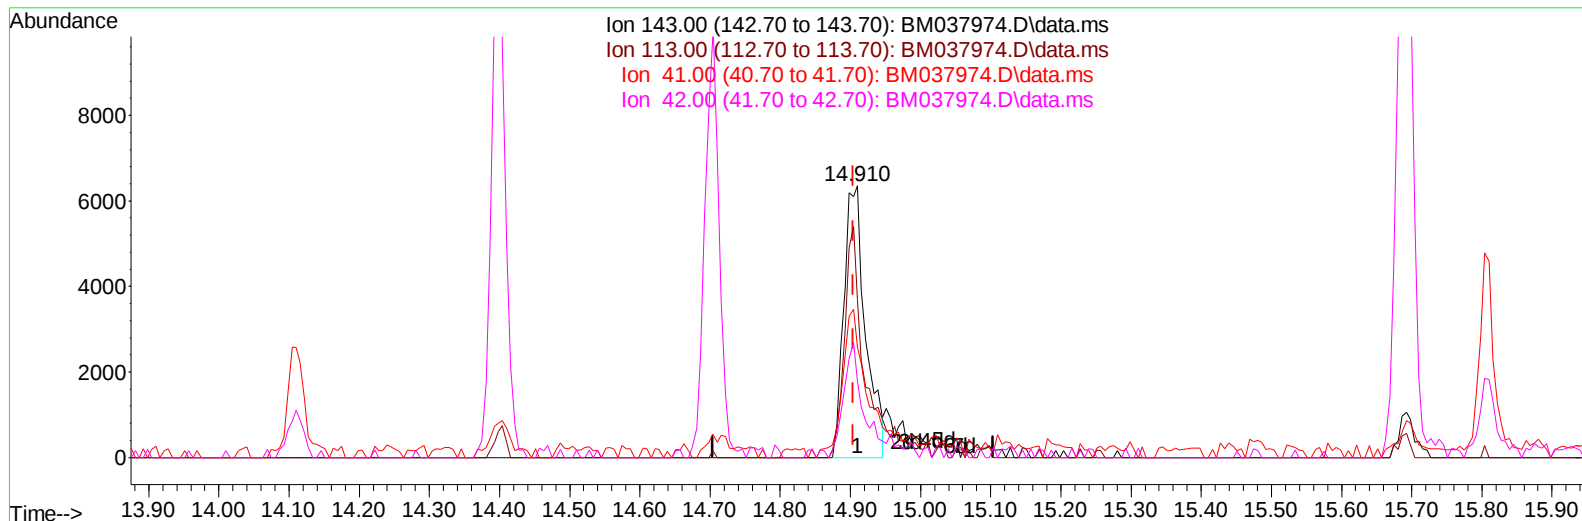

TIC: BM037974.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.006) 2.85 ng/u1

response 13683

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	60.30	58.14
41.00	43.90	40.60
42.00	30.30	28.28




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Manual IntegrationsAPPROVED

Quant Time: Dec 13 00:58:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

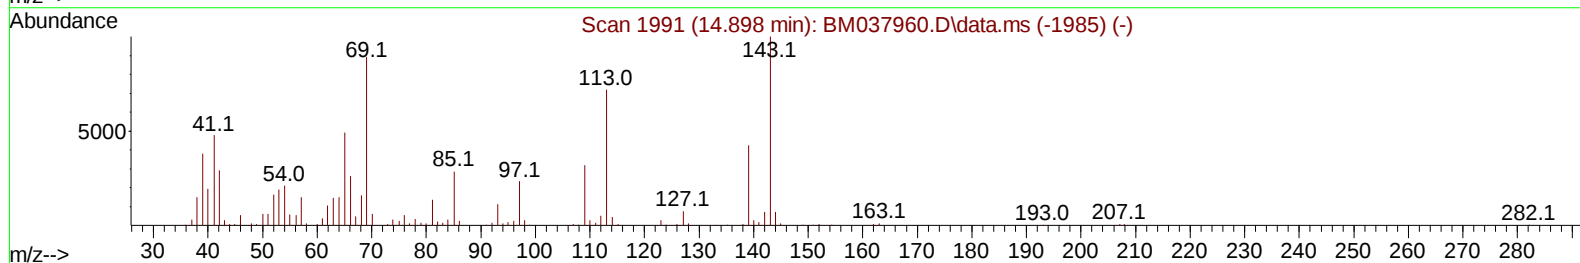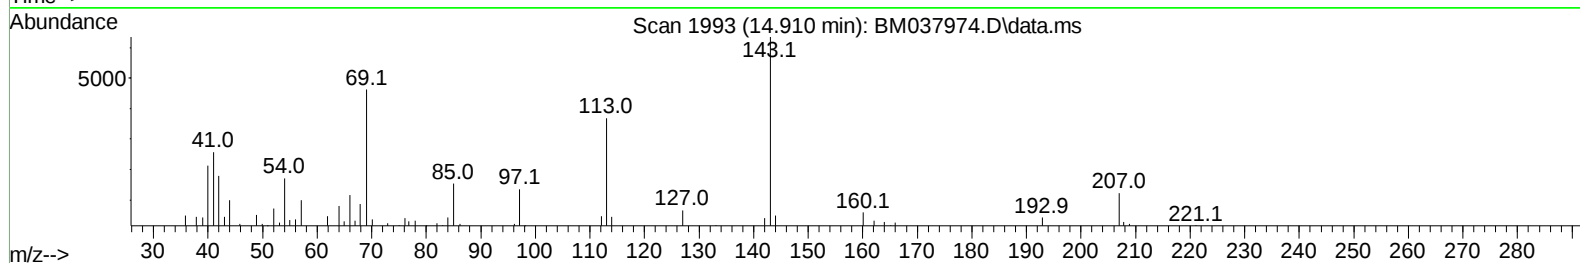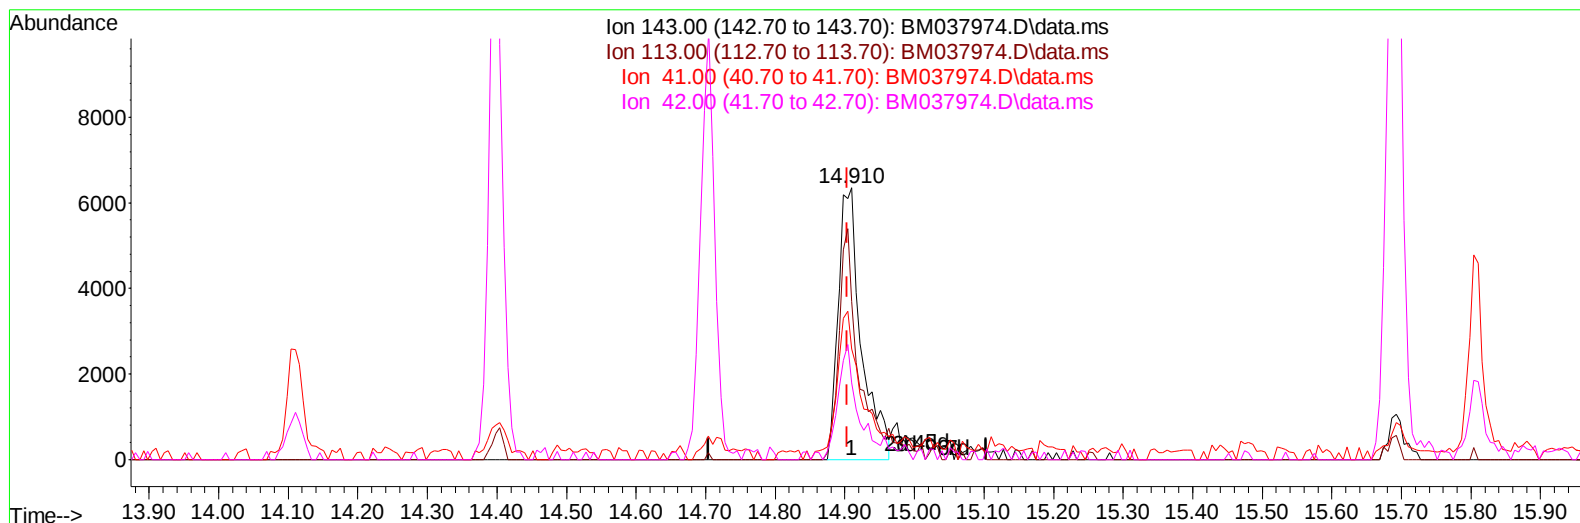

TIC: BM037974.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.006) 3.03 ng/ul m

response 14573

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	60.30	58.14
41.00	43.90	40.60
42.00	30.30	28.28

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037974.D
 Acq On : 12 Dec 2022 20:05
 Operator : CG/JU
 Sample : N5948-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB2

Manual IntegrationsAPPROVED

Quant Time: Dec 13 00:58:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/13/2022
 Supervised By :mohammad ahmed 12/14/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	172157	20.000	ng/ul	0.00
20) Naphthalene-d8	10.893	136	696902	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.704	164	395551	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.445	188	692581	20.000	ng/ul	0.00
79) Chrysene-d12	21.615	240	586247	20.000	ng/ul	0.00
88) Perylene-d12	24.092	264	637025	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.417	96	14702	3.878	ng/uL	0.00
4) Pyridine-d5	3.870	84	24782	2.203	ng/ul	0.01
7) Phenol-d5	7.228	99	87773	6.274	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.399	67	253901	29.806	ng/ul	0.00
11) 2-Chlorophenol-d4	7.599	132	231925	20.209	ng/ul	-0.01
15) 4-Methylphenol-d8	8.781	113	141350	12.944	ng/ul	-0.01
21) Nitrobenzene-d5	9.246	128	190014	34.437	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.969	143	158161	27.352	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.510	165	250443	22.803	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.028	131	170483	11.245	ng/ul	-0.01
46) Dimethylphthalate-d6	14.110	166	960539	34.062	ng/ul	-0.01
49) Acenaphthylene-d8	14.398	160	1180924	34.264	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.910	143	14573m	3.032	ng/ul	0.00
60) Fluorene-d10	15.692	176	872212	34.716	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.810	200	63756	17.218	ng/ul	0.00
73) Anthracene-d10	17.539	188	1232975	38.145	ng/ul	-0.01
81) Pyrene-d10	19.827	212	1316249	37.377	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.933	264	1233512	38.768	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/13/2022
Supervised By :mohammad ahmed 12/14/2022

Quant Time: Dec 13 00:58:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

