

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037972.D
 Acq On : 12 Dec 2022 18:51
 Operator : CG/JU
 Sample : N5948-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB7

Quant Time: Dec 13 00:58:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.075	152	196387	20.000	ng/u1	0.00
20) Naphthalene-d8	10.892	136	921313	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.704	164	576028	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1051633	20.000	ng/u1	0.00
79) Chrysene-d12	21.615	240	777719	20.000	ng/u1	0.00
88) Perylene-d12	24.091	264	819046	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.416	96	15163	3.506	ng/uL	0.00
4) Pyridine-d5	3.863	84	87164	6.793	ng/u1	0.00
7) Phenol-d5	7.228	99	73274	4.592	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.398	67	260136	26.770	ng/u1	0.00
11) 2-Chlorophenol-d4	7.604	132	262905	20.082	ng/u1	0.00
15) 4-Methylphenol-d8	8.786	113	155742	12.502	ng/u1	0.00
21) Nitrobenzene-d5	9.245	128	210136	28.807	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.975	143	224465	29.363	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	356268	24.537	ng/u1	0.00
31) 4-Chloroaniline-d4	11.039	131	331418	16.536	ng/u1	0.00
46) Dimethylphthalate-d6	14.115	166	1357359	33.052	ng/u1	0.00
49) Acenaphthylene-d8	14.404	160	1562505	31.131	ng/u1	0.00
54) 4-Nitrophenol-d4	14.904	143	26243	3.750	ng/u1	0.00
60) Fluorene-d10	15.692	176	1155767	31.589	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.809	200	132000	23.477	ng/u1	0.00
73) Anthracene-d10	17.545	188	1584673	32.287	ng/u1	0.00
81) Pyrene-d10	19.827	212	1591519	34.067	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.932	264	1376717	33.653	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.451	88	39130	8.624	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037972.D
Acq On : 12 Dec 2022 18:51
Operator : CG/JU
Sample : N5948-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB7

Quant Time: Dec 13 00:58:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration

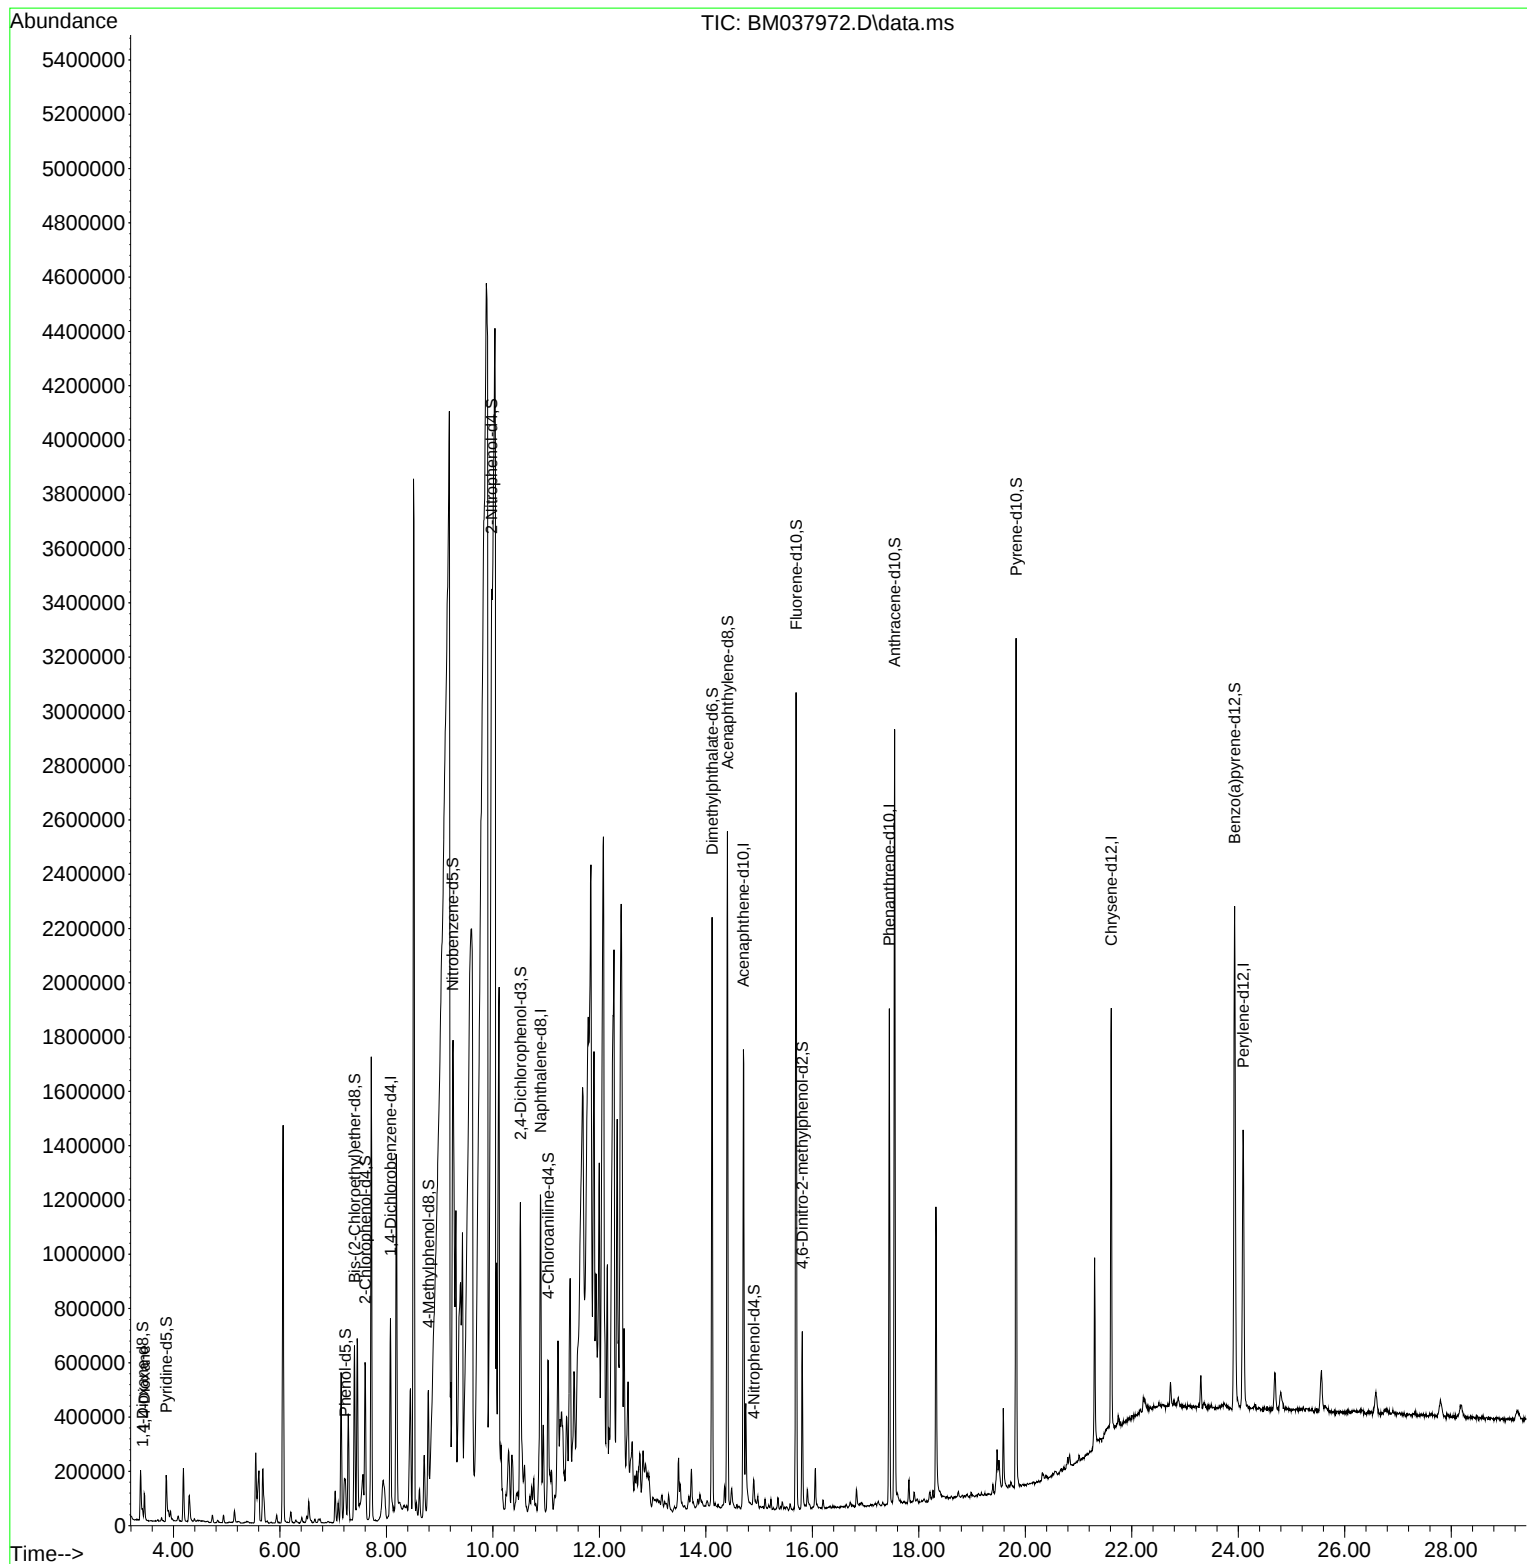

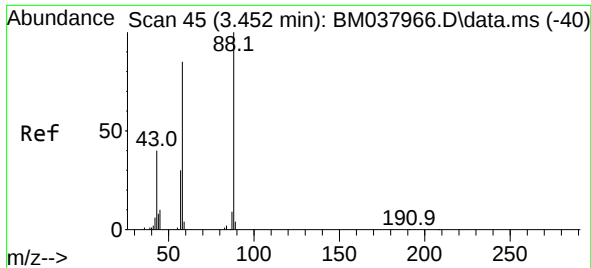

#2
 1,4-Dioxane
 Concen: 8.624 ng/uL
 RT: 3.451 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BM037972.D
 Acq: 12 Dec 2022 18:51

Instrument :
 BNA_M
 ClientSampleId :
 EXZB7

Tgt Ion: 88 Resp: 39130
 Ion Ratio Lower Upper
 88 100
 43 44.5 32.8 49.2
 58 85.4 64.6 97.0

