

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037961.D
 Acq On : 12 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149539BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	44	rVB	42019	56624	2.19%	0.158%
2	3.851	109	113	138	rBV	636389	1034262	40.02%	2.890%
3	4.187	165	170	177	rVB	123567	181029	7.00%	0.506%
4	4.728	260	262	264	rBV2	2509	3078	0.12%	0.009%
5	5.916	462	464	469	rBV6	2431	3015	0.12%	0.008%
6	6.393	541	545	546	rVB4	2221	2658	0.10%	0.007%
7	6.857	622	624	628	rBV4	2265	3024	0.12%	0.008%
8	7.181	674	679	680	rBV4	3337	4283	0.17%	0.012%
9	7.228	680	687	696	rVV	730108	1170386	45.28%	3.271%
10	7.392	709	715	725	rVB	565151	885741	34.27%	2.475%
11	7.598	743	750	759	rBV	772407	1190655	46.07%	3.327%
12	8.069	824	830	840	rVB	747100	1172541	45.37%	3.277%
13	8.439	890	893	897	rBV5	3024	3632	0.14%	0.010%
14	8.622	921	924	926	rVB4	2590	3014	0.12%	0.008%
15	8.645	926	928	931	rBV4	2500	3419	0.13%	0.010%
16	8.781	944	951	960	rBV	876725	1366115	52.85%	3.818%
17	9.145	1011	1013	1016	rVB3	2335	2970	0.11%	0.008%
18	9.245	1022	1030	1038	rBV	706973	1141616	44.17%	3.190%
19	9.410	1056	1058	1063	rVB6	3064	4464	0.17%	0.012%
20	9.969	1146	1153	1164	rBV	545728	880560	34.07%	2.461%
21	10.133	1180	1181	1185	rBV4	3510	3239	0.13%	0.009%
22	10.228	1196	1197	1201	rVB4	3178	2826	0.11%	0.008%
23	10.333	1213	1215	1218	rBV3	2128	3454	0.13%	0.010%
24	10.510	1235	1245	1264	rBV	810730	1380808	53.42%	3.859%
25	10.892	1303	1310	1323	rBV	1022469	1660009	64.23%	4.639%
26	11.028	1326	1333	1345	rBV	729623	1290343	49.92%	3.606%
27	11.880	1475	1478	1480	rBV4	3043	3653	0.14%	0.010%
28	11.910	1480	1483	1486	rVV5	2238	3627	0.14%	0.010%
29	12.057	1501	1508	1511	rBV7	4998	10499	0.41%	0.029%
30	12.469	1572	1578	1583	rBV3	13377	24656	0.95%	0.069%
31	13.033	1670	1674	1677	rBV5	2387	4325	0.17%	0.012%
32	13.304	1715	1720	1722	rVB6	1810	2810	0.11%	0.008%
33	13.598	1764	1770	1776	rVB6	7234	15085	0.58%	0.042%
34	13.674	1780	1783	1786	rVV5	2477	3622	0.14%	0.010%
35	14.110	1846	1857	1865	rBV	1229143	1688701	65.34%	4.719%
36	14.398	1899	1906	1917	rBV	1451691	2190142	84.74%	6.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037961.D
 Acq On : 12 Dec 2022 10:19
 Operator : CG/JU
 Sample : PB149539BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK539

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	14.521	1925	1927	1933	rVB6	3790	4348	0.17%	0.012%
38	14.704	1950	1958	1974	rBV	1336786	1966471	76.08%	5.495%
39	14.898	1984	1991	2005	rBV	246217	520585	20.14%	1.455%
40	15.110	2026	2027	2031	rVB4	3933	3602	0.14%	0.010%
41	15.251	2050	2051	2055	rVB4	2858	2586	0.10%	0.007%
42	15.292	2055	2058	2060	rBV4	2655	3550	0.14%	0.010%
43	15.357	2068	2069	2075	rBV6	3496	4427	0.17%	0.012%
44	15.651	2114	2119	2120	rBV4	8085	9236	0.36%	0.026%
45	15.692	2120	2126	2137	rVV	1766001	2484904	96.14%	6.944%
46	15.810	2141	2146	2158	rVB	241264	358768	13.88%	1.003%
47	15.933	2163	2167	2171	rVB4	10602	16519	0.64%	0.046%
48	16.033	2181	2184	2185	rBV3	2973	2871	0.11%	0.008%
49	16.210	2210	2214	2218	rBV6	2009	3152	0.12%	0.009%
50	16.786	2311	2312	2317	rBV4	1907	3047	0.12%	0.009%
51	16.898	2325	2331	2334	rBV7	6572	11243	0.43%	0.031%
52	17.098	2362	2365	2368	rBV5	2633	3957	0.15%	0.011%
53	17.445	2418	2424	2435	rBV	1359510	1897202	73.40%	5.302%
54	17.545	2435	2441	2456	rVB	1677268	2376557	91.95%	6.641%
55	17.804	2481	2485	2486	rBV4	3450	4339	0.17%	0.012%
56	17.962	2510	2512	2520	rVB7	5518	9017	0.35%	0.025%
57	18.074	2529	2531	2533	rBV2	2620	2657	0.10%	0.007%
58	18.398	2584	2586	2588	rBV3	4710	4697	0.18%	0.013%
59	18.533	2607	2609	2610	rBV	3433	2713	0.10%	0.008%
60	18.709	2637	2639	2640	rBV2	3160	2677	0.10%	0.007%
61	18.903	2669	2672	2678	rBV8	6808	11808	0.46%	0.033%
62	19.392	2752	2755	2760	rBV4	17933	21634	0.84%	0.060%
63	19.462	2763	2767	2771	rBV2	19167	31344	1.21%	0.088%
64	19.827	2824	2829	2840	rBV	1899493	2584652	100.00%	7.223%
65	20.803	2992	2995	2999	rVB3	35144	38071	1.47%	0.106%
66	21.509	3113	3115	3118	rBV	44245	40704	1.57%	0.114%
67	21.615	3129	3133	3143	rVB	1256479	1745785	67.54%	4.879%
68	23.938	3522	3528	3542	rVB2	1118440	2420401	93.65%	6.764%
69	24.103	3549	3556	3566	rBV	832533	1790288	69.27%	5.003%




Sum of corrected areas: 35784697

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037961.D
Acq On : 12 Dec 2022 10:19
Operator : CG/JU
Sample : PB149539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK539

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

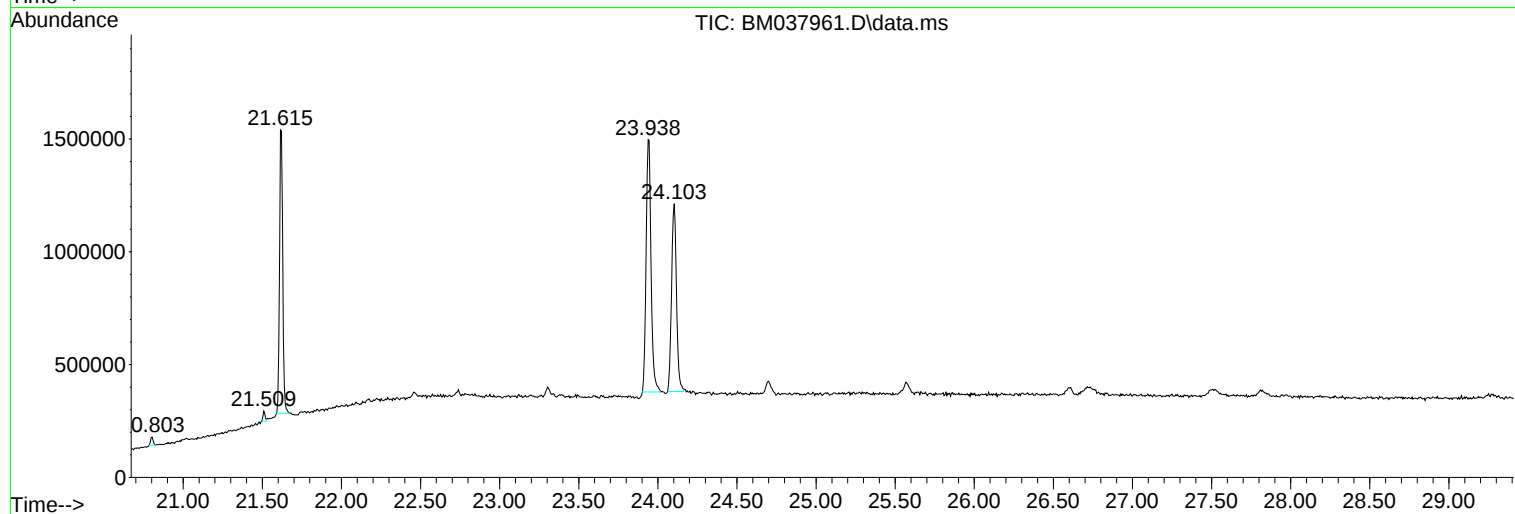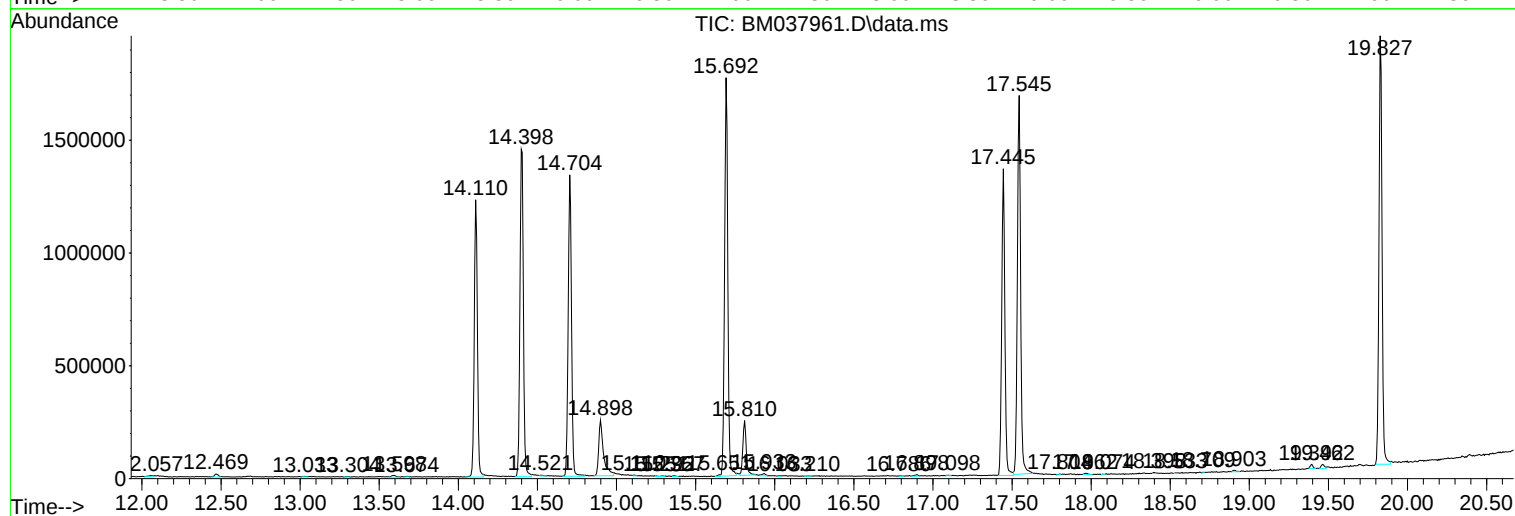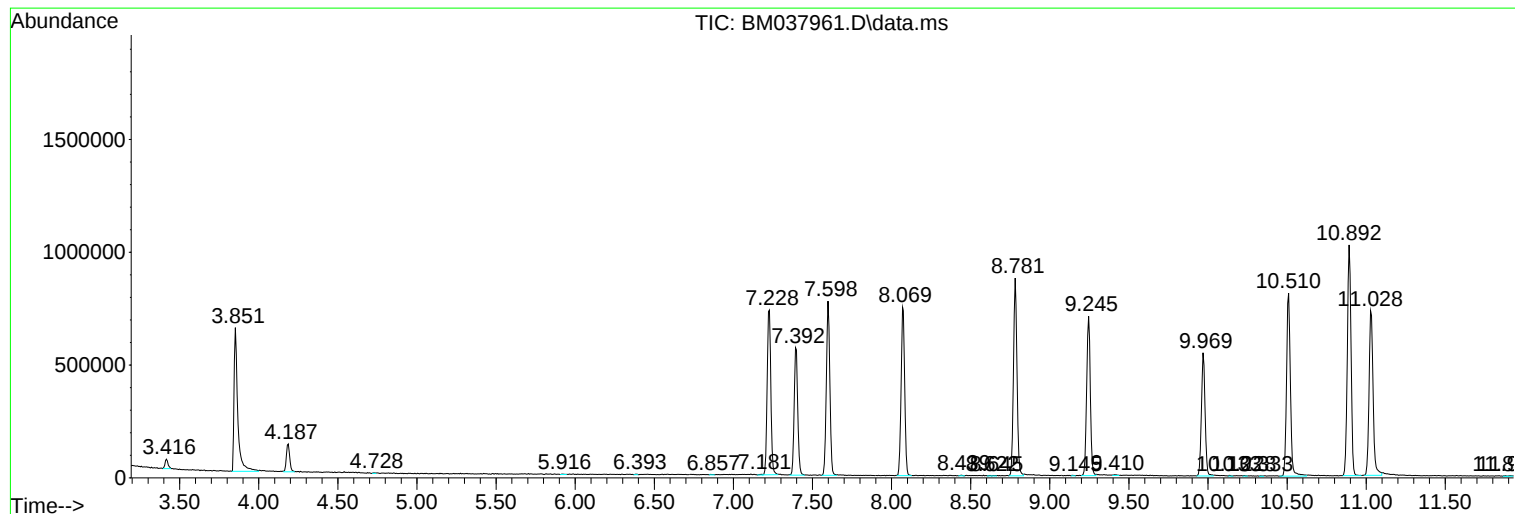

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037961.D
Acq On : 12 Dec 2022 10:19
Operator : CG/JU
Sample : PB149539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK539










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.187	3.09 ng/ul	181029	1,4-Dichlorobenzene-d4	8.069

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Toluene			92	C7H8	000108-88-3	94
2	Toluene			92	C7H8	000108-88-3	91
3	Toluene			92	C7H8	000108-88-3	91
4	Toluene			92	C7H8	000108-88-3	90
5	Toluene			92	C7H8	000108-88-3	90

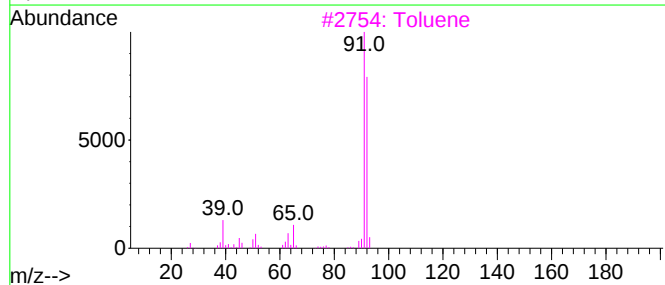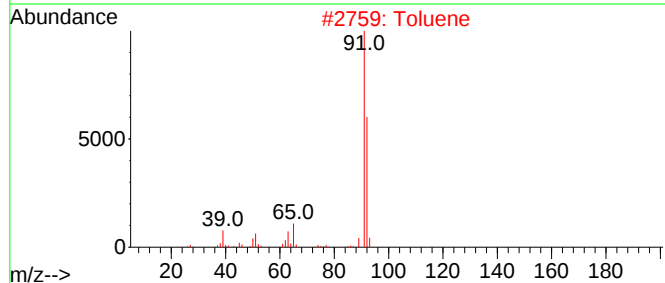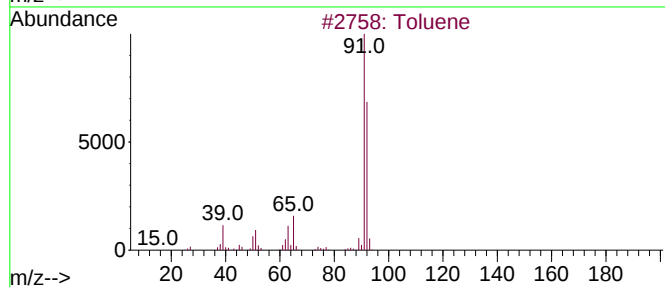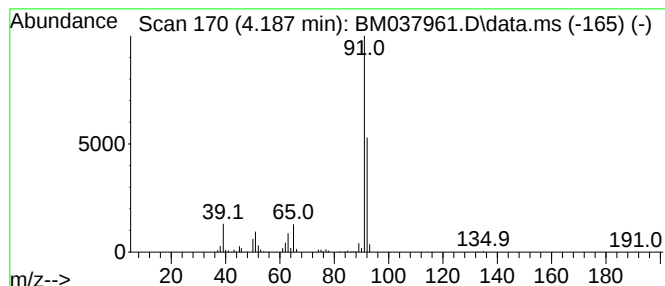

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037961.D
Acq On : 12 Dec 2022 10:19
Operator : CG/JU
Sample : PB149539BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK539

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	4.187	3.1	ng/u1	181029	1	8.069	1172540	20.0