

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037967.D
 Acq On : 12 Dec 2022 15:46
 Operator : CG/JU
 Sample : PB149528BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	48	rVB	51524	75197	2.53%	0.197%
2	3.852	109	113	132	rBV	688092	1115378	37.57%	2.928%
3	4.187	166	170	175	rVB4	10892	17654	0.59%	0.046%
4	4.975	302	304	309	rBV5	1891	3152	0.11%	0.008%
5	6.328	528	534	535	rBV6	2301	3342	0.11%	0.009%
6	6.557	570	573	577	rVB5	2948	5139	0.17%	0.013%
7	6.598	577	580	581	rBV3	2866	2978	0.10%	0.008%
8	7.228	680	687	697	rBV	890419	1347232	45.38%	3.537%
9	7.398	709	716	726	rVB	677493	1001686	33.74%	2.630%
10	7.598	743	750	760	rBV	842079	1334574	44.95%	3.504%
11	8.075	824	831	839	rVB	669857	1022793	34.45%	2.685%
12	8.786	944	952	961	rBV	982011	1570062	52.88%	4.122%
13	9.245	1023	1030	1041	rBV	793547	1287637	43.37%	3.381%
14	9.975	1146	1154	1163	rBV	622805	1021717	34.41%	2.682%
15	10.157	1183	1185	1188	rVB4	3093	3518	0.12%	0.009%
16	10.510	1237	1245	1262	rBV	951884	1587315	53.46%	4.167%
17	10.892	1303	1310	1319	rBV	882827	1434184	48.30%	3.765%
18	11.033	1326	1334	1350	rBV	875789	1526810	51.42%	4.008%
19	11.192	1359	1361	1364	rVB4	3811	3728	0.13%	0.010%
20	12.127	1517	1520	1522	rVB4	2969	3161	0.11%	0.008%
21	12.474	1574	1579	1584	rBV2	16335	27796	0.94%	0.073%
22	12.680	1610	1614	1619	rBV6	2830	4275	0.14%	0.011%
23	13.592	1765	1769	1774	rBV5	6206	9172	0.31%	0.024%
24	13.674	1781	1783	1788	rVB3	2321	3545	0.12%	0.009%
25	14.110	1851	1857	1871	rBV	1443909	1974416	66.50%	5.184%
26	14.321	1890	1893	1897	rVB4	2291	3712	0.13%	0.010%
27	14.404	1899	1907	1917	rBV	1704390	2548210	85.82%	6.690%
28	14.474	1917	1919	1923	rVB5	2956	3205	0.11%	0.008%
29	14.704	1951	1958	1967	rBV	1206524	1706202	57.47%	4.479%
30	14.898	1984	1991	2020	rBV	344468	719659	24.24%	1.889%
31	15.363	2067	2070	2073	rVB5	4161	3116	0.10%	0.008%
32	15.633	2112	2116	2118	rBV5	2595	3959	0.13%	0.010%
33	15.692	2120	2126	2138	rVV	2136163	2969082	100.00%	7.795%
34	15.810	2140	2146	2154	rVB	345016	476117	16.04%	1.250%
35	15.927	2162	2166	2173	rVB6	10850	21274	0.72%	0.056%
36	16.121	2197	2199	2203	rVB4	2915	3295	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037967.D
 Acq On : 12 Dec 2022 15:46
 Operator : CG/JU
 Sample : PB149528BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK528

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.468	2255	2258	2262	rBV6	2392	3371	0.11%	0.009%
38	17.098	2361	2365	2366	rBV3	3606	3147	0.11%	0.008%
39	17.121	2366	2369	2374	rVB7	2927	4813	0.16%	0.013%
40	17.304	2396	2400	2402	rBV3	2556	3289	0.11%	0.009%
41	17.445	2418	2424	2434	rBV	1192227	1635919	55.10%	4.295%
42	17.545	2434	2441	2452	rBV	2011756	2799437	94.29%	7.350%
43	17.809	2485	2486	2491	rBV4	3162	3730	0.13%	0.010%
44	17.927	2505	2506	2510	rBV4	3247	4579	0.15%	0.012%
45	18.404	2583	2587	2589	rBV4	5385	5740	0.19%	0.015%
46	19.392	2751	2755	2759	rVB4	21584	31146	1.05%	0.082%
47	19.462	2764	2767	2771	rVV2	19878	23526	0.79%	0.062%
48	19.827	2823	2829	2839	rBV	2249916	2925257	98.52%	7.680%
49	21.615	3129	3133	3146	rVB	1091016	1491146	50.22%	3.915%
50	23.938	3521	3528	3542	rVB	1317708	2761234	93.00%	7.249%
51	24.097	3549	3555	3568	rVB2	737898	1549328	52.18%	4.068%




Sum of corrected areas: 38089954

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037967.D
Acq On : 12 Dec 2022 15:46
Operator : CG/JU
Sample : PB149528BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

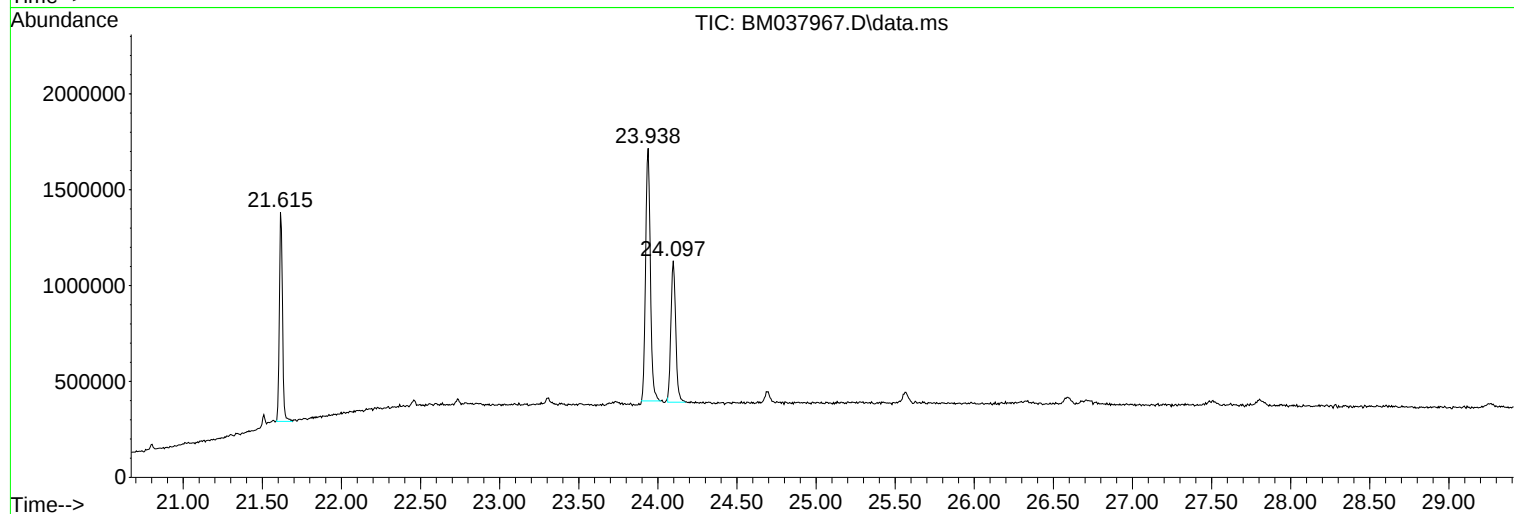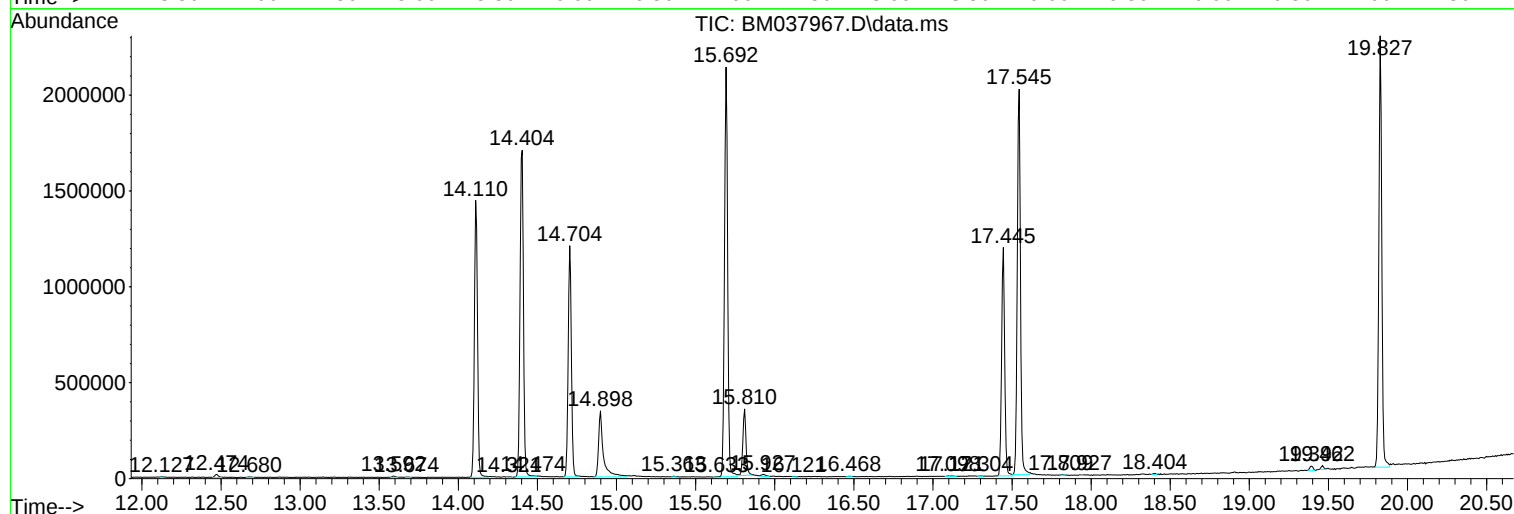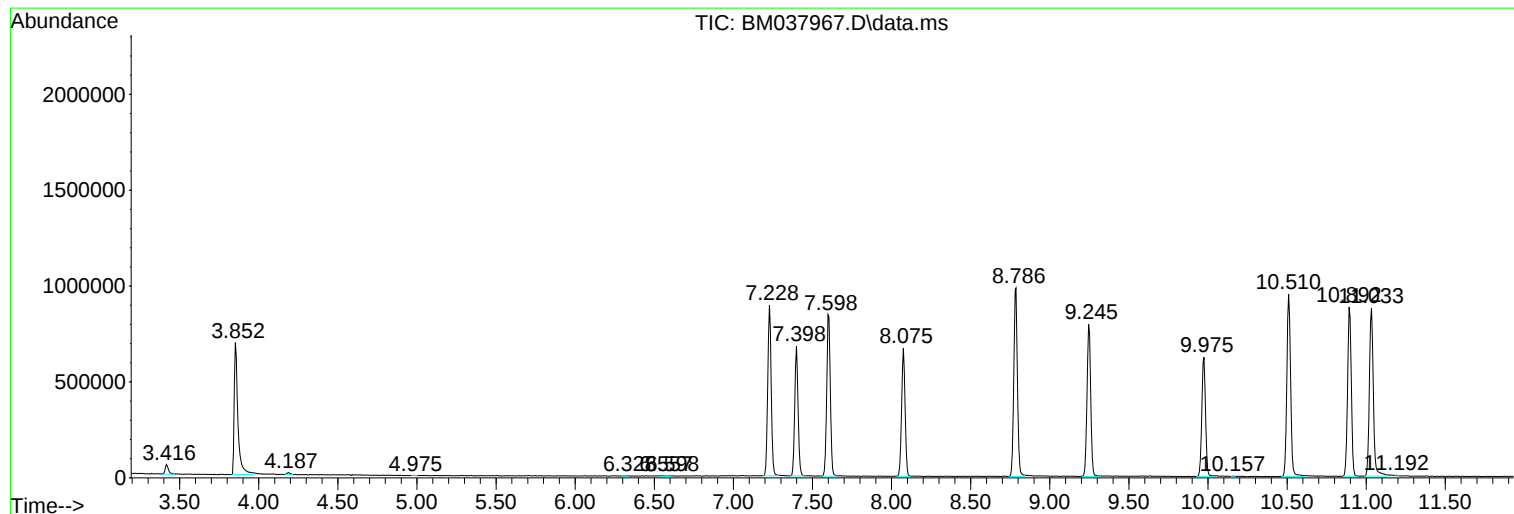

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037967.D
Acq On : 12 Dec 2022 15:46
Operator : CG/JU
Sample : PB149528BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037967.D
Acq On : 12 Dec 2022 15:46
Operator : CG/JU
Sample : PB149528BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK528

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc