

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037969.D
 Acq On : 12 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5948-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	36	rBV5	8719	11085	0.38%	0.033%
2	3.416	36	39	42	rVV	32995	42639	1.45%	0.128%
3	3.452	42	45	51	rVB	34561	48147	1.63%	0.145%
4	3.875	115	117	123	rBV	25149	42832	1.45%	0.129%
5	4.087	148	153	159	rVB	17832	27925	0.95%	0.084%
6	4.187	166	170	175	rVB	12814	17006	0.58%	0.051%
7	4.581	234	237	244	rVB6	3967	5759	0.20%	0.017%
8	4.728	257	262	270	rVB	49958	78942	2.68%	0.238%
9	6.498	558	563	565	rBV7	2561	4160	0.14%	0.013%
10	7.228	680	687	696	rVB2	171628	262987	8.92%	0.792%
11	7.357	704	709	710	rBV3	2806	4530	0.15%	0.014%
12	7.398	710	716	725	rBV	593003	901049	30.56%	2.715%
13	7.510	732	735	738	rBV5	2252	3503	0.12%	0.011%
14	7.598	744	750	759	rBV	613935	966410	32.78%	2.912%
15	7.681	761	764	774	rVB7	4340	7013	0.24%	0.021%
16	8.075	823	831	838	rBV	671371	1044692	35.44%	3.148%
17	8.134	838	841	846	rVB3	5398	7521	0.26%	0.023%
18	8.781	945	951	961	rBV	445362	704558	23.90%	2.123%
19	9.245	1023	1030	1039	rBV	762931	1208607	41.00%	3.641%
20	9.345	1044	1047	1052	rVB6	5489	8721	0.30%	0.026%
21	9.639	1093	1097	1101	rVB3	12521	16220	0.55%	0.049%
22	9.975	1145	1154	1164	rBV	548882	924171	31.35%	2.784%
23	10.122	1175	1179	1183	rBV7	2925	4819	0.16%	0.015%
24	10.192	1189	1191	1196	rBV4	3283	4403	0.15%	0.013%
25	10.510	1238	1245	1256	rVV	802951	1309493	44.42%	3.945%
26	10.616	1262	1263	1269	rVB6	2633	3246	0.11%	0.010%
27	10.892	1302	1310	1318	rBV	890978	1460293	49.53%	4.400%
28	10.951	1318	1320	1325	rVB7	2473	3253	0.11%	0.010%
29	11.033	1325	1334	1344	rBV	160159	288794	9.80%	0.870%
30	11.675	1440	1443	1448	rBV7	3322	6713	0.23%	0.020%
31	11.904	1478	1482	1483	rVB5	2913	3492	0.12%	0.011%
32	12.286	1543	1547	1553	rVB3	8960	13224	0.45%	0.040%
33	12.469	1571	1578	1584	rBV	15345	23389	0.79%	0.070%
34	12.922	1650	1655	1659	rBV4	3677	5358	0.18%	0.016%
35	13.098	1682	1685	1689	rVB6	2817	3751	0.13%	0.011%
36	13.239	1705	1709	1711	rVB4	2578	3090	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037969.D
 Acq On : 12 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5948-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	13.516	1751	1756	1760	rBV2	11702	16967	0.58%	0.051%
38	14.033	1840	1844	1848	rBV6	2449	3716	0.13%	0.011%
39	14.110	1851	1857	1870	rVV	1375586	1886252	63.98%	5.683%
40	14.398	1899	1906	1918	rBV	1655933	2479391	84.10%	7.470%
41	14.580	1933	1937	1943	rBV7	4065	8278	0.28%	0.025%
42	14.704	1951	1958	1967	rBV	1250563	1766537	59.92%	5.322%
43	14.904	1986	1992	2003	rBV2	42725	96155	3.26%	0.290%
44	15.110	2023	2027	2032	rVB7	6848	14142	0.48%	0.043%
45	15.163	2032	2036	2039	rVB5	2221	3269	0.11%	0.010%
46	15.651	2116	2119	2120	rBV2	3401	3941	0.13%	0.012%
47	15.692	2120	2126	2140	rVV	2046872	2875415	97.53%	8.663%
48	15.810	2140	2146	2160	rVV	346219	526687	17.87%	1.587%
49	15.933	2163	2167	2173	rVB7	9347	16495	0.56%	0.050%
50	16.051	2182	2187	2194	rBV	12805	18488	0.63%	0.056%
51	16.468	2255	2258	2262	rBV6	2146	2952	0.10%	0.009%
52	16.827	2316	2319	2321	rBV3	2405	3179	0.11%	0.010%
53	16.898	2328	2331	2335	rVB6	5426	4984	0.17%	0.015%
54	17.086	2359	2363	2365	rBV5	2328	3008	0.10%	0.009%
55	17.245	2387	2390	2393	rVB5	3095	4323	0.15%	0.013%
56	17.445	2418	2424	2434	rBV	1241602	1712280	58.08%	5.159%
57	17.545	2434	2441	2465	rVB	1905272	2764040	93.76%	8.328%
58	18.104	2532	2536	2542	rVB8	7147	10920	0.37%	0.033%
59	18.315	2568	2572	2579	rBV4	50111	72372	2.45%	0.218%
60	19.392	2751	2755	2761	rBV3	24922	39636	1.34%	0.119%
61	19.462	2763	2767	2770	rBV2	22568	33099	1.12%	0.100%
62	19.586	2784	2788	2794	rBV7	30652	49594	1.68%	0.149%
63	19.827	2823	2829	2837	rBV	2242867	2893544	98.15%	8.718%
64	21.297	3076	3079	3083	rBV4	67561	99899	3.39%	0.301%
65	21.615	3128	3133	3142	rBV	1219971	1616094	54.82%	4.869%
66	23.933	3520	3527	3543	rVB2	1388890	2948133	100.00%	8.882%
67	24.091	3548	3554	3566	rVB2	818548	1744810	59.18%	5.257%




Sum of corrected areas: 33190395

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037969.D
Acq On : 12 Dec 2022 17:01
Operator : CG/JU
Sample : N5948-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

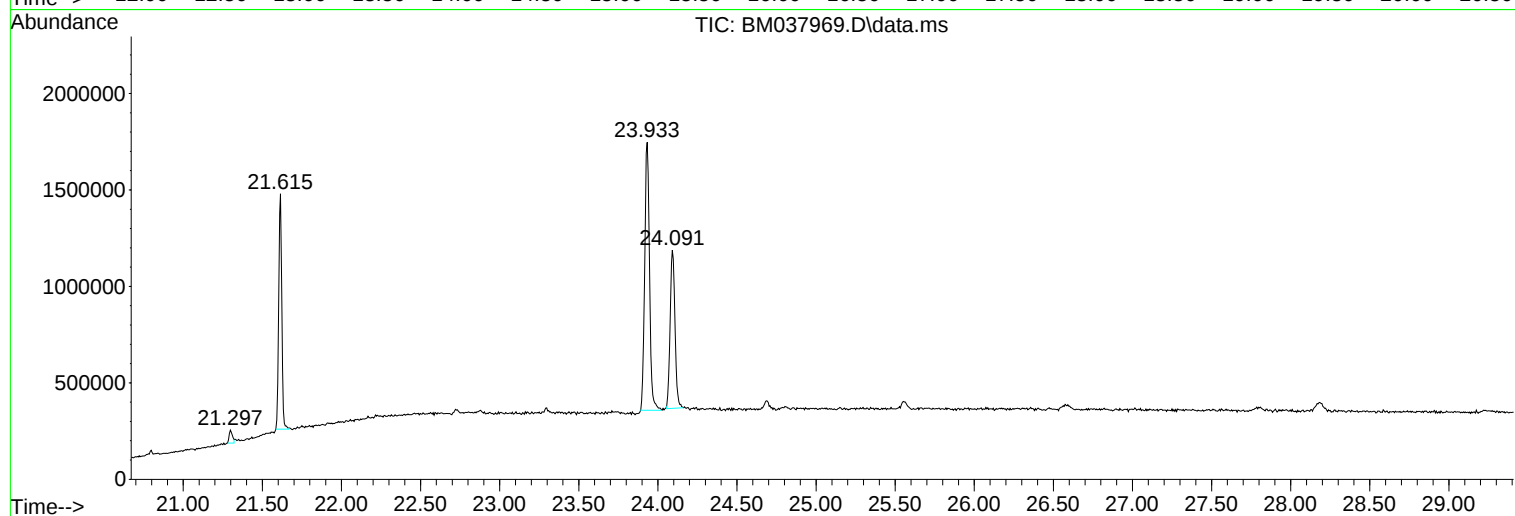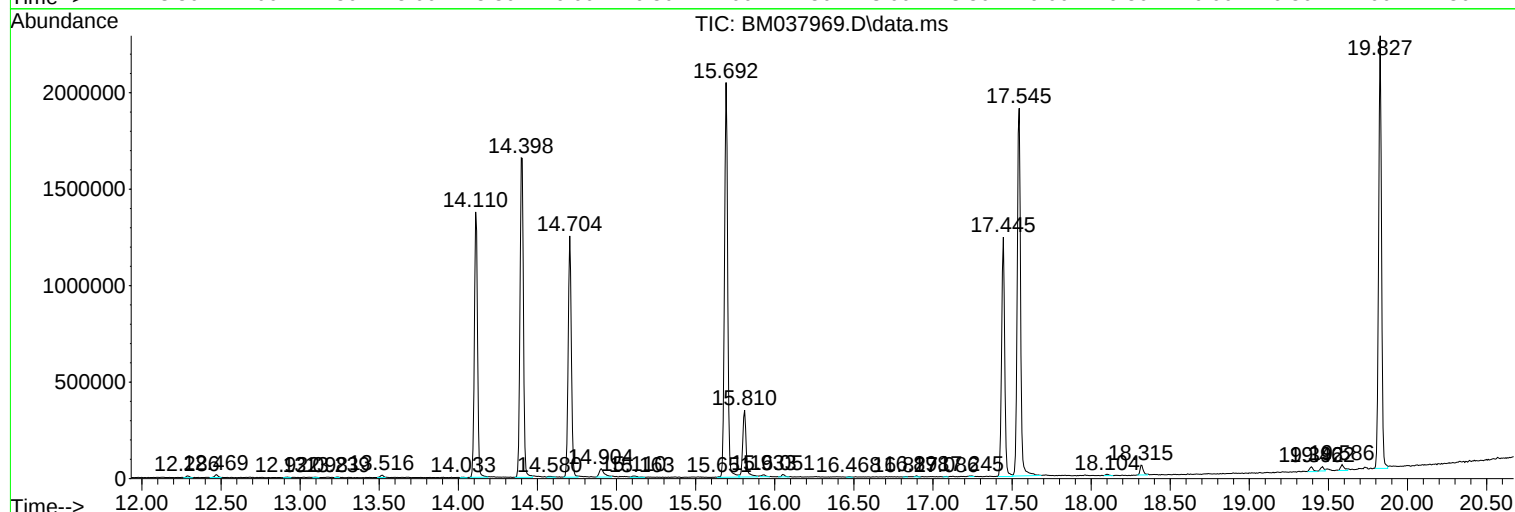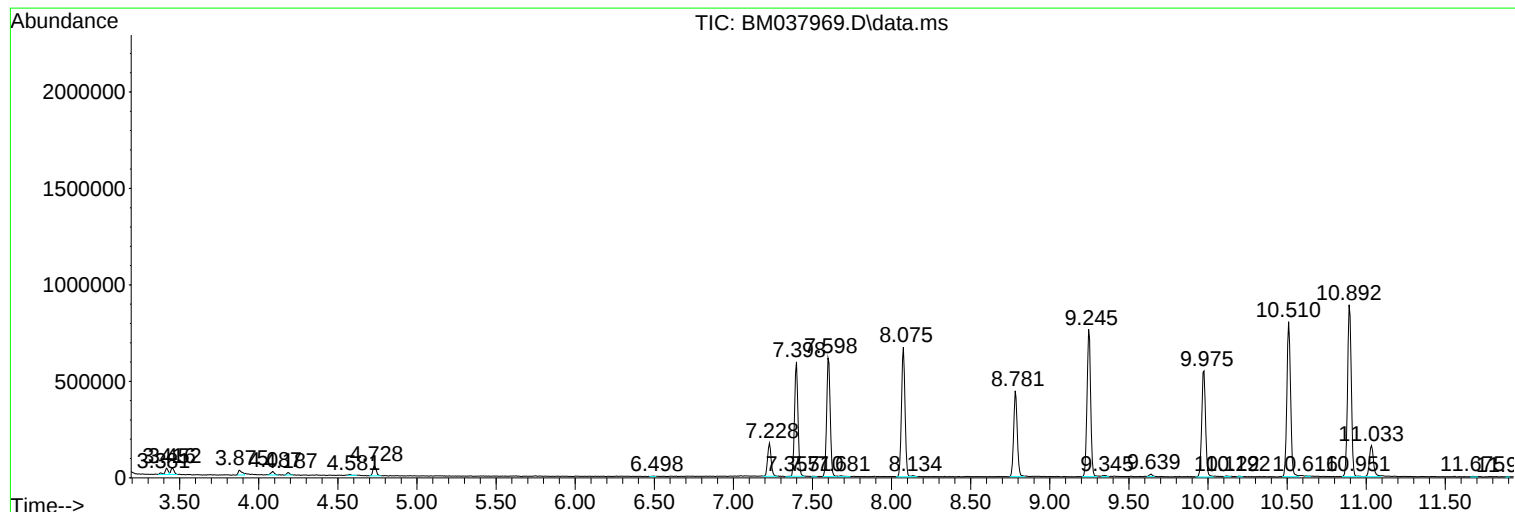

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037969.D
Acq On : 12 Dec 2022 17:01
Operator : CG/JU
Sample : N5948-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037969.D
Acq On : 12 Dec 2022 17:01
Operator : CG/JU
Sample : N5948-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc