

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037970.D
 Acq On : 12 Dec 2022 17:38
 Operator : CG/JU
 Sample : N5948-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	30	34	36	rBV4	7458	10106	0.31%	0.031%
2	3.416	36	39	42	rVV	34728	43217	1.33%	0.133%
3	3.451	42	45	52	rVB	37353	50592	1.56%	0.155%
4	3.875	114	117	127	rBV	30649	62199	1.92%	0.191%
5	4.087	148	153	159	rVB2	16793	27741	0.86%	0.085%
6	4.187	166	170	175	rVB	15351	20975	0.65%	0.064%
7	4.734	257	263	272	rBV	52164	79267	2.44%	0.243%
8	5.816	445	447	452	rVB4	2242	3345	0.10%	0.010%
9	7.228	681	687	693	rBV	169759	262662	8.10%	0.806%
10	7.398	710	716	725	rBV	574239	868163	26.77%	2.663%
11	7.598	743	750	759	rBV	551439	881279	27.17%	2.703%
12	7.681	761	764	768	rVB3	5673	5338	0.16%	0.016%
13	8.075	824	831	838	rBV	642278	995291	30.69%	3.052%
14	8.133	839	841	846	rVB5	3485	4759	0.15%	0.015%
15	8.781	943	951	961	rBV	422945	662188	20.42%	2.031%
16	9.245	1021	1030	1041	rBV	737703	1188858	36.66%	3.646%
17	9.639	1093	1097	1101	rVV2	10783	15586	0.48%	0.048%
18	9.975	1145	1154	1164	rBV	496872	838630	25.86%	2.572%
19	10.510	1233	1245	1255	rBV	719234	1186347	36.58%	3.638%
20	10.892	1304	1310	1319	rVB	863213	1389732	42.85%	4.262%
21	11.033	1324	1334	1348	rBV	201734	367383	11.33%	1.127%
22	12.292	1543	1548	1552	rVB3	7136	9759	0.30%	0.030%
23	12.469	1574	1578	1586	rVB2	15436	25160	0.78%	0.077%
24	12.951	1657	1660	1665	rVB5	2461	3474	0.11%	0.011%
25	13.021	1668	1672	1673	rBV4	2804	3395	0.10%	0.010%
26	13.092	1681	1684	1689	rVB5	2999	4327	0.13%	0.013%
27	13.180	1695	1699	1704	rVB6	3221	5771	0.18%	0.018%
28	13.233	1704	1708	1712	rBV5	2943	3950	0.12%	0.012%
29	13.521	1749	1757	1760	rBV3	9795	14413	0.44%	0.044%
30	13.592	1765	1769	1773	rBV5	3085	4925	0.15%	0.015%
31	13.680	1780	1784	1788	rVB4	3257	3887	0.12%	0.012%
32	14.027	1837	1843	1846	rBV5	2643	4600	0.14%	0.014%
33	14.110	1851	1857	1867	rBV	1345978	1824328	56.25%	5.595%
34	14.398	1900	1906	1918	rBV	1580812	2380401	73.40%	7.300%
35	14.704	1950	1958	1966	rBV	1174501	1678388	51.75%	5.147%
36	14.904	1986	1992	2004	rBV2	36947	93022	2.87%	0.285%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037970.D
 Acq On : 12 Dec 2022 17:38
 Operator : CG/JU
 Sample : N5948-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.110	2023	2027	2032	rVB7	4409	8020	0.25%	0.025%
38	15.692	2120	2126	2137	rVV	2027976	2801151	86.37%	8.591%
39	15.809	2140	2146	2159	rVB	319193	460858	14.21%	1.413%
40	15.933	2164	2167	2174	rVB6	10109	15192	0.47%	0.047%
41	16.057	2183	2188	2197	rVB2	9484	15511	0.48%	0.048%
42	16.468	2256	2258	2264	rBV4	2746	4274	0.13%	0.013%
43	17.033	2351	2354	2356	rBV4	2658	3719	0.11%	0.011%
44	17.174	2375	2378	2382	rBV4	3680	6287	0.19%	0.019%
45	17.233	2383	2388	2390	rVV4	3329	6326	0.20%	0.019%
46	17.256	2390	2392	2396	rVB4	2843	3257	0.10%	0.010%
47	17.445	2417	2424	2434	rBV	1193810	1638240	50.51%	5.024%
48	17.545	2434	2441	2462	rVB	1964062	2853101	87.97%	8.750%
49	17.709	2467	2469	2477	rVB8	3002	6728	0.21%	0.021%
50	18.315	2567	2572	2579	rBV5	36180	57787	1.78%	0.177%
51	18.933	2675	2677	2679	rBV2	4295	3470	0.11%	0.011%
52	19.068	2698	2700	2702	rBV3	4848	5560	0.17%	0.017%
53	19.392	2751	2755	2760	rBV3	24801	34216	1.06%	0.105%
54	19.456	2764	2766	2770	rVV2	20831	26726	0.82%	0.082%
55	19.492	2770	2772	2776	rVV5	9424	12366	0.38%	0.038%
56	19.586	2785	2788	2796	rBV8	16308	28676	0.88%	0.088%
57	19.733	2811	2813	2818	rVB4	10307	11101	0.34%	0.034%
58	19.827	2823	2829	2838	rBV	2380861	3043455	93.84%	9.334%
59	21.615	3128	3133	3143	rBV	1191738	1593821	49.14%	4.888%
60	23.932	3520	3527	3542	rBV2	1599611	3243148	100.00%	9.946%
61	24.091	3548	3554	3566	rVB2	818375	1700050	52.42%	5.214%


Sum of corrected areas: 32606498

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037970.D
Acq On : 12 Dec 2022 17:38
Operator : CG/JU
Sample : N5948-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

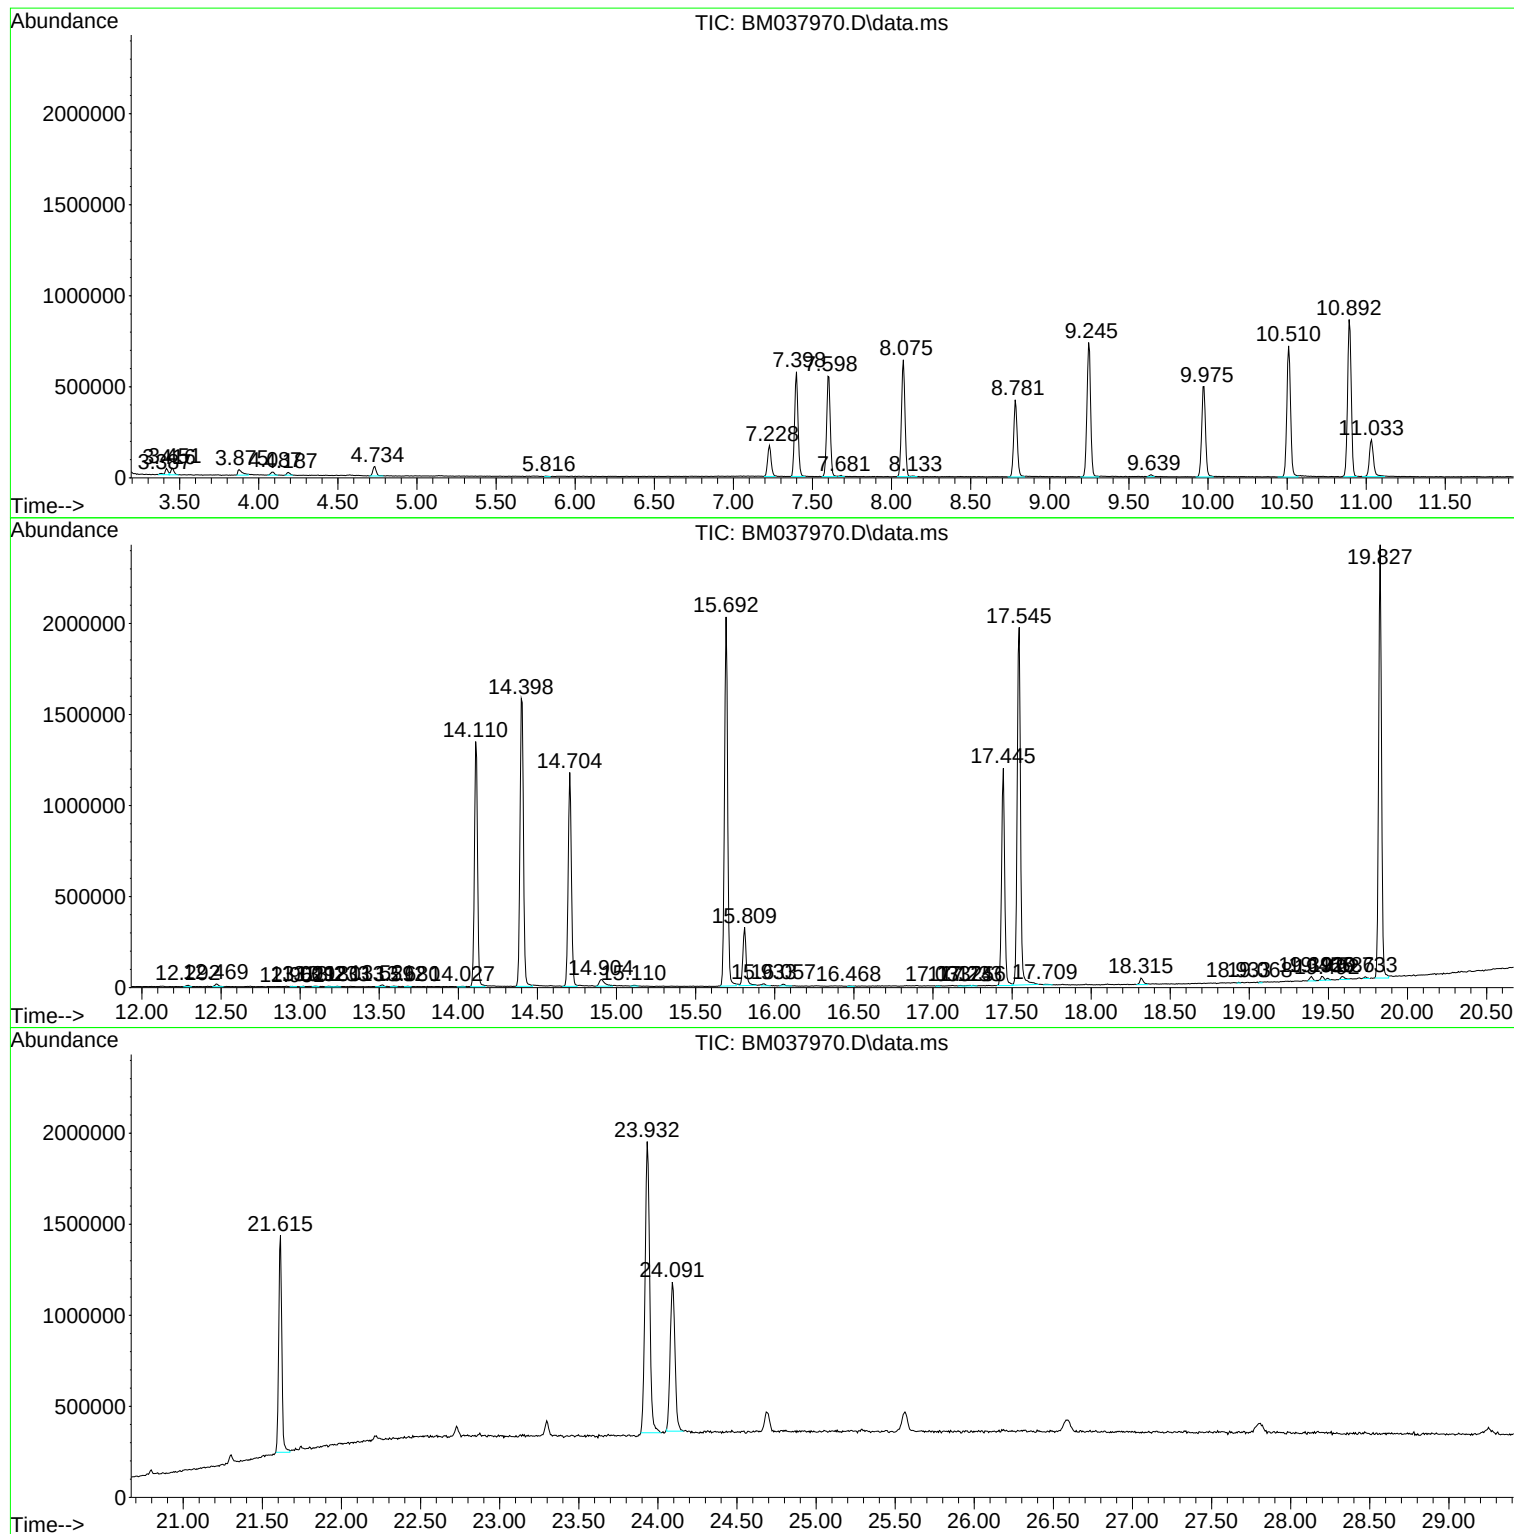

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037970.D
Acq On : 12 Dec 2022 17:38
Operator : CG/JU
Sample : N5948-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037970.D
Acq On : 12 Dec 2022 17:38
Operator : CG/JU
Sample : N5948-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
