

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037974.D
 Acq On : 12 Dec 2022 20:05
 Operator : CG/JU
 Sample : N5948-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	36	39	44	rVB	31659	38250	1.16%	0.113%
2	3.870	113	116	128	rBV	45536	91366	2.78%	0.270%
3	4.087	149	153	159	rVB	20513	32755	1.00%	0.097%
4	4.187	165	170	175	rBV	29861	40025	1.22%	0.118%
5	4.575	233	236	239	rVB5	3490	3692	0.11%	0.011%
6	4.728	257	262	267	rBV3	16418	24042	0.73%	0.071%
7	5.152	332	334	340	rVB6	3785	4705	0.14%	0.014%
8	5.746	430	435	440	rBV7	3563	8061	0.25%	0.024%
9	5.969	471	473	478	rBV4	1953	3996	0.12%	0.012%
10	6.105	490	496	498	rVB6	2435	3578	0.11%	0.011%
11	6.575	574	576	581	rBV6	2217	3506	0.11%	0.010%
12	7.228	681	687	696	rVB	177260	277492	8.44%	0.820%
13	7.399	707	716	727	rBV	608449	947269	28.81%	2.799%
14	7.599	742	750	759	rBV	533997	818523	24.90%	2.418%
15	7.681	761	764	768	rVB5	4483	6037	0.18%	0.018%
16	8.075	824	831	838	rBV	646623	1002734	30.50%	2.962%
17	8.781	943	951	962	rBV	410177	642090	19.53%	1.897%
18	9.246	1023	1030	1042	rBV	809360	1293500	39.35%	3.821%
19	9.640	1093	1097	1102	rVB5	4469	6634	0.20%	0.020%
20	9.969	1146	1153	1161	rBV	511106	829781	25.24%	2.451%
21	10.110	1174	1177	1180	rBV5	2226	3878	0.12%	0.011%
22	10.510	1237	1245	1254	rBV	672957	1120898	34.10%	3.312%
23	10.893	1301	1310	1319	rBV	884706	1420101	43.20%	4.196%
24	11.028	1326	1333	1347	rBV	308741	563495	17.14%	1.665%
25	11.669	1437	1442	1446	rBV5	2293	3901	0.12%	0.012%
26	12.010	1498	1500	1504	rBV4	2203	3583	0.11%	0.011%
27	12.122	1515	1519	1524	rVB6	2631	4283	0.13%	0.013%
28	12.469	1573	1578	1584	rVB2	15213	25365	0.77%	0.075%
29	12.669	1609	1612	1614	rBV3	2496	3554	0.11%	0.010%
30	13.592	1764	1769	1774	rBV3	7246	12744	0.39%	0.038%
31	14.110	1850	1857	1872	rBV	1494534	2001549	60.88%	5.913%
32	14.398	1899	1906	1917	rBV	1880611	2637704	80.24%	7.793%
33	14.704	1951	1958	1966	rBV	1186731	1695336	51.57%	5.009%
34	14.904	1986	1992	2004	rBV2	43710	102371	3.11%	0.302%
35	15.116	2023	2028	2032	rBV8	7548	12161	0.37%	0.036%
36	15.692	2119	2126	2139	rBV	2274487	3133686	95.32%	9.258%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037974.D
 Acq On : 12 Dec 2022 20:05
 Operator : CG/JU
 Sample : N5948-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.810	2140	2146	2156	rVB	299717	441632	13.43%	1.305%
38	15.928	2162	2166	2171	rVB5	11174	17632	0.54%	0.052%
39	16.210	2211	2214	2219	rVB5	1849	3334	0.10%	0.010%
40	16.563	2270	2274	2277	rBV3	2176	3395	0.10%	0.010%
41	17.122	2365	2369	2373	rBV6	2438	3908	0.12%	0.012%
42	17.445	2417	2424	2434	rBV	1089826	1622027	49.34%	4.792%
43	17.539	2434	2440	2454	rVV	2085650	3046553	92.67%	9.001%
44	17.957	2509	2511	2514	rBV3	3356	3383	0.10%	0.010%
45	18.092	2532	2534	2539	rVB5	3188	4444	0.14%	0.013%
46	18.316	2568	2572	2578	rBV7	17355	25899	0.79%	0.077%
47	19.392	2751	2755	2759	rVB2	25717	33280	1.01%	0.098%
48	19.457	2763	2766	2770	rBV2	21378	31058	0.94%	0.092%
49	19.586	2785	2788	2793	rBV5	20492	31473	0.96%	0.093%
50	19.827	2823	2829	2837	rBV	2540491	3280912	99.80%	9.693%
51	21.610	3128	3132	3142	rBV	1143287	1549704	47.14%	4.578%
52	23.933	3520	3527	3541	rVB	1607915	3287446	100.00%	9.712%
53	24.092	3548	3554	3566	rVB2	786507	1639264	49.86%	4.843%




Sum of corrected areas: 33847989

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

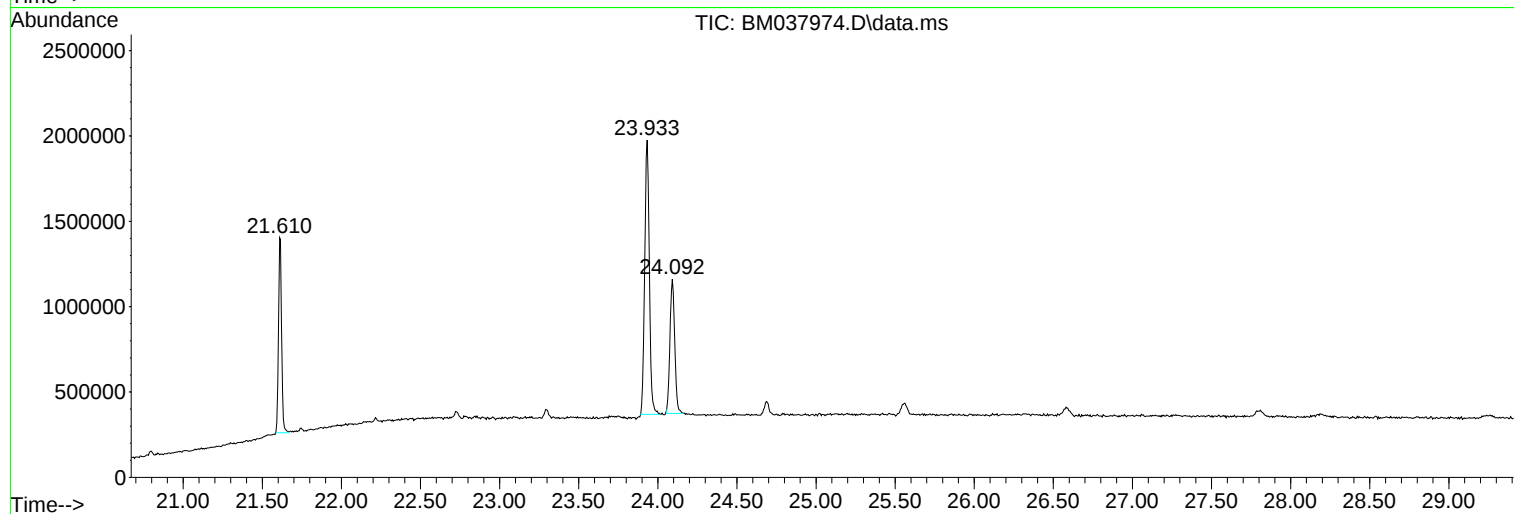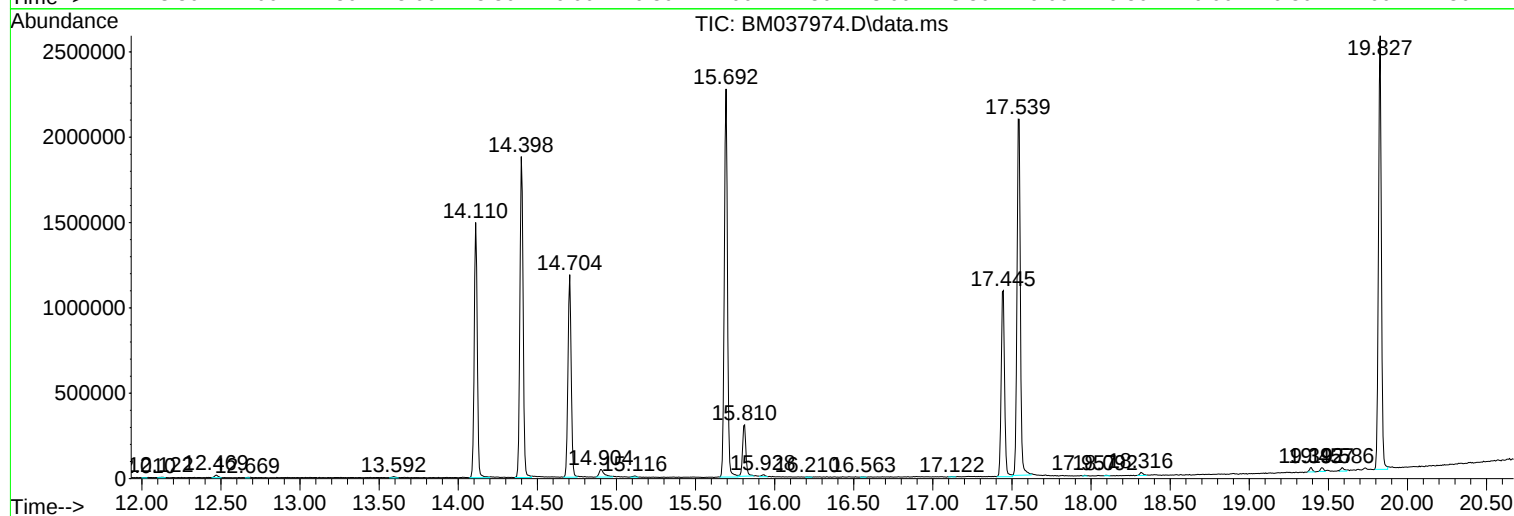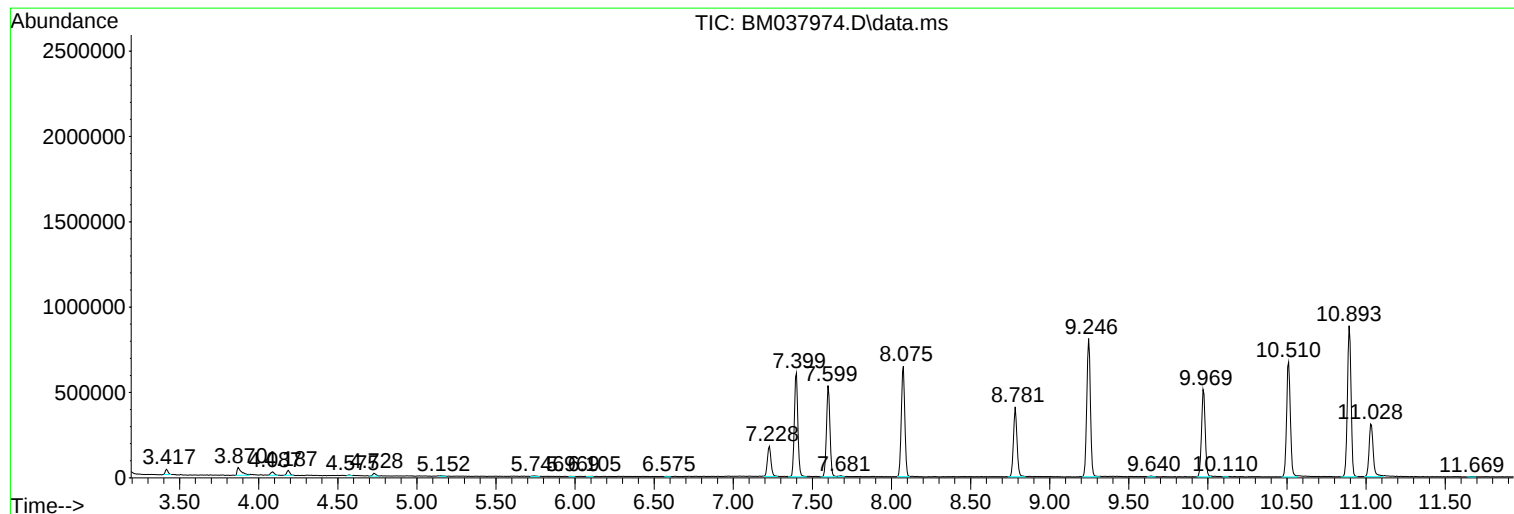

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037974.D
Acq On : 12 Dec 2022 20:05
Operator : CG/JU
Sample : N5948-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
