

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037975.D
 Acq On : 12 Dec 2022 20:42
 Operator : CG/JU
 Sample : N5948-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	36	39	47	rVB	31882	41724	1.37%	0.133%
2	3.810	105	106	109	rBV3	2635	3076	0.10%	0.010%
3	3.875	114	117	125	rBV	34607	72184	2.37%	0.229%
4	4.087	148	153	158	rVB2	18625	32268	1.06%	0.103%
5	4.134	158	161	164	rBV5	1912	3144	0.10%	0.010%
6	4.187	166	170	177	rVB	37013	50162	1.64%	0.159%
7	4.728	258	262	270	rVB4	19255	30539	1.00%	0.097%
8	5.681	422	424	429	rVB4	2583	3107	0.10%	0.010%
9	6.228	513	517	521	rVB5	2033	3477	0.11%	0.011%
10	7.228	681	687	694	rBV	165527	250989	8.23%	0.798%
11	7.398	709	716	727	rVB	550243	846379	27.74%	2.691%
12	7.598	743	750	758	rBV	518758	804197	26.36%	2.557%
13	7.681	761	764	767	rVB5	4008	4902	0.16%	0.016%
14	7.892	795	800	804	rBV6	2295	3905	0.13%	0.012%
15	8.075	824	831	838	rBV	621972	959667	31.45%	3.051%
16	8.781	944	951	962	rBV	397199	628455	20.60%	1.998%
17	9.245	1022	1030	1042	rBV	715711	1149151	37.66%	3.653%
18	9.639	1094	1097	1103	rVB5	3820	5778	0.19%	0.018%
19	9.969	1145	1153	1165	rBV	476874	787894	25.82%	2.505%
20	10.510	1238	1245	1254	rBV	672597	1097089	35.96%	3.488%
21	10.610	1260	1262	1266	rVB4	3679	3437	0.11%	0.011%
22	10.892	1302	1310	1321	rBV	850709	1361270	44.62%	4.328%
23	11.033	1327	1334	1342	rBV	245987	445463	14.60%	1.416%
24	11.563	1421	1424	1428	rBV5	1785	3510	0.12%	0.011%
25	12.127	1518	1520	1524	rVB5	2354	3058	0.10%	0.010%
26	12.469	1574	1578	1584	rVB2	13974	20706	0.68%	0.066%
27	14.110	1851	1857	1868	rBV	1350586	1791648	58.72%	5.696%
28	14.398	1900	1906	1918	rBV	1615737	2359431	77.33%	7.501%
29	14.704	1951	1958	1968	rBV	1152024	1650250	54.09%	5.246%
30	14.904	1987	1992	2001	rBV2	41833	93659	3.07%	0.298%
31	15.121	2023	2029	2031	rVB6	5576	8145	0.27%	0.026%
32	15.174	2037	2038	2043	rVB5	2446	3185	0.10%	0.010%
33	15.692	2119	2126	2139	rVV	2041419	2834825	92.91%	9.012%
34	15.810	2140	2146	2154	rVV	292853	415389	13.61%	1.321%
35	15.933	2163	2167	2175	rVB7	11831	21780	0.71%	0.069%
36	16.580	2273	2277	2282	rVB5	1697	3300	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
 Data File : BM037975.D
 Acq On : 12 Dec 2022 20:42
 Operator : CG/JU
 Sample : N5948-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.892	2327	2330	2335	rBV6	2615	3810	0.12%	0.012%
38	17.227	2384	2387	2390	rBV4	2254	3220	0.11%	0.010%
39	17.445	2418	2424	2434	rBV	1140566	1610085	52.77%	5.119%
40	17.545	2434	2441	2453	rVV	1964707	2815893	92.29%	8.952%
41	18.098	2533	2535	2537	rBV2	4221	3985	0.13%	0.013%
42	18.321	2568	2573	2578	rBV7	10536	17684	0.58%	0.056%
43	19.392	2751	2755	2759	rVB3	25394	31975	1.05%	0.102%
44	19.462	2763	2767	2770	rBV	21541	32293	1.06%	0.103%
45	19.586	2785	2788	2795	rBV8	16637	27582	0.90%	0.088%
46	19.733	2810	2813	2817	rBV6	9736	13661	0.45%	0.043%
47	19.827	2823	2829	2840	rBV	2346167	3028400	99.26%	9.627%
48	21.609	3128	3132	3143	rBV	1055622	1485477	48.69%	4.722%
49	23.933	3520	3527	3540	rBV	1478374	3051051	100.00%	9.699%
50	24.091	3548	3554	3562	rVB	760053	1533684	50.27%	4.876%




Sum of corrected areas: 31455943

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037975.D
Acq On : 12 Dec 2022 20:42
Operator : CG/JU
Sample : N5948-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

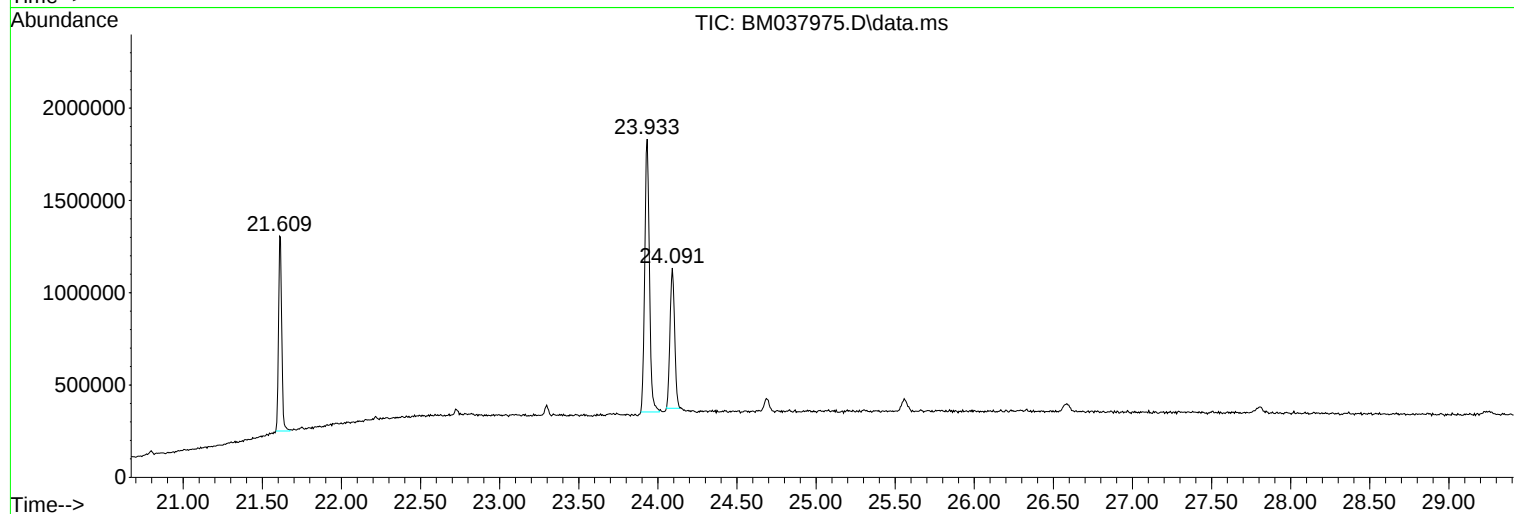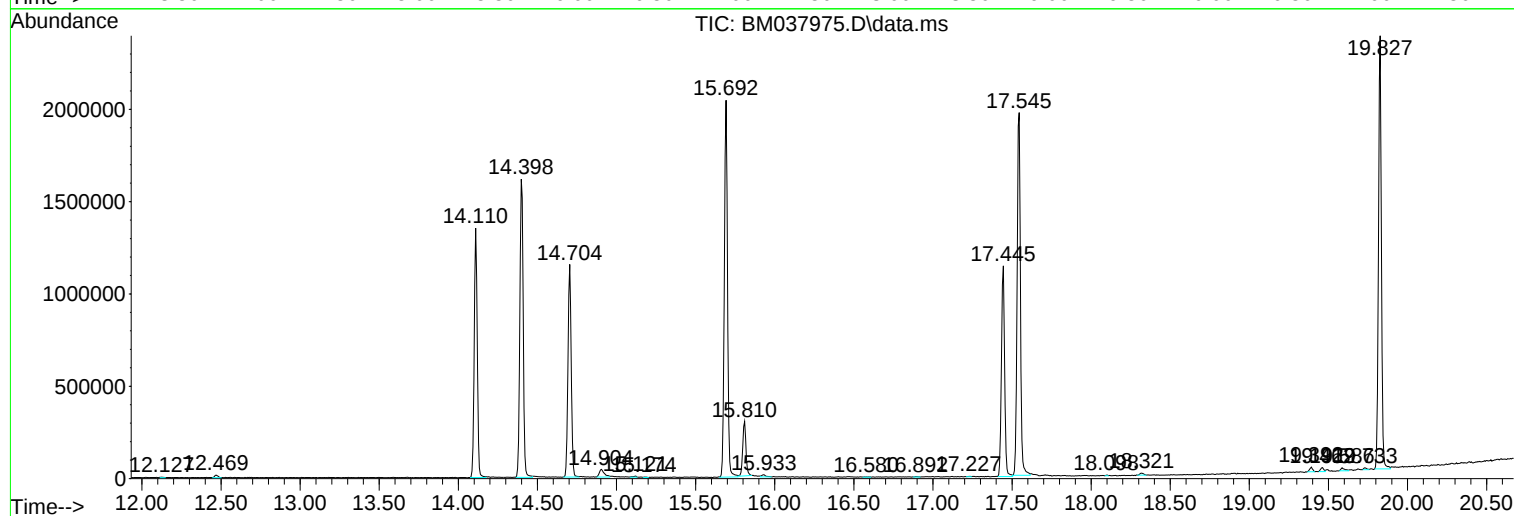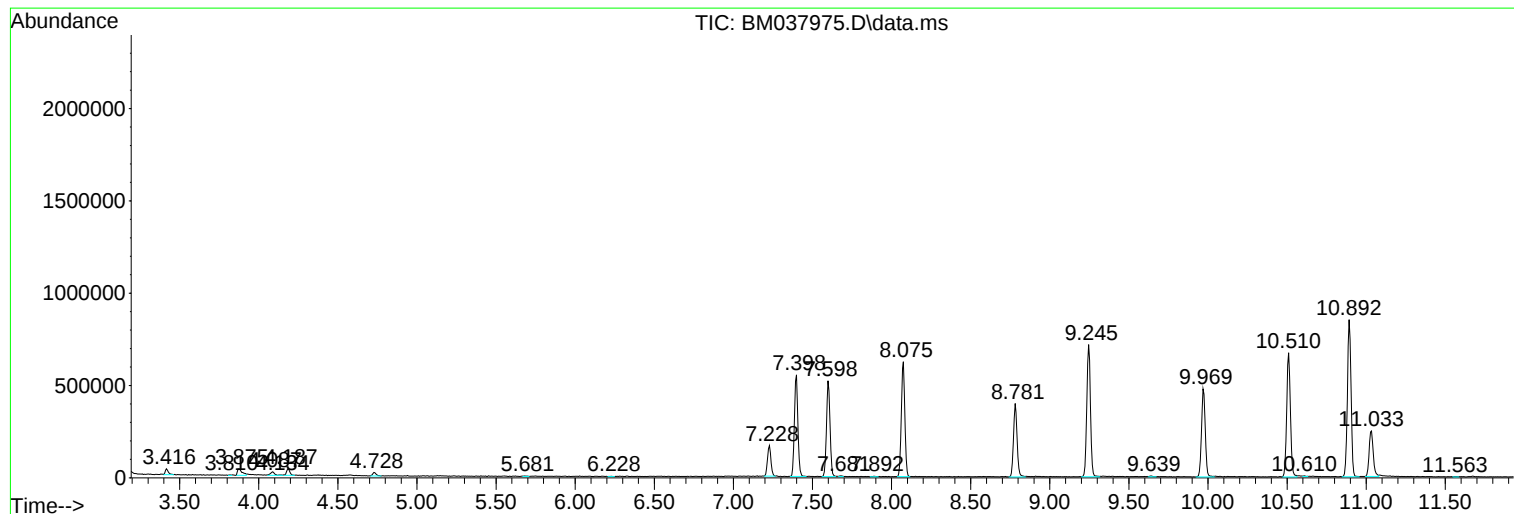

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037975.D
Acq On : 12 Dec 2022 20:42
Operator : CG/JU
Sample : N5948-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121222\
Data File : BM037975.D
Acq On : 12 Dec 2022 20:42
Operator : CG/JU
Sample : N5948-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZB3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc