

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
 Data File : BM048965.D
 Acq On : 12 Dec 2024 10:12
 Operator : RC/JU
 Sample : PB165140BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK140

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	36	rVB	67280	85388	2.70%	0.241%
2	3.540	90	94	111	rBV	754057	1092204	34.53%	3.085%
3	3.857	145	148	154	rVB2	19136	23946	0.76%	0.068%
4	4.075	183	185	190	rVB5	6540	7237	0.23%	0.020%
5	5.363	402	404	407	rBV4	3042	4149	0.13%	0.012%
6	6.757	634	641	650	rBV	743879	1161156	36.71%	3.279%
7	6.916	662	668	677	rBV	656769	1011806	31.98%	2.858%
8	7.110	694	701	713	rBV	782865	1155551	36.53%	3.264%
9	7.569	773	779	788	rBV	572533	909045	28.74%	2.567%
10	8.275	892	899	915	rBV	844320	1333939	42.17%	3.767%
11	8.398	918	920	923	rVB4	3300	3339	0.11%	0.009%
12	8.716	966	974	985	rBV	642452	1071069	33.86%	3.025%
13	9.181	1049	1053	1054	rBV3	3110	3992	0.13%	0.011%
14	9.428	1088	1095	1106	rBV	446225	719939	22.76%	2.033%
15	9.628	1126	1129	1132	rVB4	2707	3541	0.11%	0.010%
16	9.963	1179	1186	1196	rBV	757459	1211812	38.31%	3.422%
17	10.339	1242	1250	1258	rBV	722375	1207959	38.19%	3.412%
18	10.475	1266	1273	1285	rBV	721610	1268798	40.11%	3.583%
19	11.022	1360	1366	1370	rBV7	2554	5877	0.19%	0.017%
20	11.181	1387	1393	1396	rBV5	2828	4510	0.14%	0.013%
21	11.933	1517	1521	1531	rVV7	9135	20614	0.65%	0.058%
22	13.063	1710	1713	1716	rBV4	2532	3262	0.10%	0.009%
23	13.627	1802	1809	1820	rBV	1308914	1781959	56.33%	5.033%
24	13.698	1820	1821	1826	rVB4	3347	3239	0.10%	0.009%
25	13.898	1848	1855	1869	rVB	1568060	2219406	70.16%	6.268%
26	14.051	1878	1881	1885	rBV3	2164	3434	0.11%	0.010%
27	14.204	1899	1907	1918	rBV	978399	1433396	45.31%	4.048%
28	14.416	1936	1943	1962	rBV	459157	766830	24.24%	2.166%
29	14.580	1969	1971	1976	rVB6	3340	3814	0.12%	0.011%
30	14.969	2034	2037	2041	rBV5	2352	3181	0.10%	0.009%
31	15.204	2070	2077	2089	rBV	2045599	2678185	84.66%	7.564%
32	15.321	2091	2097	2108	rVV	415014	555653	17.57%	1.569%
33	15.445	2114	2118	2121	rVV5	6582	9690	0.31%	0.027%
34	16.257	2254	2256	2259	rBV3	2928	3245	0.10%	0.009%
35	16.745	2335	2339	2342	rVB6	3314	3474	0.11%	0.010%
36	16.951	2368	2374	2383	rVV	1152696	1589305	50.24%	4.489%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048965.D
Acq On : 12 Dec 2024 10:12
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK140

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

37	17.051	2383	2391	2408	rVV	2109959	2812846	88.92%	7.944%
38	17.509	2466	2469	2471	rBV3	3120	3191	0.10%	0.009%
39	18.457	2627	2630	2633	rBV4	2513	3480	0.11%	0.010%
40	18.745	2678	2679	2683	rBV4	3453	4354	0.14%	0.012%
41	18.915	2704	2708	2712	rVB6	20083	27020	0.85%	0.076%
42	18.986	2717	2720	2725	rVB	18241	22138	0.70%	0.063%
43	19.351	2776	2782	2793	rBV	2434513	3163397	100.00%	8.934%
44	21.180	3087	3093	3100	rBV	1170461	1533323	48.47%	4.330%
45	23.797	3530	3538	3552	rBV	1324193	2913266	92.09%	8.228%
46	23.991	3563	3571	3580	rBV	713798	1561117	49.35%	4.409%




Sum of corrected areas: 35408076

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048965.D
Acq On : 12 Dec 2024 10:12
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

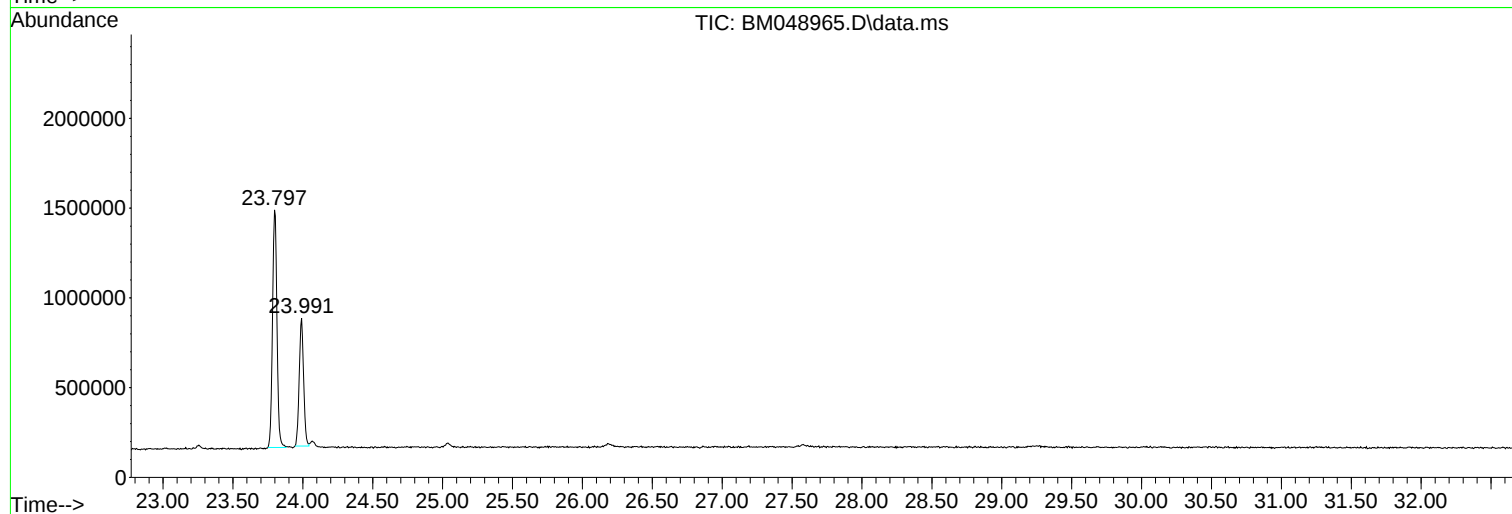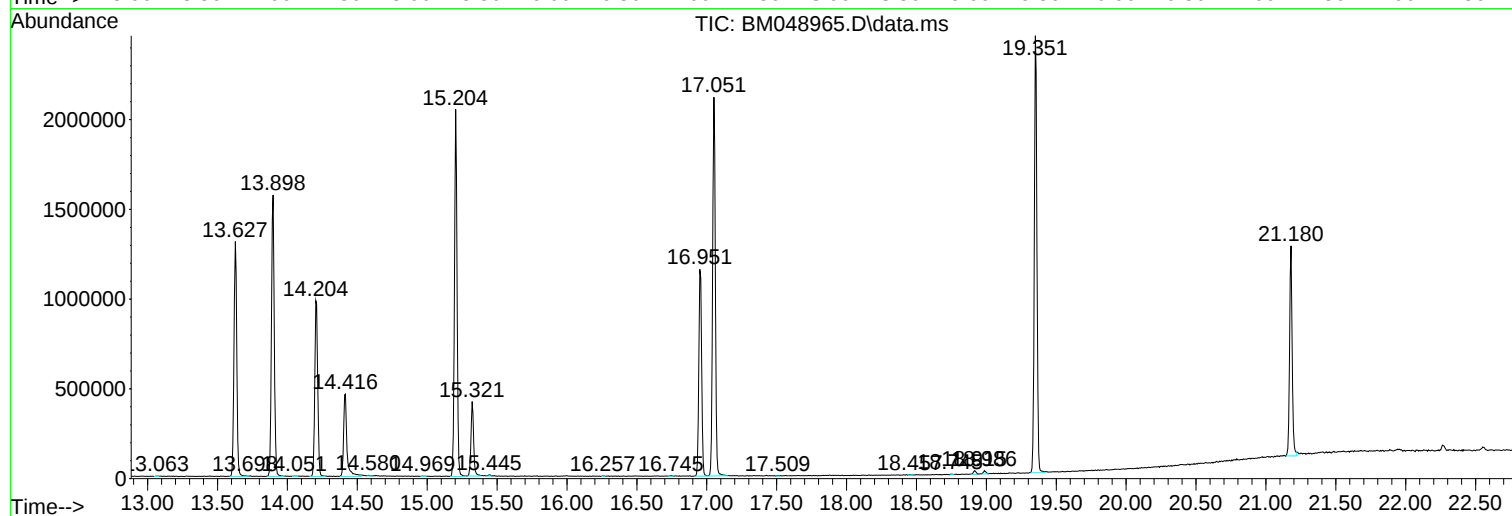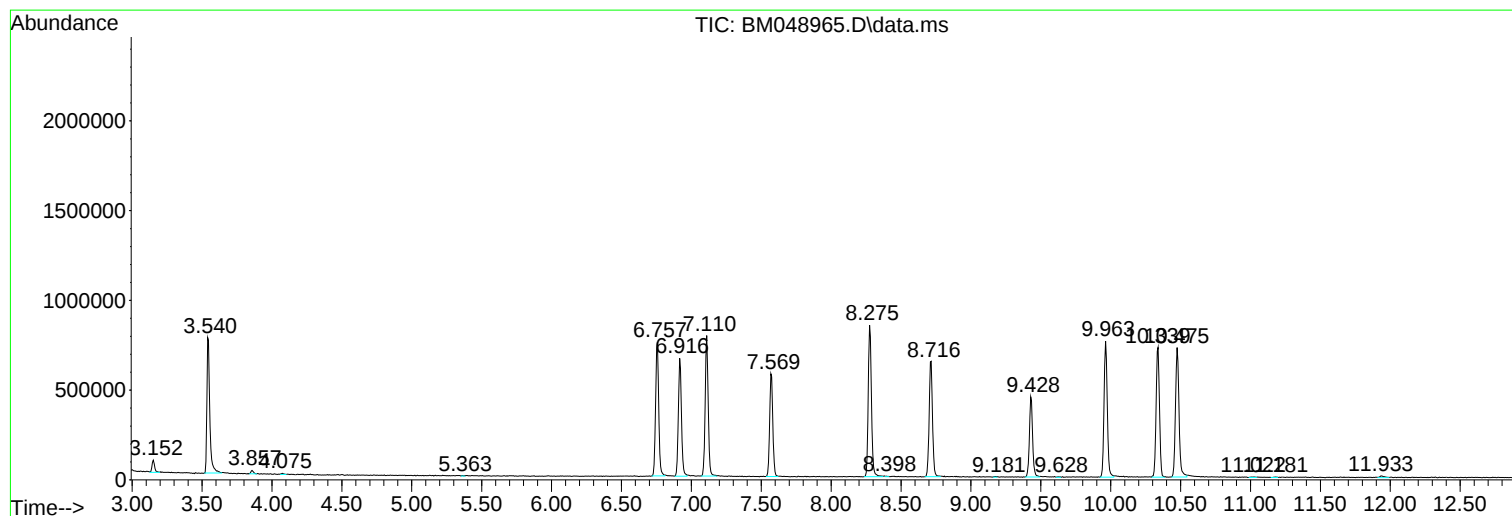

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048965.D
Acq On : 12 Dec 2024 10:12
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048965.D
Acq On : 12 Dec 2024 10:12
Operator : RC/JU
Sample : PB165140BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK140

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc