

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
 Data File : BM048966.D
 Acq On : 12 Dec 2024 10:51
 Operator : RC/JU
 Sample : PB165114BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	36	rVB	67241	86783	3.05%	0.270%
2	3.546	91	95	112	rBV	721600	1058934	37.19%	3.296%
3	3.857	145	148	154	rVB	17686	21979	0.77%	0.068%
4	4.075	183	185	187	rBV3	4532	3905	0.14%	0.012%
5	4.469	250	252	256	rVB3	5408	4368	0.15%	0.014%
6	5.416	412	413	417	rVB4	2995	3584	0.13%	0.011%
7	6.116	530	532	535	rVB4	2735	3029	0.11%	0.009%
8	6.163	535	540	541	rBV5	2759	4576	0.16%	0.014%
9	6.757	635	641	654	rBV	718871	1110237	39.00%	3.456%
10	6.916	662	668	678	rBV	620305	965721	33.92%	3.006%
11	7.110	694	701	714	rBV	739974	1100787	38.67%	3.426%
12	7.416	752	753	758	rVB4	3986	4781	0.17%	0.015%
13	7.569	773	779	789	rVB	514114	815025	28.63%	2.537%
14	8.122	871	873	878	rVB5	2580	2894	0.10%	0.009%
15	8.275	892	899	911	rBV	790533	1249528	43.89%	3.889%
16	8.528	939	942	945	rBV5	2411	2927	0.10%	0.009%
17	8.716	966	974	983	rBV	612170	997328	35.03%	3.104%
18	9.428	1088	1095	1104	rVV	411186	659915	23.18%	2.054%
19	9.963	1180	1186	1200	rBV	720021	1153255	40.51%	3.590%
20	10.339	1242	1250	1257	rVV	633430	1066056	37.45%	3.318%
21	10.475	1266	1273	1286	rBV	685757	1191919	41.87%	3.710%
22	10.781	1321	1325	1327	rBV4	2654	3404	0.12%	0.011%
23	10.881	1340	1342	1345	rVB4	3423	3633	0.13%	0.011%
24	10.910	1345	1347	1350	rBV4	3609	4194	0.15%	0.013%
25	11.098	1377	1379	1381	rBV3	2559	3076	0.11%	0.010%
26	11.939	1517	1522	1528	rBV6	7708	16003	0.56%	0.050%
27	13.627	1803	1809	1819	rBV	1174014	1589062	55.82%	4.946%
28	13.898	1848	1855	1867	rBV	1414302	2053906	72.14%	6.393%
29	14.210	1901	1908	1918	rBV	863903	1260281	44.27%	3.923%
30	14.416	1936	1943	1956	rBV	401239	650820	22.86%	2.026%
31	14.633	1978	1980	1986	rBV6	2160	3418	0.12%	0.011%
32	15.204	2071	2077	2087	rBV	1860859	2437605	85.62%	7.587%
33	15.321	2092	2097	2109	rVB	356326	473075	16.62%	1.472%
34	15.445	2115	2118	2123	rBV5	6728	9064	0.32%	0.028%
35	15.704	2159	2162	2164	rBV4	2787	3421	0.12%	0.011%
36	15.992	2209	2211	2215	rBV3	3902	6278	0.22%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048966.D
Acq On : 12 Dec 2024 10:51
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

37	16.733	2335	2337	2340	rBV3	2971	3379	0.12%	0.011%
38	16.951	2368	2374	2382	rBV	967578	1350982	47.45%	4.205%
39	17.051	2385	2391	2407	rVV2	1864961	2548869	89.53%	7.934%
40	17.880	2528	2532	2536	rBV7	2587	4500	0.16%	0.014%
41	18.921	2705	2709	2712	rBV4	16598	22912	0.80%	0.071%
42	18.992	2716	2721	2725	rVB3	12816	19616	0.69%	0.061%
43	19.027	2725	2727	2731	rBV3	3179	3729	0.13%	0.012%
44	19.168	2749	2751	2754	rBV4	5367	7047	0.25%	0.022%
45	19.356	2775	2783	2791	rBV	2103619	2846981	100.00%	8.861%
46	21.180	3087	3093	3102	rBV	946916	1297095	45.56%	4.037%
47	23.797	3530	3538	3549	rBV2	1240604	2662741	93.53%	8.288%
48	23.991	3563	3571	3579	rBV	593946	1335032	46.89%	4.155%


Sum of corrected areas: 32127654

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048966.D
Acq On : 12 Dec 2024 10:51
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

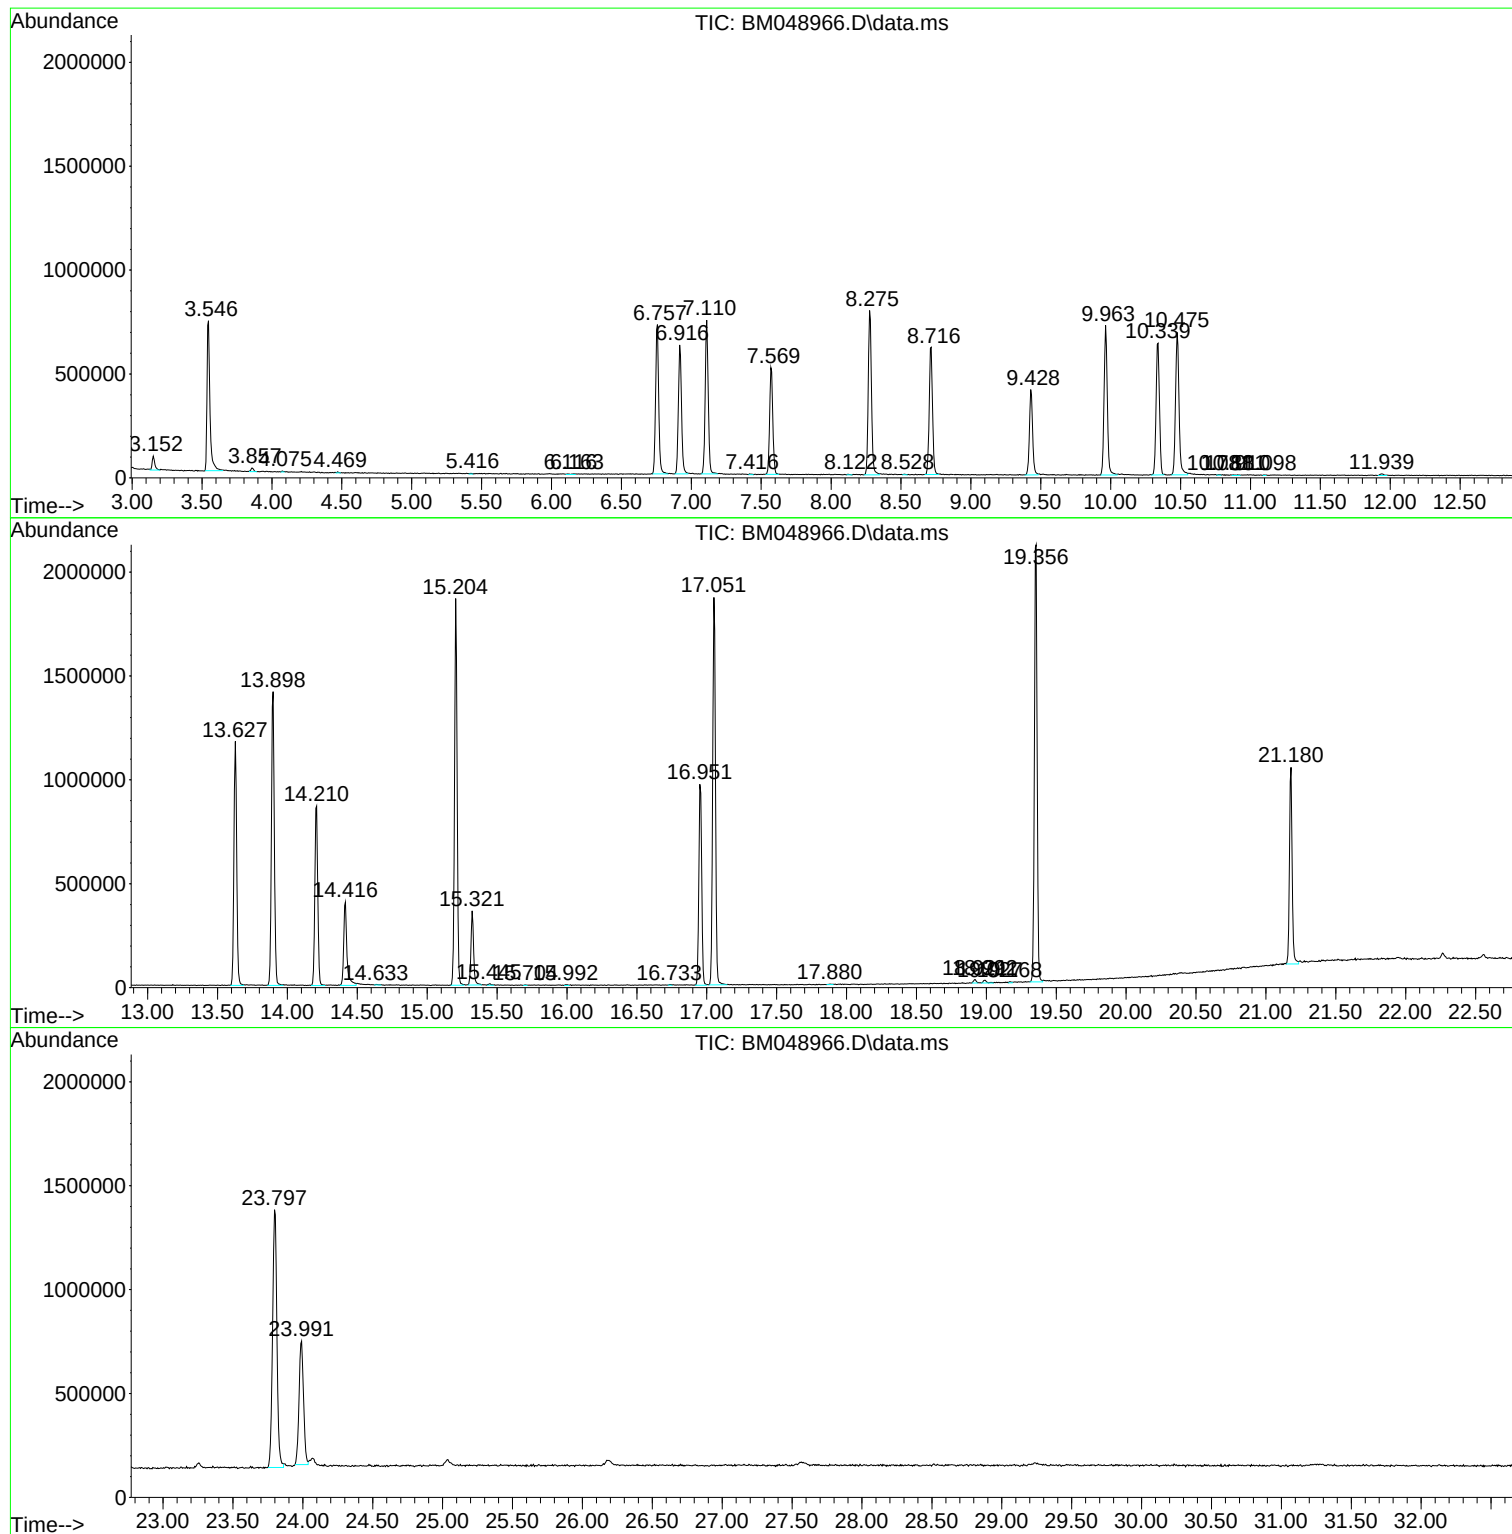

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048966.D
Acq On : 12 Dec 2024 10:51
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048966.D
Acq On : 12 Dec 2024 10:51
Operator : RC/JU
Sample : PB165114BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK114

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc