

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
 Data File : BM048970.D
 Acq On : 12 Dec 2024 13:39
 Operator : RC/JU
 Sample : PB165141BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK141

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	33	rBV	70040	83324	2.67%	0.235%
2	3.546	91	95	110	rBV	841906	1197195	38.33%	3.381%
3	3.857	145	148	154	rVB	19306	22234	0.71%	0.063%
4	4.075	181	185	190	rBV7	7227	10753	0.34%	0.030%
5	4.628	276	279	280	rBV3	2971	3454	0.11%	0.010%
6	5.699	459	461	463	rBV3	4060	3587	0.11%	0.010%
7	6.757	634	641	652	rVV	812568	1257549	40.27%	3.551%
8	6.916	662	668	680	rBV	695476	1080407	34.60%	3.051%
9	7.110	692	701	716	rBV	821124	1263094	40.44%	3.567%
10	7.340	738	740	743	rBV3	3376	3148	0.10%	0.009%
11	7.569	773	779	790	rVB	575910	924980	29.62%	2.612%
12	8.275	891	899	914	rBV	882974	1420169	45.47%	4.010%
13	8.469	928	932	936	rBV5	2877	5213	0.17%	0.015%
14	8.716	966	974	983	rBV	685238	1139409	36.48%	3.217%
15	8.928	1008	1010	1013	rVB4	3365	3329	0.11%	0.009%
16	9.181	1051	1053	1056	rVB4	3811	4324	0.14%	0.012%
17	9.428	1087	1095	1104	rBV	459815	741415	23.74%	2.094%
18	9.657	1131	1134	1138	rBV5	2348	3592	0.12%	0.010%
19	9.716	1141	1144	1148	rBV5	2032	3141	0.10%	0.009%
20	9.963	1179	1186	1201	rBV	816497	1306968	41.85%	3.691%
21	10.339	1242	1250	1258	rVB	733773	1202963	38.52%	3.397%
22	10.475	1266	1273	1285	rBV	770867	1340717	42.93%	3.786%
23	10.598	1292	1294	1299	rVB5	3686	5167	0.17%	0.015%
24	10.733	1315	1317	1323	rVB5	2908	4948	0.16%	0.014%
25	11.663	1473	1475	1478	rBV3	2815	3254	0.10%	0.009%
26	11.939	1518	1522	1525	rVV5	9497	14198	0.45%	0.040%
27	13.627	1803	1809	1819	rBV	1274335	1735895	55.58%	4.902%
28	13.792	1834	1837	1840	rVB4	2775	3197	0.10%	0.009%
29	13.898	1847	1855	1864	rBV	1555215	2238916	71.69%	6.322%
30	14.210	1901	1908	1915	rBV	919453	1367976	43.80%	3.863%
31	14.416	1934	1943	1957	rBV	429869	704166	22.55%	1.988%
32	14.574	1969	1970	1977	rVB7	2963	4202	0.13%	0.012%
33	15.204	2070	2077	2089	rBV	2023840	2662479	85.25%	7.518%
34	15.321	2091	2097	2108	rVV	378720	501997	16.07%	1.418%
35	15.445	2113	2118	2125	rVB10	6307	12692	0.41%	0.036%
36	16.739	2335	2338	2341	rBV4	3591	4858	0.16%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048970.D
Acq On : 12 Dec 2024 13:39
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK141

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Title : SVOA CALIBRATION

37	16.951	2369	2374	2381	rBV	1040914	1463108	46.85%	4.132%
38	17.051	2385	2391	2405	rVB	2038623	2741631	87.79%	7.742%
39	17.445	2454	2458	2462	rBV4	2570	4339	0.14%	0.012%
40	18.262	2593	2597	2600	rBV4	2278	3715	0.12%	0.010%
41	18.380	2614	2617	2618	rBV3	3216	3307	0.11%	0.009%
42	18.527	2639	2642	2645	rBV5	2872	3689	0.12%	0.010%
43	18.915	2705	2708	2713	rBV5	17580	24348	0.78%	0.069%
44	18.986	2717	2720	2725	rVB3	15063	20684	0.66%	0.058%
45	19.351	2776	2782	2793	rBV	2471807	3123013	100.00%	8.819%
46	21.180	3087	3093	3102	rBV	1022648	1412152	45.22%	3.988%
47	23.797	3530	3538	3550	rBV2	1333871	2878441	92.17%	8.128%
48	23.986	3563	3570	3579	rBV	641473	1449549	46.42%	4.093%




Sum of corrected areas: 35412886

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048970.D
Acq On : 12 Dec 2024 13:39
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

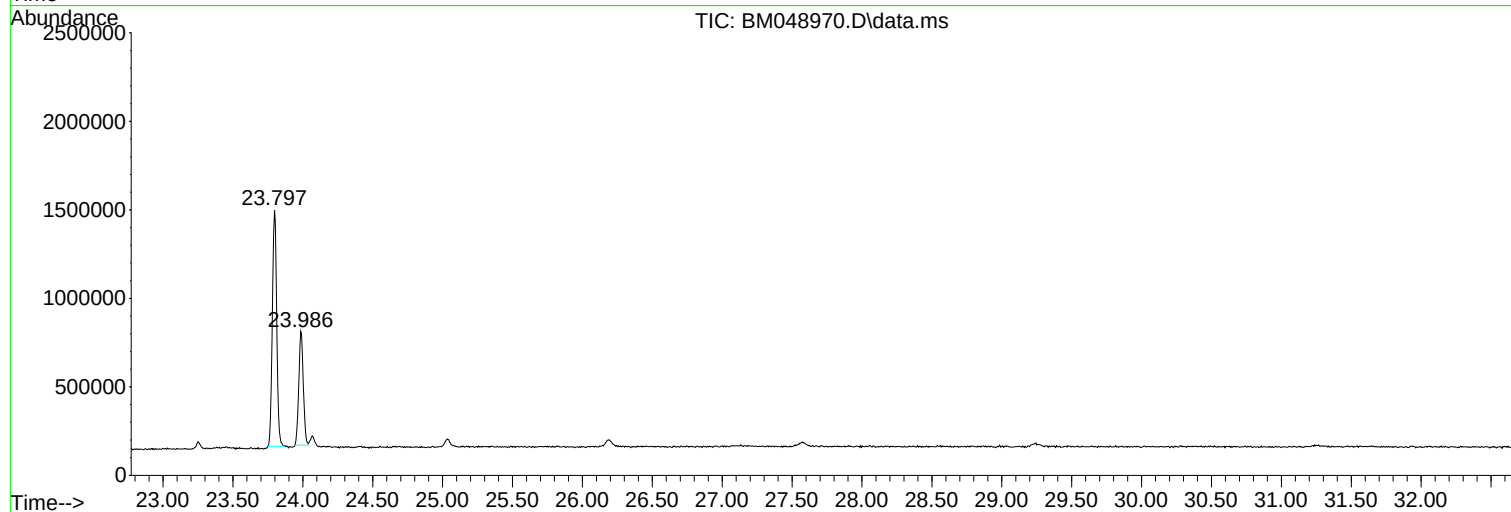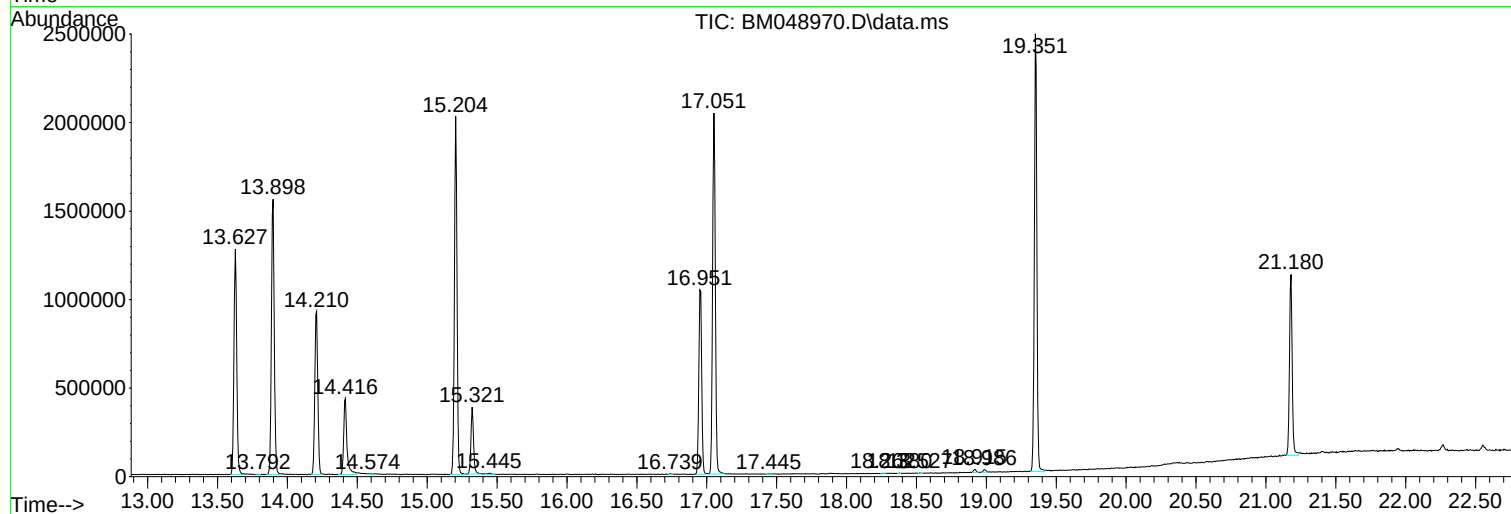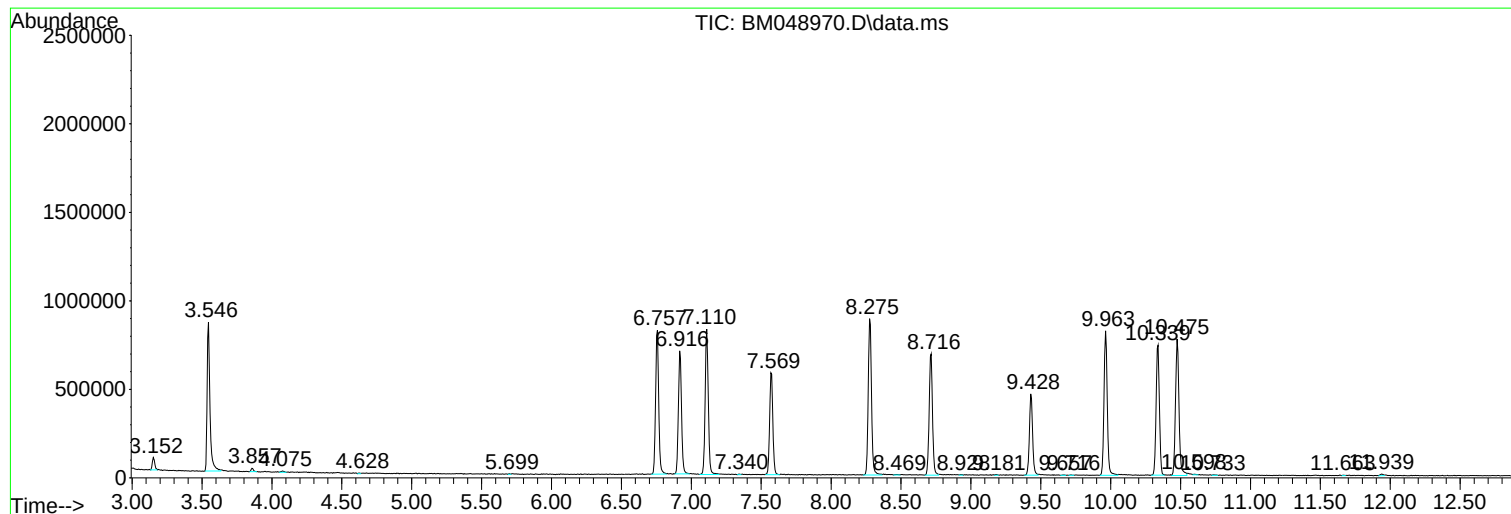

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048970.D
Acq On : 12 Dec 2024 13:39
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121224\
Data File : BM048970.D
Acq On : 12 Dec 2024 13:39
Operator : RC/JU
Sample : PB165141BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK141

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc