

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
 Data File : BM003520.D
 Acq On : 13 Dec 2015 21:49
 Operator : UM/IZ
 Sample : G4722-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C6

Quant Time: Dec 14 05:46:02 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 14 04:23:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	70227	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	300459	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	153076	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	303387	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	307891	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	302963	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	2203	1.56	ng/uL	0.00
5) Phenol-d5	6.89	99	43685	7.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	115187	37.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	142252	30.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	83441	17.74	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	84568	41.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	89479	41.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	144590	34.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	8654	1.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	441590	38.37	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	553223	39.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	8583	4.16	ng/ul	0.00
58) Fluorene-d10	15.36	176	378275	38.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	45225	29.14	ng/ul	0.00
71) Anthracene-d10	17.22	188	521974	38.73	ng/ul	0.00
79) Pyrene-d10	19.52	212	556823	36.94	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	490206	33.54	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.79	165	2452	1.13 ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003520.D
Acq On : 13 Dec 2015 21:49
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Time: Dec 14 05:46:02 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 14 04:23:11 2015
Response via : Initial Calibration

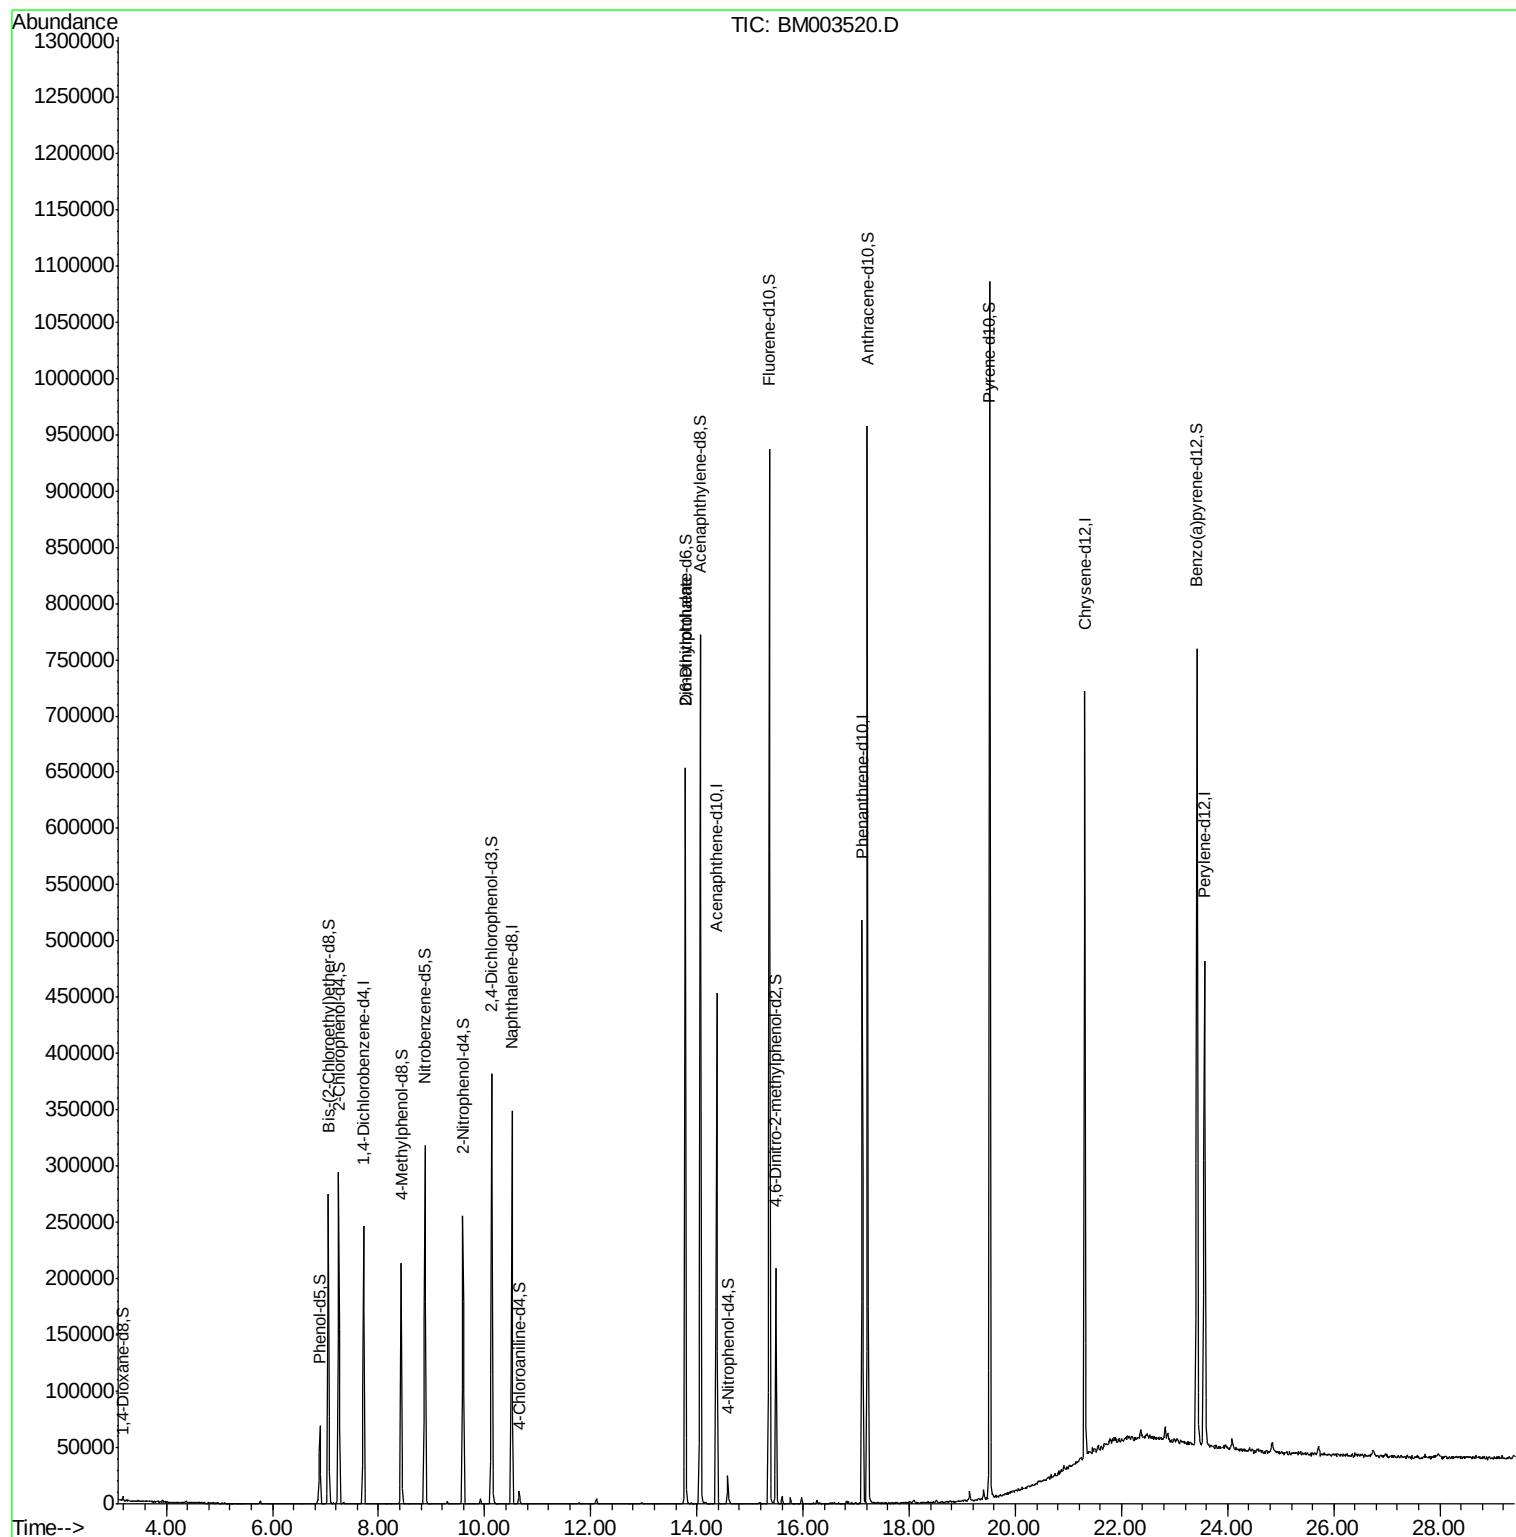

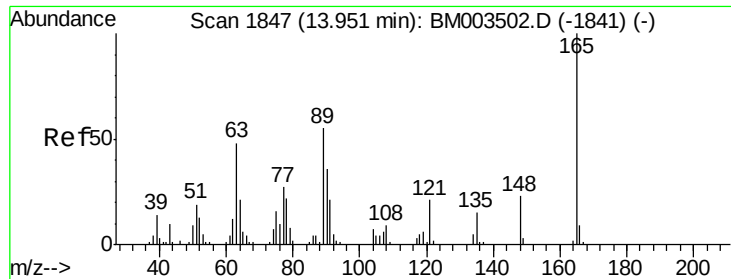

#46

2,6-Dinitrotoluene

Concen: 1.13 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.16 min

Lab File: BM003520.D


Acq: 13 Dec 2015 21:49

Instrument :

BNA_M

ClientSampleId :

C04C6

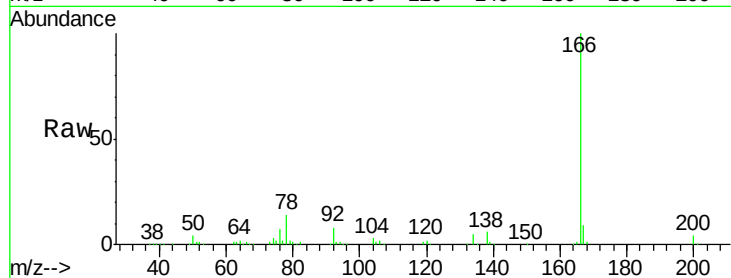

Tgt Ion:	165	Resp:	2452
Ion Ratio	Lower	Upper	
165	100		
89	0.0	42.0	63.0#
121	32.5	16.6	24.8#

