

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
 Data File : BM003525.D
 Acq On : 14 Dec 2015 00:49
 Operator : UM/IZ
 Sample : G4722-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D7

Quant Time: Dec 14 05:46:48 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 14 04:23:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	73790	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	330696	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	176301	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	335784	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	294179	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	284695	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	2361	1.59	ng/uL	0.00
5) Phenol-d5	6.89	99	55649	9.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	128780	39.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	166890	34.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	107172	21.69	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	99657	44.18	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	109159	46.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	184786	39.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	2503	0.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	585484	44.17	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	720518	44.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	12978	5.46	ng/ul	0.01
58) Fluorene-d10	15.37	176	485433	42.56	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	60137	35.00	ng/ul	0.00
71) Anthracene-d10	17.22	188	657627	44.08	ng/ul	0.00
79) Pyrene-d10	19.52	212	647612	44.97	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	556598	40.52	ng/ul	0.00


Target Compounds					Qvalue
46) 2,6-Dinitrotoluene	13.79	165	3466	1.39 ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003525.D
Acq On : 14 Dec 2015 00:49
Operator : UM/IZ
Sample : G4722-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C04D7

Quant Time: Dec 14 05:46:48 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 14 04:23:11 2015
Response via : Initial Calibration

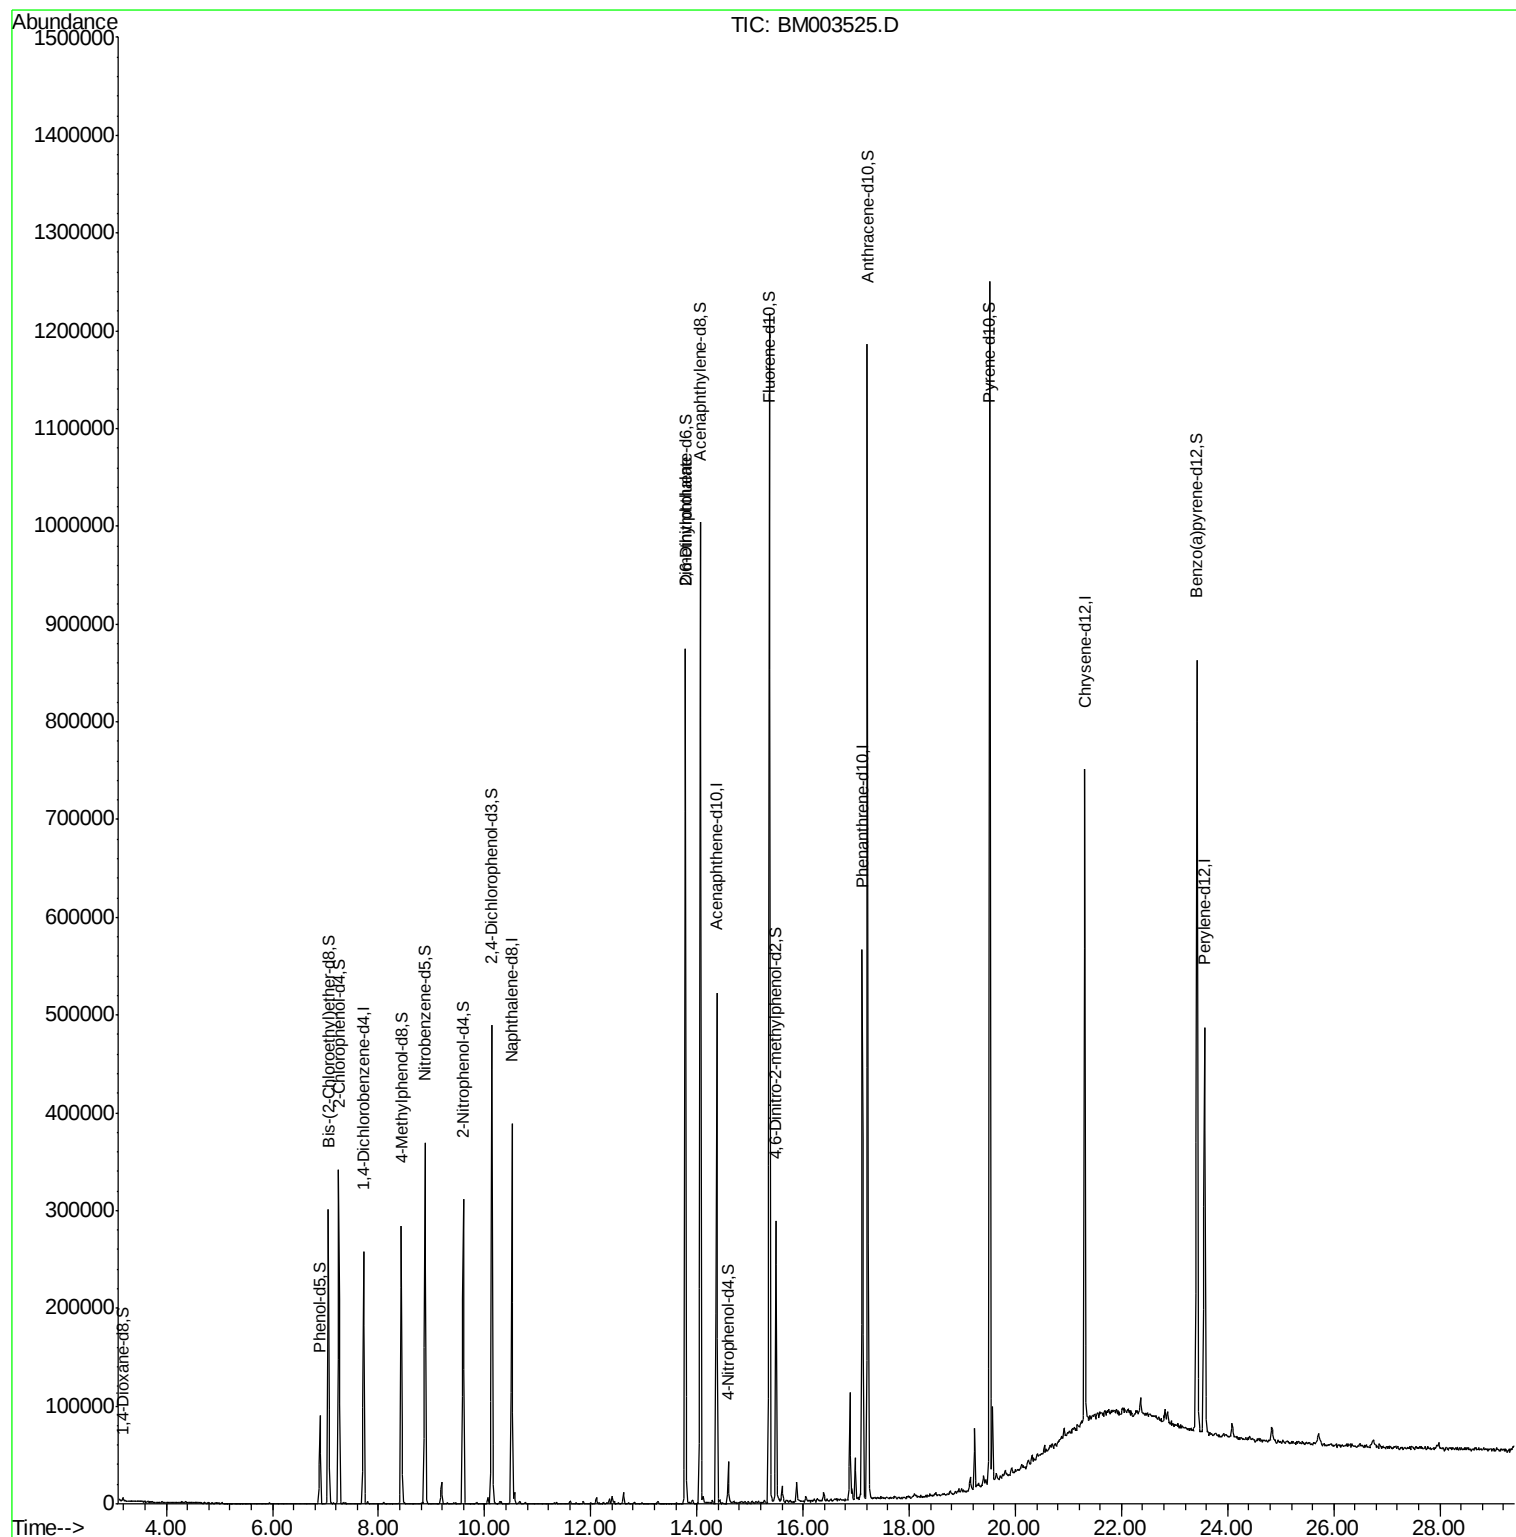

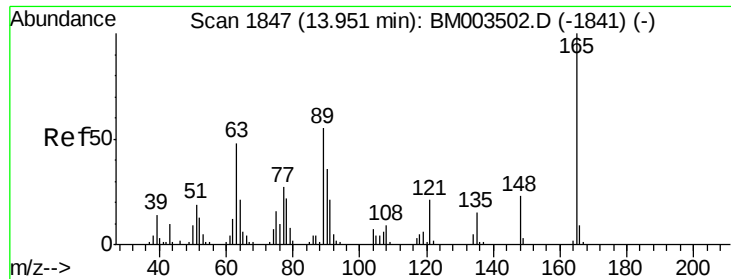

#46

2,6-Dinitrotoluene

Concen: 1.39 ng/ul

RT: 13.79 min Scan# 1819

Delta R.T. -0.16 min

Lab File: BM003525.D


Acq: 14 Dec 2015 00:49

Instrument :

BNA_M

ClientSampleId :

C04D7

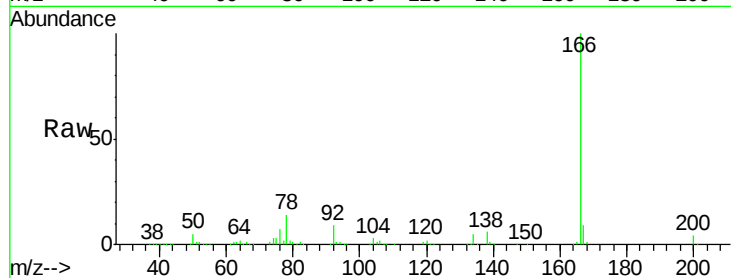

Tgt Ion:	165	Resp:	3466
Ion Ratio	Lower	Upper	
165	100		
89	0.0	42.0	63.0#
121	34.4	16.6	24.8#

