

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003527.D
 Acq On : 14 Dec 2015 02:01
 Operator : UM/IZ
 Sample : G4722-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D8

Quant Time: Dec 14 05:47:06 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 14 04:23:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	68518	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	318186	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.37	164	178326	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.12	188	350098	20.00	ng/ul	0.00
78) Chrysene-d12	21.31	240	315097	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	299258	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	1274	0.92	ng/uL	0.00
5) Phenol-d5	6.89	99	33864	6.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	75191	24.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	97960	21.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	65822	14.34	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	56057	25.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	61240	26.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	112500	25.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	132492	26.03	ng/ul	0.00
44) Dimethylphthalate-d6	13.78	166	363721	27.13	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	421775	25.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.59	143	6900	2.87	ng/ul	0.01
58) Fluorene-d10	15.36	176	290845	25.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.49	200	24009	13.40	ng/ul	0.00
71) Anthracene-d10	17.22	188	396320	25.48	ng/ul	0.00
79) Pyrene-d10	19.52	212	403362	26.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	316304	21.91	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.83	163	49029	3.55	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003527.D
Acq On : 14 Dec 2015 02:01
Operator : UM/IZ
Sample : G4722-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D8

Quant Time: Dec 14 05:47:06 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 14 04:23:11 2015
Response via : Initial Calibration

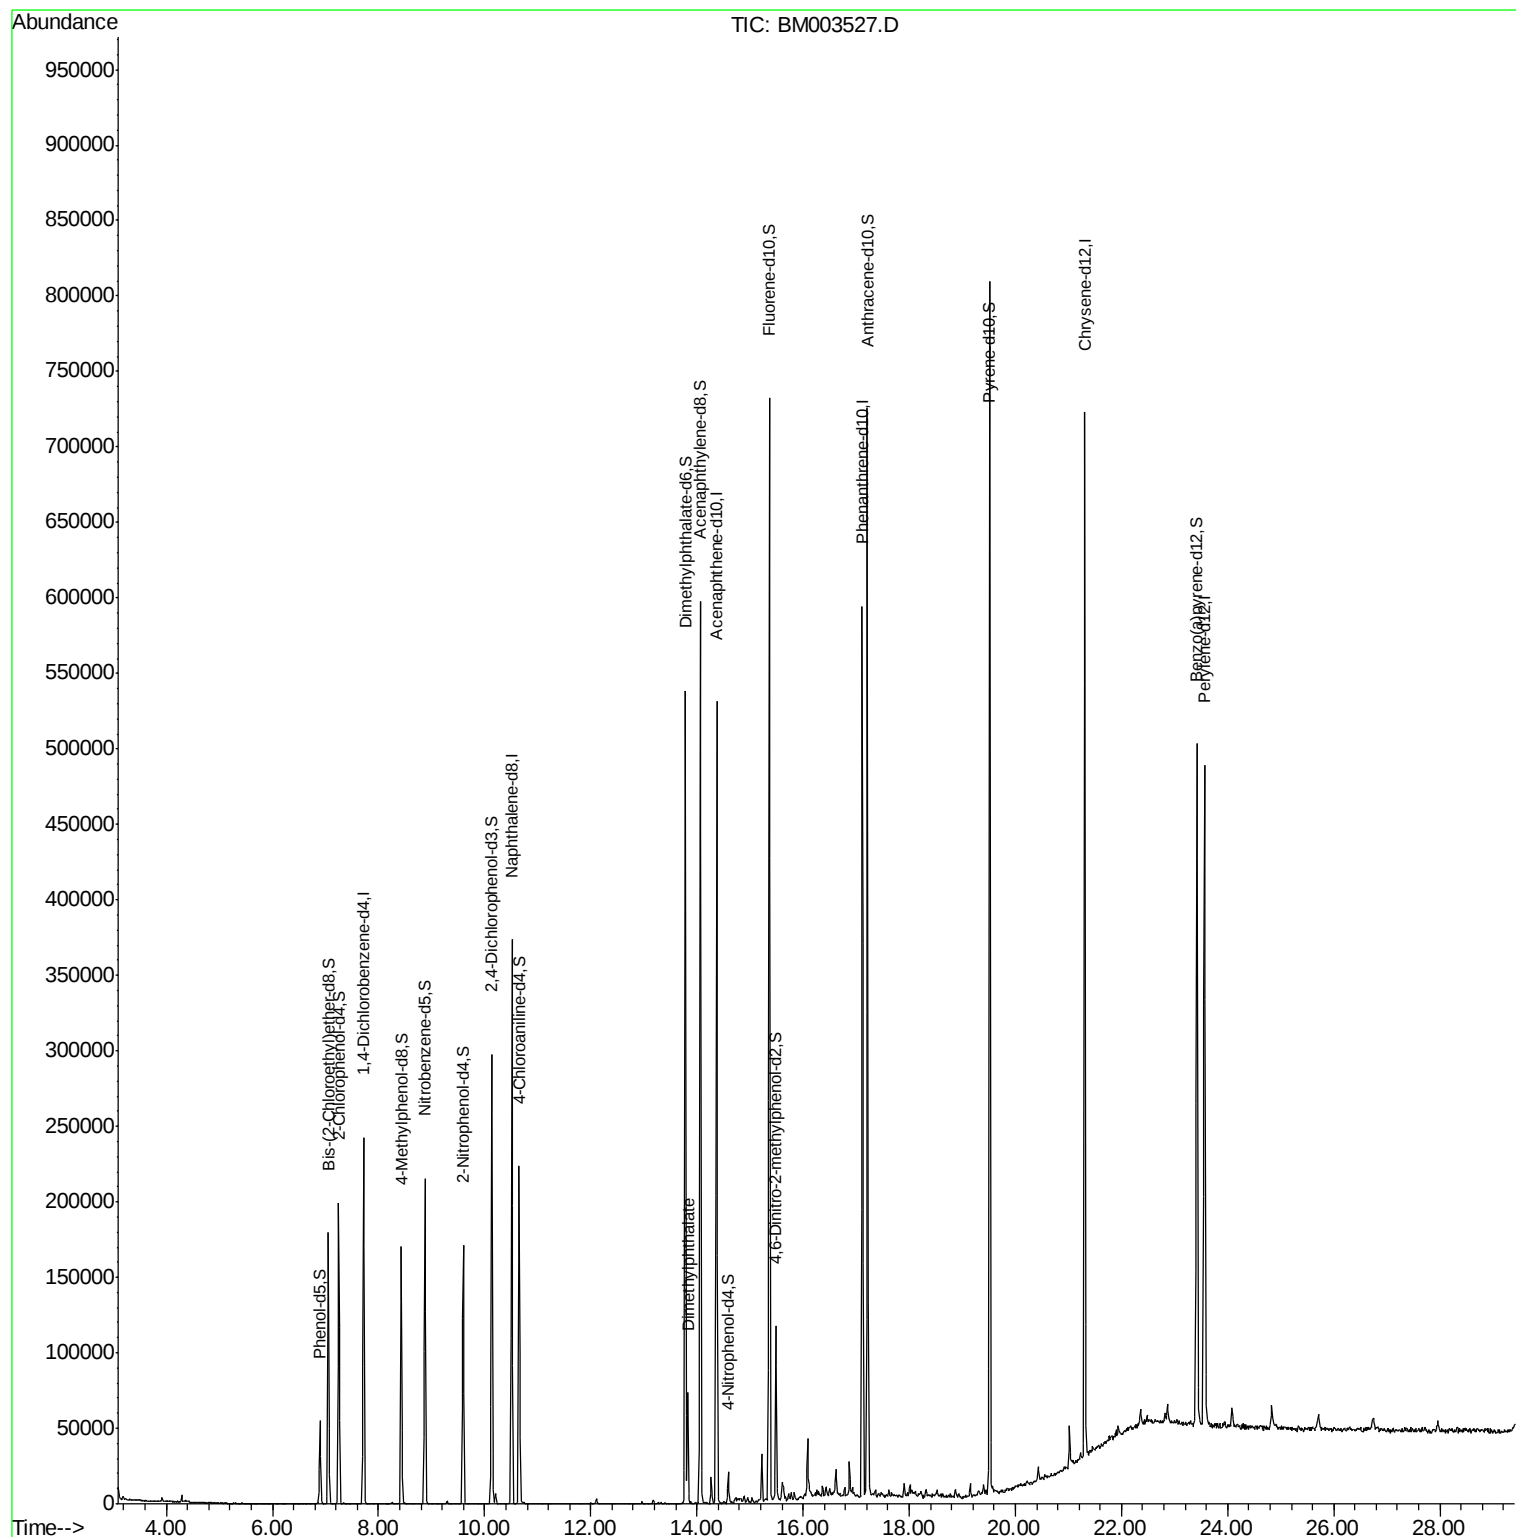

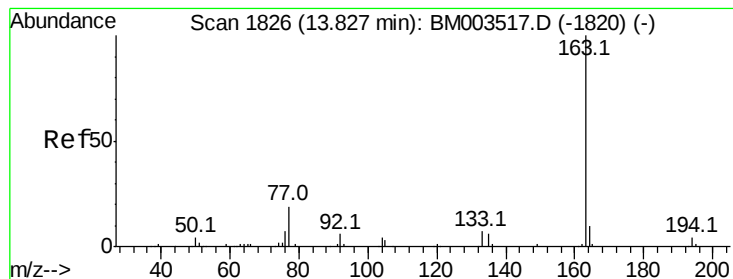

#45

Dimethylphthalate

Concen: 3.55 ng/ul

RT: 13.83 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BM003527.D

Acq: 14 Dec 2015 02:01

Instrument :

BNA_M

ClientSampleId :

C04D8


Tot Ion:163 Resp: 49029

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.7 8.3 12.5

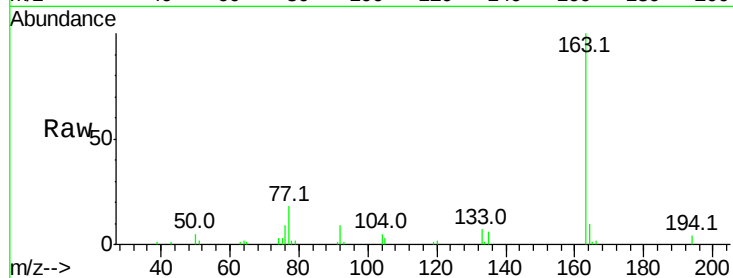

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

