

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003507.D
 Acq On : 13 Dec 2015 13:22
 Operator : UM/IZ
 Sample : G4734-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4KX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB	4136	4166	0.26%	0.026%
2	6.887	641	646	653	rBV	64705	94687	6.01%	0.582%
3	7.051	668	674	682	rBV	259756	397659	25.25%	2.442%
4	7.251	702	708	717	rBB	275354	420560	26.71%	2.583%
5	7.722	781	788	795	rBB	283111	447416	28.41%	2.748%
6	8.422	901	907	920	rBB	208623	319361	20.28%	1.961%
7	8.875	978	984	994	rBB	307194	482561	30.64%	2.964%
8	9.592	1100	1106	1114	rBB	237522	390597	24.80%	2.399%
9	10.128	1191	1197	1210	rBV	363969	613537	38.96%	3.768%
10	10.510	1255	1262	1272	rBB	441155	723745	45.96%	4.445%
11	10.651	1280	1286	1292	rBB	16267	25248	1.60%	0.155%
12	12.104	1529	1533	1537	rBB	4901	6811	0.43%	0.042%
13	13.780	1812	1818	1829	rBV	675486	913067	57.98%	5.607%
14	14.063	1859	1866	1878	rBV	816079	1170947	74.36%	7.191%
15	14.368	1912	1918	1928	rBB2	572805	892652	56.69%	5.482%
16	14.574	1949	1953	1962	rBB2	18358	29022	1.84%	0.178%
17	15.362	2081	2087	2102	rVB	972003	1431117	90.88%	8.789%
18	15.486	2103	2108	2114	rBV	198018	251195	15.95%	1.543%
19	15.604	2124	2128	2133	rBB	7756	9926	0.63%	0.061%
20	15.786	2155	2159	2164	rVB	28020	33425	2.12%	0.205%
21	16.204	2227	2230	2233	rBV2	1186	1735	0.11%	0.011%
22	16.586	2293	2295	2301	rBB2	1095	1707	0.11%	0.010%
23	16.904	2346	2349	2354	rBB	1767	2487	0.16%	0.015%
24	17.115	2379	2385	2392	rBV2	662170	936954	59.50%	5.754%
25	17.215	2396	2402	2417	rBV2	1003570	1418402	90.07%	8.711%
26	19.150	2727	2731	2735	rVB	6920	9075	0.58%	0.056%
27	19.403	2769	2774	2780	rBV	6459	9182	0.58%	0.056%
28	19.515	2787	2793	2808	rVB	1140150	1574713	100.00%	9.671%
29	20.927	3030	3033	3036	rBV4	1397	1920	0.12%	0.012%
30	21.309	3093	3098	3107	rBV	880985	1068349	67.84%	6.561%
31	22.491	3296	3299	3305	rVB2	8408	9691	0.62%	0.060%
32	22.821	3352	3355	3360	rVB3	8158	12326	0.78%	0.076%
33	23.421	3449	3457	3468	rBV	829121	1515117	96.22%	9.305%
34	23.568	3474	3482	3495	rVB2	562878	1063645	67.55%	6.532%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003507.D
Acq On : 13 Dec 2015 13:22
Operator : UM/IZ
Sample : G4734-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KX6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


Sum of corrected areas: 16283002

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003507.D
Acq On : 13 Dec 2015 13:22
Operator : UM/IZ
Sample : G4734-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KX6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

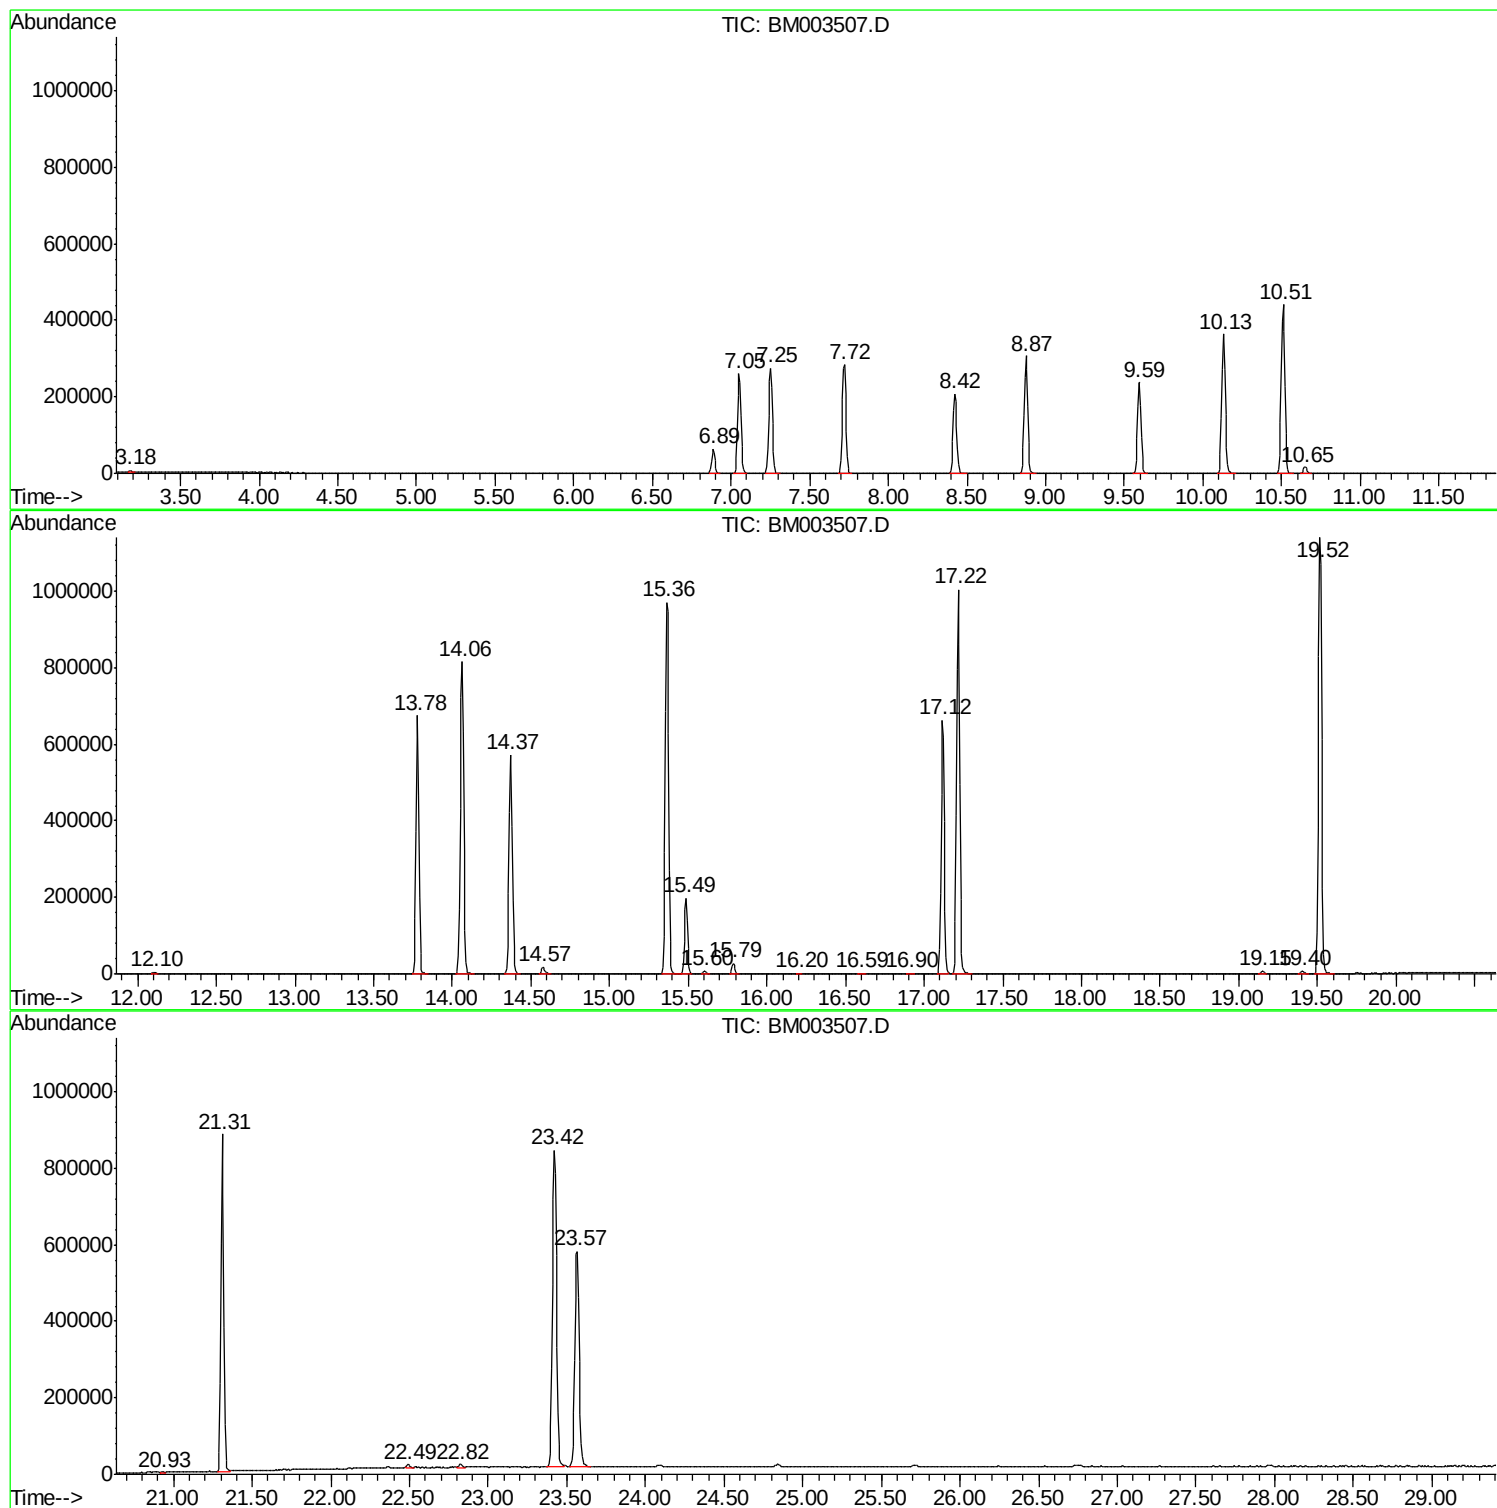

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003507.D
Acq On : 13 Dec 2015 13:22
Operator : UM/IZ
Sample : G4734-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KX6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003507.D
Acq On : 13 Dec 2015 13:22
Operator : UM/IZ
Sample : G4734-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KX6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc