

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003511.D
 Acq On : 13 Dec 2015 15:47
 Operator : UM/IZ
 Sample : G4734-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4KY1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	20	rVB	2019	2770	0.17%	0.017%
2	4.840	296	298	301	rVB	2483	2473	0.15%	0.015%
3	6.887	641	646	655	rBB	55387	84664	5.27%	0.513%
4	7.051	668	674	684	rBB	223457	335849	20.91%	2.034%
5	7.251	702	708	717	rBB	233451	354996	22.11%	2.150%
6	7.716	781	787	795	rBB	264673	423783	26.39%	2.567%
7	8.422	898	907	917	rBB	186175	286381	17.83%	1.735%
8	8.875	977	984	994	rVB	276536	431507	26.87%	2.614%
9	9.292	1051	1055	1058	rBB	2178	2692	0.17%	0.016%
10	9.592	1100	1106	1115	rBB	218091	353023	21.98%	2.138%
11	10.133	1191	1198	1212	rBV	345728	577369	35.95%	3.497%
12	10.510	1255	1262	1271	rBB	430977	708017	44.09%	4.289%
13	10.651	1281	1286	1292	rBB	12318	17680	1.10%	0.107%
14	12.104	1529	1533	1537	rBB	4668	6763	0.42%	0.041%
15	13.780	1812	1818	1823	rBV	710927	980468	61.06%	5.939%
16	13.821	1823	1825	1831	rVB	27073	34237	2.13%	0.207%
17	14.063	1859	1866	1877	rBV	831460	1206468	75.13%	7.308%
18	14.268	1897	1901	1905	rVB	13125	16191	1.01%	0.098%
19	14.368	1911	1918	1927	rBB2	640504	991279	61.73%	6.005%
20	14.574	1949	1953	1963	rBB	17500	29284	1.82%	0.177%
21	14.715	1974	1977	1984	rBB4	2250	3789	0.24%	0.023%
22	14.768	1984	1986	1989	rBB	1895	2152	0.13%	0.013%
23	14.827	1992	1996	2000	rBB2	1610	1994	0.12%	0.012%
24	14.886	2003	2006	2010	rBB	3608	4275	0.27%	0.026%
25	14.957	2015	2018	2022	rVB	2328	2279	0.14%	0.014%
26	15.186	2051	2057	2059	rBV2	1585	2082	0.13%	0.013%
27	15.221	2059	2063	2068	rVB	28785	36466	2.27%	0.221%
28	15.280	2068	2073	2078	rBV	2537	3904	0.24%	0.024%
29	15.368	2081	2088	2101	rVB	1051987	1535113	95.59%	9.299%
30	15.486	2103	2108	2114	rBV	200147	260678	16.23%	1.579%
31	15.604	2124	2128	2132	rBV2	13521	23189	1.44%	0.140%
32	15.668	2136	2139	2142	rVV2	2951	3448	0.21%	0.021%
33	15.727	2144	2149	2154	rVB	3959	4906	0.31%	0.030%
34	15.780	2154	2158	2163	rBV3	7356	10299	0.64%	0.062%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003511.D
 Acq On : 13 Dec 2015 15:47
 Operator : UM/IZ
 Sample : G4734-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4KY1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.845	2165	2169	2173	rVB2	5021	6694	0.42%	0.041%
36	16.027	2196	2200	2201	rBV2	1935	1811	0.11%	0.011%
37	16.086	2205	2210	2218	rBV	37462	60459	3.76%	0.366%
38	16.204	2226	2230	2234	rVB3	2170	3282	0.20%	0.020%
39	16.262	2234	2240	2242	rVV3	3682	4725	0.29%	0.029%
40	16.292	2242	2245	2249	rVV	2714	4107	0.26%	0.025%
41	16.351	2252	2255	2259	rVB2	2657	3687	0.23%	0.022%
42	16.427	2264	2268	2276	rBV2	5377	12174	0.76%	0.074%
43	16.492	2276	2279	2280	rBV2	3934	4465	0.28%	0.027%
44	16.545	2285	2288	2292	rVV	3616	4106	0.26%	0.025%
45	16.592	2292	2296	2302	rVB4	3646	5845	0.36%	0.035%
46	16.662	2304	2308	2310	rBV	3546	4757	0.30%	0.029%
47	16.692	2310	2313	2316	rVB3	2430	2657	0.17%	0.016%
48	16.833	2334	2337	2340	rBV	1135	1717	0.11%	0.010%
49	16.880	2340	2345	2348	rVV	20638	27472	1.71%	0.166%
50	16.927	2351	2353	2357	rVB3	5477	7686	0.48%	0.047%
51	17.021	2367	2369	2374	rVB	1417	1681	0.10%	0.010%
52	17.115	2379	2385	2393	rVV2	785017	1107789	68.98%	6.710%
53	17.215	2393	2402	2416	rVV2	1111239	1577635	98.24%	9.556%
54	17.357	2424	2426	2431	rVB2	2260	3127	0.19%	0.019%
55	17.498	2446	2450	2453	rVB4	1617	1698	0.11%	0.010%
56	17.615	2466	2470	2475	rVB	5379	6216	0.39%	0.038%
57	17.909	2513	2520	2526	rBV2	6910	11724	0.73%	0.071%
58	18.009	2531	2537	2542	rVV	10475	15299	0.95%	0.093%
59	18.062	2542	2546	2548	rVB3	2291	2568	0.16%	0.016%
60	18.309	2585	2588	2593	rVB2	3514	4006	0.25%	0.024%
61	18.521	2619	2624	2630	rVB	3618	6437	0.40%	0.039%
62	18.786	2662	2669	2672	rVB3	1327	1979	0.12%	0.012%
63	18.868	2680	2683	2692	rBV4	4864	6915	0.43%	0.042%
64	19.151	2726	2731	2736	rBV	8193	10049	0.63%	0.061%
65	19.298	2752	2756	2760	rBV	3085	2800	0.17%	0.017%
66	19.403	2769	2774	2778	rBV	6720	9100	0.57%	0.055%
67	19.515	2787	2793	2803	rBV2	1189039	1605876	100.00%	9.728%
68	21.021	3044	3049	3056	rBV3	11709	18507	1.15%	0.112%
69	21.227	3081	3084	3086	rBV	3608	3364	0.21%	0.020%
70	21.309	3093	3098	3109	rBV	778794	990230	61.66%	5.998%
71	22.362	3275	3277	3281	rVB4	4872	3995	0.25%	0.024%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003511.D
Acq On : 13 Dec 2015 15:47
Operator : UM/IZ
Sample : G4734-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KY1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	22.827	3353	3356	3359	rVB3	6889	8814	0.55%	0.053%
73	22.868	3360	3363	3367	rVB2	5408	7741	0.48%	0.047%
74	23.421	3449	3457	3474	rBV	697422	1264776	78.76%	7.661%
75	23.562	3474	3481	3495	rVB2	481647	924232	57.55%	5.598%
76	24.832	3695	3697	3704	rVB4	8721	15935	0.99%	0.097%


Sum of corrected areas: 16508605

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003511.D
Acq On : 13 Dec 2015 15:47
Operator : UM/IZ
Sample : G4734-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KY1

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

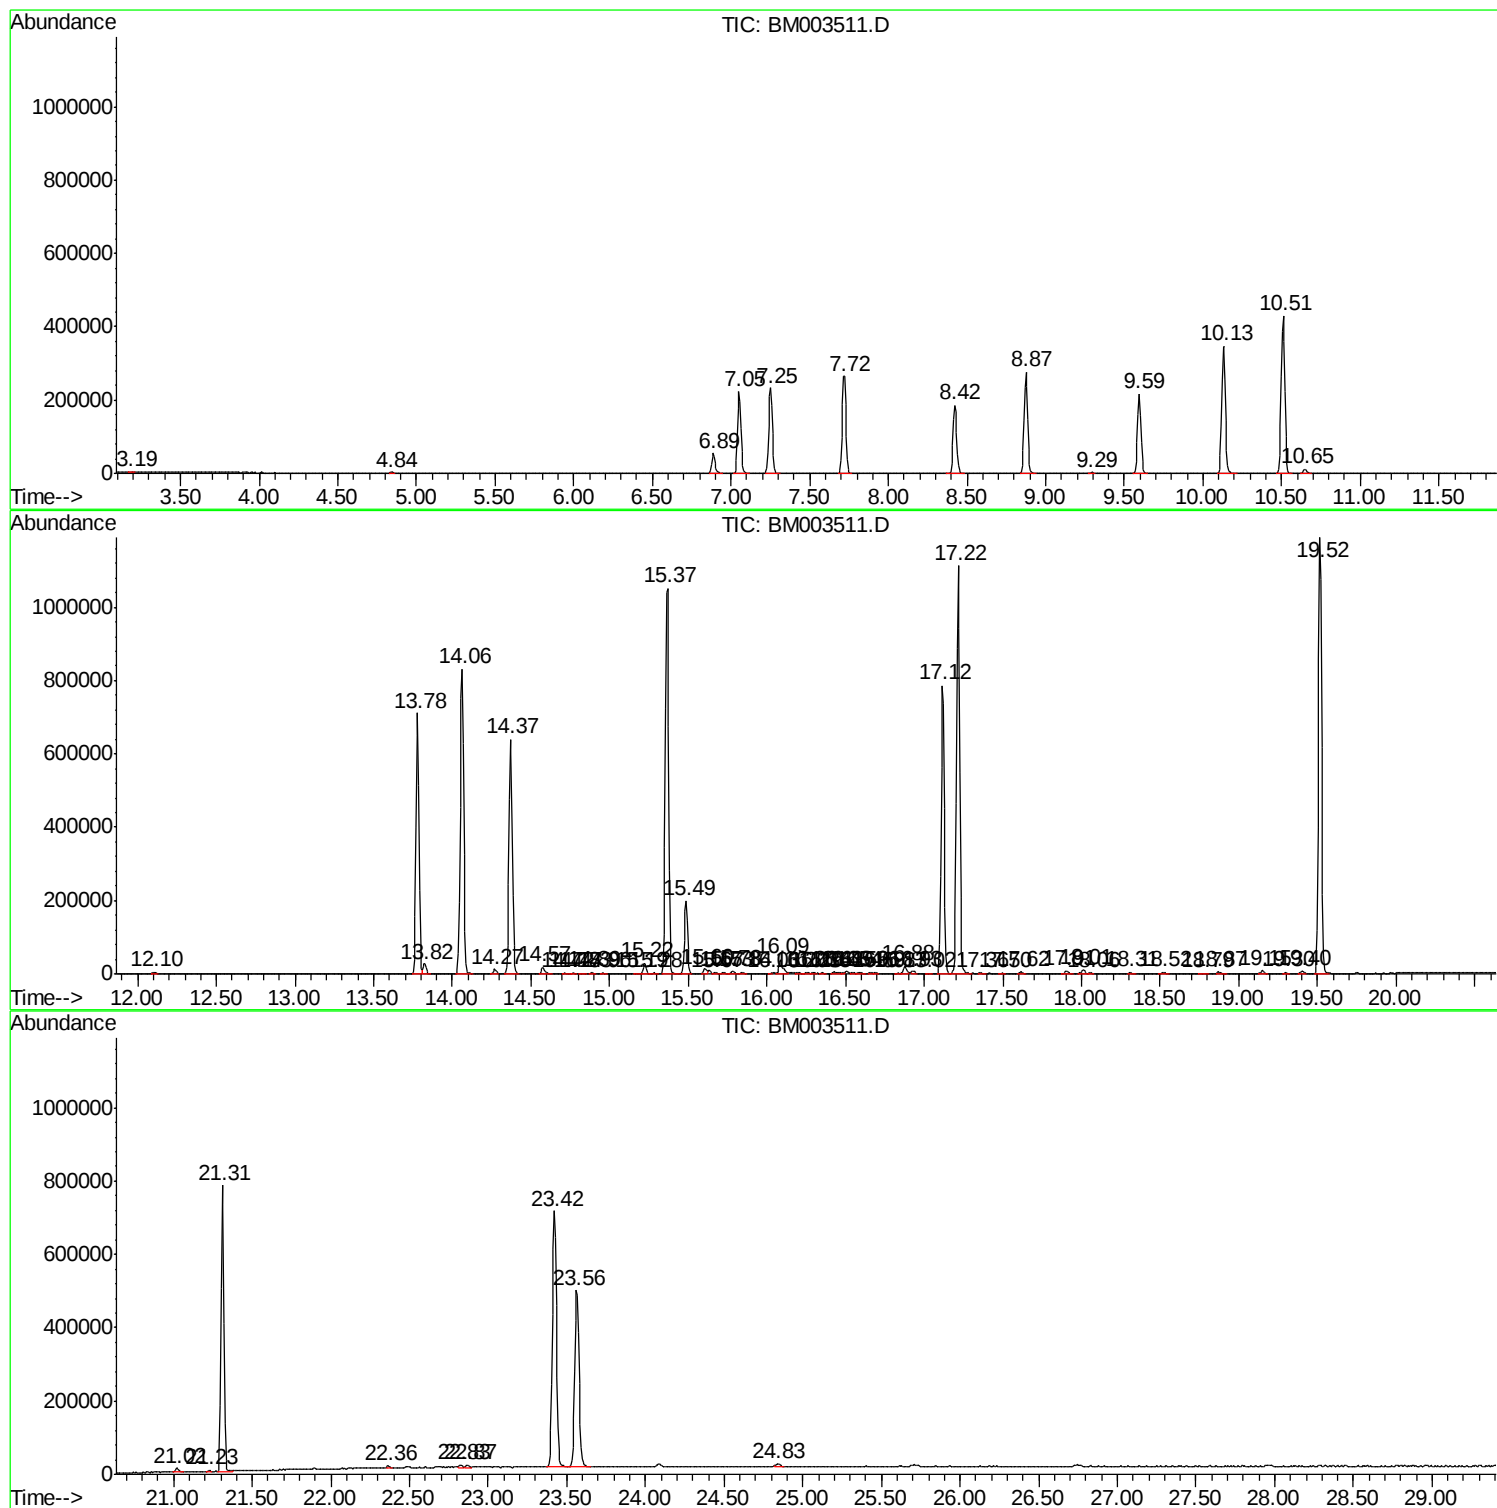

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003511.D
Acq On : 13 Dec 2015 15:47
Operator : UM/IZ
Sample : G4734-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KY1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003511.D
Acq On : 13 Dec 2015 15:47
Operator : UM/IZ
Sample : G4734-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4KY1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc