

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003513.D
 Acq On : 13 Dec 2015 17:00
 Operator : UM/IZ
 Sample : G4722-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04B3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rBV	4566	4736	0.29%	0.029%
2	3.922	139	142	145	rVB2	1560	1918	0.12%	0.012%
3	4.363	212	217	224	rBV2	9580	14763	0.91%	0.090%
4	5.046	327	333	341	rVB	173552	254645	15.73%	1.557%
5	5.175	349	355	358	rVB2	1734	2562	0.16%	0.016%
6	6.887	638	646	657	rBB	70415	110791	6.84%	0.677%
7	7.051	668	674	685	rBB	274342	413006	25.52%	2.525%
8	7.251	701	708	717	rBB	296226	460206	28.43%	2.813%
9	7.463	740	744	746	rBB	3066	3440	0.21%	0.021%
10	7.610	765	769	773	rBB	6765	8918	0.55%	0.055%
11	7.716	781	787	797	rBV	223453	374542	23.14%	2.290%
12	7.804	797	802	806	rVB3	4649	8591	0.53%	0.053%
13	8.422	901	907	914	rBV	218960	337602	20.86%	2.064%
14	8.775	962	967	971	rBV	10740	17323	1.07%	0.106%
15	8.816	971	974	978	rVV	2986	4307	0.27%	0.026%
16	8.875	978	984	993	rVB	310324	496337	30.66%	3.034%
17	9.104	1019	1023	1032	rBB2	4058	8204	0.51%	0.050%
18	9.181	1032	1036	1038	rBB2	2328	2708	0.17%	0.017%
19	9.228	1038	1044	1048	rBB2	24214	36567	2.26%	0.224%
20	9.298	1052	1056	1057	rBV	1539	2122	0.13%	0.013%
21	9.328	1057	1061	1073	rVB2	17568	33590	2.08%	0.205%
22	9.592	1100	1106	1114	rBB	255582	419052	25.89%	2.562%
23	10.016	1174	1178	1180	rBV3	2305	3865	0.24%	0.024%
24	10.057	1180	1185	1190	rVB3	3701	6823	0.42%	0.042%
25	10.133	1191	1198	1207	rVV	383055	648242	40.05%	3.963%
26	10.286	1221	1224	1228	rVV2	972	1703	0.11%	0.010%
27	10.351	1230	1235	1238	rBV3	2455	4947	0.31%	0.030%
28	10.410	1241	1245	1250	rVB5	4533	7171	0.44%	0.044%
29	10.510	1255	1262	1272	rBB	315866	532146	32.88%	3.253%
30	10.651	1278	1286	1293	rBV5	6335	18538	1.15%	0.113%
31	10.751	1301	1303	1307	rBV2	1437	2397	0.15%	0.015%
32	10.857	1318	1321	1323	rBV2	1838	2166	0.13%	0.013%
33	10.916	1327	1331	1332	rBV	1718	1715	0.11%	0.010%
34	11.080	1353	1359	1365	rBV3	3344	8103	0.50%	0.050%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003513.D
 Acq On : 13 Dec 2015 17:00
 Operator : UM/IZ
 Sample : G4722-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04B3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	11.151	1368	1371	1377	rVB2	1494	2472	0.15%	0.015%
36	11.227	1377	1384	1390	rBV5	3547	8974	0.55%	0.055%
37	11.351	1398	1405	1412	rBV4	6031	14653	0.91%	0.090%
38	11.416	1414	1416	1421	rVB3	3291	3970	0.25%	0.024%
39	11.475	1421	1426	1430	rBV3	2863	4573	0.28%	0.028%
40	11.575	1438	1443	1448	rBV3	1149	2415	0.15%	0.015%
41	11.639	1450	1454	1458	rVB2	2130	3531	0.22%	0.022%
42	11.710	1460	1466	1468	rBV3	2660	4080	0.25%	0.025%
43	11.857	1483	1491	1496	rBV3	10113	18680	1.15%	0.114%
44	11.957	1504	1508	1516	rVB4	2719	6556	0.41%	0.040%
45	12.051	1519	1524	1525	rBV3	1328	1799	0.11%	0.011%
46	12.104	1525	1533	1538	rBV2	5412	11999	0.74%	0.073%
47	12.180	1540	1546	1550	rVV7	2844	7109	0.44%	0.043%
48	12.233	1550	1555	1562	rVV3	12092	21885	1.35%	0.134%
49	12.298	1562	1566	1570	rVV4	2966	5603	0.35%	0.034%
50	12.345	1572	1574	1577	rVB4	2953	2324	0.14%	0.014%
51	12.392	1577	1582	1586	rBV4	2740	4392	0.27%	0.027%
52	12.563	1603	1611	1613	rBV6	2967	8116	0.50%	0.050%
53	12.586	1613	1615	1618	rVV4	2207	2695	0.17%	0.016%
54	12.622	1618	1621	1624	rVV4	2683	3661	0.23%	0.022%
55	12.657	1624	1627	1629	rBV5	1712	2123	0.13%	0.013%
56	12.739	1635	1641	1642	rBV4	1959	3443	0.21%	0.021%
57	12.816	1650	1654	1657	rBV5	1872	3251	0.20%	0.020%
58	12.851	1657	1660	1662	rVV2	3280	4270	0.26%	0.026%
59	12.880	1663	1665	1670	rVB4	4061	5151	0.32%	0.031%
60	12.933	1670	1674	1676	rBV4	2814	3523	0.22%	0.022%
61	12.969	1676	1680	1683	rVB4	2669	4110	0.25%	0.025%
62	13.027	1683	1690	1696	rBV9	3691	8652	0.53%	0.053%
63	13.086	1696	1700	1704	rBV5	3334	4926	0.30%	0.030%
64	13.163	1705	1713	1717	rBV5	5099	11981	0.74%	0.073%
65	13.216	1720	1722	1729	rVB5	4139	5130	0.32%	0.031%
66	13.304	1733	1737	1738	rBV3	2847	3167	0.20%	0.019%
67	13.374	1744	1749	1756	rBV4	10506	21316	1.32%	0.130%
68	13.433	1757	1759	1762	rBV4	1636	2084	0.13%	0.013%
69	13.551	1774	1779	1782	rBV4	4853	9575	0.59%	0.059%
70	13.592	1782	1786	1789	rVV4	4379	7125	0.44%	0.044%
71	13.669	1795	1799	1801	rBV3	5398	6792	0.42%	0.042%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003513.D
Acq On : 13 Dec 2015 17:00
Operator : UM/IZ
Sample : G4722-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


72	13.780	1812	1818	1826	rVB	687134	975156	60.25%	5.962%
73	13.857	1828	1831	1832	rBV3	2830	2856	0.18%	0.017%
74	14.063	1859	1866	1878	rVB	810291	1201739	74.24%	7.347%
75	14.180	1881	1886	1893	rVV5	7458	15488	0.96%	0.095%
76	14.292	1901	1905	1910	rVB4	15536	22195	1.37%	0.136%
77	14.368	1912	1918	1925	rVV2	415987	651816	40.27%	3.985%
78	14.580	1949	1954	1962	rBV	46574	90458	5.59%	0.553%
79	15.363	2081	2087	2102	rVB	983309	1474125	91.07%	9.012%
80	15.486	2102	2108	2114	rBV	265301	384383	23.75%	2.350%
81	15.604	2125	2128	2135	rVB2	25260	36878	2.28%	0.225%
82	15.880	2171	2175	2180	rBV3	22784	37361	2.31%	0.228%
83	16.621	2298	2301	2309	rVB3	25682	42941	2.65%	0.263%
84	17.115	2380	2385	2394	rVB2	491154	724732	44.77%	4.431%
85	17.215	2396	2402	2412	rVV2	1030999	1472739	90.99%	9.004%
86	18.021	2536	2539	2544	rBV5	29584	55863	3.45%	0.342%
87	19.515	2788	2793	2799	rBV	1143693	1618639	100.00%	9.896%
88	21.315	3094	3099	3105	rVB	603026	806482	49.82%	4.930%
89	23.427	3451	3458	3466	rVB	711447	1379891	85.25%	8.436%
90	23.568	3475	3482	3491	rVB	450845	863650	53.36%	5.280%

Sum of corrected areas: 16357244

Instrument :
BNA_M
ClientSampleId :
C04B3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

```
TIC Library      : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P
```

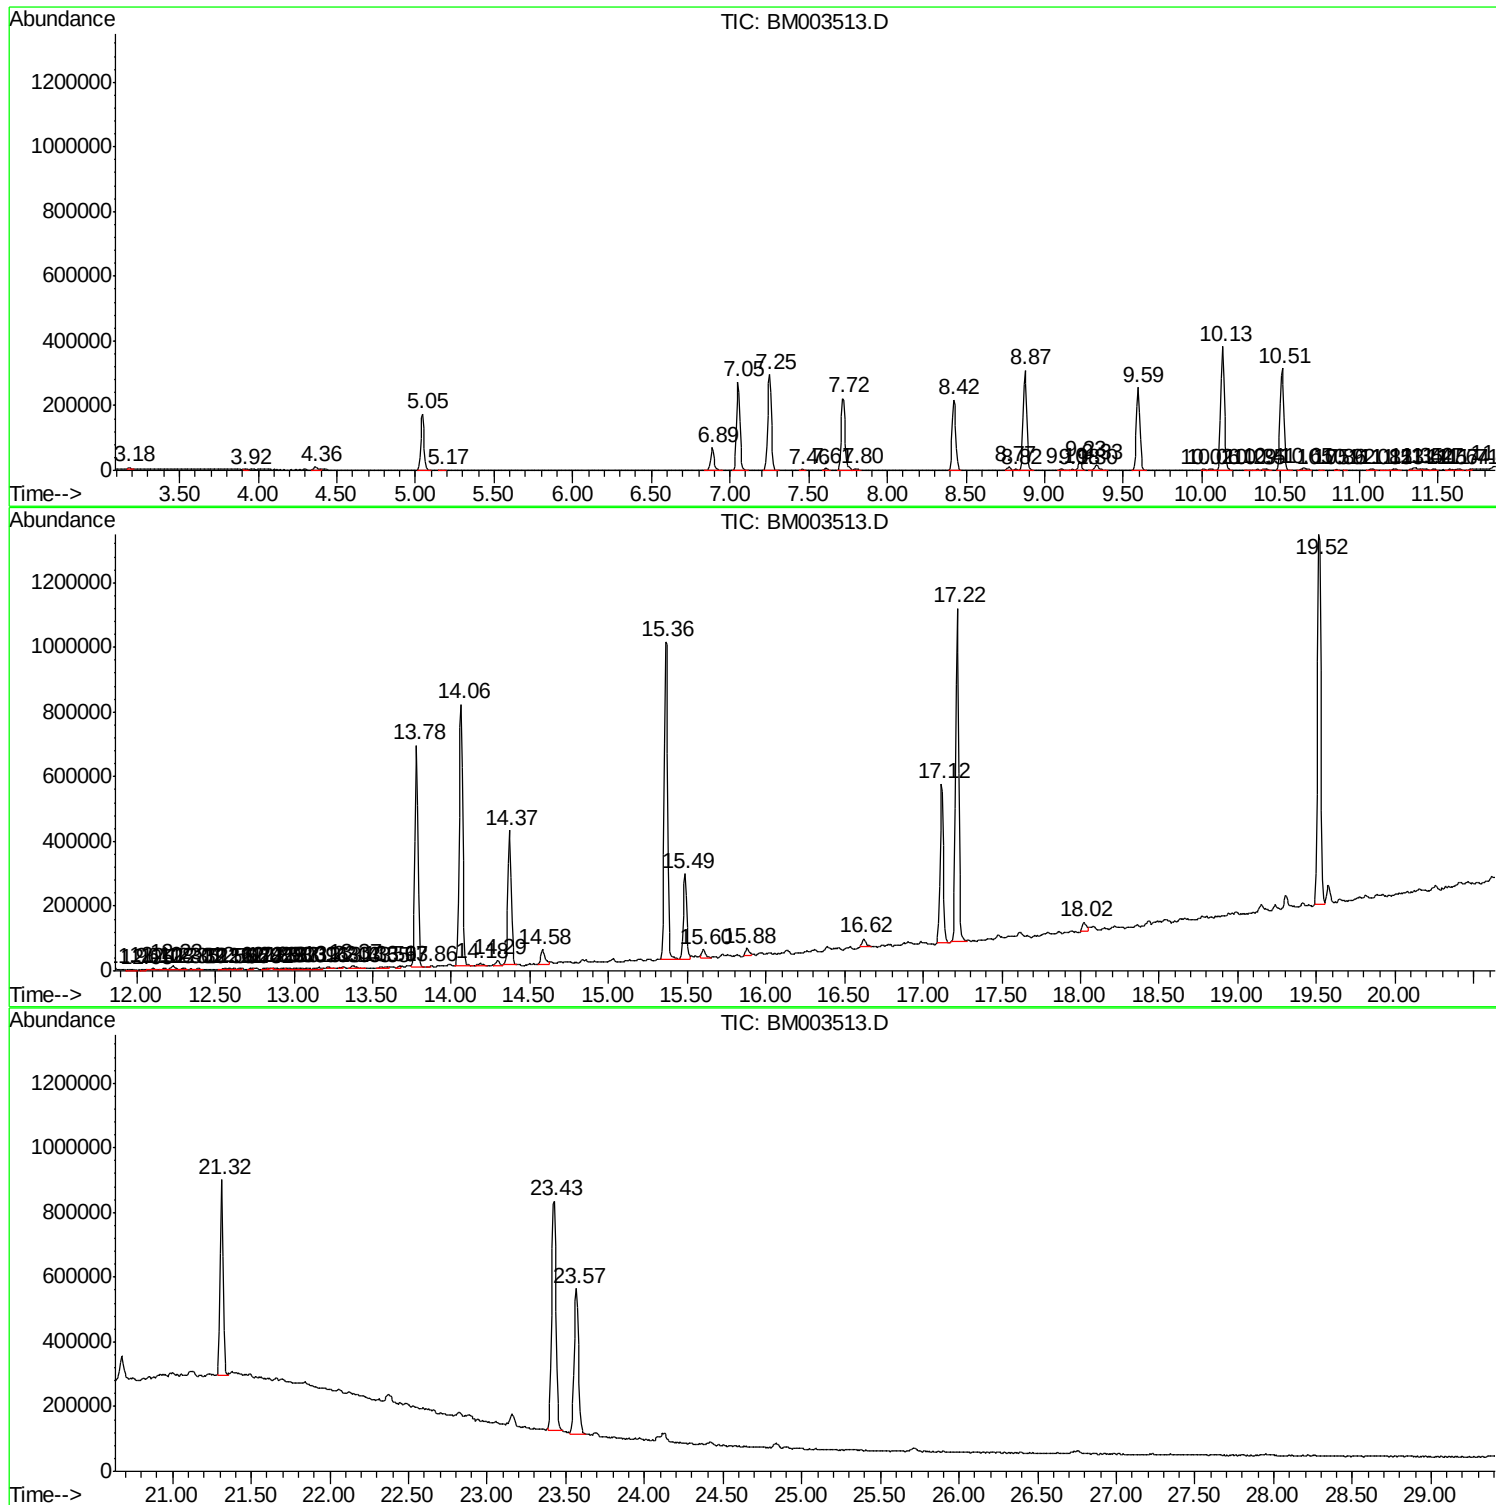

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003513.D
Acq On : 13 Dec 2015 17:00
Operator : UM/IZ
Sample : G4722-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003513.D
Acq On : 13 Dec 2015 17:00
Operator : UM/IZ
Sample : G4722-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B3

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc