

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003514.D
 Acq On : 13 Dec 2015 17:36
 Operator : UM/IZ
 Sample : G4722-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04B7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	14	16	21	rVB	3068	3554	0.23%	0.023%
2	3.475	60	66	74	rBV3	4276	9206	0.60%	0.059%
3	6.887	641	646	654	rBB	61966	93412	6.12%	0.595%
4	7.052	668	674	684	rBB	261206	395306	25.91%	2.516%
5	7.252	702	708	716	rBB	277817	425844	27.91%	2.710%
6	7.716	781	787	794	rBB	244005	387049	25.36%	2.463%
7	7.811	800	803	806	rBB	2457	2371	0.16%	0.015%
8	8.428	902	908	915	rBV	203479	318655	20.88%	2.028%
9	8.875	977	984	995	rBB	322750	505423	33.12%	3.217%
10	9.593	1100	1106	1114	rBB	265740	431858	28.30%	2.749%
11	10.134	1191	1198	1209	rBV	402941	654539	42.89%	4.166%
12	10.510	1255	1262	1269	rBV	375968	620290	40.65%	3.948%
13	10.652	1281	1286	1292	rBB	9077	12872	0.84%	0.082%
14	11.763	1470	1475	1478	rBB	934	1624	0.11%	0.010%
15	12.104	1529	1533	1537	rBB	5319	7505	0.49%	0.048%
16	12.887	1662	1666	1669	rBV2	1329	2055	0.13%	0.013%
17	12.969	1677	1680	1683	rVB	1509	1730	0.11%	0.011%
18	13.257	1727	1729	1734	rVB	1678	2149	0.14%	0.014%
19	13.687	1795	1802	1807	rBV3	2141	4987	0.33%	0.032%
20	13.781	1812	1818	1826	rVV	727452	1025510	67.20%	6.527%
21	13.969	1845	1850	1855	rBV3	1939	3714	0.24%	0.024%
22	14.063	1859	1866	1877	rVV	851934	1265499	82.93%	8.055%
23	14.292	1900	1905	1909	rVB3	7177	9433	0.62%	0.060%
24	14.369	1912	1918	1931	rVB2	522548	809642	53.06%	5.153%
25	14.581	1948	1954	1964	rBV	30032	54473	3.57%	0.347%
26	14.792	1987	1990	1992	rBV3	1896	2044	0.13%	0.013%
27	14.828	1992	1996	2000	rVV3	2701	5036	0.33%	0.032%
28	14.863	2000	2002	2006	rVB2	2437	2342	0.15%	0.015%
29	14.904	2006	2009	2011	rBV4	2709	3389	0.22%	0.022%
30	15.028	2028	2030	2034	rBV3	1216	1625	0.11%	0.010%
31	15.110	2040	2044	2047	rBV4	4459	6273	0.41%	0.040%
32	15.192	2054	2058	2065	rVB2	3003	4086	0.27%	0.026%
33	15.363	2081	2087	2097	rVV	1029514	1525961	100.00%	9.712%
34	15.486	2102	2108	2115	rBV	265031	363779	23.84%	2.315%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003514.D
 Acq On : 13 Dec 2015 17:36
 Operator : UM/IZ
 Sample : G4722-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04B7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.604	2125	2128	2133	rVB	10933	13605	0.89%	0.087%
36	15.869	2171	2173	2176	rBV4	2719	3141	0.21%	0.020%
37	16.263	2237	2240	2243	rBV2	3199	3693	0.24%	0.024%
38	16.428	2265	2268	2272	rBV6	3237	3675	0.24%	0.023%
39	16.528	2282	2285	2287	rBV4	2384	2138	0.14%	0.014%
40	16.710	2314	2316	2320	rBV5	1918	2098	0.14%	0.013%
41	16.863	2337	2342	2344	rBV5	5429	7704	0.50%	0.049%
42	16.898	2346	2348	2353	rVB3	4886	7989	0.52%	0.051%
43	17.116	2379	2385	2395	rBV	588300	831634	54.50%	5.293%
44	17.216	2395	2402	2413	rBV2	992088	1445946	94.76%	9.203%
45	17.463	2440	2444	2446	rBV3	2866	3989	0.26%	0.025%
46	17.486	2446	2448	2450	rBV3	2947	3026	0.20%	0.019%
47	18.016	2534	2538	2542	rBV2	14401	20101	1.32%	0.128%
48	18.080	2547	2549	2555	rVB5	3765	4434	0.29%	0.028%
49	19.151	2728	2731	2734	rVB	12047	14716	0.96%	0.094%
50	19.298	2753	2756	2760	rBV3	17164	21413	1.40%	0.136%
51	19.404	2772	2774	2778	rVB	10682	11886	0.78%	0.076%
52	19.516	2787	2793	2800	rBV2	1094881	1505300	98.65%	9.581%
53	21.310	3093	3098	3108	rBV	632824	835276	54.74%	5.316%
54	23.421	3450	3457	3469	rVB	649660	1225828	80.33%	7.802%
55	23.562	3475	3481	3491	rVB2	408310	780671	51.16%	4.969%


Sum of corrected areas: 15711498

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003514.D
Acq On : 13 Dec 2015 17:36
Operator : UM/IZ
Sample : G4722-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

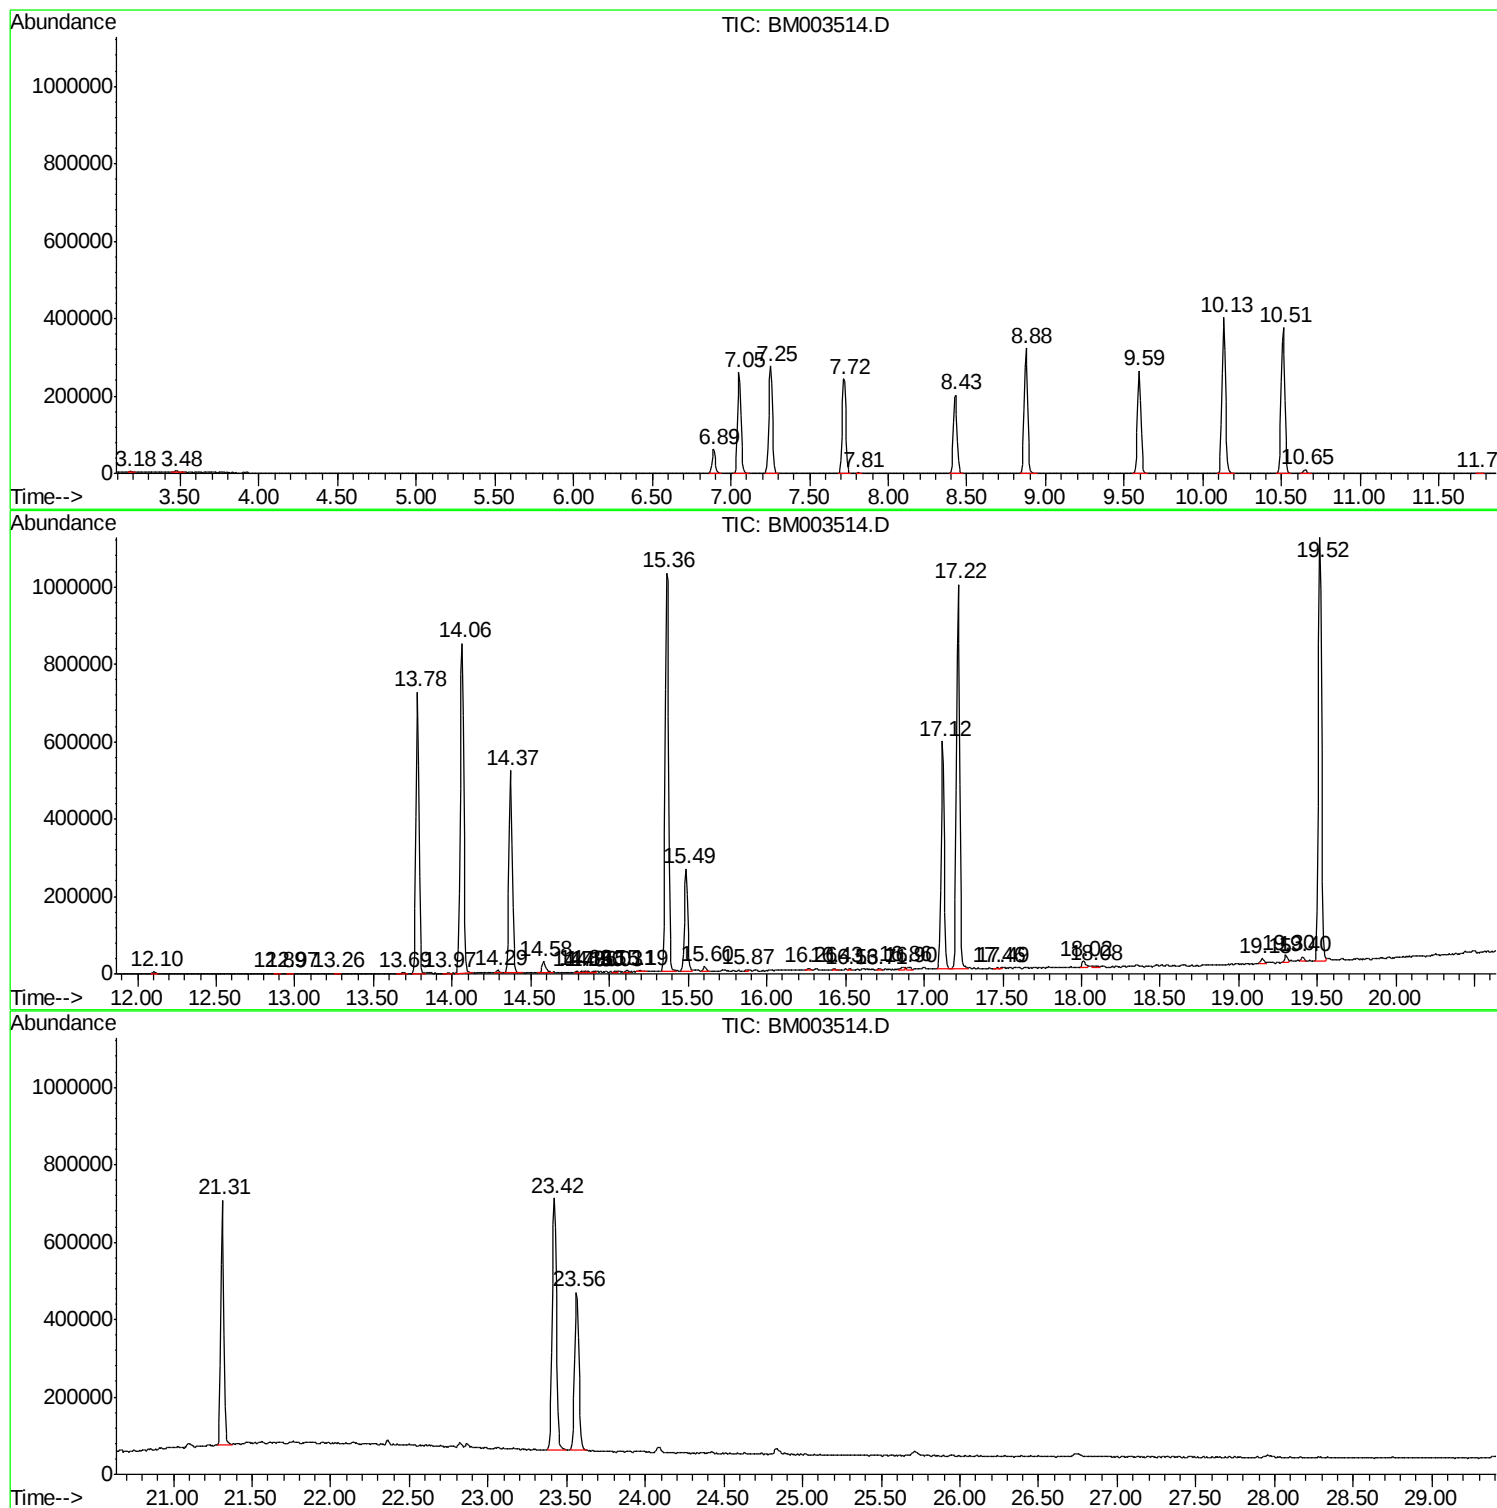

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003514.D
Acq On : 13 Dec 2015 17:36
Operator : UM/IZ
Sample : G4722-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003514.D
Acq On : 13 Dec 2015 17:36
Operator : UM/IZ
Sample : G4722-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04B7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc