

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003518.D
 Acq On : 13 Dec 2015 20:36
 Operator : UM/IZ
 Sample : PB87247BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	24	rVB	20134	23163	1.34%	0.132%
2	3.740	108	111	116	rVB3	2602	3172	0.18%	0.018%
3	6.893	640	647	658	rBV	322201	505473	29.14%	2.881%
4	7.051	668	674	683	rBV	277018	418931	24.15%	2.388%
5	7.251	701	708	715	rBV	358821	548076	31.60%	3.124%
6	7.716	781	787	794	rVB	232775	366490	21.13%	2.089%
7	8.428	899	908	920	rBB	435216	678701	39.13%	3.868%
8	8.875	978	984	991	rBV	315956	499447	28.79%	2.846%
9	9.598	1100	1107	1114	rBB	252493	411600	23.73%	2.346%
10	10.134	1191	1198	1208	rBV	415541	671185	38.69%	3.825%
11	10.510	1255	1262	1270	rVB	341913	564065	32.52%	3.215%
12	10.645	1279	1285	1293	rBV	413461	696875	40.18%	3.972%
13	12.104	1529	1533	1538	rBB	5141	7176	0.41%	0.041%
14	13.780	1812	1818	1830	rBV	709145	967254	55.76%	5.513%
15	14.063	1859	1866	1880	rBV	831452	1197705	69.05%	6.826%
16	14.369	1912	1918	1926	rVB2	461296	704812	40.63%	4.017%
17	14.574	1947	1953	1964	rBV	204276	309199	17.83%	1.762%
18	15.363	2081	2087	2102	rBV	995284	1461503	84.26%	8.329%
19	15.486	2102	2108	2116	rVV	177250	224002	12.91%	1.277%
20	15.604	2124	2128	2132	rBV	8576	9812	0.57%	0.056%
21	17.115	2379	2385	2392	rBV2	535201	739257	42.62%	4.213%
22	17.215	2396	2402	2415	rVV2	1085186	1459256	84.13%	8.317%
23	19.151	2727	2731	2736	rBV	7877	9745	0.56%	0.056%
24	19.404	2770	2774	2780	rVB	6030	8580	0.49%	0.049%
25	19.515	2787	2793	2805	rBV	1206898	1623785	93.61%	9.254%
26	21.309	3093	3098	3110	rBV	685393	846066	48.78%	4.822%
27	22.821	3352	3355	3360	rBV3	8607	12504	0.72%	0.071%
28	23.421	3449	3457	3471	rBV	938317	1734583	100.00%	9.886%
29	23.562	3474	3481	3495	rVB2	450685	843702	48.64%	4.808%


Sum of corrected areas: 17546119

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003518.D
Acq On : 13 Dec 2015 20:36
Operator : UM/IZ
Sample : PB87247BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

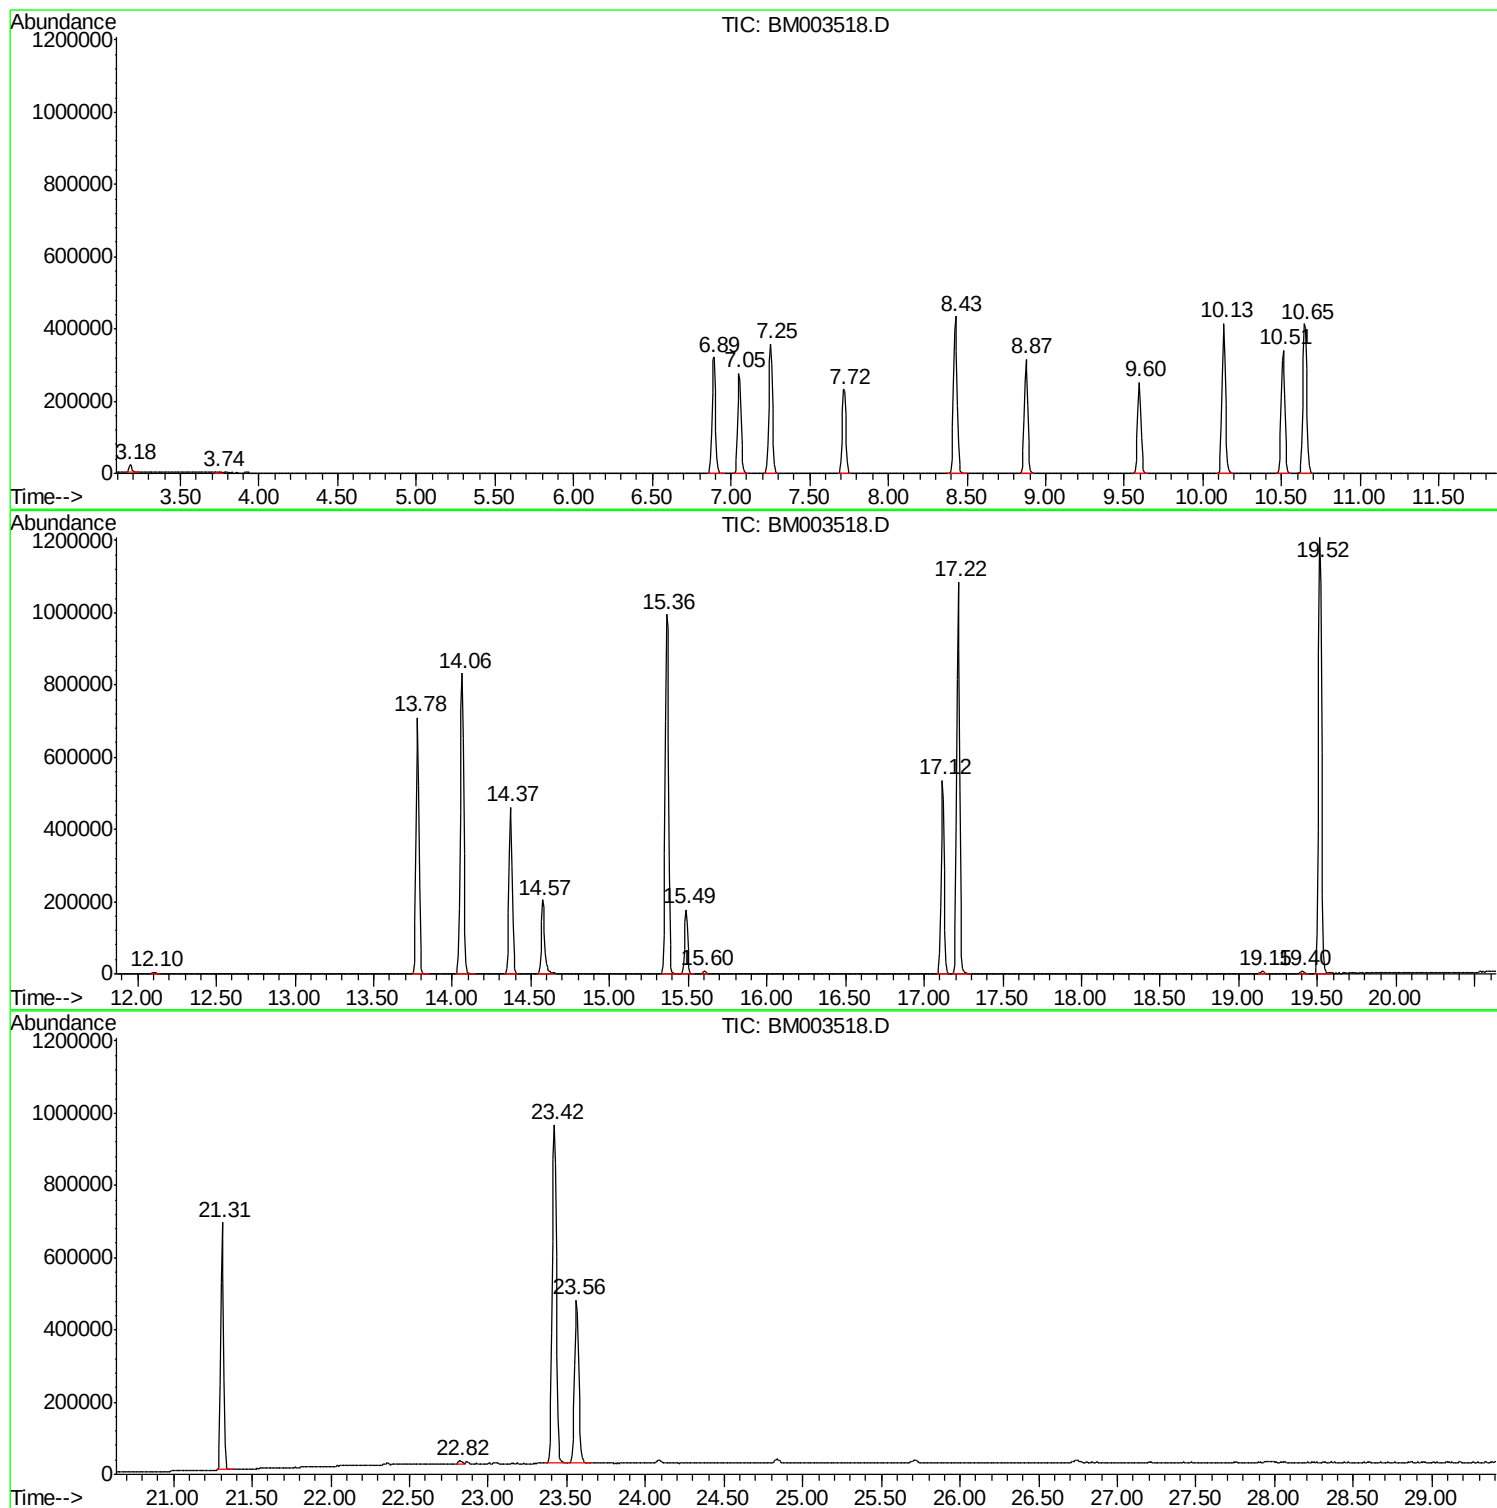

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003518.D
Acq On : 13 Dec 2015 20:36
Operator : UM/IZ
Sample : PB87247BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003518.D
Acq On : 13 Dec 2015 20:36
Operator : UM/IZ
Sample : PB87247BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK47

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc