

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003520.D
 Acq On : 13 Dec 2015 21:49
 Operator : UM/IZ
 Sample : G4722-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB	4276	4634	0.31%	0.031%
2	3.928	139	143	146	rBV	1567	1970	0.13%	0.013%
3	4.369	214	218	225	rVB2	1002	2235	0.15%	0.015%
4	5.769	453	456	459	rBB	2485	2639	0.18%	0.018%
5	6.857	637	641	642	rBV	3491	4229	0.28%	0.028%
6	6.893	642	647	654	rVB	69230	105309	7.03%	0.707%
7	7.051	668	674	684	rBB	275014	416396	27.81%	2.796%
8	7.251	702	708	716	rBB	294250	450290	30.08%	3.023%
9	7.716	781	787	794	rBB	247028	393443	26.28%	2.642%
10	8.428	902	908	917	rBB	214210	331642	22.15%	2.227%
11	8.875	977	984	992	rBV	318652	502104	33.54%	3.371%
12	9.292	1051	1055	1059	rBB	2193	2963	0.20%	0.020%
13	9.592	1100	1106	1114	rBB	255499	414223	27.67%	2.781%
14	9.922	1159	1162	1166	rBB	4830	5527	0.37%	0.037%
15	10.134	1191	1198	1214	rBB	381994	619475	41.38%	4.159%
16	10.510	1255	1262	1270	rBB	348628	577682	38.59%	3.879%
17	10.651	1281	1286	1292	rBB	11041	17255	1.15%	0.116%
18	12.104	1529	1533	1537	rBB	5083	7008	0.47%	0.047%
19	13.780	1811	1818	1834	rBV	654074	888132	59.32%	5.963%
20	14.063	1859	1866	1887	rBV	771992	1124652	75.12%	7.551%
21	14.369	1912	1918	1927	rBB2	453479	688738	46.00%	4.624%
22	14.580	1950	1954	1964	rBB	24742	40086	2.68%	0.269%
23	15.363	2081	2087	2102	rBV	937516	1369069	91.44%	9.192%
24	15.486	2102	2108	2117	rVB	209073	273895	18.29%	1.839%
25	15.604	2124	2128	2133	rVB	7458	9423	0.63%	0.063%
26	15.763	2151	2155	2159	rBB2	6008	7235	0.48%	0.049%
27	15.968	2187	2190	2194	rBB	5225	6215	0.42%	0.042%
28	16.263	2237	2240	2244	rBB2	3188	3411	0.23%	0.023%
29	16.586	2292	2295	2299	rBB	1550	1592	0.11%	0.011%
30	16.821	2331	2335	2337	rBV	2462	3325	0.22%	0.022%
31	16.851	2337	2340	2343	rVB	1959	2248	0.15%	0.015%
32	16.910	2344	2350	2352	rBV	1330	2190	0.15%	0.015%
33	16.992	2359	2364	2366	rBB	1171	1700	0.11%	0.011%
34	17.115	2379	2385	2396	rBV2	518533	730986	48.83%	4.908%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003520.D
Acq On : 13 Dec 2015 21:49
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

35	17.215	2396	2402	2417	rVV2	957020	1337063	89.31%	8.977%
36	18.010	2531	2537	2539	rBV3	1382	2295	0.15%	0.015%
37	18.086	2546	2550	2554	rBV	2616	3367	0.22%	0.023%
38	18.351	2591	2595	2599	rVB4	1607	2338	0.16%	0.016%
39	18.515	2619	2623	2630	rBV4	2211	3642	0.24%	0.024%
40	19.145	2726	2730	2734	rVB3	8868	12067	0.81%	0.081%
41	19.404	2769	2774	2780	rBV	9011	12780	0.85%	0.086%
42	19.515	2787	2793	2800	rVV2	1081555	1497152	100.00%	10.052%
43	19.562	2800	2801	2807	rVV5	5127	6825	0.46%	0.046%
44	19.609	2807	2809	2811	rVV3	2130	2147	0.14%	0.014%
45	19.656	2815	2817	2821	rVV4	1412	1695	0.11%	0.011%
46	19.804	2840	2842	2846	rBV3	1658	2284	0.15%	0.015%
47	21.309	3093	3098	3106	rBV	681553	870589	58.15%	5.845%
48	23.421	3450	3457	3467	rVB	704900	1305163	87.18%	8.763%
49	23.562	3475	3481	3491	rVB2	429200	822303	54.92%	5.521%


Sum of corrected areas: 14893631

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003520.D
Acq On : 13 Dec 2015 21:49
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

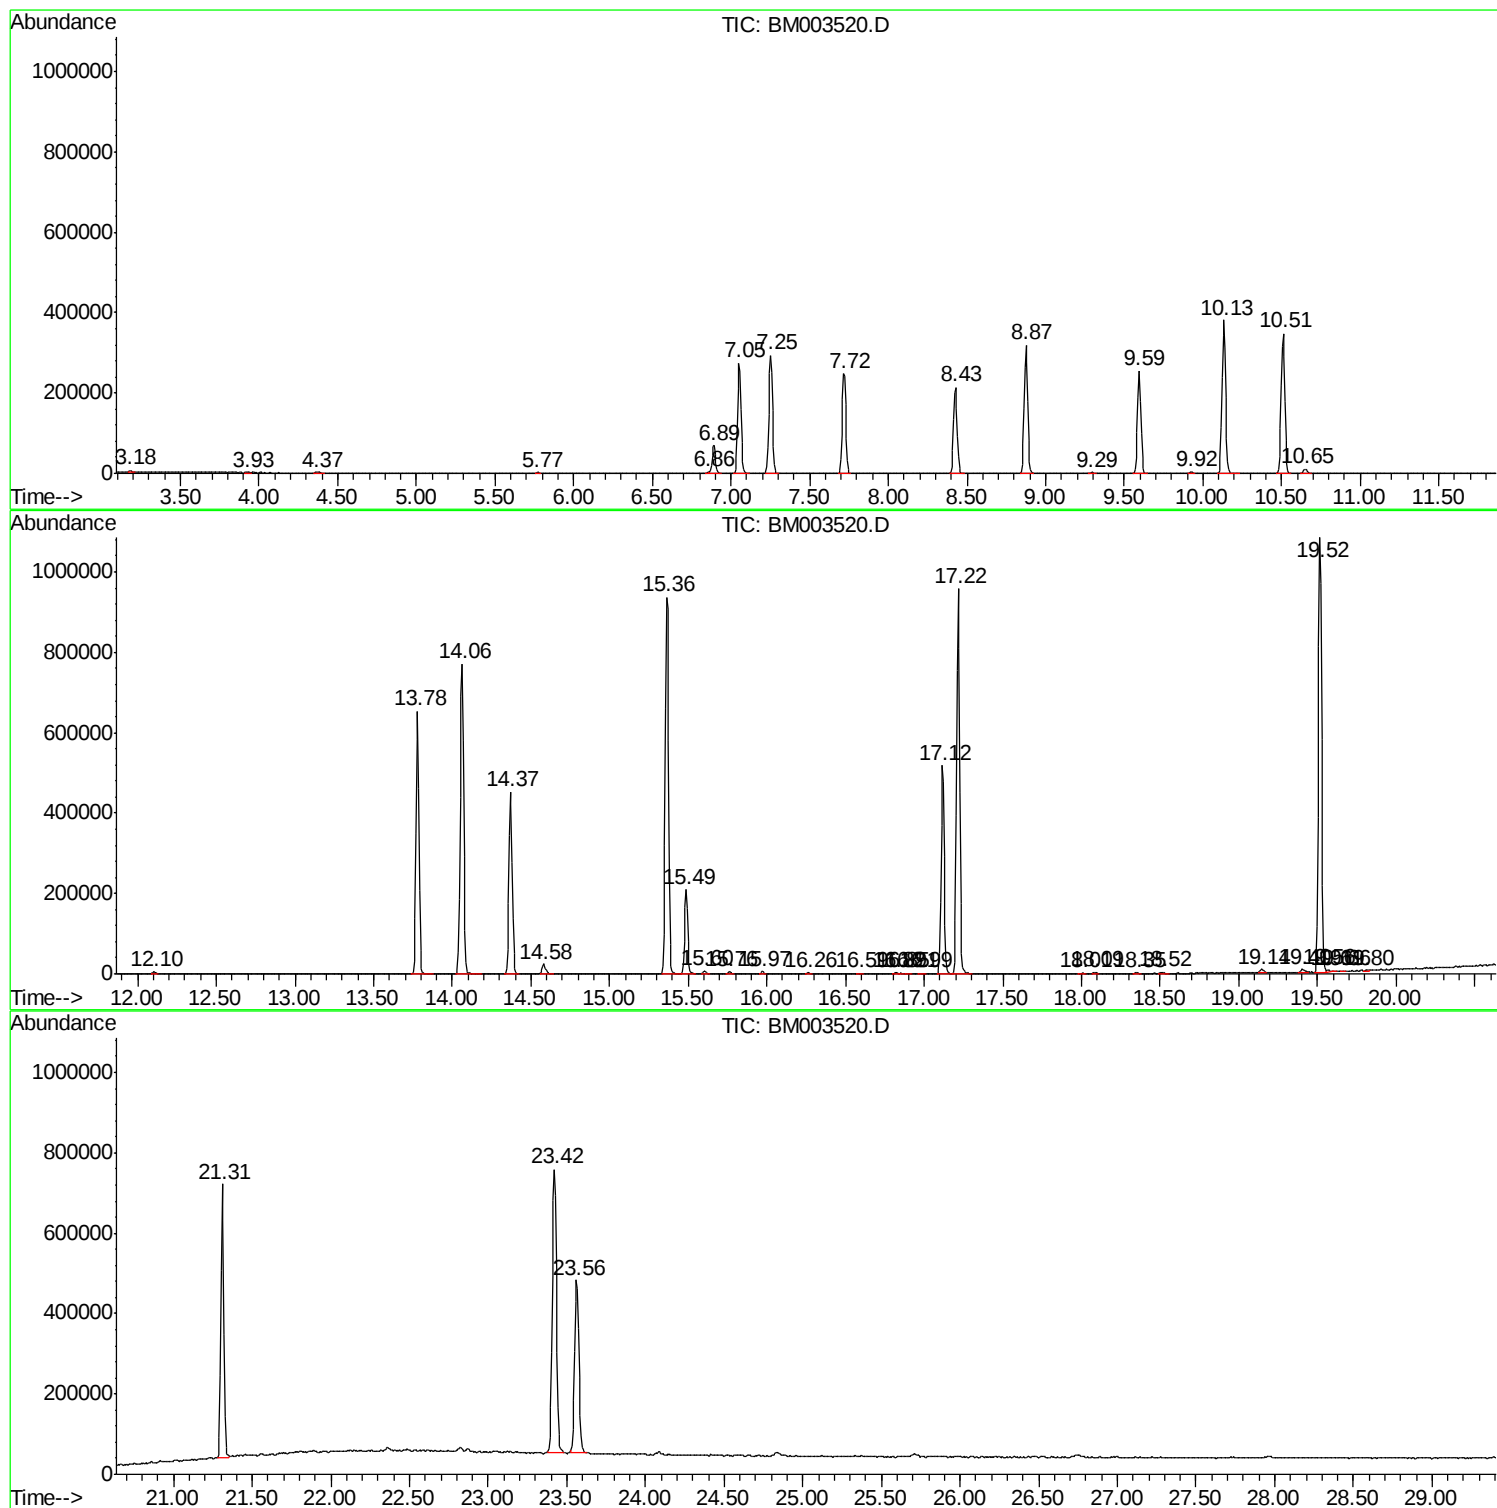

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003520.D
Acq On : 13 Dec 2015 21:49
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003520.D
Acq On : 13 Dec 2015 21:49
Operator : UM/IZ
Sample : G4722-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc