

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003523.D
 Acq On : 13 Dec 2015 23:37
 Operator : UM/IZ
 Sample : G4722-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB2	2560	3420	0.29%	0.024%
2	3.922	138	142	146	rBV	3060	4382	0.37%	0.031%
3	6.892	640	647	656	rBB2	57558	95704	8.03%	0.666%
4	7.051	668	674	683	rBB	192312	292036	24.50%	2.034%
5	7.251	702	708	716	rBB	213900	329615	27.66%	2.295%
6	7.722	781	788	794	rBB	258432	410630	34.46%	2.860%
7	8.428	902	908	917	rBB	182250	276466	23.20%	1.925%
8	8.875	978	984	993	rBB	238396	374303	31.41%	2.607%
9	9.292	1051	1055	1059	rBB2	2778	3991	0.33%	0.028%
10	9.592	1100	1106	1114	rBB	189897	313607	26.31%	2.184%
11	10.133	1192	1198	1206	rBV	320680	514056	43.13%	3.580%
12	10.204	1206	1210	1216	rVB	6398	10014	0.84%	0.070%
13	10.510	1255	1262	1271	rBB	403119	653852	54.86%	4.553%
14	10.651	1279	1286	1302	rBV	284055	477021	40.03%	3.322%
15	11.780	1475	1478	1482	rBB	1099	1369	0.11%	0.010%
16	12.104	1529	1533	1537	rBB	3401	4931	0.41%	0.034%
17	12.969	1678	1680	1684	rBB2	2269	1860	0.16%	0.013%
18	13.192	1715	1718	1721	rBB	3653	3948	0.33%	0.027%
19	13.316	1736	1739	1741	rBB2	2477	2823	0.24%	0.020%
20	13.404	1751	1754	1757	rBB	1372	1800	0.15%	0.013%
21	13.780	1812	1818	1823	rBV	587007	813097	68.23%	5.662%
22	13.827	1823	1826	1834	rVV	28070	38086	3.20%	0.265%
23	13.892	1834	1837	1840	rVB	1368	1425	0.12%	0.010%
24	13.968	1848	1850	1853	rBB	1209	1333	0.11%	0.009%
25	14.021	1854	1859	1860	rBV2	2375	2976	0.25%	0.021%
26	14.063	1860	1866	1879	rVB	647575	937814	78.69%	6.531%
27	14.268	1897	1901	1910	rBV2	21020	33797	2.84%	0.235%
28	14.374	1910	1919	1929	rVB2	541351	864613	72.55%	6.021%
29	14.510	1938	1942	1947	rBV2	2646	4319	0.36%	0.030%
30	14.586	1949	1955	1967	rBV	25403	45398	3.81%	0.316%
31	14.668	1967	1969	1972	rVV2	1689	1477	0.12%	0.010%
32	14.721	1972	1978	1979	rVV2	2771	4607	0.39%	0.032%
33	14.739	1979	1981	1984	rVV3	3449	3896	0.33%	0.027%
34	14.774	1984	1987	1989	rVV3	3415	4311	0.36%	0.030%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003523.D
 Acq On : 13 Dec 2015 23:37
 Operator : UM/IZ
 Sample : G4722-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	14.827	1992	1996	2000	rVV2	3319	6021	0.51%	0.042%
36	14.886	2002	2006	2012	rVB5	6615	12972	1.09%	0.090%
37	14.963	2012	2019	2023	rBV2	3691	6568	0.55%	0.046%
38	15.039	2027	2032	2040	rVB5	5648	12527	1.05%	0.087%
39	15.110	2040	2044	2046	rBV	1921	3004	0.25%	0.021%
40	15.157	2050	2052	2055	rBV3	932	1231	0.10%	0.009%
41	15.221	2058	2063	2068	rVB	34603	43177	3.62%	0.301%
42	15.286	2068	2074	2078	rBV2	2658	6117	0.51%	0.043%
43	15.362	2081	2087	2094	rBV	790040	1151600	96.63%	8.020%
44	15.486	2102	2108	2113	rBV	138882	186185	15.62%	1.297%
45	15.610	2122	2129	2137	rBV6	13673	37063	3.11%	0.258%
46	15.668	2137	2139	2142	rVV2	4621	4439	0.37%	0.031%
47	15.727	2144	2149	2154	rBV3	3935	7517	0.63%	0.052%
48	15.780	2154	2158	2163	rVB3	4542	6868	0.58%	0.048%
49	15.839	2163	2168	2172	rVB3	5079	7750	0.65%	0.054%
50	15.933	2179	2184	2186	rBV4	2828	4398	0.37%	0.031%
51	16.027	2197	2200	2201	rBV2	2364	2934	0.25%	0.020%
52	16.086	2206	2210	2218	rVV	38682	58240	4.89%	0.406%
53	16.227	2232	2234	2237	rVB3	1595	1475	0.12%	0.010%
54	16.262	2237	2240	2242	rBV2	4440	4707	0.39%	0.033%
55	16.298	2244	2246	2248	rVV2	4507	3539	0.30%	0.025%
56	16.368	2252	2258	2264	rBV4	10572	14939	1.25%	0.104%
57	16.427	2264	2268	2276	rBV3	6086	10382	0.87%	0.072%
58	16.504	2276	2281	2286	rVB3	4775	8881	0.75%	0.062%
59	16.545	2286	2288	2291	rBV4	2808	1972	0.17%	0.014%
60	16.615	2291	2300	2306	rBV2	22235	39954	3.35%	0.278%
61	16.692	2311	2313	2316	rVB3	2151	1643	0.14%	0.011%
62	16.739	2319	2321	2324	rBV3	1279	1392	0.12%	0.010%
63	16.786	2324	2329	2335	rVB2	8501	11567	0.97%	0.081%
64	16.833	2335	2337	2339	rBV3	1388	1567	0.13%	0.011%
65	16.880	2340	2345	2349	rBV	20388	26636	2.24%	0.185%
66	16.927	2351	2353	2357	rVB3	3246	3835	0.32%	0.027%
67	17.015	2366	2368	2371	rVB4	1454	1321	0.11%	0.009%
68	17.115	2379	2385	2392	rBV2	619738	905530	75.98%	6.306%
69	17.215	2394	2402	2415	rVB2	796177	1142555	95.87%	7.957%
70	17.362	2422	2427	2431	rVB3	5232	8457	0.71%	0.059%
71	17.421	2433	2437	2439	rVB4	1497	2119	0.18%	0.015%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003523.D
 Acq On : 13 Dec 2015 23:37
 Operator : UM/IZ
 Sample : G4722-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04C9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	17.480	2443	2447	2448	rBV3	2867	2774	0.23%	0.019%
73	17.580	2461	2464	2465	rBV3	1752	1459	0.12%	0.010%
74	17.615	2468	2470	2473	rVV	4197	4099	0.34%	0.029%
75	17.662	2474	2478	2483	rVB6	3113	6086	0.51%	0.042%
76	17.909	2514	2520	2526	rBV3	9246	16670	1.40%	0.116%
77	17.962	2527	2529	2532	rBV2	3383	3521	0.30%	0.025%
78	18.015	2534	2538	2541	rVV2	8030	10620	0.89%	0.074%
79	18.309	2584	2588	2593	rBV5	4761	8724	0.73%	0.061%
80	18.398	2601	2603	2606	rBV4	1572	2446	0.21%	0.017%
81	18.421	2606	2607	2612	rBV3	2427	2534	0.21%	0.018%
82	18.468	2613	2615	2618	rBV3	1580	1685	0.14%	0.012%
83	18.509	2619	2622	2623	rBV	3899	3597	0.30%	0.025%
84	18.639	2641	2644	2652	rBV8	3200	5391	0.45%	0.038%
85	18.715	2654	2657	2659	rVB3	2075	2118	0.18%	0.015%
86	18.868	2678	2683	2691	rBV5	5643	12222	1.03%	0.085%
87	18.933	2691	2694	2700	rBV6	2085	4771	0.40%	0.033%
88	19.121	2718	2726	2727	rBV7	1813	4104	0.34%	0.029%
89	19.150	2727	2731	2736	rVB	8438	13743	1.15%	0.096%
90	19.303	2753	2757	2758	rBV3	4679	5082	0.43%	0.035%
91	19.403	2771	2774	2781	rVB	6390	10023	0.84%	0.070%
92	19.456	2781	2783	2787	rVB3	2546	1474	0.12%	0.010%
93	19.515	2787	2793	2799	rBV2	871985	1191753	100.00%	8.299%
94	20.227	2912	2914	2916	rBV2	3485	2421	0.20%	0.017%
95	20.433	2945	2949	2956	rBV2	11827	17088	1.43%	0.119%
96	21.021	3045	3049	3056	rBV	41482	63145	5.30%	0.440%
97	21.309	3093	3098	3104	rBV	725559	913430	76.65%	6.361%
98	23.421	3450	3457	3467	rVB	473568	891942	74.84%	6.212%
99	23.562	3474	3481	3491	rVB2	457646	872479	73.21%	6.076%


Sum of corrected areas: 14359460

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003523.D
Acq On : 13 Dec 2015 23:37
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

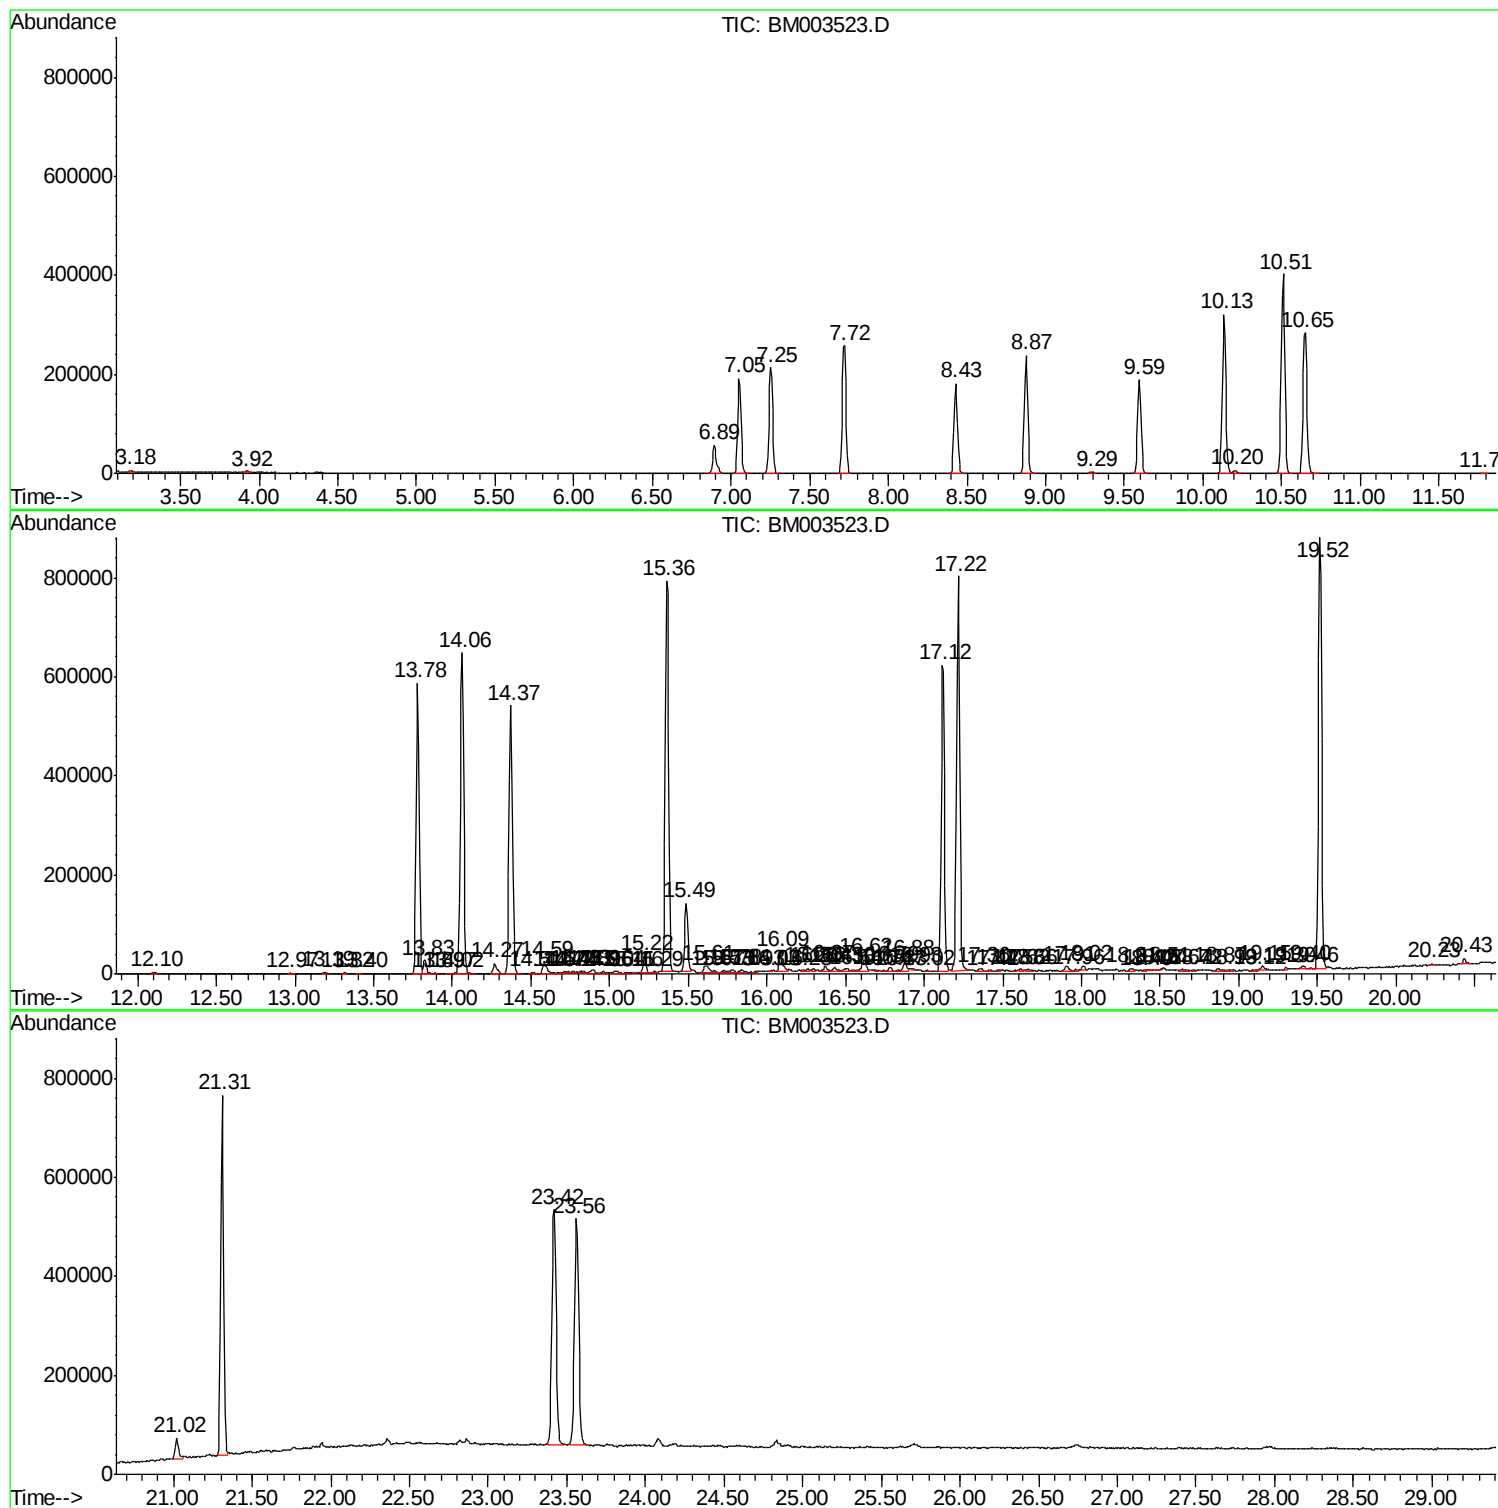

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003523.D
Acq On : 13 Dec 2015 23:37
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003523.D
Acq On : 13 Dec 2015 23:37
Operator : UM/IZ
Sample : G4722-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04C9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc