

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003526.D
 Acq On : 14 Dec 2015 01:25
 Operator : UM/IZ
 Sample : PB87248BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	23	rVB	22423	26170	1.41%	0.142%
2	3.740	108	111	117	rVB2	3281	3844	0.21%	0.021%
3	6.893	641	647	660	rBB	355214	542357	29.19%	2.953%
4	7.051	668	674	686	rBB	283584	436066	23.47%	2.374%
5	7.251	702	708	716	rBV	380545	582058	31.33%	3.169%
6	7.716	781	787	794	rBB	231933	365854	19.69%	1.992%
7	8.428	902	908	918	rBV	451762	716754	38.58%	3.902%
8	8.875	978	984	993	rBV	331126	526075	28.32%	2.864%
9	9.598	1100	1107	1114	rBB	272528	436790	23.51%	2.378%
10	10.134	1192	1198	1210	rBV	441858	706823	38.04%	3.848%
11	10.510	1255	1262	1270	rBB	346285	557237	29.99%	3.034%
12	10.651	1279	1286	1305	rBV	419684	723426	38.94%	3.939%
13	12.104	1529	1533	1537	rBB2	5325	7725	0.42%	0.042%
14	13.780	1812	1818	1828	rBV	742760	1006286	54.16%	5.479%
15	14.063	1859	1866	1880	rBV	855136	1248821	67.22%	6.799%
16	14.369	1912	1918	1926	rBB2	454638	691591	37.23%	3.765%
17	14.580	1949	1954	1976	rBV	236625	363294	19.55%	1.978%
18	15.363	2081	2087	2099	rBV	1019015	1509728	81.26%	8.220%
19	15.486	2103	2108	2114	rBV	211669	264538	14.24%	1.440%
20	15.604	2123	2128	2132	rBV2	9363	11450	0.62%	0.062%
21	16.904	2344	2349	2352	rBV2	1502	2388	0.13%	0.013%
22	17.115	2379	2385	2396	rBV2	530704	744905	40.09%	4.056%
23	17.215	2396	2402	2416	rVV2	1091883	1550377	83.45%	8.441%
24	19.151	2727	2731	2737	rVB	9593	12001	0.65%	0.065%
25	19.404	2770	2774	2779	rVB	6830	8714	0.47%	0.047%
26	19.515	2787	2793	2807	rBV2	1276703	1746774	94.02%	9.511%
27	20.068	2885	2887	2891	rBV3	1373	2153	0.12%	0.012%
28	21.309	3093	3098	3106	rBV	700045	861608	46.38%	4.691%
29	23.421	3449	3457	3470	rBV	988150	1857866	100.00%	10.115%
30	23.562	3474	3481	3494	rVB2	465127	853105	45.92%	4.645%


Sum of corrected areas: 18366778

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003526.D
Acq On : 14 Dec 2015 01:25
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

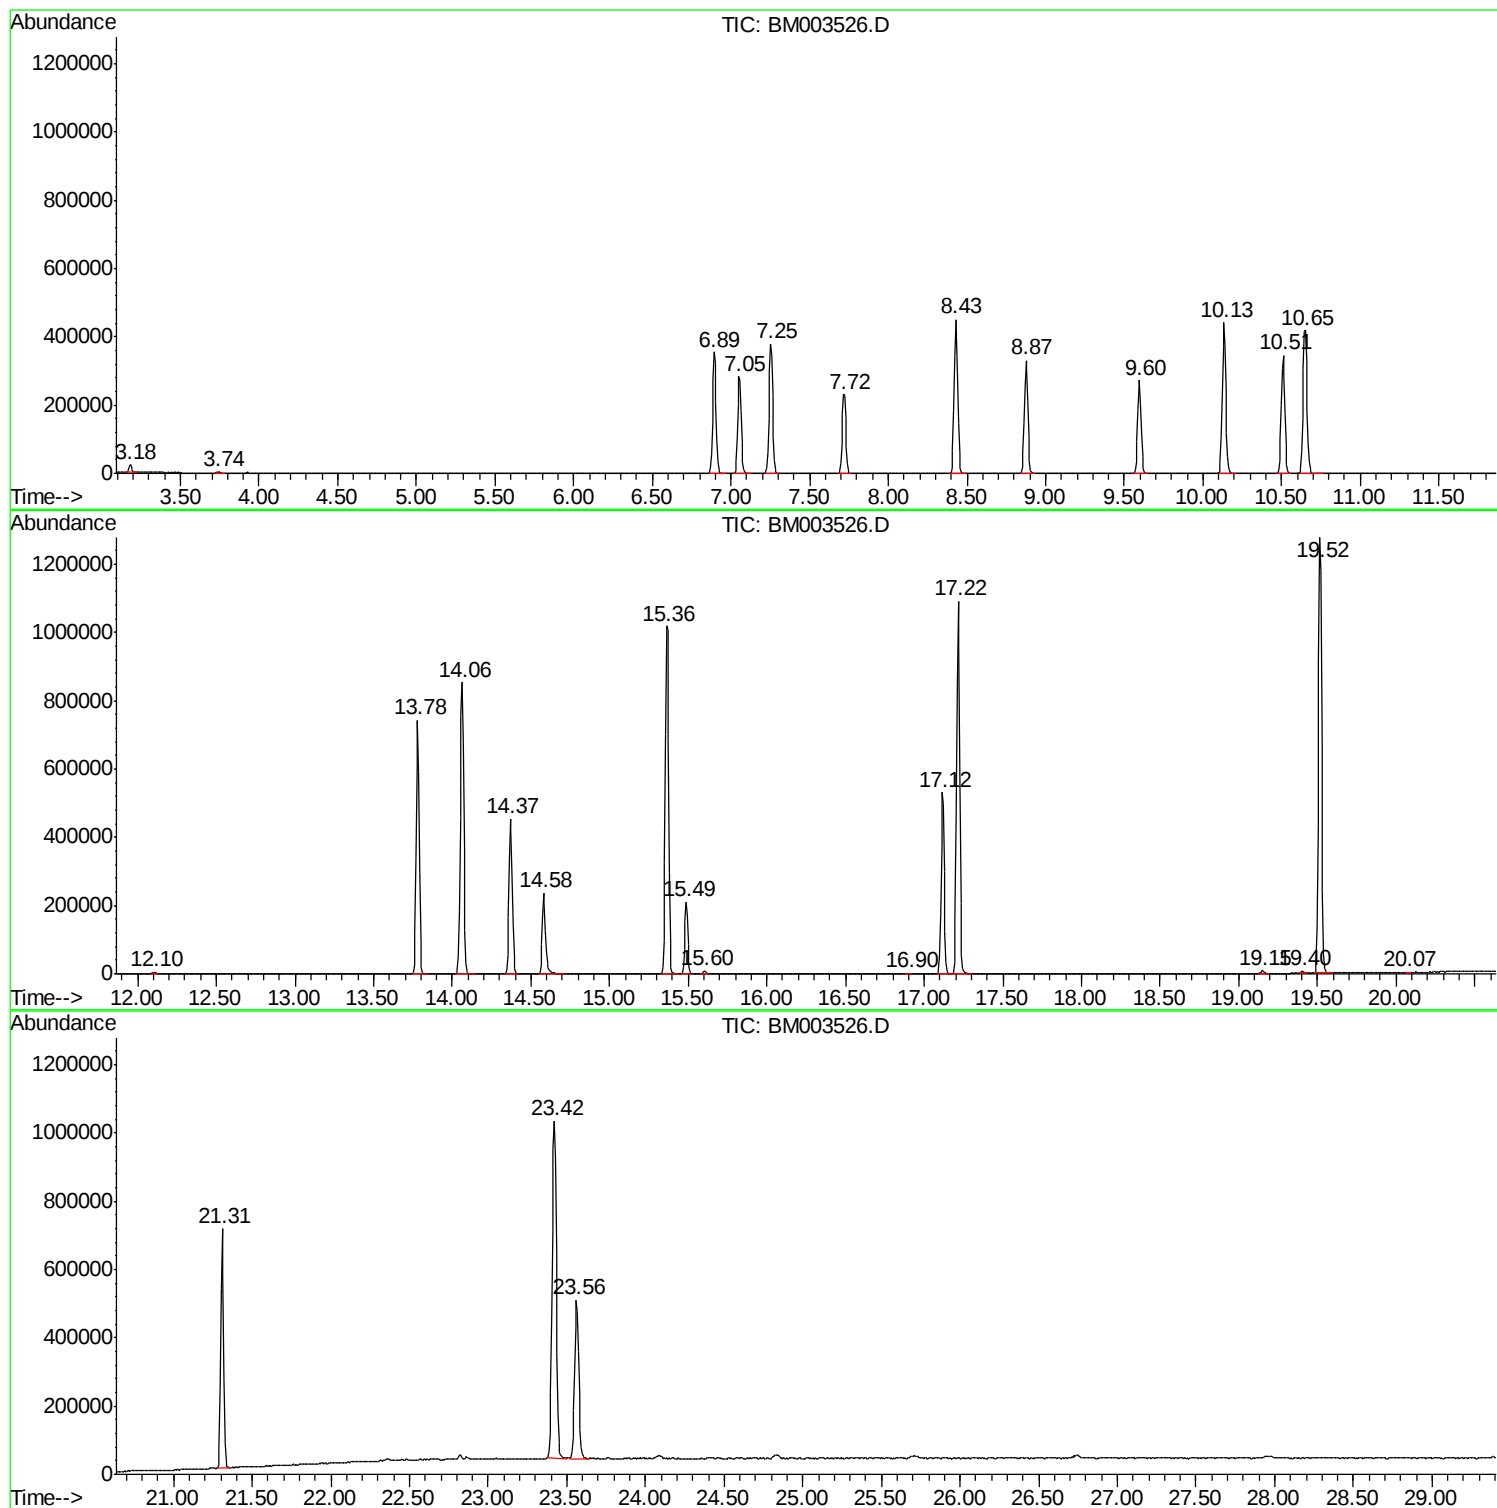

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003526.D
Acq On : 14 Dec 2015 01:25
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003526.D
Acq On : 14 Dec 2015 01:25
Operator : UM/IZ
Sample : PB87248BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK48

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc