

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003527.D
 Acq On : 14 Dec 2015 02:01
 Operator : UM/IZ
 Sample : G4722-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	14	16	20	rVB2	2244	2338	0.22%	0.018%
2	3.922	138	142	148	rVB	2931	4190	0.39%	0.032%
3	4.287	200	204	207	rVB	4905	5767	0.53%	0.044%
4	4.363	215	217	224	rBV2	1386	1408	0.13%	0.011%
5	6.893	642	647	656	rVB2	54744	89305	8.28%	0.676%
6	7.051	668	674	684	rBB	179552	270091	25.03%	2.043%
7	7.251	702	708	716	rBB	199568	306775	28.43%	2.320%
8	7.716	781	787	796	rBB	242814	383747	35.57%	2.903%
9	8.428	901	908	916	rBV	170408	259612	24.06%	1.964%
10	8.875	978	984	992	rBB	215759	339242	31.44%	2.566%
11	9.292	1051	1055	1058	rBB	1861	2240	0.21%	0.017%
12	9.598	1100	1107	1113	rBB	171669	279913	25.94%	2.117%
13	10.134	1192	1198	1206	rBV	297831	474008	43.93%	3.585%
14	10.204	1206	1210	1216	rVB2	6648	11073	1.03%	0.084%
15	10.510	1255	1262	1271	rBB	373842	611315	56.66%	4.624%
16	10.651	1279	1286	1306	rBB	223583	382442	35.45%	2.893%
17	12.104	1529	1533	1537	rBB	3283	4563	0.42%	0.035%
18	12.969	1677	1680	1683	rBB2	1400	1358	0.13%	0.010%
19	13.186	1715	1717	1720	rBB	2467	2606	0.24%	0.020%
20	13.780	1812	1818	1822	rBV	538751	736507	68.26%	5.571%
21	13.827	1822	1826	1833	rVB	73412	102469	9.50%	0.775%
22	13.886	1834	1836	1840	rBB	1317	1760	0.16%	0.013%
23	14.063	1859	1866	1874	rVV	597056	847284	78.53%	6.409%
24	14.269	1895	1901	1909	rBV2	17593	27843	2.58%	0.211%
25	14.369	1909	1918	1928	rVV2	531066	809247	75.01%	6.121%
26	14.510	1938	1942	1944	rBV	1519	2108	0.20%	0.016%
27	14.586	1949	1955	1964	rVV2	21039	37681	3.49%	0.285%
28	14.657	1964	1967	1970	rVV2	1150	1443	0.13%	0.011%
29	14.716	1973	1977	1978	rBV	3561	5273	0.49%	0.040%
30	14.733	1978	1980	1983	rVV2	3405	4415	0.41%	0.033%
31	14.769	1983	1986	1989	rVV	2950	4704	0.44%	0.036%
32	14.821	1993	1995	1999	rVV2	2750	4236	0.39%	0.032%
33	14.886	2003	2006	2014	rVB2	4770	8893	0.82%	0.067%
34	14.957	2014	2018	2023	rBV2	3235	5253	0.49%	0.040%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003527.D
 Acq On : 14 Dec 2015 02:01
 Operator : UM/IZ
 Sample : G4722-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.039	2025	2032	2036	rBV5	3733	7130	0.66%	0.054%
36	15.104	2041	2043	2045	rBV5	1381	1588	0.15%	0.012%
37	15.163	2049	2053	2055	rBV3	2233	3309	0.31%	0.025%
38	15.221	2055	2063	2068	rVB	31618	40746	3.78%	0.308%
39	15.286	2068	2074	2076	rBV4	1966	3531	0.33%	0.027%
40	15.363	2081	2087	2098	rVV	729949	1057179	97.98%	7.997%
41	15.486	2103	2108	2115	rBV	114507	155458	14.41%	1.176%
42	15.610	2123	2129	2131	rBV	12131	18628	1.73%	0.141%
43	15.668	2136	2139	2143	rVB4	3766	5811	0.54%	0.044%
44	15.721	2143	2148	2152	rBV4	5224	8766	0.81%	0.066%
45	15.774	2154	2157	2163	rVB3	5246	6835	0.63%	0.052%
46	15.839	2163	2168	2172	rVB2	5085	7292	0.68%	0.055%
47	15.927	2181	2183	2186	rBV2	919	1442	0.13%	0.011%
48	16.027	2196	2200	2201	rBV2	2888	3748	0.35%	0.028%
49	16.086	2205	2210	2213	rBV	37875	51390	4.76%	0.389%
50	16.257	2236	2239	2243	rBV4	4279	5348	0.50%	0.040%
51	16.292	2243	2245	2249	rVV2	3661	3617	0.34%	0.027%
52	16.368	2253	2258	2262	rBV4	7258	10747	1.00%	0.081%
53	16.433	2265	2269	2275	rVB2	5932	10140	0.94%	0.077%
54	16.504	2275	2281	2286	rBV4	4816	9123	0.85%	0.069%
55	16.580	2292	2294	2295	rBV2	2610	2252	0.21%	0.017%
56	16.615	2296	2300	2305	rVB	16080	23910	2.22%	0.181%
57	16.786	2324	2329	2332	rBV3	6654	9283	0.86%	0.070%
58	16.874	2340	2344	2348	rBV	21907	26721	2.48%	0.202%
59	16.927	2351	2353	2356	rVB2	4205	3798	0.35%	0.029%
60	17.010	2365	2367	2377	rVB6	2007	4404	0.41%	0.033%
61	17.115	2380	2385	2392	rVV2	589985	853670	79.12%	6.457%
62	17.215	2393	2402	2413	rVB	720296	1031320	95.59%	7.801%
63	17.362	2422	2427	2431	rVB5	5545	9672	0.90%	0.073%
64	17.421	2431	2437	2439	rBV4	2522	4654	0.43%	0.035%
65	17.480	2444	2447	2449	rBV4	2808	3500	0.32%	0.026%
66	17.568	2459	2462	2464	rBV2	1460	1824	0.17%	0.014%
67	17.615	2467	2470	2473	rVV2	4065	4546	0.42%	0.034%
68	17.662	2476	2478	2481	rBV4	2364	2621	0.24%	0.020%
69	17.798	2498	2501	2502	rBV3	1437	1425	0.13%	0.011%
70	17.904	2514	2519	2525	rBV3	9708	18134	1.68%	0.137%
71	17.974	2528	2531	2532	rVB2	1825	1832	0.17%	0.014%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003527.D
 Acq On : 14 Dec 2015 02:01
 Operator : UM/IZ
 Sample : G4722-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

72	18.015	2532	2538	2541	rBV4	6901	10428	0.97%	0.079%
73	18.057	2543	2545	2547	rVB2	2422	1900	0.18%	0.014%
74	18.174	2562	2565	2567	rBV3	2064	1960	0.18%	0.015%
75	18.221	2567	2573	2575	rVV5	3147	4419	0.41%	0.033%
76	18.262	2579	2580	2582	rBV	2021	1493	0.14%	0.011%
77	18.309	2585	2588	2594	rBV4	5302	9148	0.85%	0.069%
78	18.427	2607	2608	2611	rBV2	2506	1899	0.18%	0.014%
79	18.521	2622	2624	2628	rVB	3861	5057	0.47%	0.038%
80	18.633	2642	2643	2648	rVB3	1890	2570	0.24%	0.019%
81	18.774	2665	2667	2672	rBV3	2439	3171	0.29%	0.024%
82	18.862	2679	2682	2686	rBV2	4596	7374	0.68%	0.056%
83	18.933	2690	2694	2699	rVB3	2907	4282	0.40%	0.032%
84	19.109	2723	2724	2727	rVV3	1372	1428	0.13%	0.011%
85	19.151	2727	2731	2738	rVB	8899	12641	1.17%	0.096%
86	19.292	2753	2755	2757	rBV2	2275	2228	0.21%	0.017%
87	19.362	2764	2767	2770	rBV4	1809	2108	0.20%	0.016%
88	19.404	2771	2774	2778	rVB	6032	7166	0.66%	0.054%
89	19.456	2781	2783	2785	rVB3	3147	2047	0.19%	0.015%
90	19.515	2787	2793	2799	rBV	802234	1078921	100.00%	8.161%
91	19.704	2823	2825	2829	rBV5	2337	4089	0.38%	0.031%
92	19.804	2841	2842	2844	rBV2	2054	1560	0.14%	0.012%
93	19.945	2863	2866	2869	rBV4	2695	4328	0.40%	0.033%
94	20.103	2891	2893	2896	rVB3	2113	1898	0.18%	0.014%
95	20.433	2945	2949	2954	rBV4	8516	10545	0.98%	0.080%
96	20.545	2967	2968	2970	rBV	3429	3340	0.31%	0.025%
97	21.021	3045	3049	3054	rBV2	27338	40182	3.72%	0.304%
98	21.309	3093	3098	3106	rBV	692076	869899	80.63%	6.580%
99	23.421	3450	3457	3467	rVB	450730	858496	79.57%	6.494%
100	23.562	3474	3481	3493	rVB2	436862	819154	75.92%	6.196%


Sum of corrected areas: 13220234

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003527.D
Acq On : 14 Dec 2015 02:01
Operator : UM/IZ
Sample : G4722-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

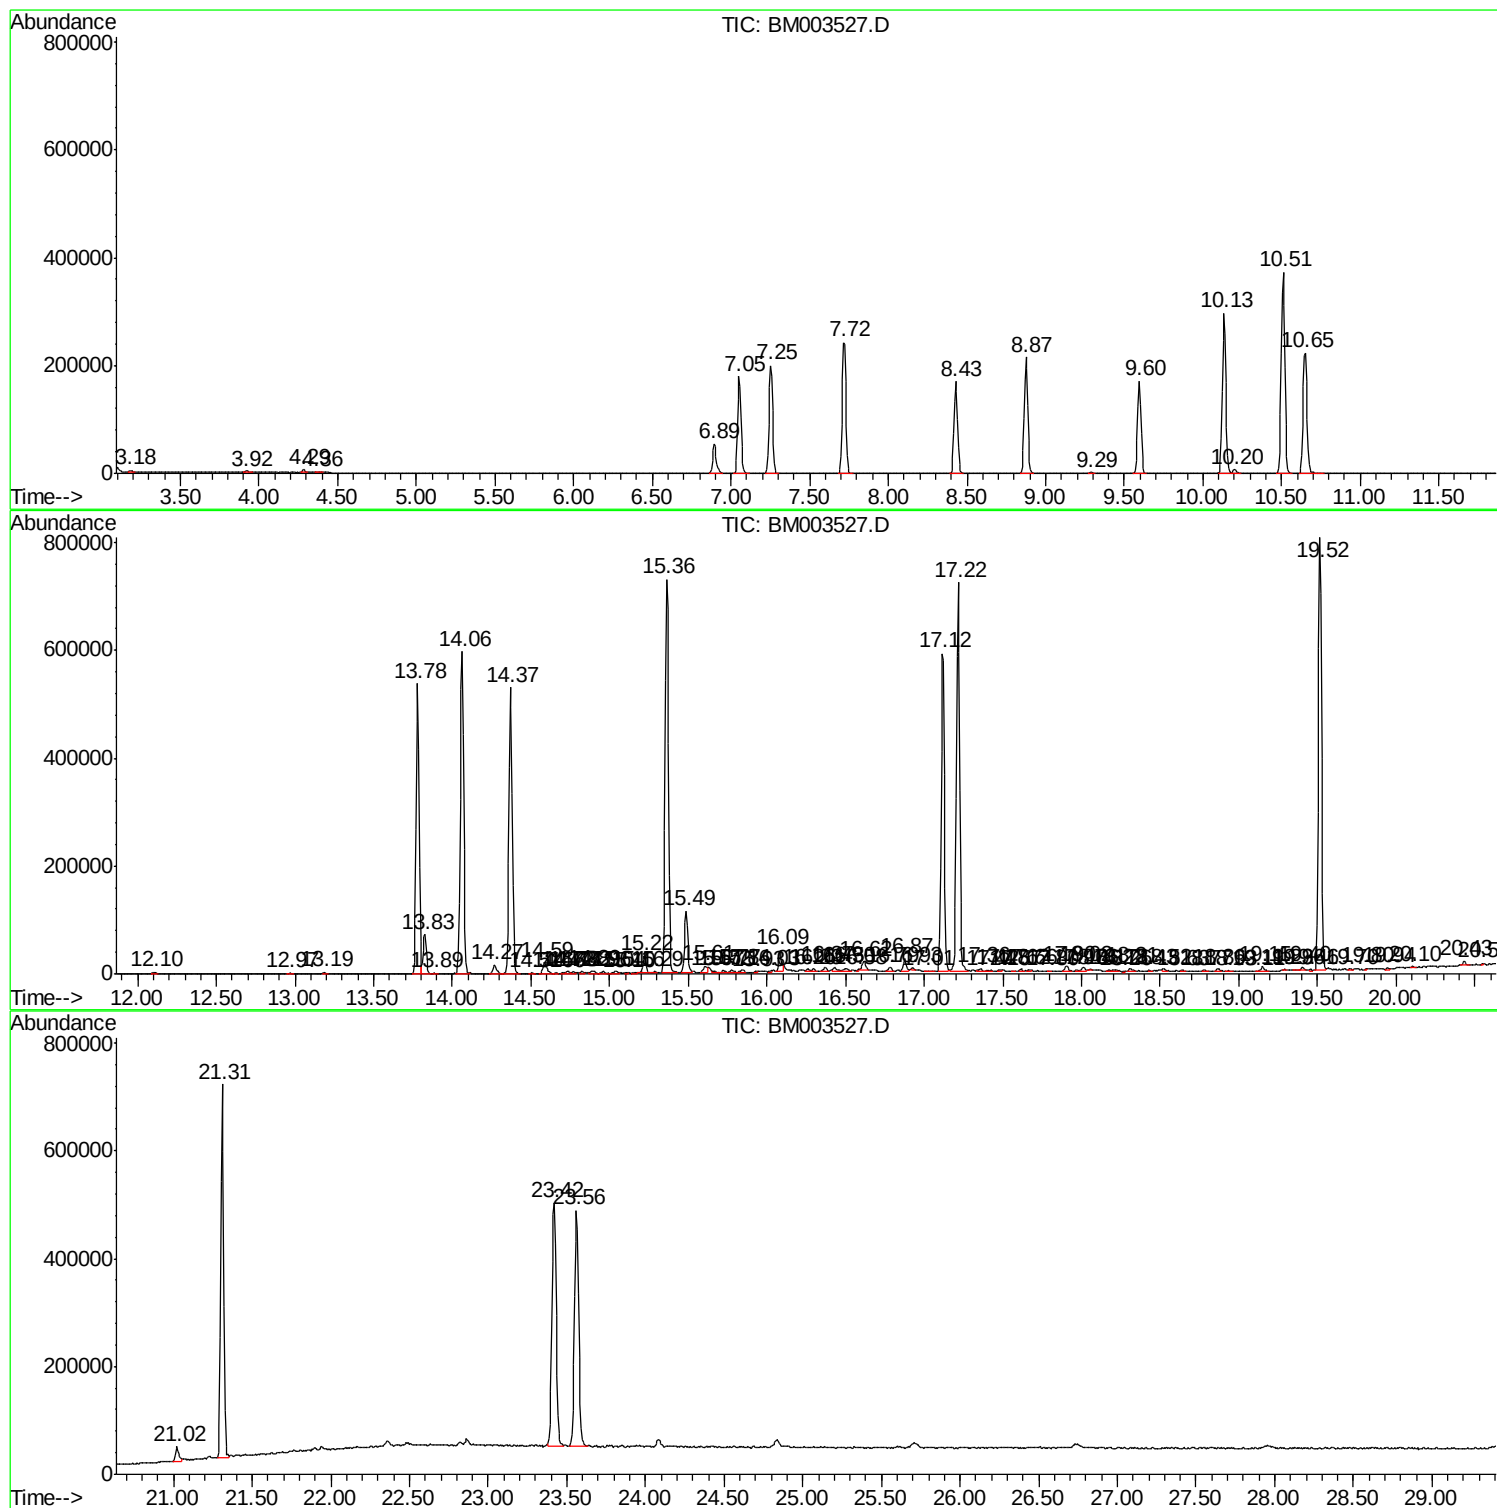

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003527.D
Acq On : 14 Dec 2015 02:01
Operator : UM/IZ
Sample : G4722-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003527.D
Acq On : 14 Dec 2015 02:01
Operator : UM/IZ
Sample : G4722-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04D8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc