

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003530.D
 Acq On : 14 Dec 2015 03:50
 Operator : UM/IZ
 Sample : G4722-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	20	rVB	1509	1701	0.19%	0.017%
2	3.469	62	65	67	rVB3	1158	1028	0.11%	0.010%
3	5.240	361	366	370	rBB2	3450	5113	0.56%	0.051%
4	6.892	641	647	656	rBB2	31437	51612	5.67%	0.513%
5	7.051	669	674	683	rBB	120750	181571	19.96%	1.805%
6	7.251	702	708	715	rBB	128427	196959	21.65%	1.958%
7	7.716	781	787	795	rBB	249414	400152	43.98%	3.978%
8	7.781	795	798	802	rBB	3071	3011	0.33%	0.030%
9	8.086	847	850	855	rBB	3715	5307	0.58%	0.053%
10	8.428	903	908	916	rBB	101000	154945	17.03%	1.540%
11	8.875	978	984	992	rBB	139391	219206	24.09%	2.179%
12	9.292	1052	1055	1058	rBB	1483	1840	0.20%	0.018%
13	9.598	1101	1107	1113	rBB	108957	174053	19.13%	1.730%
14	10.133	1192	1198	1209	rBB	183046	294916	32.42%	2.931%
15	10.510	1255	1262	1267	rBV	382109	630697	69.33%	6.269%
16	10.557	1267	1270	1276	rVB	23462	34597	3.80%	0.344%
17	10.651	1279	1286	1301	rBB	167866	281042	30.89%	2.794%
18	12.104	1530	1533	1536	rBB2	1853	2382	0.26%	0.024%
19	12.180	1542	1546	1550	rBB	3117	4744	0.52%	0.047%
20	12.398	1579	1583	1587	rBB	3930	5774	0.63%	0.057%
21	13.186	1715	1717	1721	rBB	2348	2286	0.25%	0.023%
22	13.780	1812	1818	1823	rBV	336021	462065	50.79%	4.593%
23	13.827	1823	1826	1834	rVB	26658	33322	3.66%	0.331%
24	14.063	1859	1866	1877	rBV	362437	525555	57.77%	5.224%
25	14.268	1897	1901	1905	rBB	13463	16247	1.79%	0.161%
26	14.368	1912	1918	1927	rBV2	521851	808724	88.89%	8.039%
27	14.433	1927	1929	1932	rVB	1823	2039	0.22%	0.020%
28	14.592	1951	1956	1964	rBB2	8519	14791	1.63%	0.147%
29	14.715	1974	1977	1979	rBV	1738	2253	0.25%	0.022%
30	14.739	1979	1981	1983	rVB2	1869	1517	0.17%	0.015%
31	14.768	1983	1986	1989	rBB	1733	2083	0.23%	0.021%
32	14.827	1993	1996	1999	rVB	2174	2044	0.22%	0.020%
33	14.886	2003	2006	2010	rBB2	3275	4217	0.46%	0.042%
34	14.957	2016	2018	2022	rBB	2237	2149	0.24%	0.021%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
 Data File : BM003530.D
 Acq On : 14 Dec 2015 03:50
 Operator : UM/IZ
 Sample : G4722-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

35	15.115	2041	2045	2048	rBB	2176	2669	0.29%	0.027%
36	15.168	2052	2054	2056	rBV	1485	1560	0.17%	0.016%
37	15.221	2058	2063	2069	rVB	20853	26830	2.95%	0.267%
38	15.280	2070	2073	2079	rBV2	2541	3566	0.39%	0.035%
39	15.362	2082	2087	2095	rVV	457215	663748	72.96%	6.598%
40	15.415	2095	2096	2101	rVV	2457	2968	0.33%	0.030%
41	15.486	2104	2108	2116	rVV	63310	83651	9.19%	0.831%
42	15.604	2125	2128	2136	rBV3	6389	16126	1.77%	0.160%
43	15.668	2136	2139	2143	rVB	2128	2462	0.27%	0.024%
44	15.721	2143	2148	2154	rVB	3078	4316	0.47%	0.043%
45	15.780	2154	2158	2162	rBV2	5006	7312	0.80%	0.073%
46	15.839	2165	2168	2174	rVB2	3675	4896	0.54%	0.049%
47	16.021	2197	2199	2200	rVV2	2070	1663	0.18%	0.017%
48	16.039	2200	2202	2206	rVV	1561	2423	0.27%	0.024%
49	16.086	2206	2210	2217	rVV	22417	36799	4.04%	0.366%
50	16.139	2217	2219	2222	rVV3	2702	3398	0.37%	0.034%
51	16.168	2222	2224	2227	rVV2	1373	1152	0.13%	0.011%
52	16.209	2227	2231	2234	rVB4	1353	2044	0.22%	0.020%
53	16.262	2237	2240	2242	rVB2	2373	2597	0.29%	0.026%
54	16.292	2242	2245	2248	rBV2	2301	3497	0.38%	0.035%
55	16.345	2252	2254	2256	rBV	1599	1291	0.14%	0.013%
56	16.433	2263	2269	2271	rBV2	3404	5621	0.62%	0.056%
57	16.504	2275	2281	2285	rVV3	3201	7545	0.83%	0.075%
58	16.551	2285	2289	2291	rVV2	1762	2595	0.29%	0.026%
59	16.574	2291	2293	2294	rVV2	1913	1581	0.17%	0.016%
60	16.592	2294	2296	2302	rVV3	2603	3508	0.39%	0.035%
61	16.657	2305	2307	2310	rVV3	2609	2680	0.29%	0.027%
62	16.692	2310	2313	2315	rVB	1768	1714	0.19%	0.017%
63	16.780	2325	2328	2329	rBV2	1450	1180	0.13%	0.012%
64	16.874	2337	2344	2348	rVV2	13992	20451	2.25%	0.203%
65	16.951	2351	2357	2360	rVV3	6065	12785	1.41%	0.127%
66	16.980	2360	2362	2365	rVV2	1588	1703	0.19%	0.017%
67	17.021	2365	2369	2373	rVB2	1763	3504	0.39%	0.035%
68	17.115	2379	2385	2391	rBV2	585331	840620	92.40%	8.356%
69	17.215	2395	2402	2413	rVV2	456132	654744	71.97%	6.508%
70	17.298	2415	2416	2420	rVV	745	1130	0.12%	0.011%
71	17.356	2422	2426	2430	rVB2	2109	2948	0.32%	0.029%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003530.D
Acq On : 14 Dec 2015 03:50
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04F4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

72	17.574	2459	2463	2467	rBV2	982	1472	0.16%	0.015%
73	17.615	2467	2470	2474	rVV	3732	5113	0.56%	0.051%
74	17.645	2474	2475	2479	rVB2	1064	1025	0.11%	0.010%
75	17.839	2506	2508	2514	rBV2	682	1471	0.16%	0.015%
76	17.903	2514	2519	2524	rVV	4938	8177	0.90%	0.081%
77	17.962	2527	2529	2532	rVV2	1525	1972	0.22%	0.020%
78	18.009	2532	2537	2540	rVV4	3230	5860	0.64%	0.058%
79	18.051	2542	2544	2547	rVV2	2033	2526	0.28%	0.025%
80	18.086	2547	2550	2554	rVB2	1650	2042	0.22%	0.020%
81	18.180	2561	2566	2568	rBV2	1006	1179	0.13%	0.012%
82	18.321	2584	2590	2593	rBV2	1874	2390	0.26%	0.024%
83	18.527	2620	2625	2628	rBV2	2780	4427	0.49%	0.044%
84	18.674	2644	2650	2651	rVB2	1076	1878	0.21%	0.019%
85	18.721	2655	2658	2662	rBV3	802	1458	0.16%	0.014%
86	18.874	2678	2684	2686	rVB3	2265	3248	0.36%	0.032%
87	18.986	2701	2703	2708	rVB3	788	1216	0.13%	0.012%
88	19.150	2727	2731	2734	rBV	3181	4385	0.48%	0.044%
89	19.403	2771	2774	2779	rBV	2614	3856	0.42%	0.038%
90	19.515	2787	2793	2800	rVV	527541	694616	76.35%	6.904%
91	19.562	2800	2801	2804	rVB	2164	2035	0.22%	0.020%
92	19.650	2815	2816	2820	rBV3	1255	1557	0.17%	0.015%
93	19.886	2852	2856	2857	rBV4	1150	1261	0.14%	0.013%
94	19.992	2872	2874	2876	rBV3	882	1109	0.12%	0.011%
95	20.668	2987	2989	2992	rBV4	2145	2356	0.26%	0.023%
96	21.021	3045	3049	3054	rBV3	25136	36002	3.96%	0.358%
97	21.221	3081	3083	3086	rVB	7468	8251	0.91%	0.082%
98	21.309	3093	3098	3108	rBV	719312	909766	100.00%	9.043%
99	23.421	3450	3457	3468	rBV	256597	490249	53.89%	4.873%
100	23.562	3474	3481	3493	rVB2	461596	890271	97.86%	8.849%


Sum of corrected areas: 10060387

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121315\
Data File : BM003530.D
Acq On : 14 Dec 2015 03:50
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C04F4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

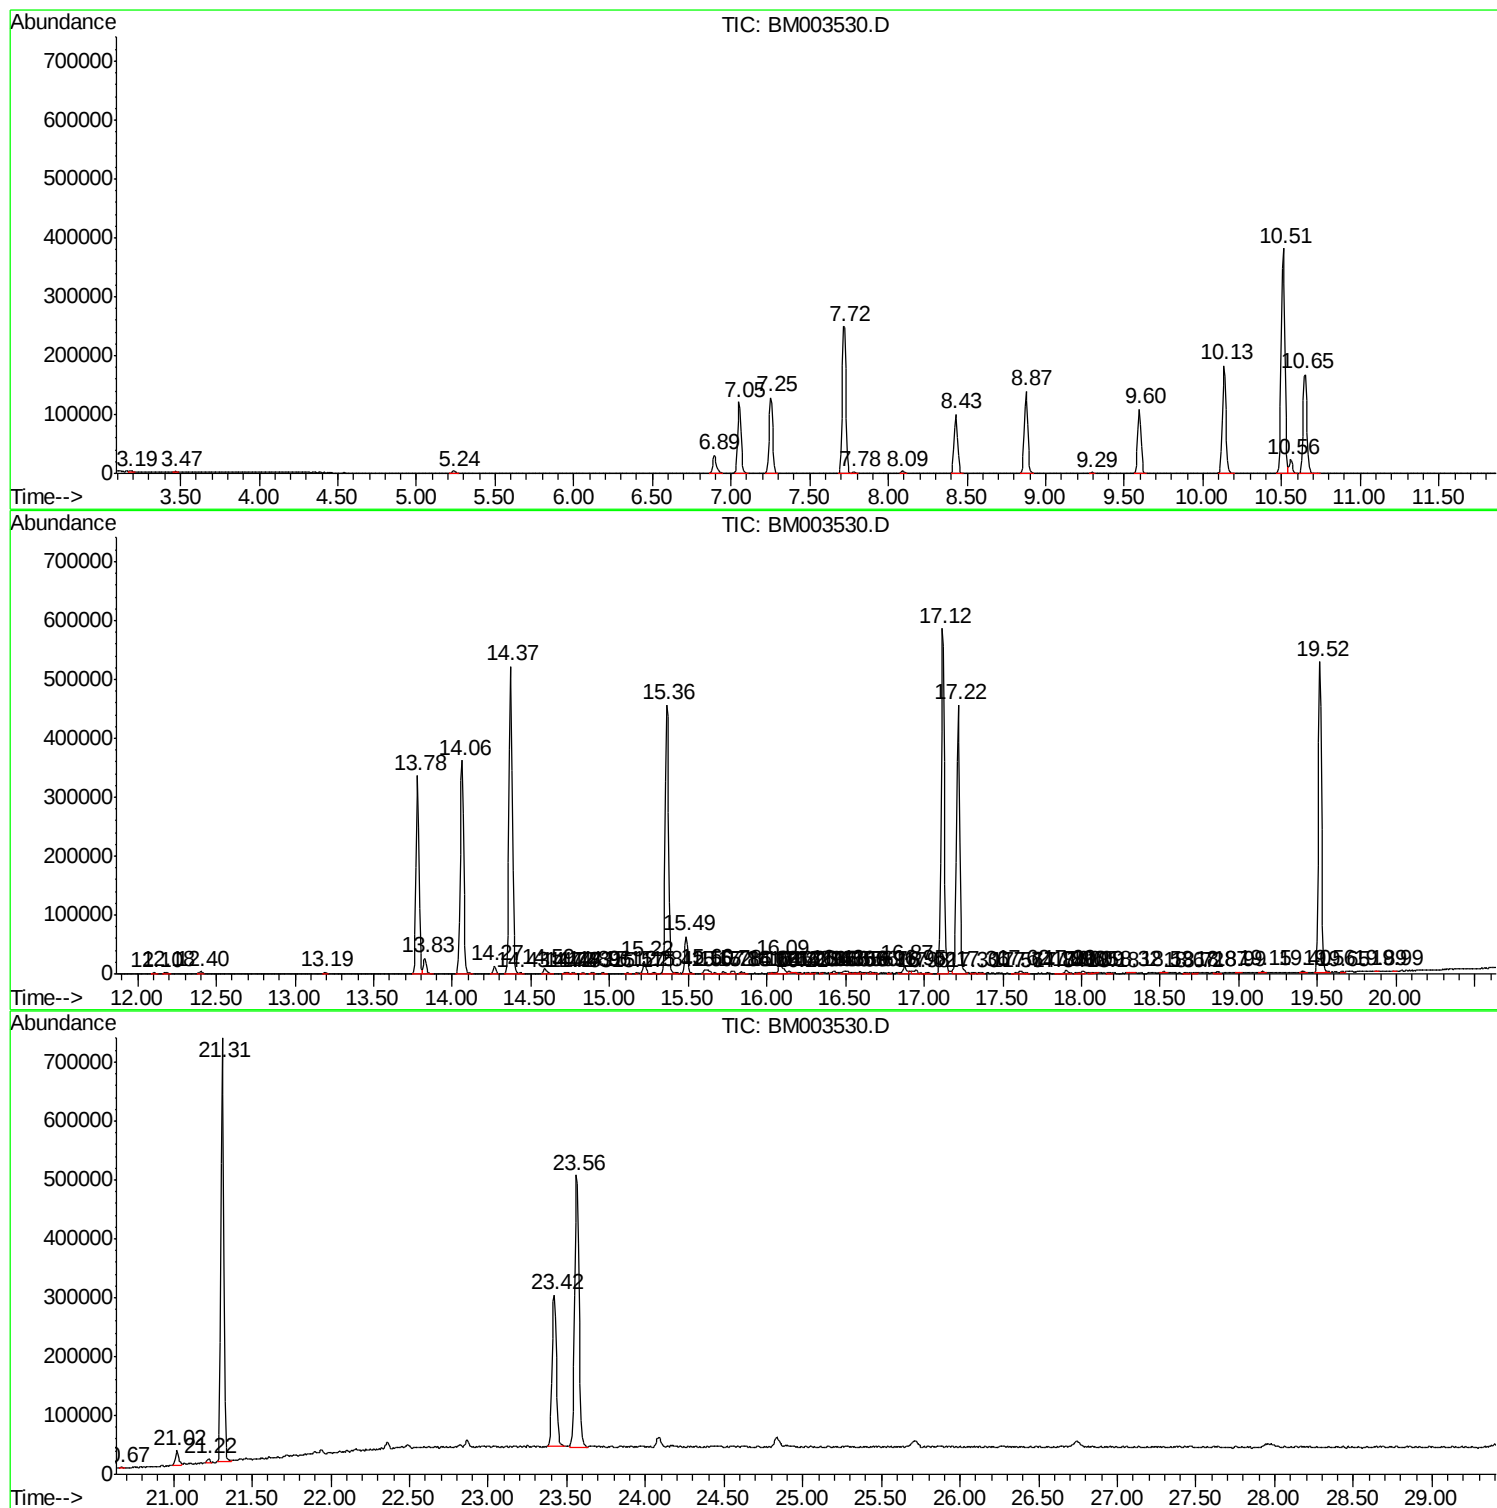

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003530.D
Acq On : 14 Dec 2015 03:50
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121315\
Data File : BM003530.D
Acq On : 14 Dec 2015 03:50
Operator : UM/IZ
Sample : G4722-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04F4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc