

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM121317\
 Data File : BM013374.D
 Acq On : 13 Dec 2017 15:25
 Operator : SJ/JU
 Sample : PB104951BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 13 17:32:04 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 04:59:25 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	147301	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	686074	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	447816	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1176110	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1346801	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	1145650	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	17913	6.02	ng/uL	0.00
5) Phenol-d5	6.86	99	381916	29.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	222667	30.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.22	132	308388	30.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.39	113	330797	30.38	ng/ul	0.00
19) Nitrobenzene-d5	8.84	128	168643	31.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	180093	30.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.09	165	337685	28.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	480503	43.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1240505	31.13	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1498066	30.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	205289	29.65	ng/ul	0.00
57) Fluorene-d10	15.32	176	1099320	32.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	161281	21.80	ng/ul	0.00
70) Anthracene-d10	17.17	188	1966932	33.39	ng/ul	0.00
76) Pyrene-d10	19.47	212	2319536	34.57	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	2001110	34.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.39	70	9165	1.099	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM121317\
Data File : BM013374.D
Acq On : 13 Dec 2017 15:25
Operator : SJ/JU
Sample : PB104951BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 13 17:32:04 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM113017.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 04:59:25 2017
Response via : Initial Calibration

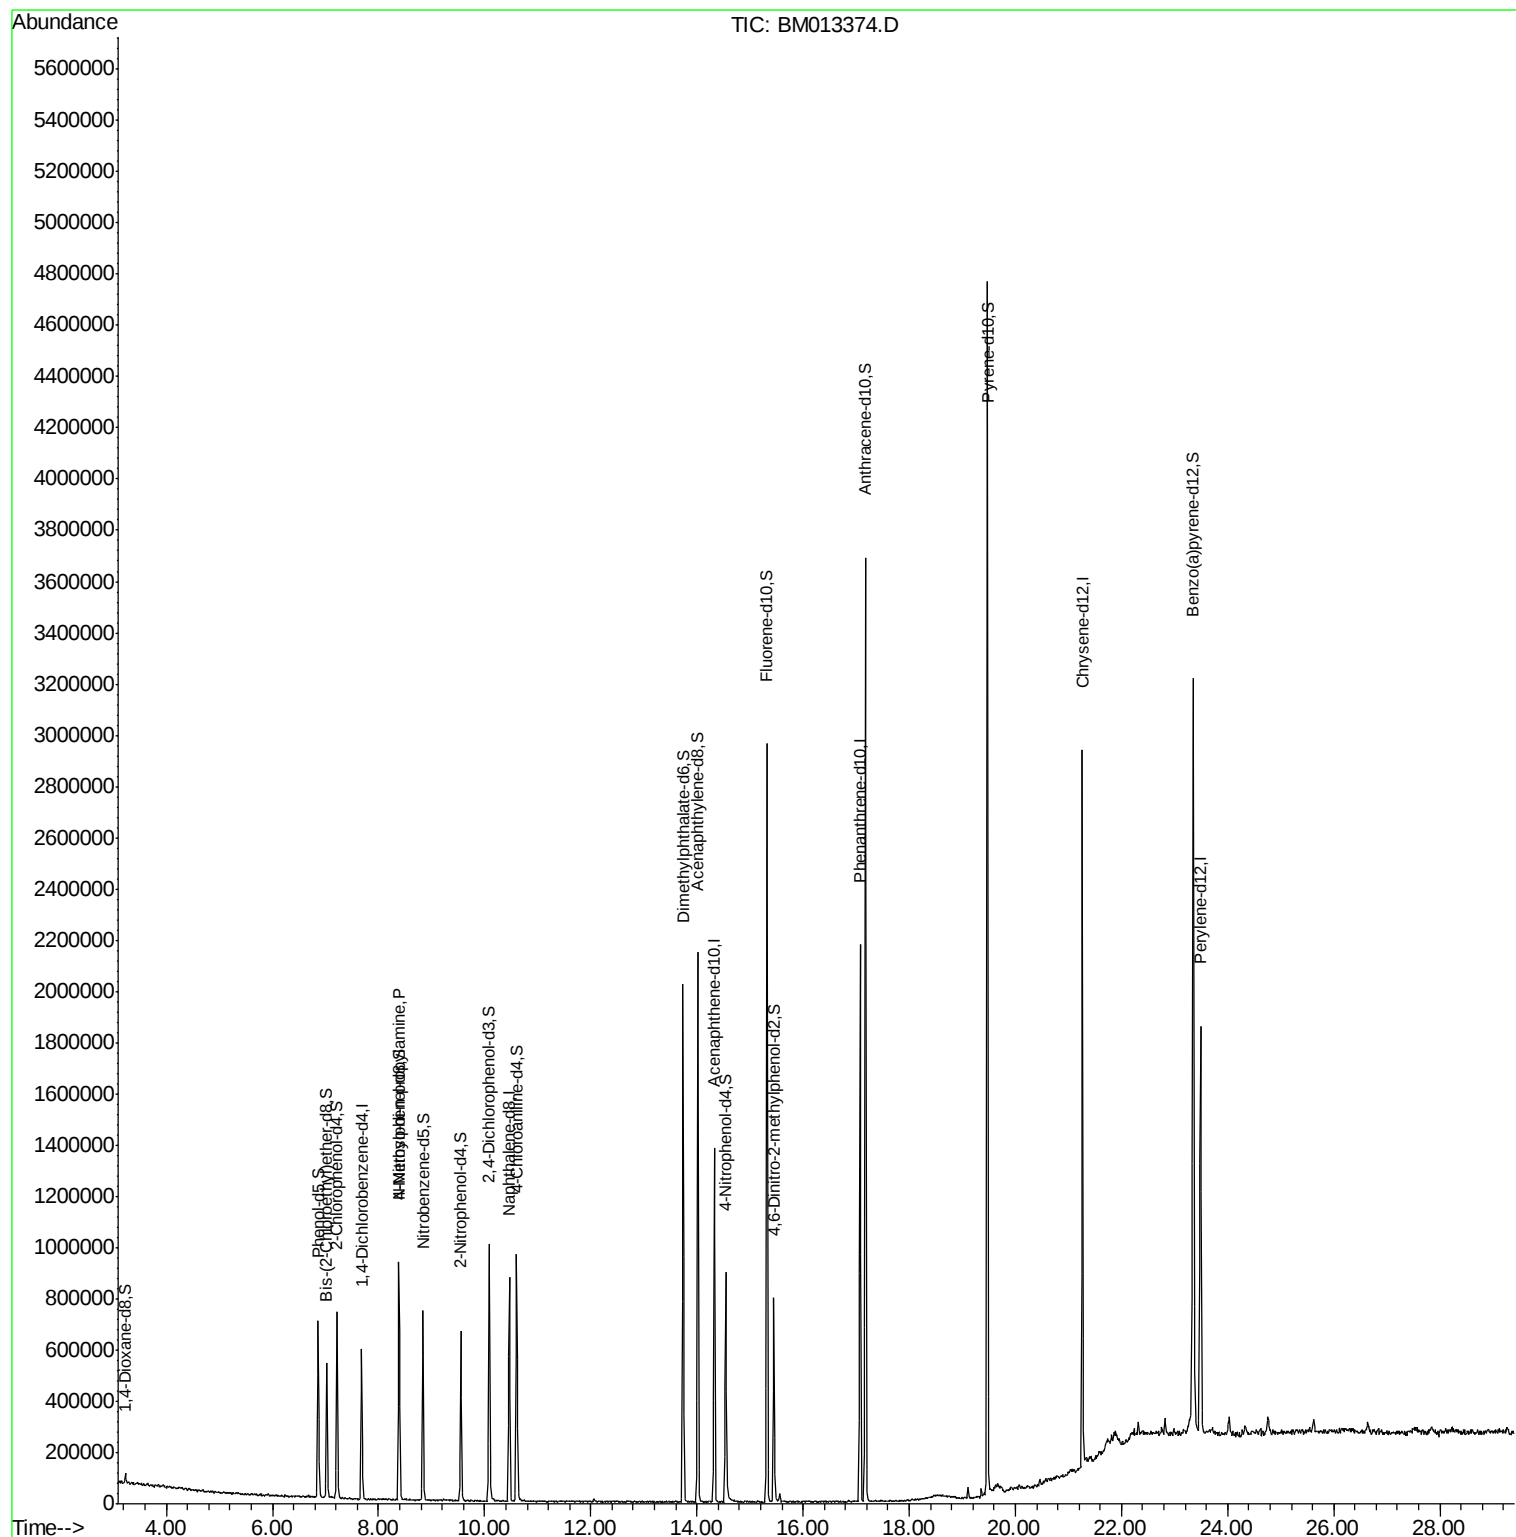

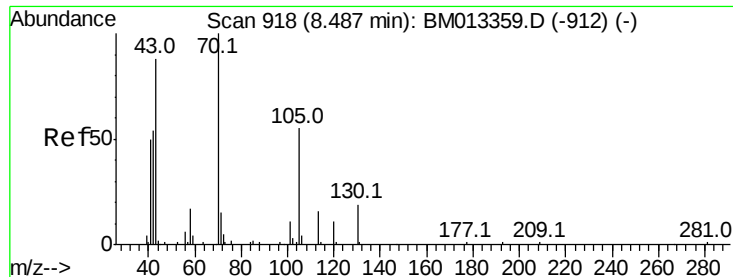

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.099 ng/ul
 RT: 8.39 min Scan# 902
 Delta R.T. -0.09 min
 Lab File: BM013374.D
 Acq: 13 Dec 2017 15:25

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 9165
 Ion Ratio Lower Upper
 70 100
 42 373.3 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

